

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD122920\
 Data File : PD060856.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Dec 2020 13:17
 Operator : DD\AJ
 Sample : INDA401
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 29 14:05:49 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD122920CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 29 13:12:41 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.500	4.021	42781901	192.5E6	36.298	38.033
27)	SA Decachlor...	8.285	9.103	105.4E6	305.3E6	72.666	73.764
Target Compounds							
2)	A alpha-BHC	3.941	4.411	64608106	291.7E6	39.313	39.579
3)	MA gamma-BHC...	4.227	4.697	60969784	264.5E6	38.680	39.578
4)	MA Heptachlor	4.532	5.208	64733562	262.2E6	38.497	38.619
9)	A Endosulfan I	5.570	6.259	54003054	211.8E6	37.514	38.652
13)	MA Dieldrin	5.815	6.516	123.2E6	460.8E6	80.608	79.025
14)	MA Endrin	6.073	6.734	102.2E6	369.2E6	77.410	78.245
16)	A 4,4'-DDD	6.197	6.854	97155426	360.6E6	79.550	78.730
17)	MA 4,4'-DDT	6.440	7.153	104.7E6	369.2E6	82.342	81.186
20)	A Methoxychlor	6.987	7.610	265.9E6	870.2E6	389.367	374.291


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD122920\
Data File : PD060856.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Dec 2020 13:17
Operator : DD\AJ
Sample : INDA401
Misc :
ALS Vial : 15 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 29 14:05:49 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD122920CLP.M
Quant Title : GC Extractables
QLast Update : Tue Dec 29 13:12:41 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

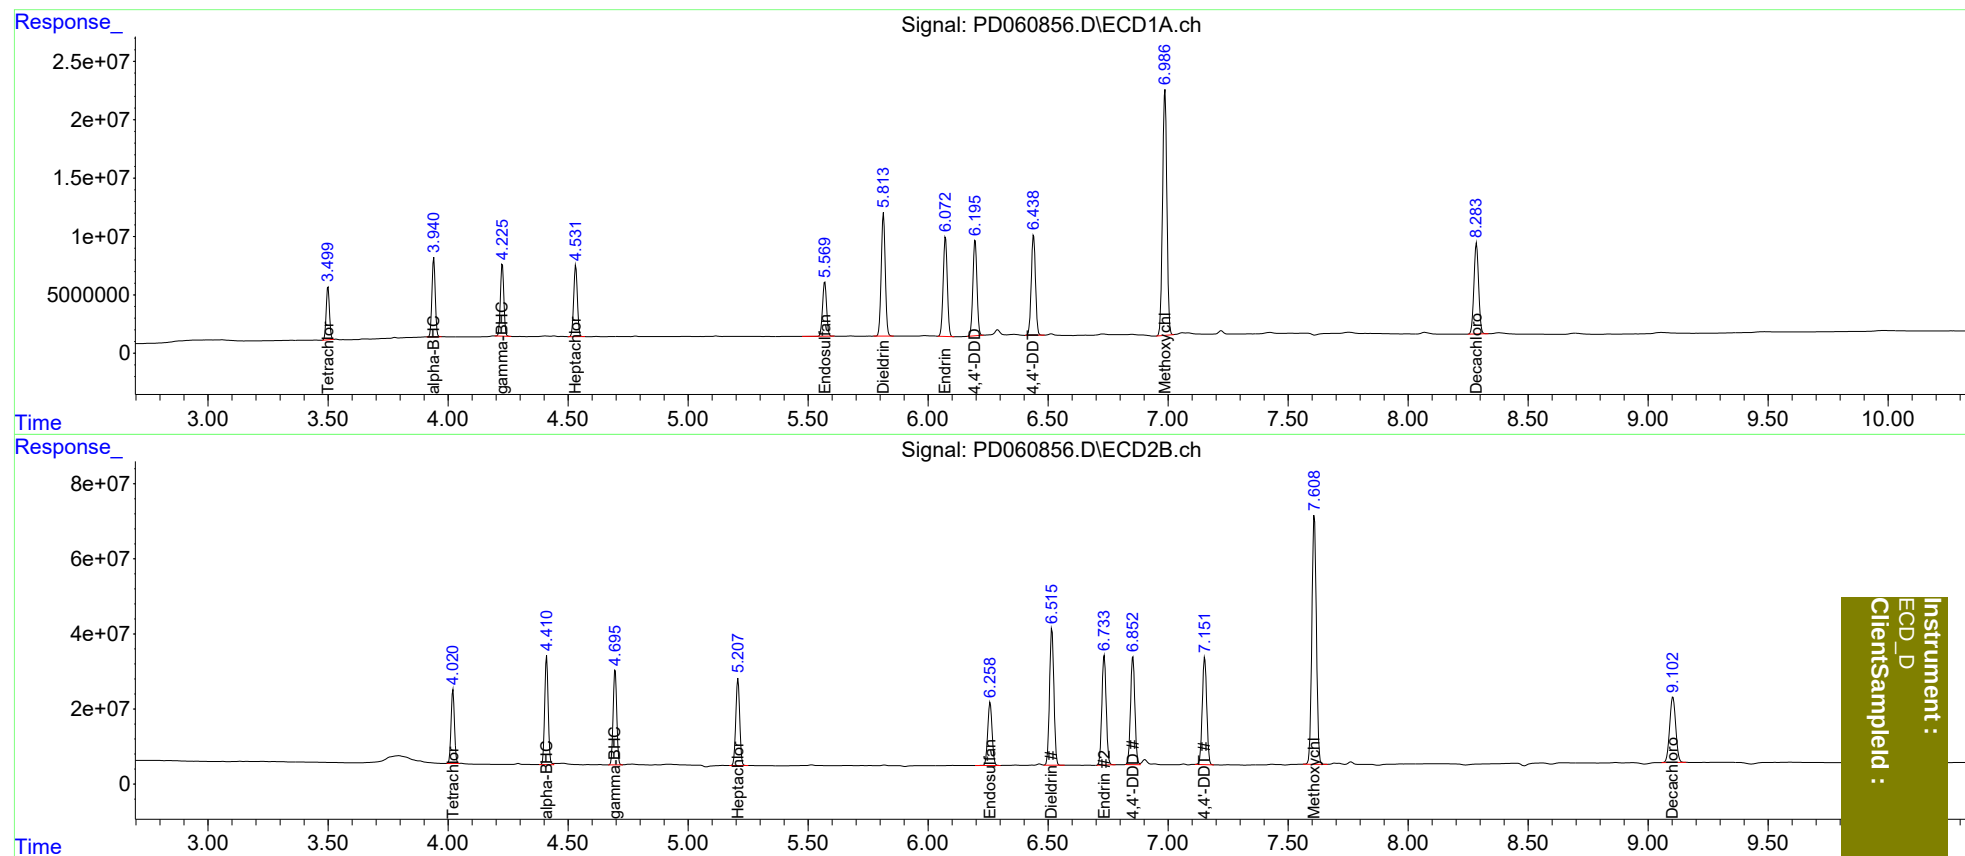


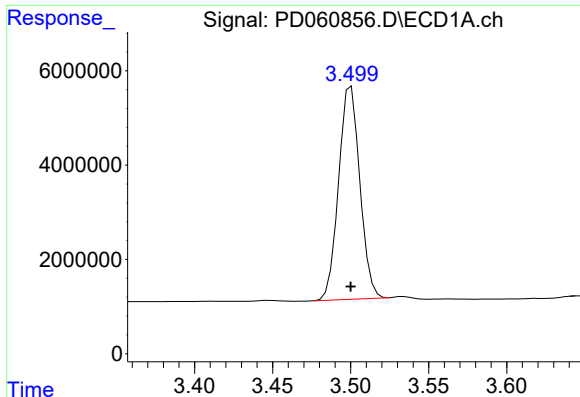

#1 Tetrachloro-m-xylene


R.T.: 3.500 min
Delta R.T.: 0.000 min
Response: 42781901
Conc: 36.30 ng/ml

Instrument :
ECD_D
ClientSampleId :

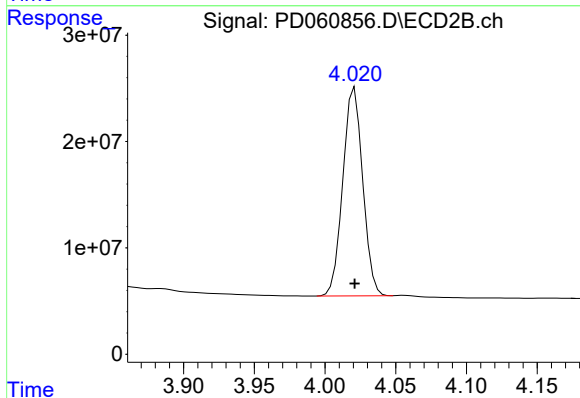


#1 Tetrachloro-m-xylene

R.T.: 4.021 min
Delta R.T.: 0.000 min
Response: 192506475
Conc: 38.03 ng/ml

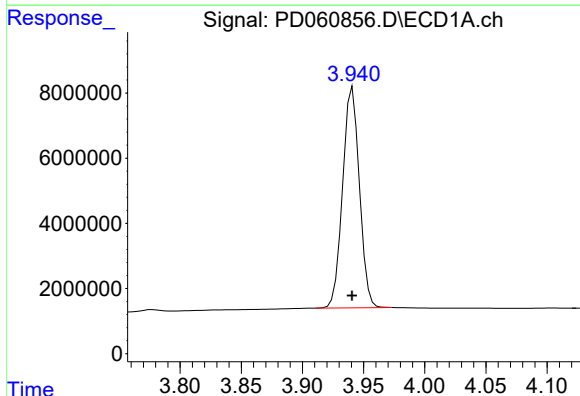


#2 alpha-BHC

R.T.: 3.941 min
Delta R.T.: 0.000 min
Response: 64608106
Conc: 39.31 ng/ml

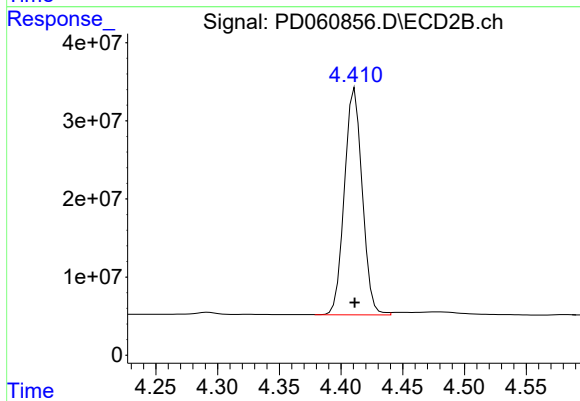

#2 alpha-BHC


R.T.: 4.411 min
Delta R.T.: 0.000 min
Response: 291745375
Conc: 39.58 ng/ml

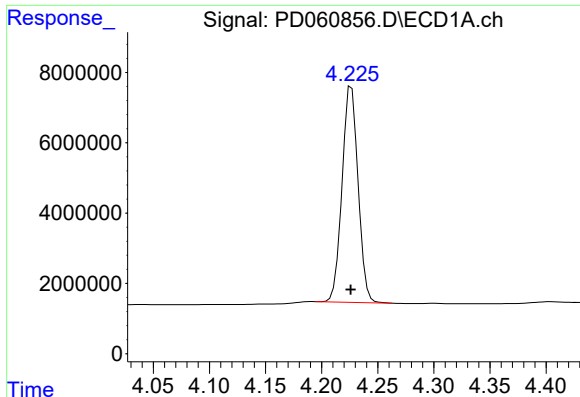

#3 gamma-BHC (Lindane)


R.T.: 4.227 min
Delta R.T.: 0.000 min
Response: 60969784
Conc: 38.68 ng/ml

Instrument :
ECD_D
ClientSampleId :

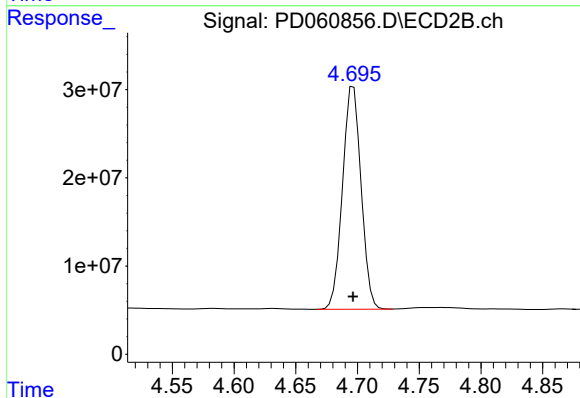


#3 gamma-BHC (Lindane)

R.T.: 4.697 min
Delta R.T.: 0.000 min
Response: 264495178
Conc: 39.58 ng/ml

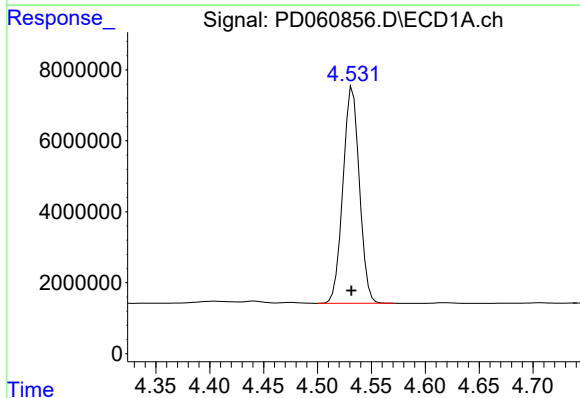


#4 Heptachlor

R.T.: 4.532 min
Delta R.T.: 0.001 min
Response: 64733562
Conc: 38.50 ng/ml

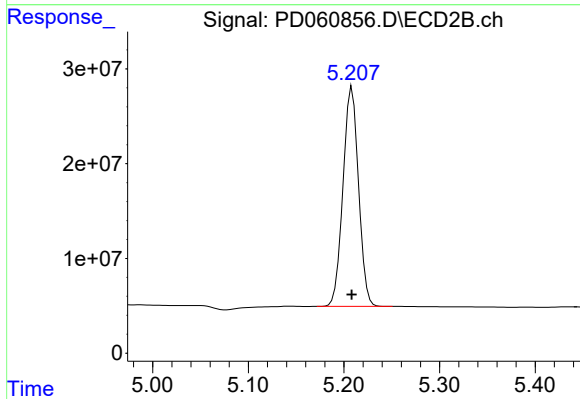

#4 Heptachlor


R.T.: 5.208 min
Delta R.T.: 0.000 min
Response: 262197438
Conc: 38.62 ng/ml

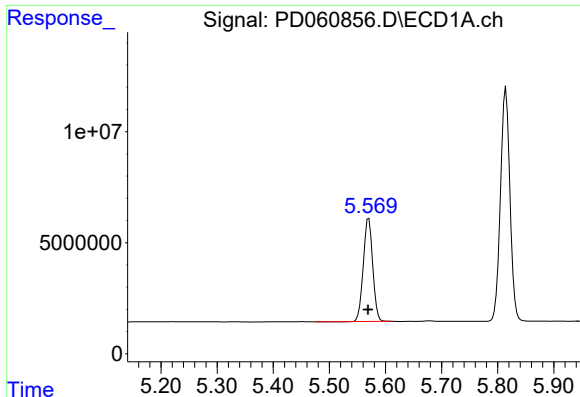

#9 Endosulfan I


R.T.: 5.570 min
Delta R.T.: 0.001 min
Response: 54003054
Conc: 37.51 ng/ml

Instrument :
ECD_D
ClientSampleId :

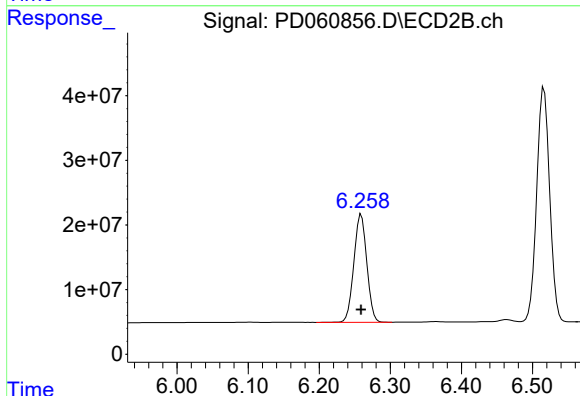


#9 Endosulfan I

R.T.: 6.259 min
Delta R.T.: 0.000 min
Response: 211752797
Conc: 38.65 ng/ml

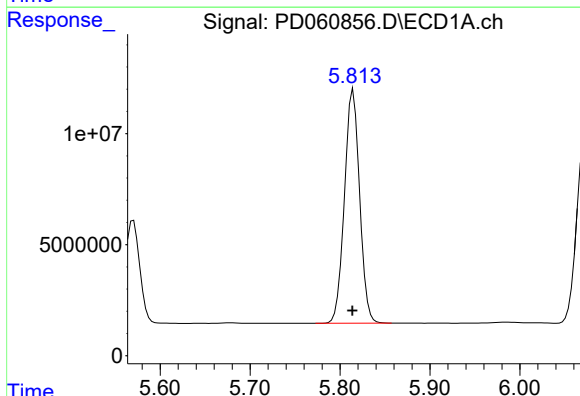


#13 Dieldrin

R.T.: 5.815 min
Delta R.T.: 0.000 min
Response: 123162400
Conc: 80.61 ng/ml

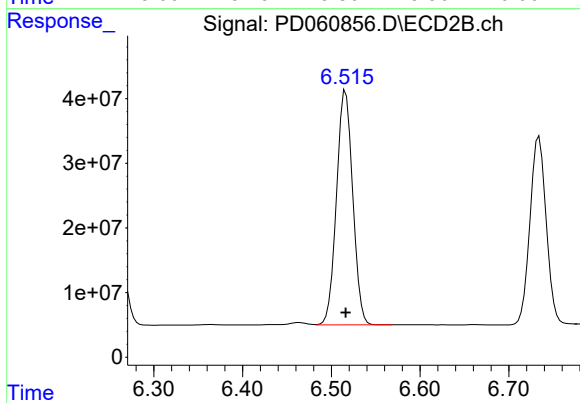

#13 Dieldrin


R.T.: 6.516 min
Delta R.T.: 0.000 min
Response: 460784224
Conc: 79.02 ng/ml

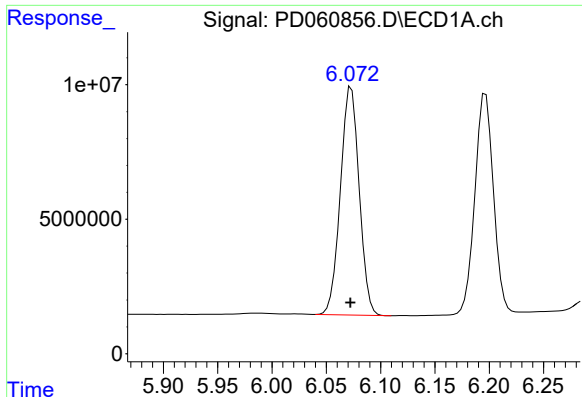

#14 Endrin


R.T.: 6.073 min
Delta R.T.: 0.000 min
Response: 102203616
Conc: 77.41 ng/ml

Instrument :
ECD_D
ClientSampleId :

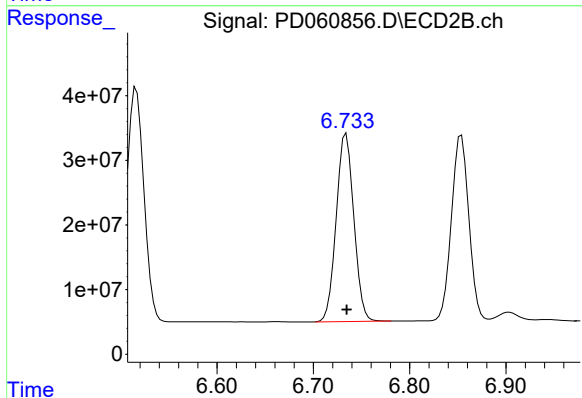


#14 Endrin

R.T.: 6.734 min
Delta R.T.: 0.000 min
Response: 369165246
Conc: 78.24 ng/ml

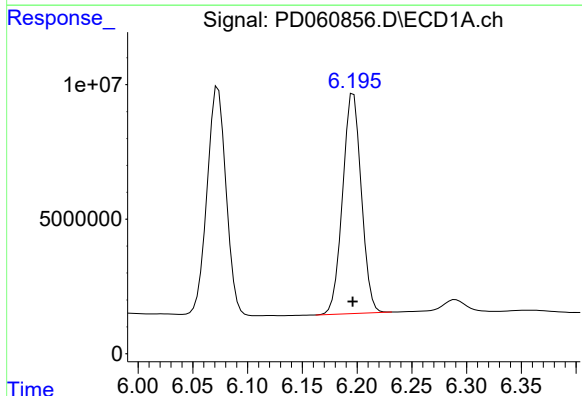


#16 4,4'-DDD

R.T.: 6.197 min
Delta R.T.: 0.000 min
Response: 97155426
Conc: 79.55 ng/ml

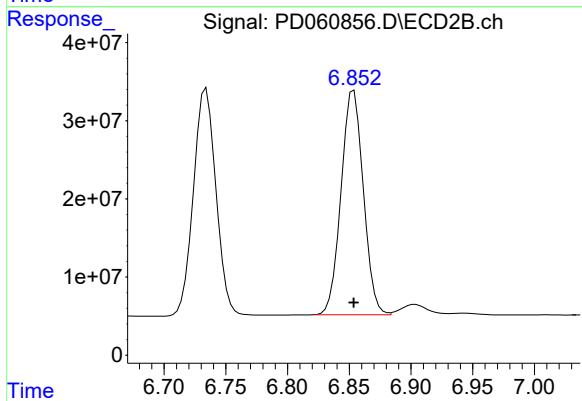

#16 4,4'-DDD


R.T.: 6.854 min
Delta R.T.: 0.000 min
Response: 360645454
Conc: 78.73 ng/ml

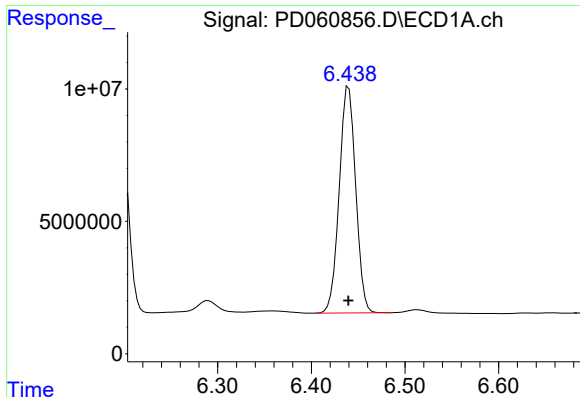

#17 4,4'-DDT


R.T.: 6.440 min
Delta R.T.: 0.000 min
Response: 104662302
Conc: 82.34 ng/ml

Instrument :
ECD_D
ClientSampleId :

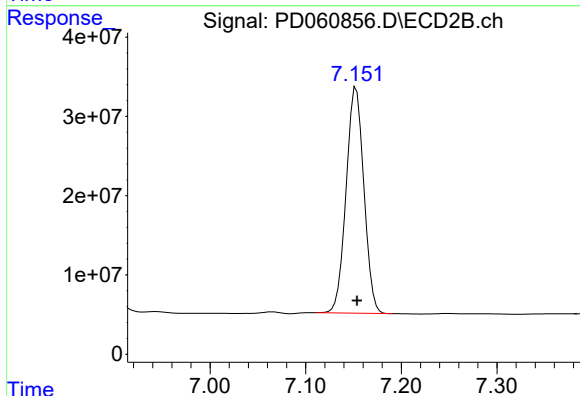


#17 4,4'-DDT

R.T.: 7.153 min
Delta R.T.: 0.000 min
Response: 369197575
Conc: 81.19 ng/ml

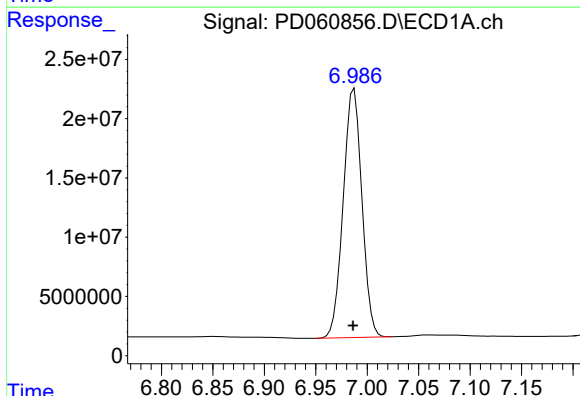


#20 Methoxychlor

R.T.: 6.987 min
Delta R.T.: 0.001 min
Response: 265926540
Conc: 389.37 ng/ml

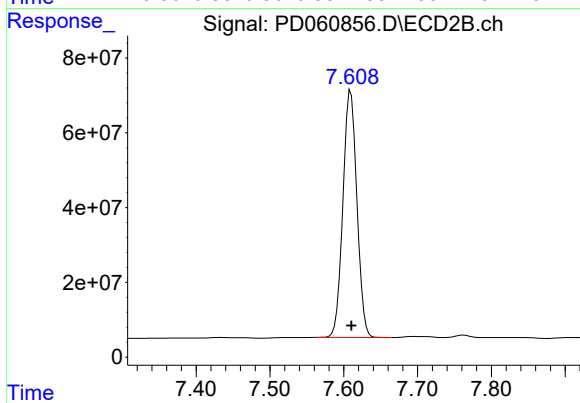

#20 Methoxychlor


R.T.: 7.610 min
Delta R.T.: 0.000 min
Response: 870174801
Conc: 374.29 ng/ml

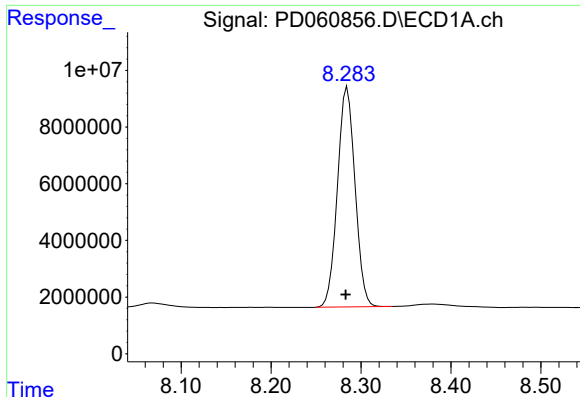

#27 Decachlorobiphenyl

R.T.: 8.285 min
Delta R.T.: 0.002 min
Response: 105359359
Conc: 72.67 ng/ml

Instrument :
ECD_D
ClientSampleId :

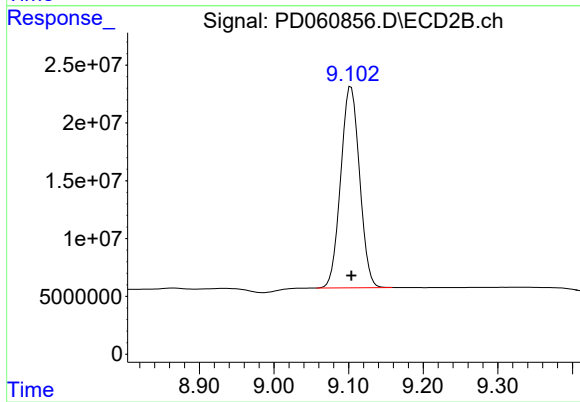

#27 Decachlorobiphenyl

R.T.: 9.103 min
Delta R.T.: 0.000 min
Response: 305334964
Conc: 73.76 ng/ml