

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD122920\
 Data File : PD060858.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Dec 2020 13:45
 Operator : DD\AJ
 Sample : INDA501
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 29 14:05:58 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD122920CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 29 13:12:41 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.500	4.021	83108444	370.3E6	70.513	73.166
27)	SA Decachlor...	8.285	9.104	196.8E6	564.3E6	135.748	136.320
Target Compounds							
2)	A alpha-BHC	3.941	4.411	129.1E6	566.9E6	78.576	76.904
3)	MA gamma-BHC...	4.227	4.697	120.3E6	513.8E6	76.313	76.890
4)	MA Heptachlor	4.532	5.209	126.7E6	503.2E6	75.378	74.119
9)	A Endosulfan I	5.570	6.259	105.3E6	402.7E6	73.122	73.511
13)	MA Dieldrin	5.815	6.516	243.5E6	883.7E6	159.348	151.563
14)	MA Endrin	6.073	6.735	197.3E6	700.5E6	149.413	148.467
16)	A 4,4'-DDD	6.197	6.854	191.4E6	690.7E6	156.746	150.783
17)	MA 4,4'-DDT	6.439	7.154	207.8E6	710.5E6	163.483	156.235
20)	A Methoxychlor	6.987	7.611	496.9E6	1595.7E6	727.616	686.343


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD122920\
Data File : PD060858.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Dec 2020 13:45
Operator : DD\AJ
Sample : INDA501
Misc :
ALS Vial : 17 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 29 14:05:58 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD122920CLP.M
Quant Title : GC Extractables
QLast Update : Tue Dec 29 13:12:41 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

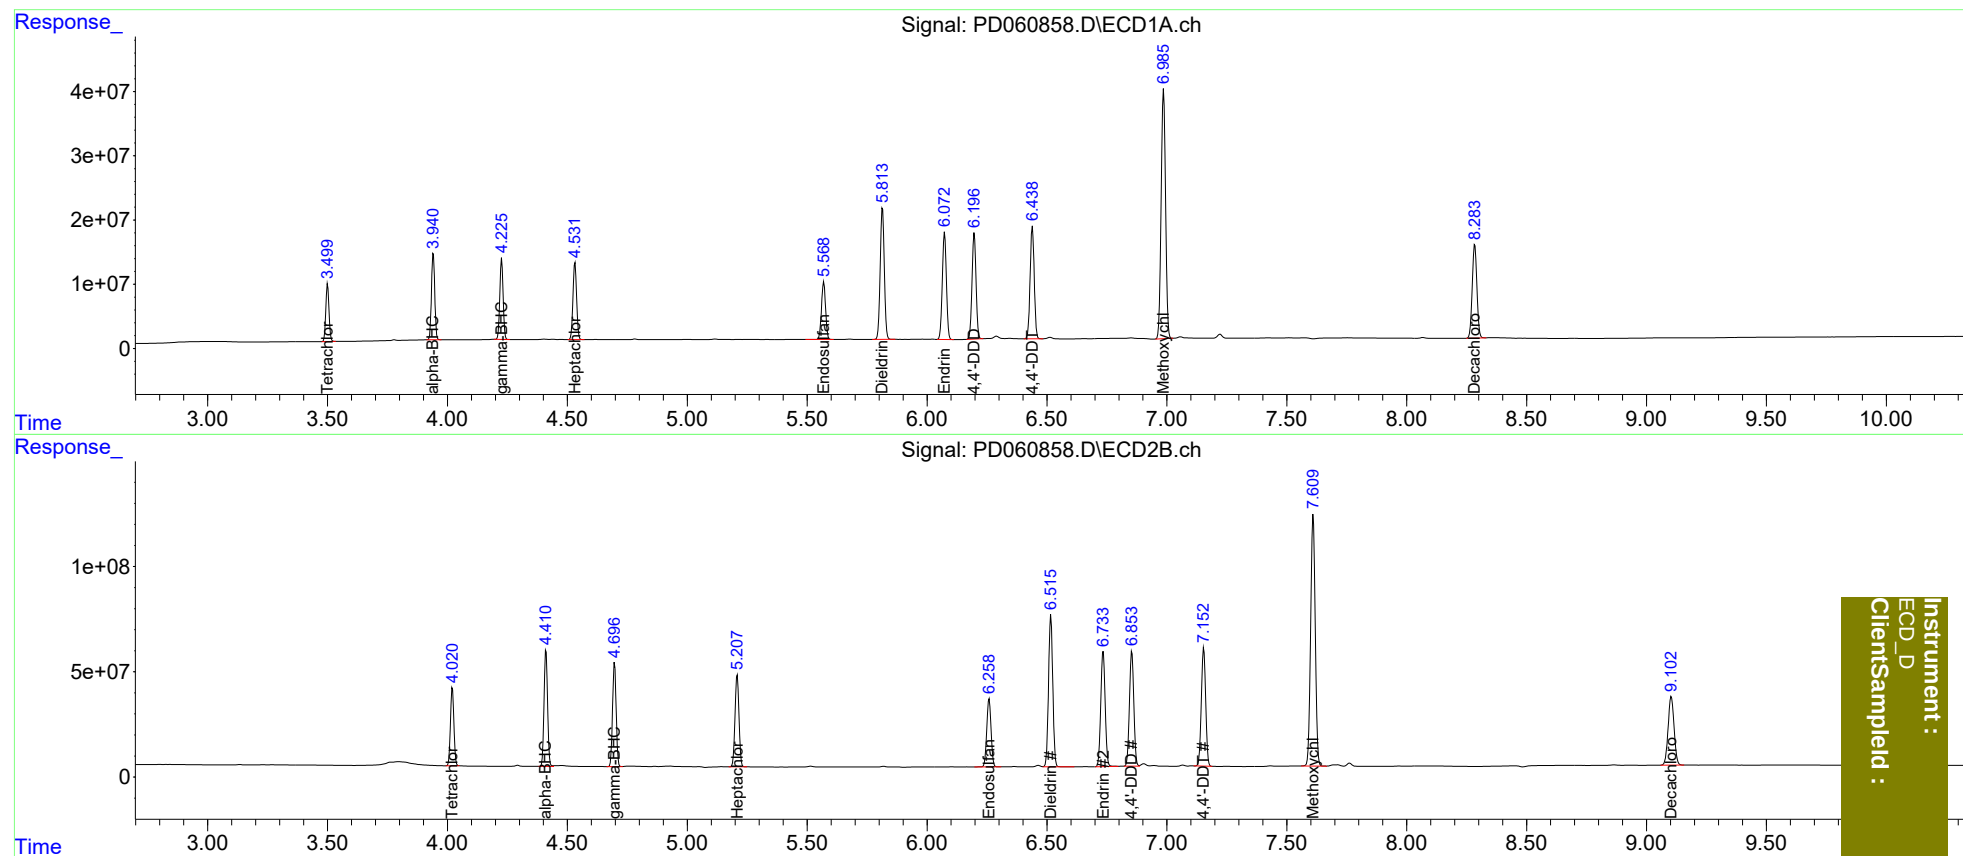


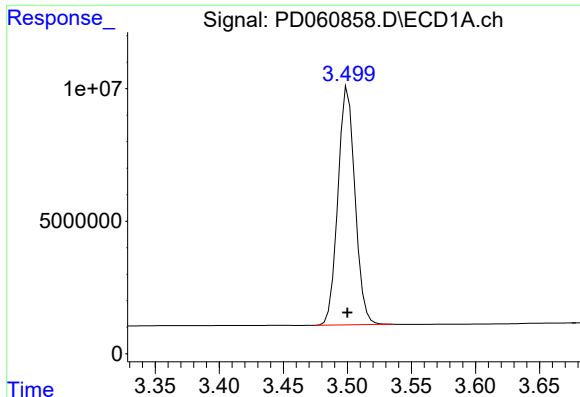

#1 Tetrachloro-m-xylene


R.T.: 3.500 min
Delta R.T.: 0.000 min
Response: 83108444
Conc: 70.51 ng/ml

Instrument :
ECD_D
ClientSampleId :

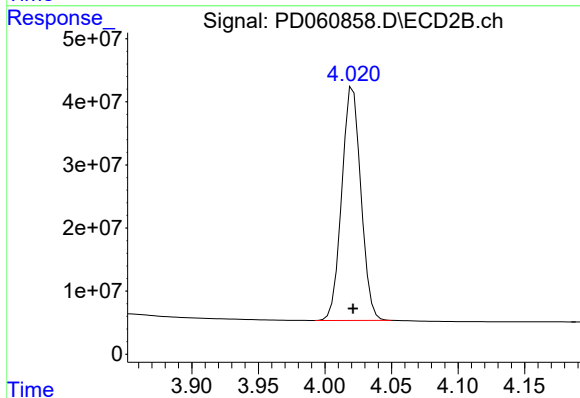


#1 Tetrachloro-m-xylene

R.T.: 4.021 min
Delta R.T.: 0.000 min
Response: 370331881
Conc: 73.17 ng/ml

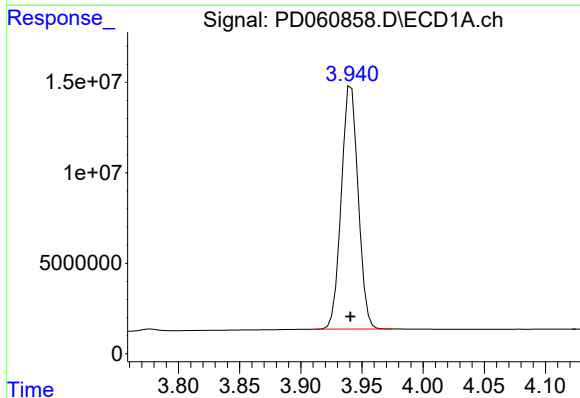


#2 alpha-BHC

R.T.: 3.941 min
Delta R.T.: 0.000 min
Response: 129134980
Conc: 78.58 ng/ml

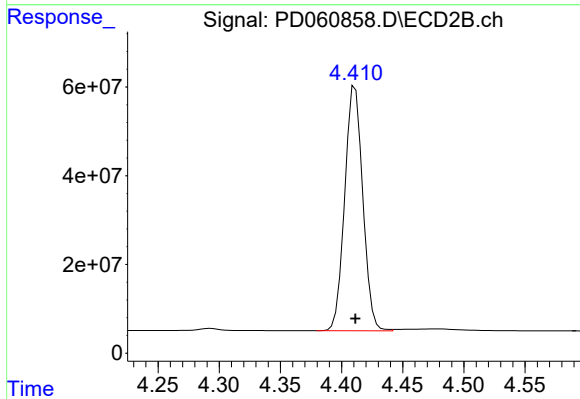

#2 alpha-BHC


R.T.: 4.411 min
Delta R.T.: 0.000 min
Response: 566874391
Conc: 76.90 ng/ml

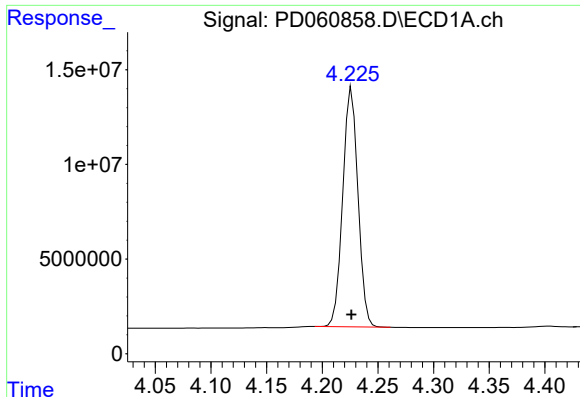

#3 gamma-BHC (Lindane)


R.T.: 4.227 min
Delta R.T.: 0.000 min
Response: 120288668
Conc: 76.31 ng/ml

Instrument :
ECD_D
ClientSampleId :

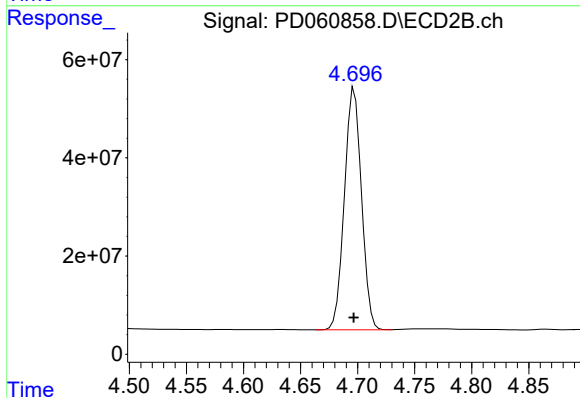


#3 gamma-BHC (Lindane)

R.T.: 4.697 min
Delta R.T.: 0.000 min
Response: 513843734
Conc: 76.89 ng/ml

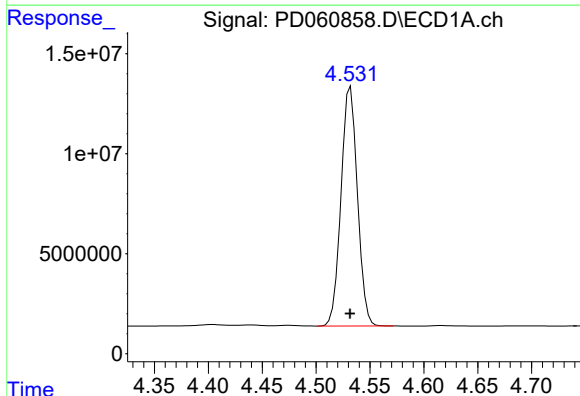


#4 Heptachlor

R.T.: 4.532 min
Delta R.T.: 0.000 min
Response: 126748394
Conc: 75.38 ng/ml

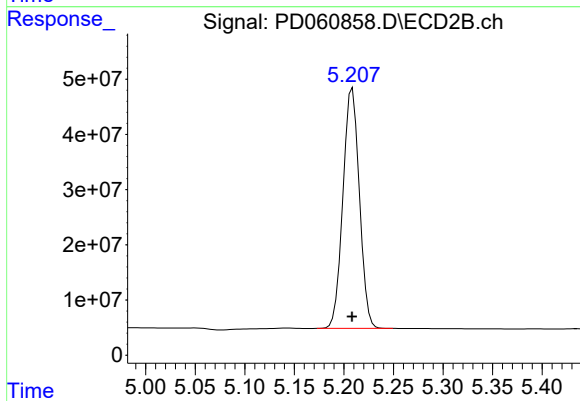

#4 Heptachlor


R.T.: 5.209 min
Delta R.T.: 0.000 min
Response: 503216735
Conc: 74.12 ng/ml

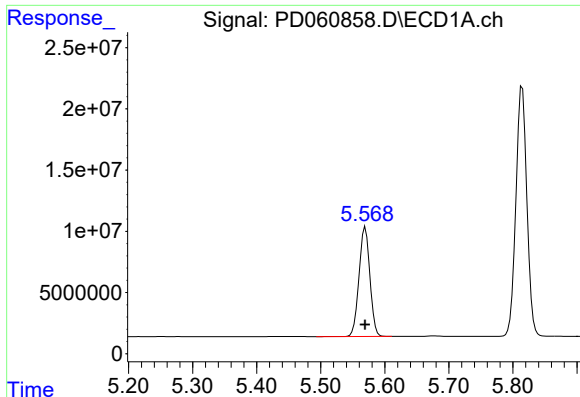

#9 Endosulfan I


R.T.: 5.570 min
Delta R.T.: 0.000 min
Response: 105262671
Conc: 73.12 ng/ml

Instrument :
ECD_D
ClientSampleId :

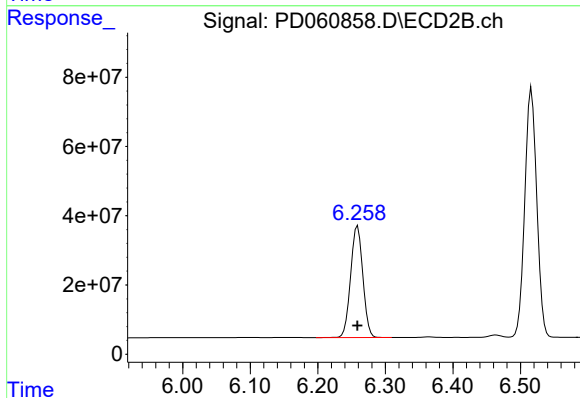


#9 Endosulfan I

R.T.: 6.259 min
Delta R.T.: 0.000 min
Response: 402727996
Conc: 73.51 ng/ml

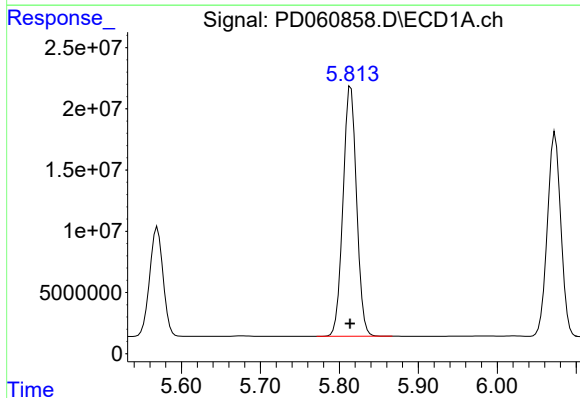


#13 Dieldrin

R.T.: 5.815 min
Delta R.T.: 0.000 min
Response: 243471365
Conc: 159.35 ng/ml

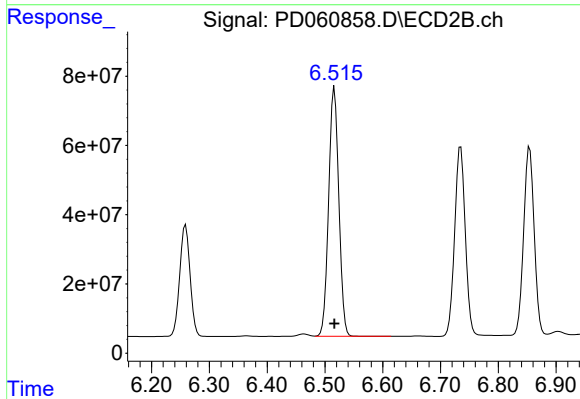

#13 Dieldrin


R.T.: 6.516 min
Delta R.T.: 0.000 min
Response: 883745567
Conc: 151.56 ng/ml

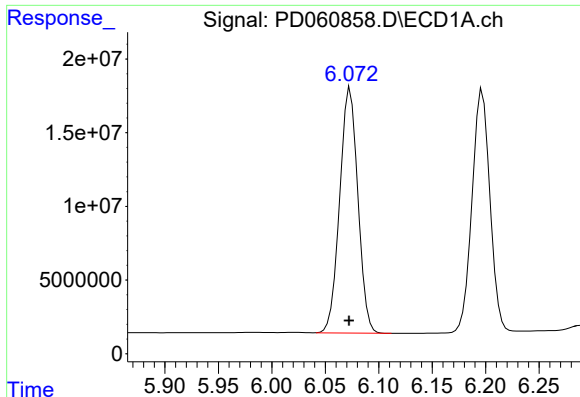

#14 Endrin


R.T.: 6.073 min
Delta R.T.: 0.001 min
Response: 197268559
Conc: 149.41 ng/ml

Instrument :
ECD_D
ClientSampleId :

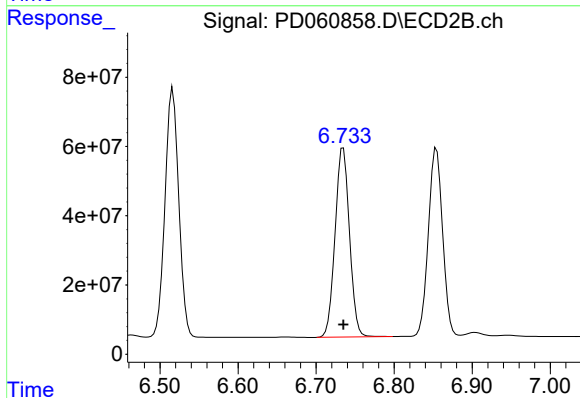


#14 Endrin

R.T.: 6.735 min
Delta R.T.: 0.000 min
Response: 700477255
Conc: 148.47 ng/ml

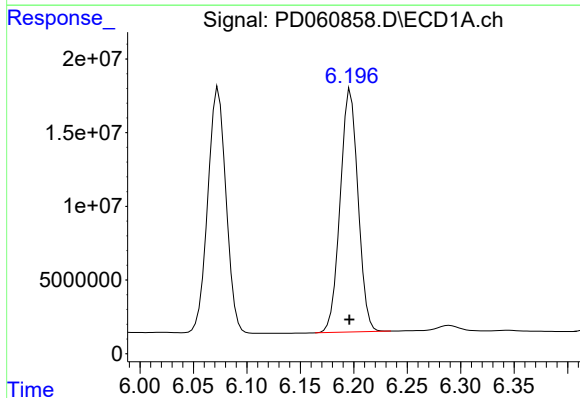


#16 4,4'-DDD

R.T.: 6.197 min
Delta R.T.: 0.001 min
Response: 191437095
Conc: 156.75 ng/ml

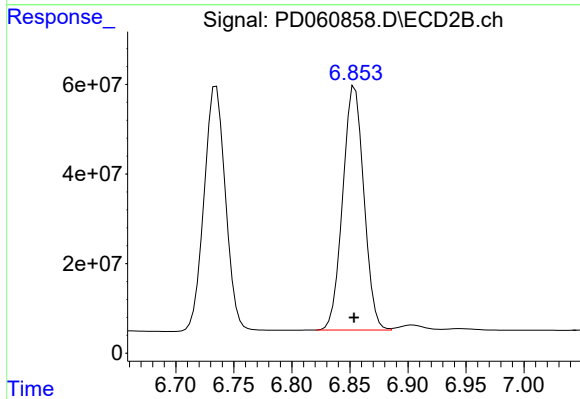

#16 4,4'-DDD


R.T.: 6.854 min
Delta R.T.: 0.000 min
Response: 690703814
Conc: 150.78 ng/ml

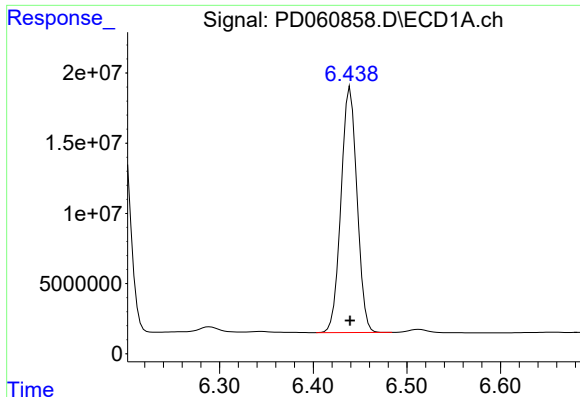

#17 4,4'-DDT


R.T.: 6.439 min
Delta R.T.: 0.000 min
Response: 207797229
Conc: 163.48 ng/ml

Instrument :
ECD_D
ClientSampleId :

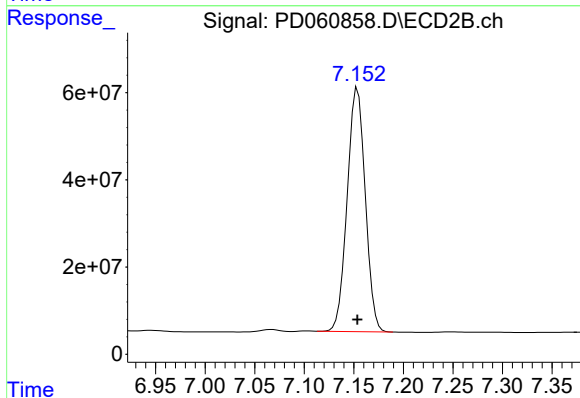


#17 4,4'-DDT

R.T.: 7.154 min
Delta R.T.: 0.000 min
Response: 710485563
Conc: 156.23 ng/ml

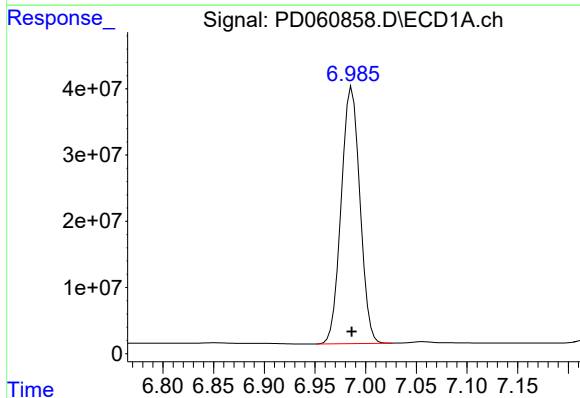


#20 Methoxychlor

R.T.: 6.987 min
Delta R.T.: 0.000 min
Response: 496941393
Conc: 727.62 ng/ml

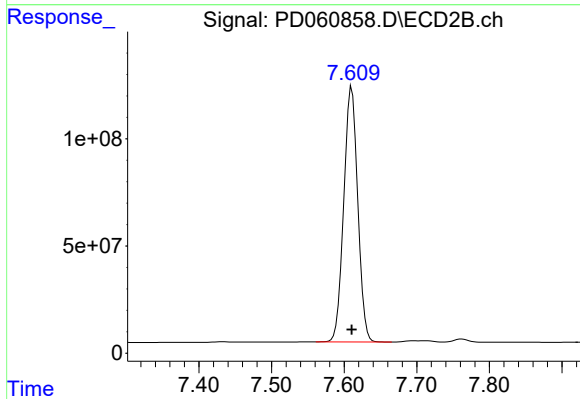

#20 Methoxychlor

R.T.: 7.611 min
Delta R.T.: 0.000 min
Response: 1595653643
Conc: 686.34 ng/ml

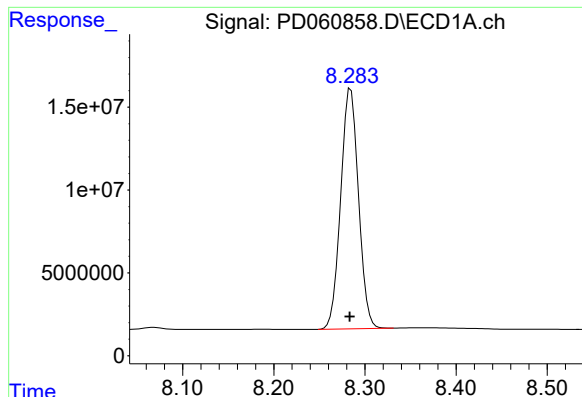

#27 Decachlorobiphenyl


R.T.: 8.285 min

Delta R.T.: 0.001 min

Response: 196823424

Conc: 135.75 ng/ml

Instrument :
ECD_D
ClientSampleId :

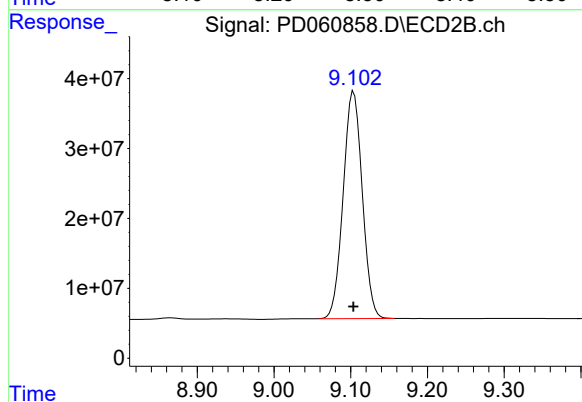

#27 Decachlorobiphenyl

R.T.: 9.104 min

Delta R.T.: 0.000 min

Response: 564276130

Conc: 136.32 ng/ml