

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD122920\
 Data File : PD060843.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Dec 2020 10:14
 Operator : DD\AJ
 Sample : RESC13
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 RESC013

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 30 01:16:49 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD122920CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Dec 30 01:06:43 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.500	4.021	22412757	99336080	19.854	20.169
27)	SA Decachlor...	8.284	9.103	53585474	156.2E6	38.848	39.517
Target Compounds							
2)	A alpha-BHC	3.941	4.412	16050161	72881299	9.835	9.986
3)	MA gamma-BHC...	4.226	4.697	15336248	66713630	9.886	10.083
4)	MA Heptachlor	4.532	5.209	16565657	65153364	10.043	9.808
5)	MB Aldrin	4.783	5.515	15435246	61070933	10.058	10.060
6)	B beta-BHC	4.476	4.865	7925177	31463033	10.701	10.621
7)	B delta-BHC	4.683	5.085	15187097	47586157	9.978	8.755
8)	B Heptachlo...	5.229	5.901	14742142	45860915	10.099	9.099
9)	A Endosulfan I	5.569	6.259	14077004	53347831	10.077	9.967
10)	B trans-Chl...	5.457	6.136	15232577	57007799	10.046	9.901
11)	B cis-Chlor...	5.515	6.208	14977275	56600346	10.057	10.149
12)	B 4,4'-DDE	5.679	6.364	28863693	108.1E6	19.727	19.868
13)	MA Dieldrin	5.815	6.517	29679553	113.0E6	19.411	19.636
14)	MA Endrin	6.073	6.735	25917343	93341826	20.025	20.163
15)	B Endosulfa...	6.346	6.943	23149554	94738118	19.170	20.787
16)	A 4,4'-DDD	6.197	6.854	23559609	90907613	19.391	20.141
17)	MA 4,4'-DDT	6.440	7.154	24640715	92240635	19.190	20.319
18)	B Endrin al...	6.515	7.067	22257423	76669342	21.115	20.416
19)	B Endosulfa...	6.729	7.290	23704028	91822243	20.362	20.532
20)	A Methoxychlor	6.987	7.610	67833406	227.9E6	101.702	102.229
21)	B Endrin ke...	7.224	7.762	28551429	95219263	20.674	20.427

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD122920\
Data File : PD060843.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Dec 2020 10:14
Operator : DD\AJ
Sample : RESC13
Misc :
ALS Vial : 2 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 30 01:16:49 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD122920CLP.M
Quant Title : GC Extractables
QLast Update : Wed Dec 30 01:06:43 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

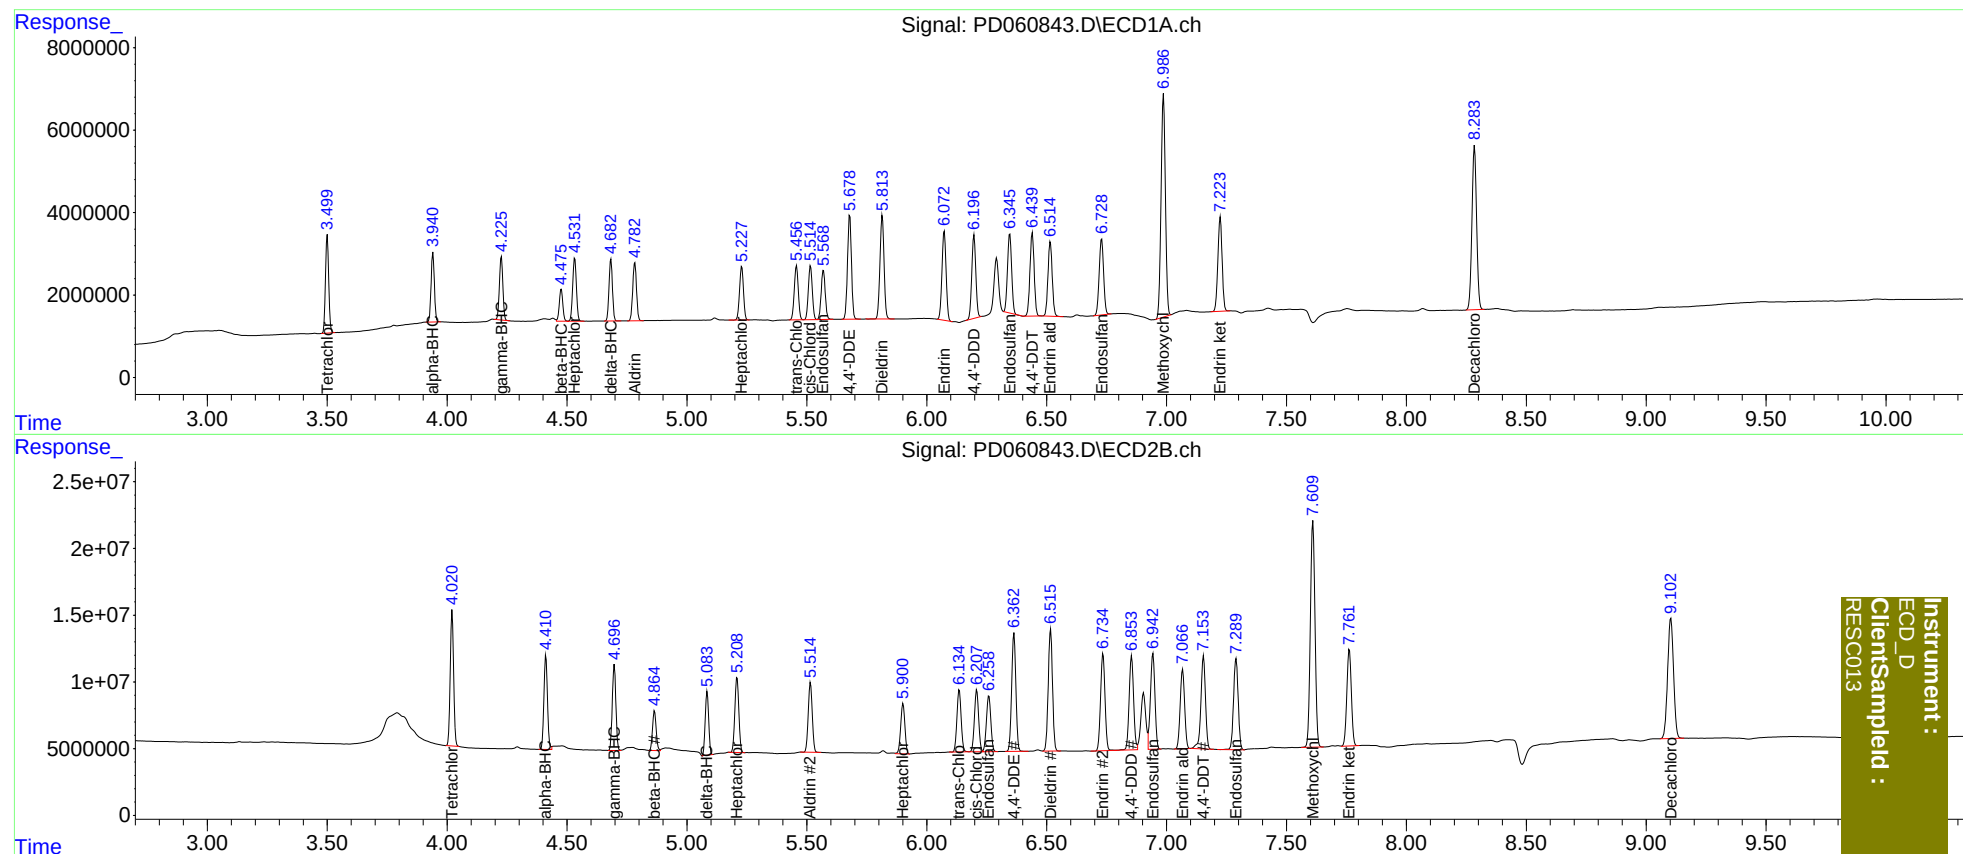

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD122920\
Data File : PD060843.D
Acq On : 29 Dec 2020 10:14
Operator : DD\AJ
Sample : RESC13
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESC013

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e

Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD122920CLP.M
Title : GC Extractables
Last Update : Wed Dec 30 01:06:43 2020
Integrator: ChemStation

RT#1	RT#2	Resolution
3.500	3.941	100.00%
3.941	4.226	100.00%
4.226	4.476	100.00%
4.476	4.532	98.47%
4.532	4.683	100.00%
4.683	4.783	100.00%
4.783	5.229	100.00%
5.229	5.457	100.00%
5.457	5.515	100.00%
5.515	5.569	99.58%
5.569	5.679	100.00%
5.679	5.815	100.00%
5.815	6.073	100.00%
6.073	6.197	100.00%
6.197	6.346	100.00%
6.346	6.440	100.00%
6.440	6.515	100.00%
6.515	6.730	100.00%
6.730	6.987	100.00%
6.987	7.224	100.00%
7.224	8.284	100.00%

Signal #2


4.021	4.412	100.00%
4.412	4.697	100.00%
4.697	4.865	100.00%
4.865	5.085	100.00%
5.085	5.209	100.00%
5.209	5.515	100.00%
5.515	5.901	100.00%
5.901	6.136	100.00%
6.136	6.208	100.00%
6.208	6.259	98.43%
6.259	6.364	100.00%
6.364	6.517	100.00%
6.517	6.735	100.00%
6.735	6.854	100.00%
6.854	6.943	100.00%
6.943	7.067	100.00%
7.067	7.154	100.00%
7.154	7.290	100.00%
7.290	7.610	100.00%
7.610	7.762	100.00%
7.762	9.103	100.00%

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD122920\
Data File : PD060843.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Dec 2020 10:14
Operator : DD\AJ
Sample : RESC13
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESC013

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 30 01:16:49 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD122920CLP.M
Quant Title : GC Extractables
QLast Update : Wed Dec 30 01:06:43 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

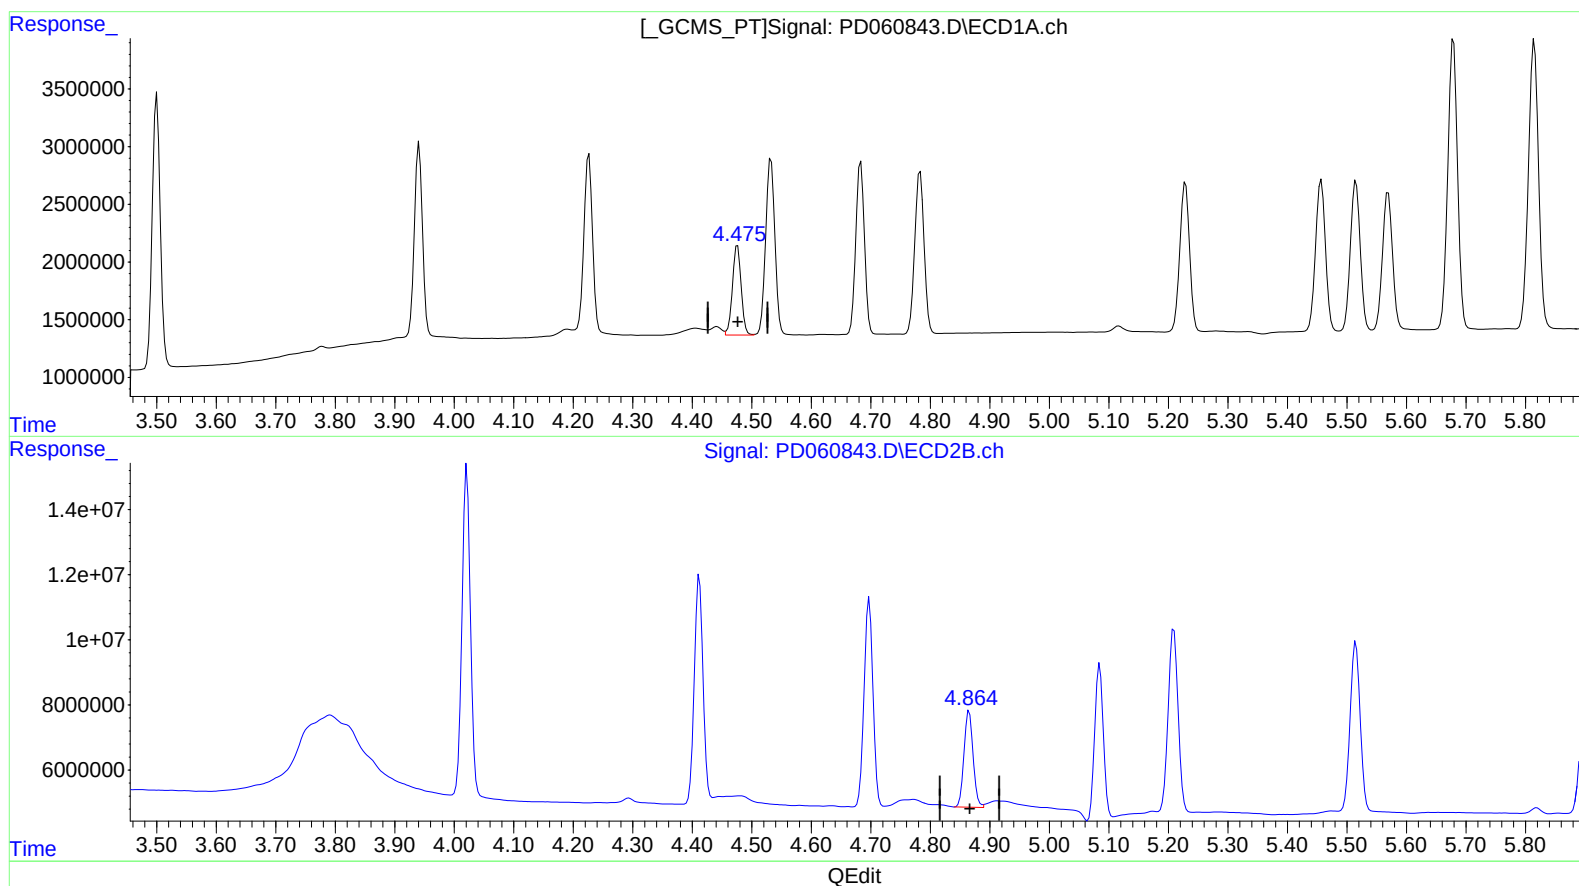

(6) beta-BHC (B)

4.476min 10.701 ng/ml

response 7925177

(6) beta-BHC #2 (B)

4.865min 10.621 ng/ml


response 31463033

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD122920\
Data File : PD060843.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Dec 2020 10:14
Operator : DD\AJ
Sample : RESC13
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESC013

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 30 01:16:49 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD122920CLP.M
Quant Title : GC Extractables
QLast Update : Wed Dec 30 01:06:43 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

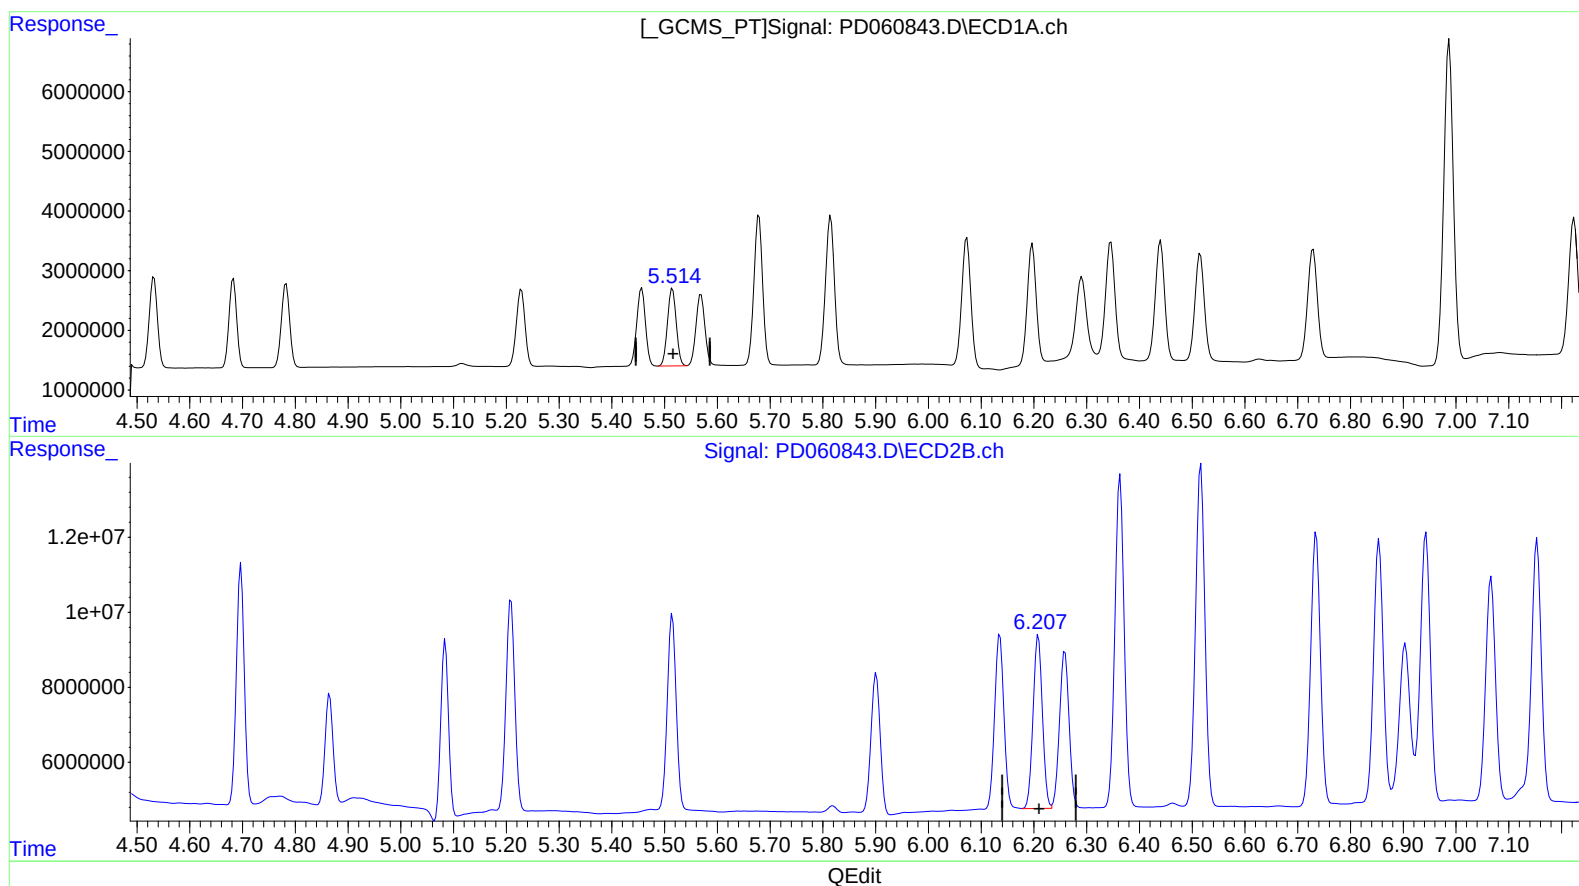

(11) cis-Chlordane (B)

5.515min 10.057 ng/ml

response 14977275

(11) cis-Chlordane #2 (B)

6.208min 10.149 ng/ml

response 56600346