

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD122920\
 Data File : PD060854.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Dec 2020 12:49
 Operator : DD\AJ
 Sample : INDA301
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 INDA3001

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 29 13:09:40 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD122920CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 29 13:09:22 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.500	4.021	22639366	99817749	20.000	20.000
27)	SA Decachlor...	8.285	9.104	55195468	159.0E6	40.000	40.000
Target Compounds							
2)	A alpha-BHC	3.941	4.411	32150541	146.7E6	20.000	20.000
3)	MA gamma-BHC...	4.226	4.697	30746187	133.3E6	20.000	20.000
4)	MA Heptachlor	4.532	5.208	32778646	132.9E6	20.000	20.000
9)	A Endosulfan I	5.569	6.259	27828756	107.7E6	20.000	20.000
13)	MA Dieldrin	5.815	6.517	60707101	232.2E6	40.000	40.000
14)	MA Endrin	6.073	6.735	51079773	185.4E6	40.000	40.000
16)	A 4,4'-DDD	6.197	6.854	48385910	180.6E6	40.000	40.000
17)	MA 4,4'-DDT	6.440	7.153	51125194	180.6E6	40.000	40.000
20)	A Methoxychlor	6.987	7.610	131.6E6	443.3E6	200.000	200.000

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD122920\
Data File : PD060854.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Dec 2020 12:49
Operator : DD\AJ
Sample : INDA301
Misc :
ALS Vial : 13 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 29 13:09:40 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD122920CLP.M
Quant Title : GC Extractables
QLast Update : Tue Dec 29 13:09:22 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

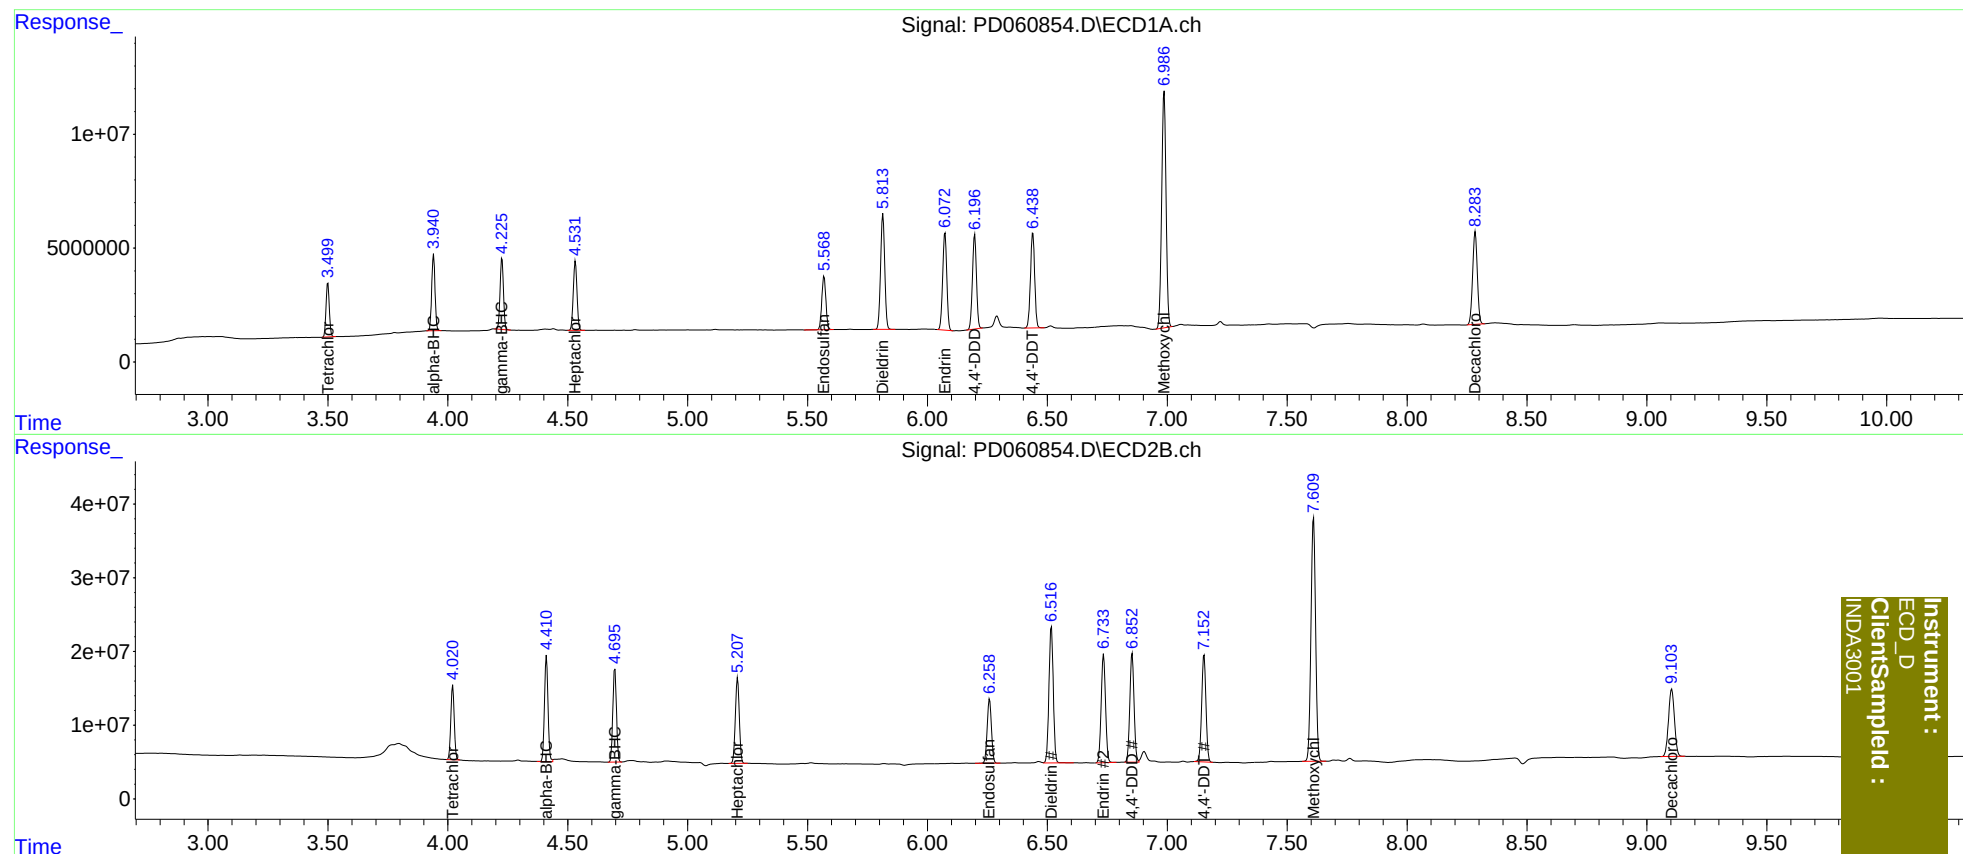

Instrument :
ECD_D
ClientSampled :
INDA3001