

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD122921\
 Data File : PD067544.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Dec 2021 10:54
 Operator : AR\AJ
 Sample : INDA101
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 28 13:49:37 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD122921CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 28 13:49:05 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.434	3.964	12605036	47340323	5.717	5.939
27)	SA Decachlor...	8.157	9.020	11443251	57997637	12.148	11.531
Target Compounds							
2)	A alpha-BHC	3.870	4.358	16392855	56025883	4.983	5.393
3)	MA gamma-BHC...	4.151	4.643	16509533	53265754	5.325	5.422
4)	MA Heptachlor	4.444	5.142	15775018	49411093	5.155	5.580
9)	A Endosulfan I	5.466	6.192	14067912	38774582	5.408	5.398
13)	MA Dieldrin	5.708	6.450	27763848	80662723	9.877	10.803
14)	MA Endrin	5.965	6.667	23688618	62581933	10.995	11.442
16)	A 4,4'-DDD	6.089	6.796	20087630	62352528	10.172	10.629
17)	MA 4,4'-DDT	6.328	7.093	21339584	60020386	10.525	10.327
20)	A Methoxychlor	6.876	7.555	47714819	155.0E6	54.812	56.493


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD122921\
Data File : PD067544.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Dec 2021 10:54
Operator : AR\AJ
Sample : INDA101
Misc :
ALS Vial : 31 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 28 13:49:37 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD122921CLP.M
Quant Title : GC Extractables
QLast Update : Tue Dec 28 13:49:05 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

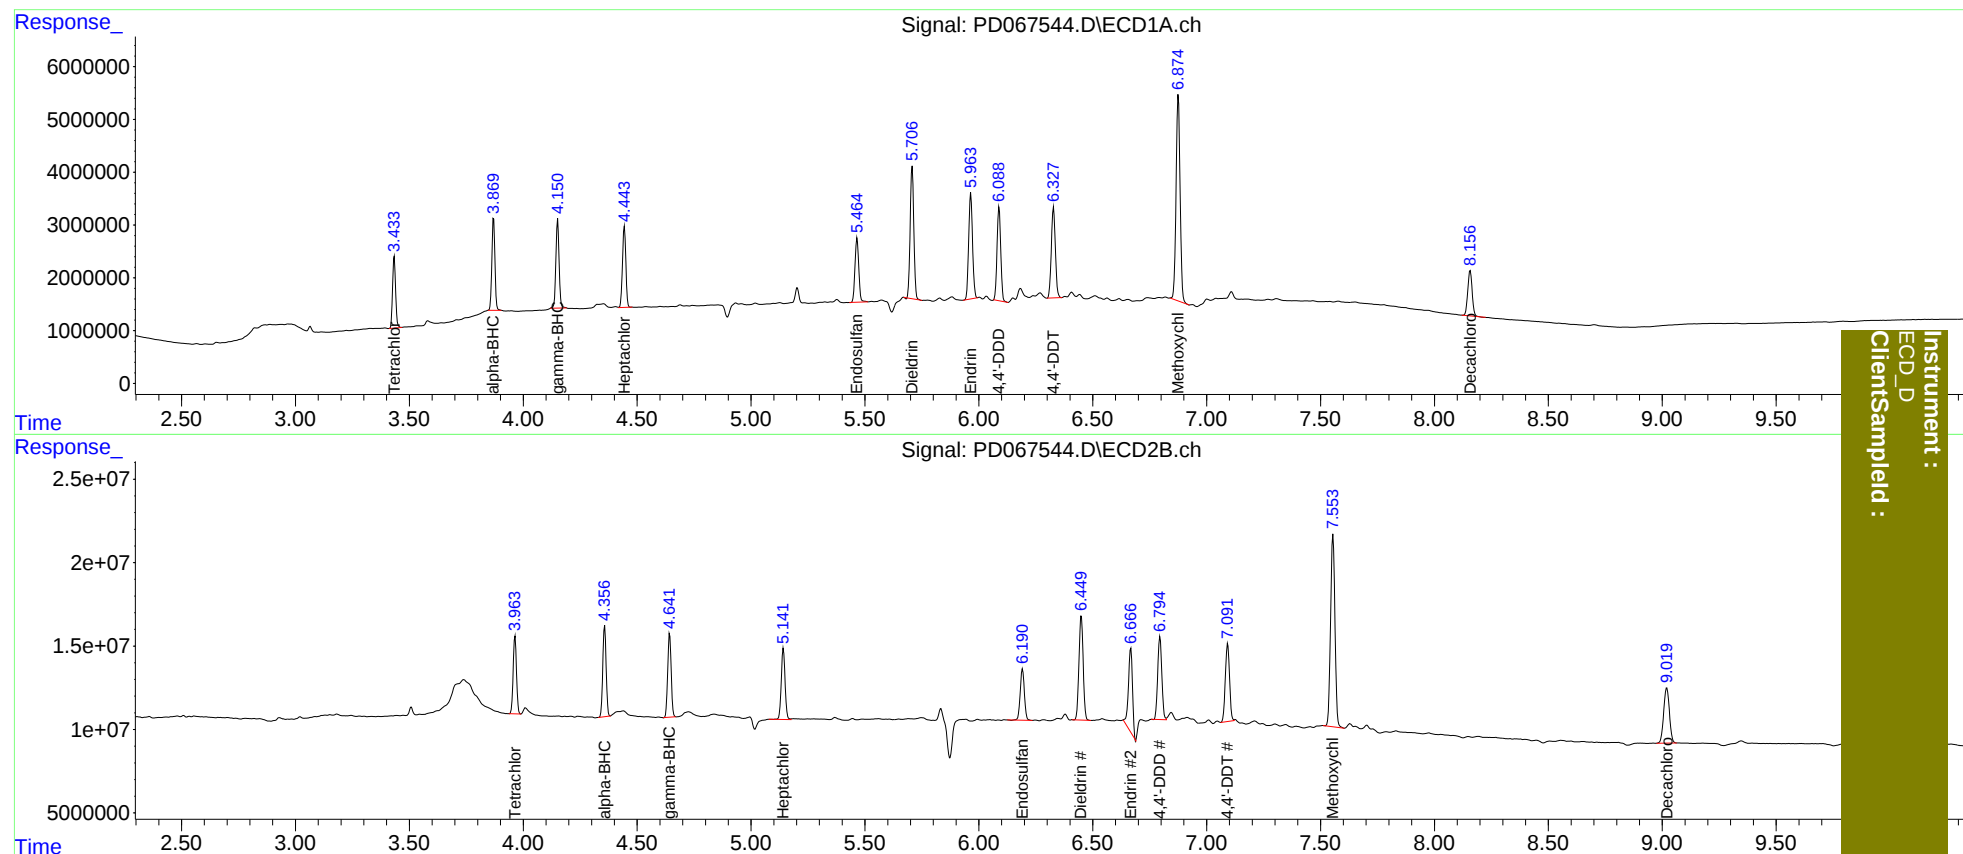


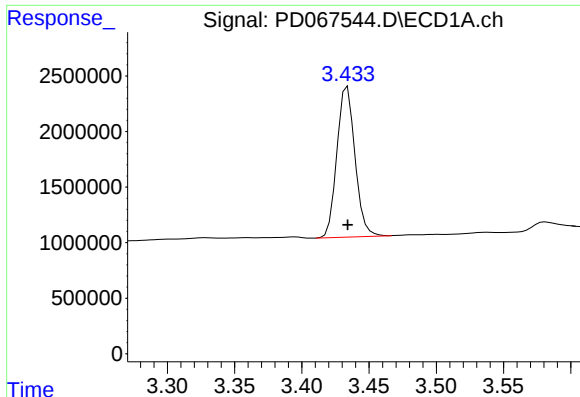

#1 Tetrachloro-m-xylene


R.T.: 3.434 min
Delta R.T.: 0.000 min
Response: 12605036
Conc: 5.72 ng/ml

Instrument :
ECD_D
ClientSampleId :

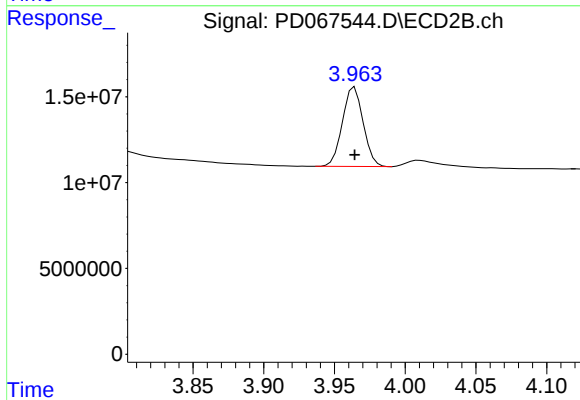


#1 Tetrachloro-m-xylene

R.T.: 3.964 min
Delta R.T.: 0.000 min
Response: 47340323
Conc: 5.94 ng/ml

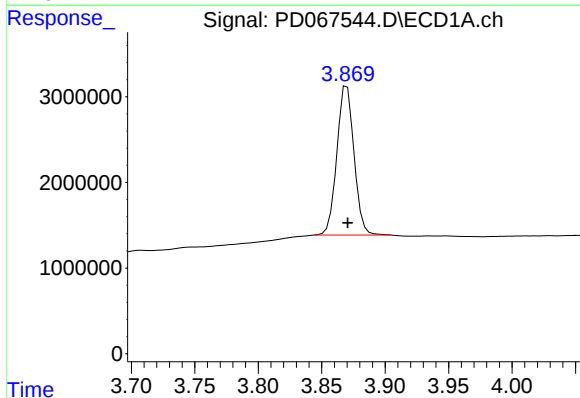


#2 alpha-BHC

R.T.: 3.870 min
Delta R.T.: 0.000 min
Response: 16392855
Conc: 4.98 ng/ml

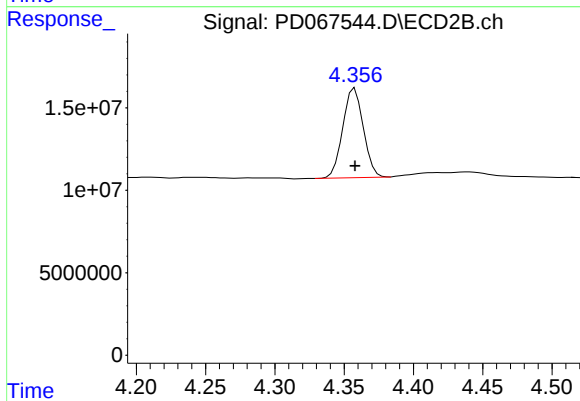

#2 alpha-BHC


R.T.: 4.358 min
Delta R.T.: 0.000 min
Response: 56025883
Conc: 5.39 ng/ml

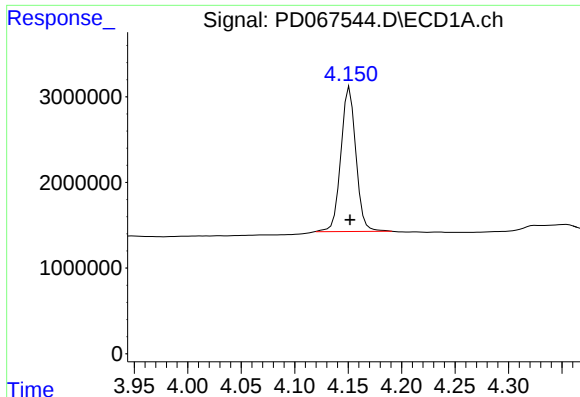

#3 gamma-BHC (Lindane)


R.T.: 4.151 min
Delta R.T.: 0.000 min
Response: 16509533
Conc: 5.33 ng/ml

Instrument :
ECD_D
ClientSampleId :

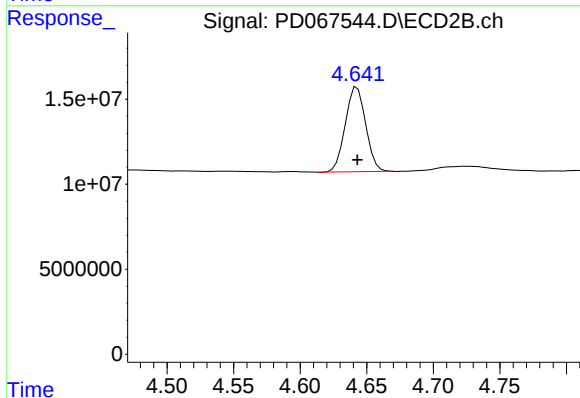


#3 gamma-BHC (Lindane)

R.T.: 4.643 min
Delta R.T.: 0.000 min
Response: 53265754
Conc: 5.42 ng/ml

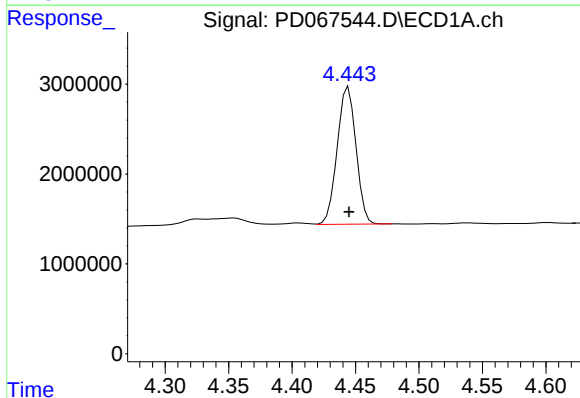


#4 Heptachlor

R.T.: 4.444 min
Delta R.T.: 0.000 min
Response: 15775018
Conc: 5.16 ng/ml

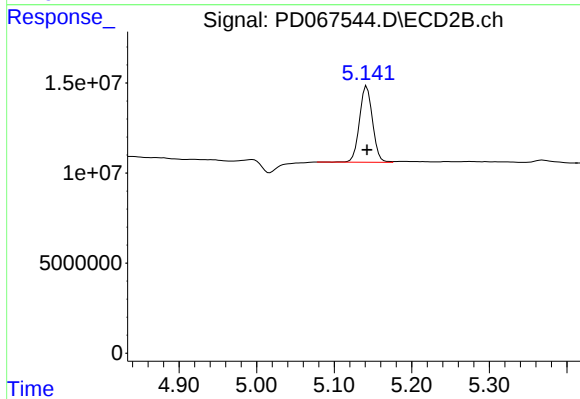

#4 Heptachlor


R.T.: 5.142 min
Delta R.T.: 0.000 min
Response: 49411093
Conc: 5.58 ng/ml

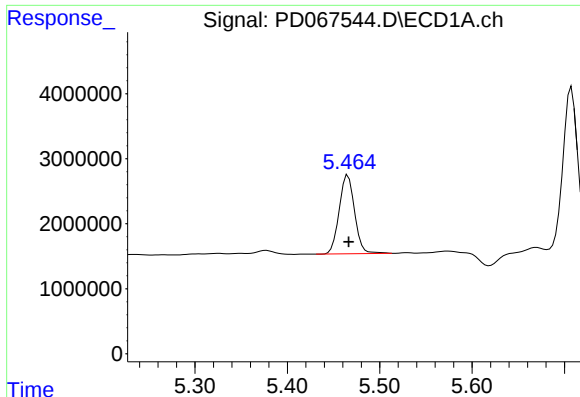

#9 Endosulfan I


R.T.: 5.466 min
Delta R.T.: 0.000 min
Response: 14067912
Conc: 5.41 ng/ml

Instrument :
ECD_D
ClientSampleId :

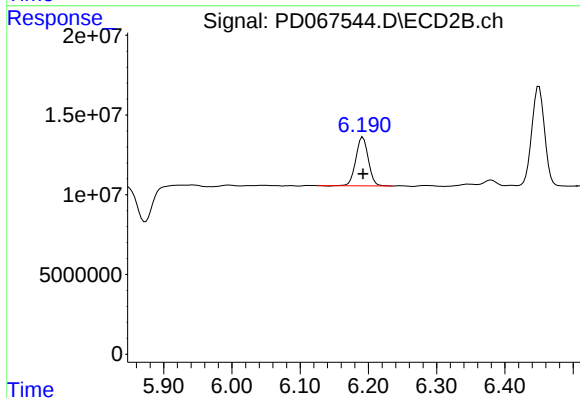


#9 Endosulfan I

R.T.: 6.192 min
Delta R.T.: 0.000 min
Response: 38774582
Conc: 5.40 ng/ml

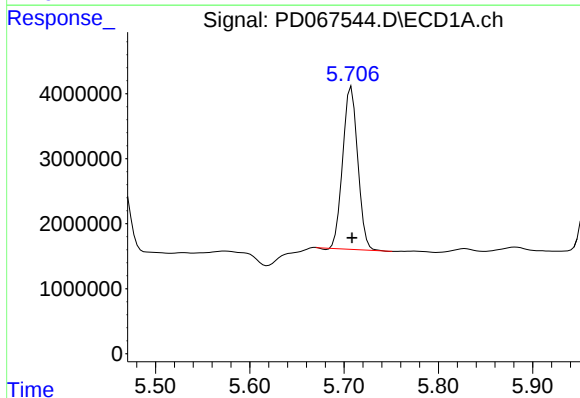


#13 Dieldrin

R.T.: 5.708 min
Delta R.T.: 0.000 min
Response: 27763848
Conc: 9.88 ng/ml

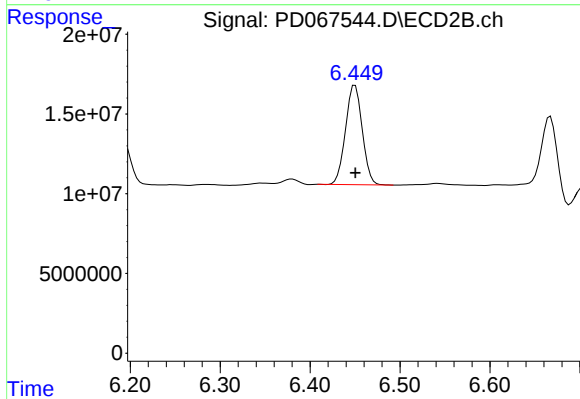

#13 Dieldrin


R.T.: 6.450 min
Delta R.T.: 0.000 min
Response: 80662723
Conc: 10.80 ng/ml

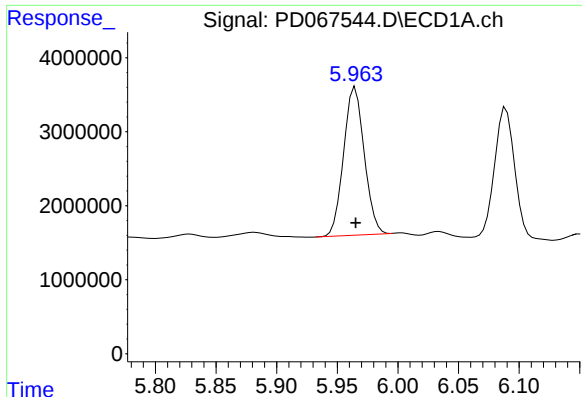

#14 Endrin


R.T.: 5.965 min
Delta R.T.: 0.000 min
Response: 23688618
Conc: 11.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

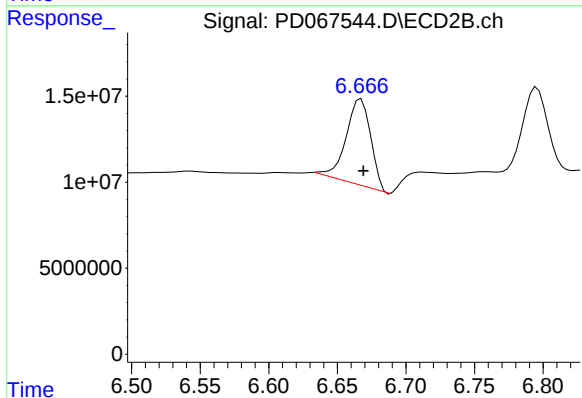


#14 Endrin

R.T.: 6.667 min
Delta R.T.: -0.002 min
Response: 62581933
Conc: 11.44 ng/ml

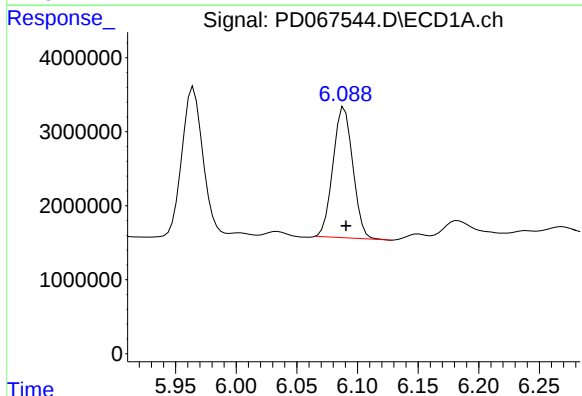


#16 4,4'-DDD

R.T.: 6.089 min
Delta R.T.: -0.002 min
Response: 20087630
Conc: 10.17 ng/ml

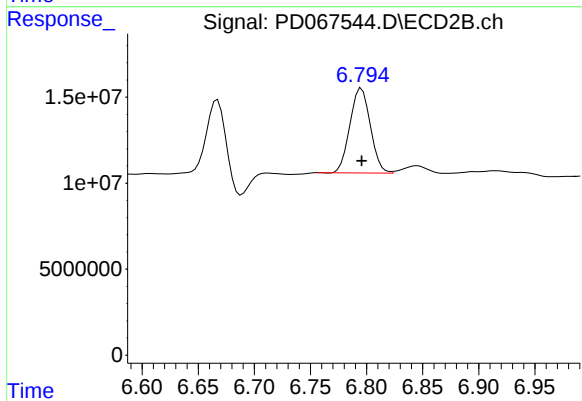

#16 4,4'-DDD


R.T.: 6.796 min
Delta R.T.: 0.000 min
Response: 62352528
Conc: 10.63 ng/ml

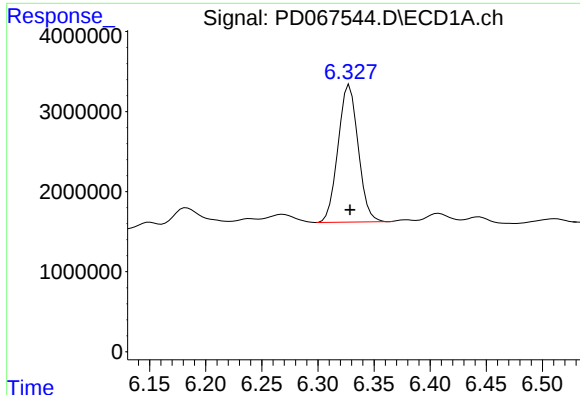

#17 4,4'-DDT


R.T.: 6.328 min
Delta R.T.: 0.000 min
Response: 21339584
Conc: 10.53 ng/ml

Instrument :
ECD_D
ClientSampleId :

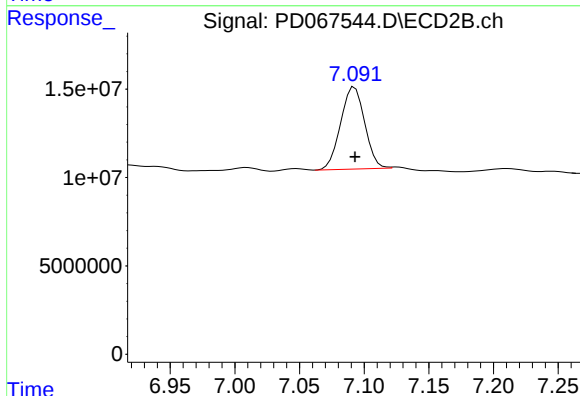


#17 4,4'-DDT

R.T.: 7.093 min
Delta R.T.: 0.000 min
Response: 60020386
Conc: 10.33 ng/ml

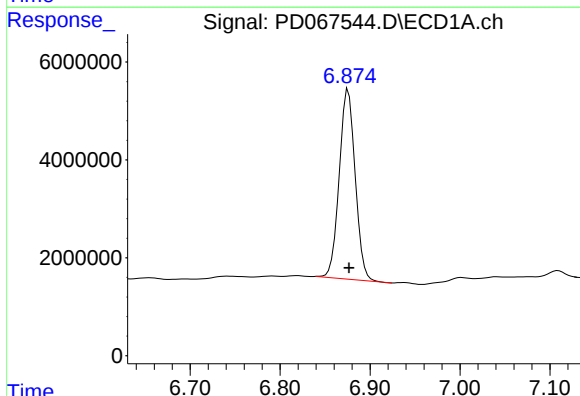


#20 Methoxychlor

R.T.: 6.876 min
Delta R.T.: 0.000 min
Response: 47714819
Conc: 54.81 ng/ml

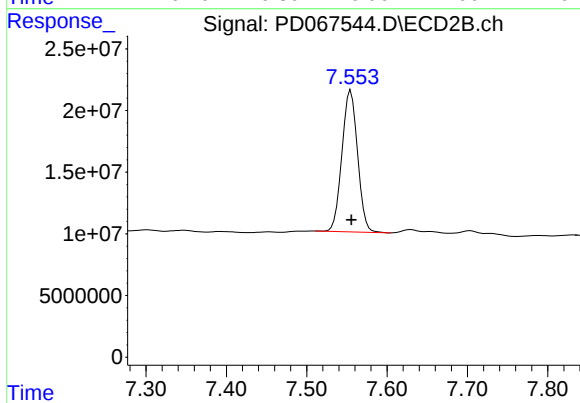

#20 Methoxychlor


R.T.: 7.555 min
Delta R.T.: 0.000 min
Response: 155001137
Conc: 56.49 ng/ml

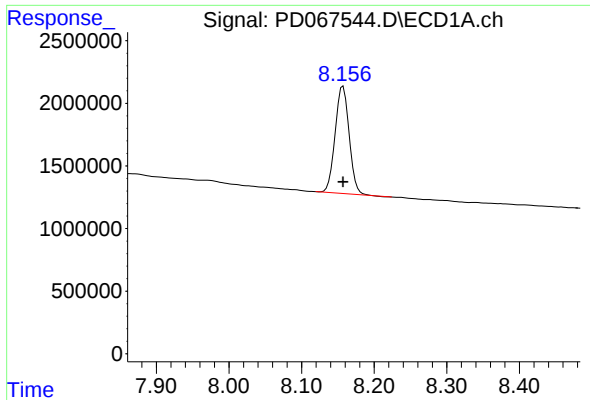

#27 Decachlorobiphenyl

R.T.: 8.157 min
Delta R.T.: 0.000 min
Response: 11443251
Conc: 12.15 ng/ml

Instrument :
ECD_D
ClientSampleId :

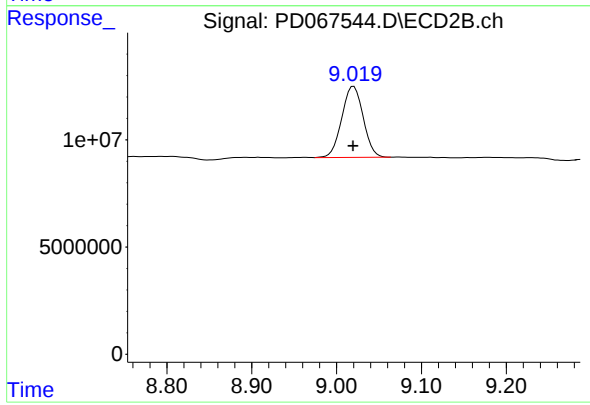

#27 Decachlorobiphenyl

R.T.: 9.020 min
Delta R.T.: 0.000 min
Response: 57997637
Conc: 11.53 ng/ml