

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD122921\
 Data File : PD067546.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Dec 2021 11:22
 Operator : AR\AJ
 Sample : INDA201
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 28 13:49:44 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD122921CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 28 13:49:05 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.434	3.964	23431528	86258581	10.627	10.822
27)	SA Decachlor...	8.157	9.020	20386837	107.5E6	21.642	21.374
Target Compounds							
2)	A alpha-BHC	3.871	4.358	33112913	109.5E6	10.066	10.537
3)	MA gamma-BHC...	4.152	4.643	31870521	103.4E6	10.280	10.530
4)	MA Heptachlor	4.445	5.143	31411595	95543132	10.265	10.790
9)	A Endosulfan I	5.466	6.192	27276858	77139698	10.485	10.740
13)	MA Dieldrin	5.709	6.450	56862316	159.0E6	20.229	21.301
14)	MA Endrin	5.965	6.668	46742194	116.0E6	21.696	21.208
16)	A 4,4'-DDD	6.091	6.795	40576840	124.3E6	20.548	21.197
17)	MA 4,4'-DDT	6.330	7.093	41148901	124.5E6	20.296	21.415
20)	A Methoxychlor	6.877	7.555	92533980	300.7E6	106.298	109.601


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD122921\
Data File : PD067546.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Dec 2021 11:22
Operator : AR\AJ
Sample : INDA201
Misc :
ALS Vial : 33 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 28 13:49:44 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD122921CLP.M
Quant Title : GC Extractables
QLast Update : Tue Dec 28 13:49:05 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

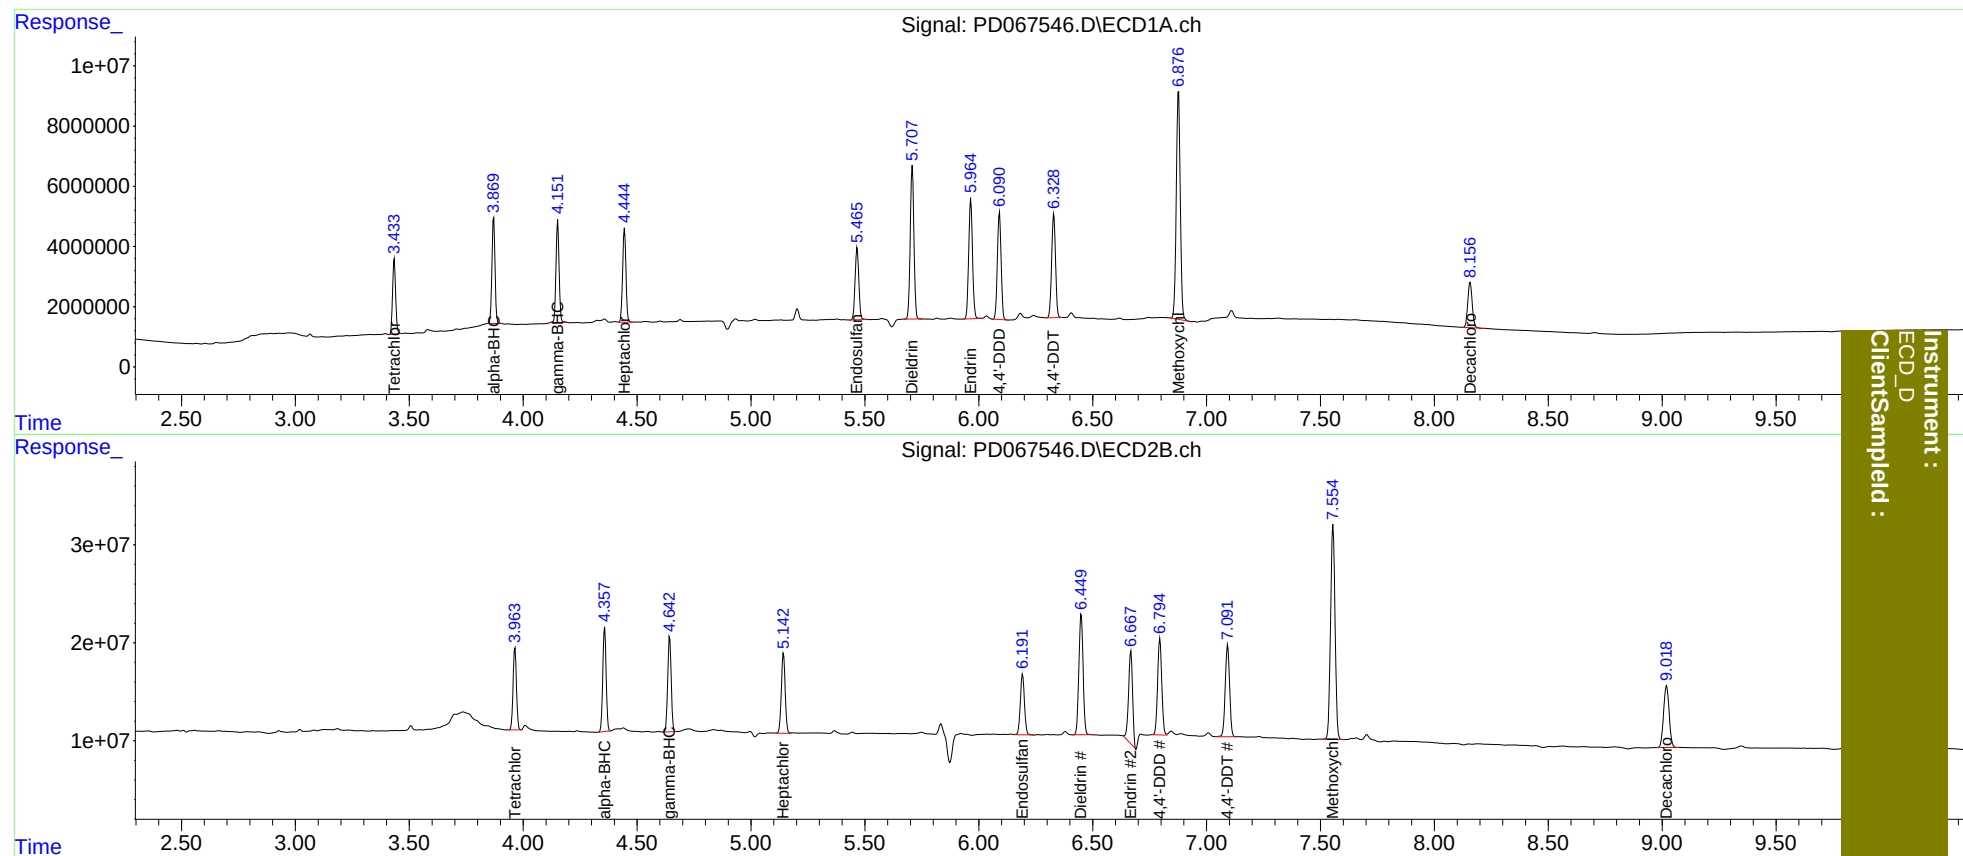


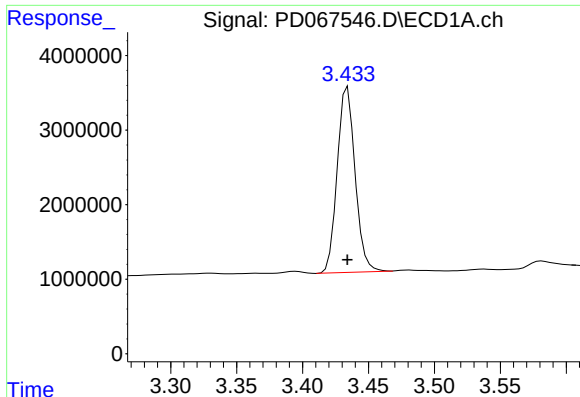

#1 Tetrachloro-m-xylene


R.T.: 3.434 min
Delta R.T.: 0.000 min
Response: 23431528
Conc: 10.63 ng/ml

Instrument :
ECD_D
ClientSampleId :

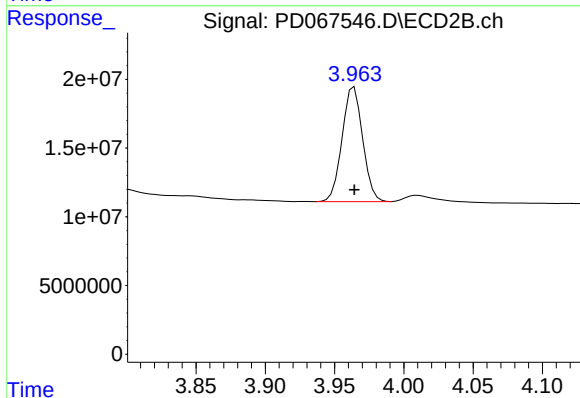


#1 Tetrachloro-m-xylene

R.T.: 3.964 min
Delta R.T.: 0.000 min
Response: 86258581
Conc: 10.82 ng/ml

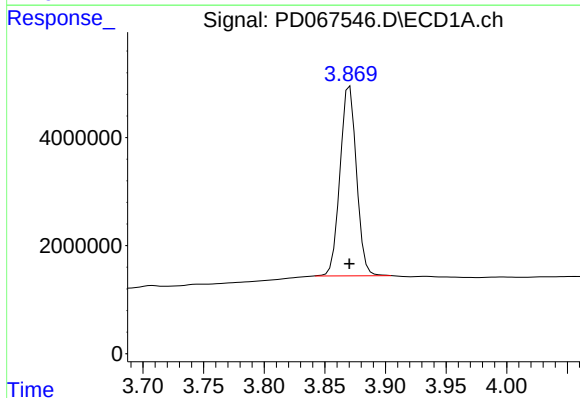


#2 alpha-BHC

R.T.: 3.871 min
Delta R.T.: 0.000 min
Response: 33112913
Conc: 10.07 ng/ml

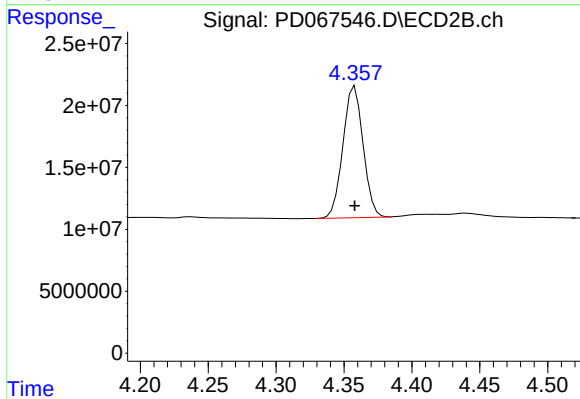

#2 alpha-BHC


R.T.: 4.358 min
Delta R.T.: 0.000 min
Response: 109462714
Conc: 10.54 ng/ml

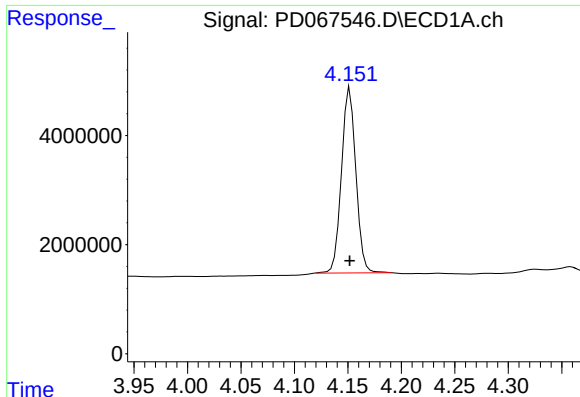

#3 gamma-BHC (Lindane)


R.T.: 4.152 min
Delta R.T.: 0.000 min
Response: 31870521
Conc: 10.28 ng/ml

Instrument :
ECD_D
ClientSampleId :

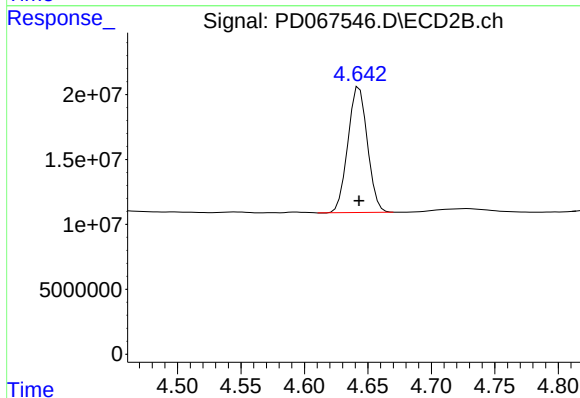


#3 gamma-BHC (Lindane)

R.T.: 4.643 min
Delta R.T.: 0.000 min
Response: 103448488
Conc: 10.53 ng/ml

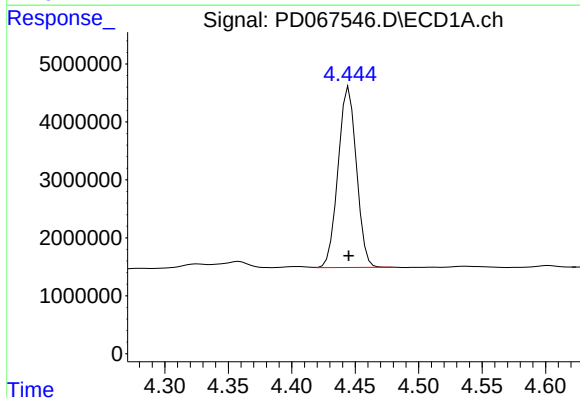


#4 Heptachlor

R.T.: 4.445 min
Delta R.T.: 0.000 min
Response: 31411595
Conc: 10.27 ng/ml

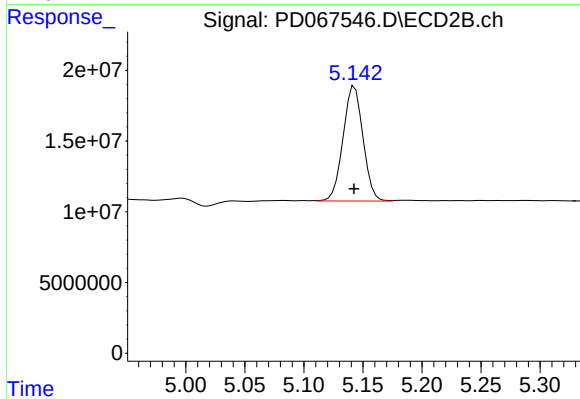

#4 Heptachlor


R.T.: 5.143 min
Delta R.T.: 0.000 min
Response: 95543132
Conc: 10.79 ng/ml

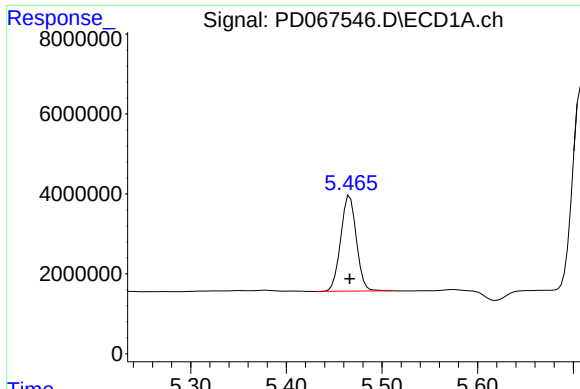

#9 Endosulfan I


R.T.: 5.466 min
Delta R.T.: 0.000 min
Response: 27276858
Conc: 10.49 ng/ml

Instrument :
ECD_D
ClientSampleId :

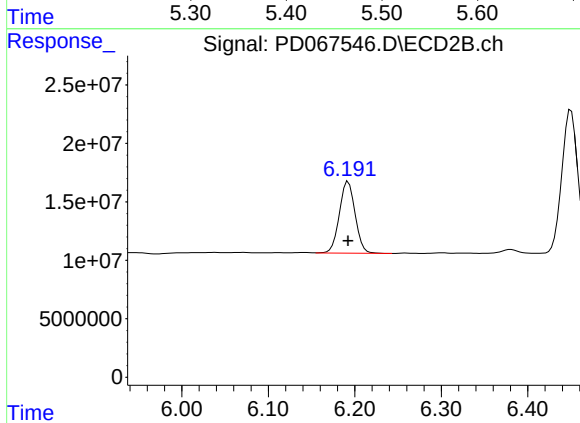


#9 Endosulfan I

R.T.: 6.192 min
Delta R.T.: 0.000 min
Response: 77139698
Conc: 10.74 ng/ml

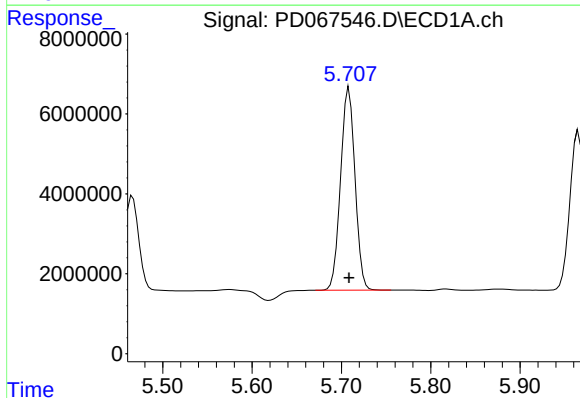


#13 Dieldrin

R.T.: 5.709 min
Delta R.T.: 0.000 min
Response: 56862316
Conc: 20.23 ng/ml

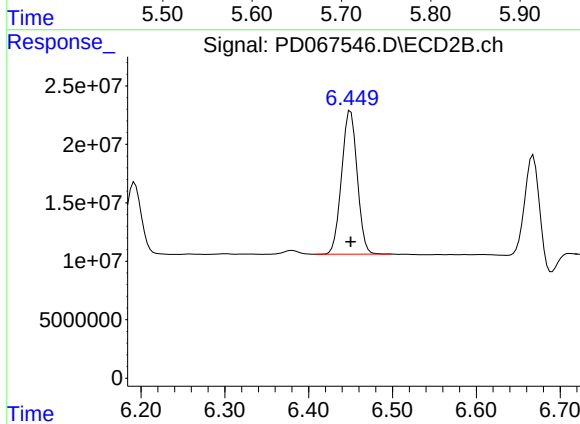

#13 Dieldrin


R.T.: 6.450 min
Delta R.T.: 0.000 min
Response: 159041857
Conc: 21.30 ng/ml

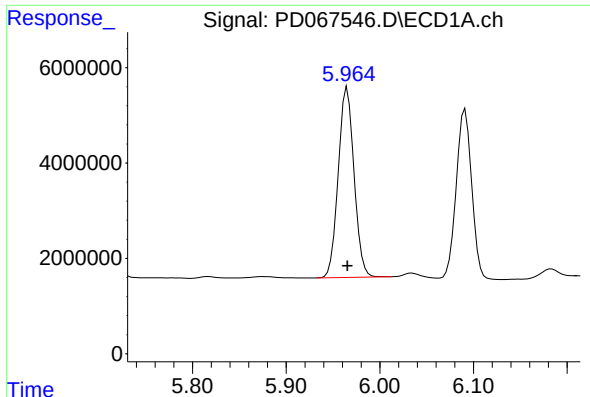

#14 Endrin


R.T.: 5.965 min
Delta R.T.: 0.000 min
Response: 46742194
Conc: 21.70 ng/ml

Instrument :
ECD_D
ClientSampleId :

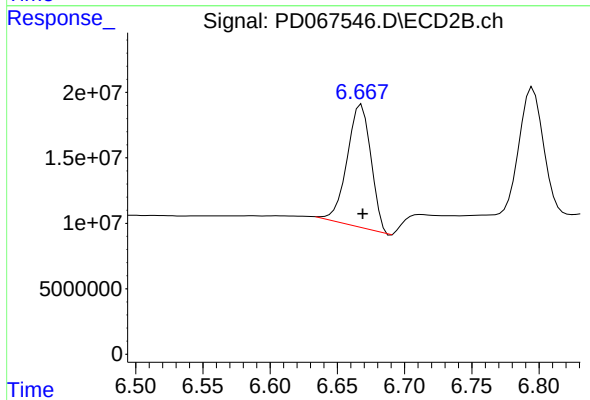


#14 Endrin

R.T.: 6.668 min
Delta R.T.: -0.001 min
Response: 115993045
Conc: 21.21 ng/ml

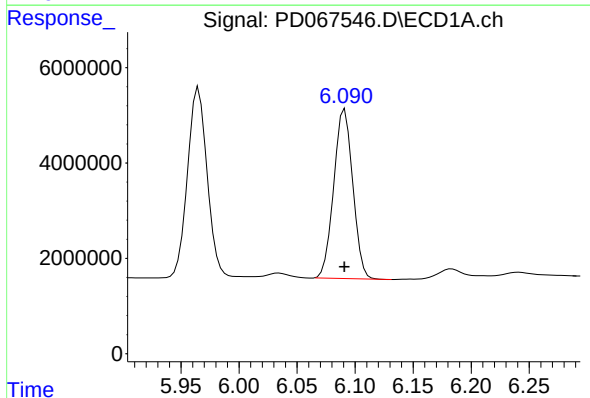


#16 4,4'-DDD

R.T.: 6.091 min
Delta R.T.: 0.000 min
Response: 40576840
Conc: 20.55 ng/ml

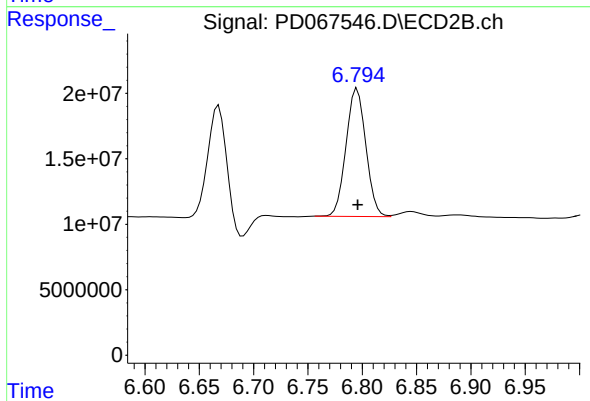

#16 4,4'-DDD


R.T.: 6.795 min
Delta R.T.: 0.000 min
Response: 124344499
Conc: 21.20 ng/ml

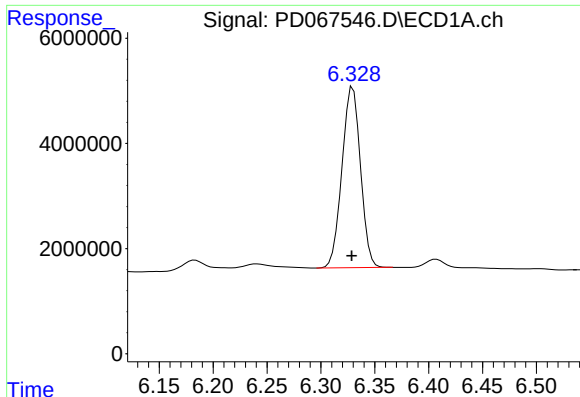

#17 4,4'-DDT


R.T.: 6.330 min
Delta R.T.: 0.001 min
Response: 41148901
Conc: 20.30 ng/ml

Instrument :
ECD_D
ClientSampleId :

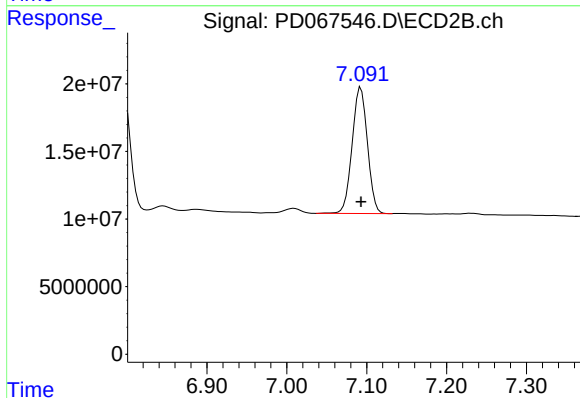


#17 4,4'-DDT

R.T.: 7.093 min
Delta R.T.: 0.000 min
Response: 124463450
Conc: 21.41 ng/ml

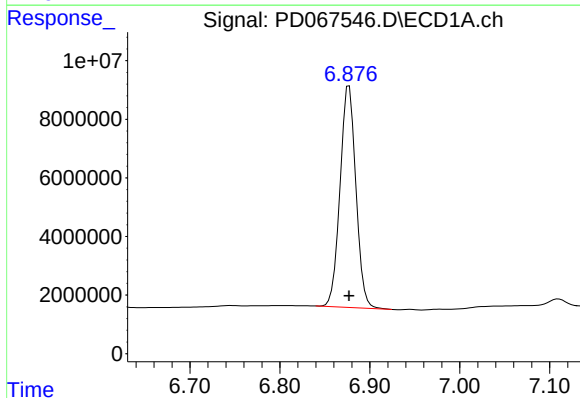


#20 Methoxychlor

R.T.: 6.877 min
Delta R.T.: 0.000 min
Response: 92533980
Conc: 106.30 ng/ml

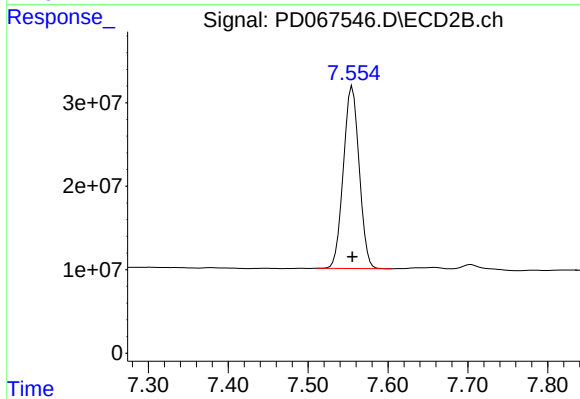

#20 Methoxychlor


R.T.: 7.555 min
Delta R.T.: 0.000 min
Response: 300718043
Conc: 109.60 ng/ml

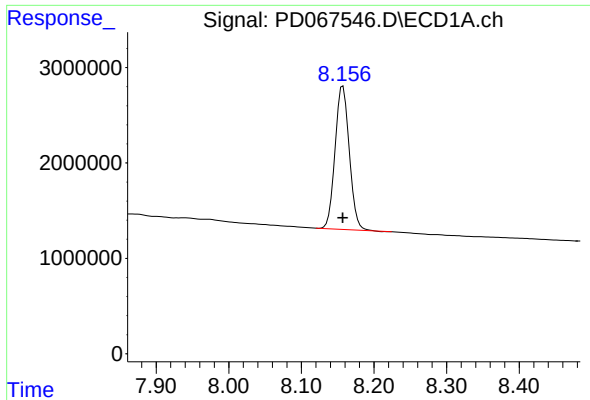

#27 Decachlorobiphenyl

R.T.: 8.157 min
Delta R.T.: 0.000 min
Response: 20386837
Conc: 21.64 ng/ml

Instrument :
ECD_D
ClientSampleId :

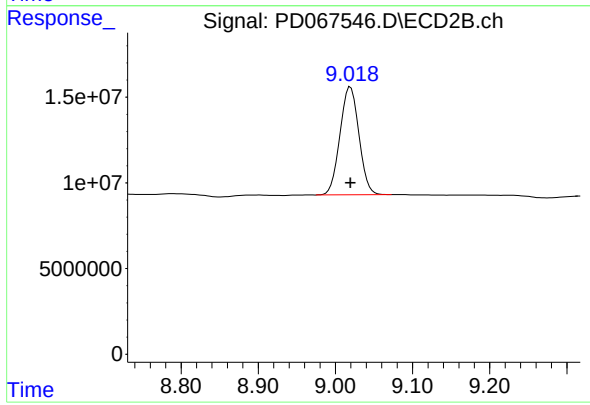

#27 Decachlorobiphenyl

R.T.: 9.020 min
Delta R.T.: 0.000 min
Response: 107507754
Conc: 21.37 ng/ml