

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD122921\
 Data File : PD067548.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Dec 2021 11:49
 Operator : AR\AJ
 Sample : INDA301
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 28 13:49:54 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD122921CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 28 13:49:05 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.434	3.964	44099414	159.4E6	20.000	20.000
27)	SA Decachlor...	8.157	9.020	37680086	201.2E6	40.000	40.000
Target Compounds							
2)	A alpha-BHC	3.870	4.358	65792164	207.8E6	20.000	20.000
3)	MA gamma-BHC...	4.152	4.643	62003705	196.5E6	20.000	20.000
4)	MA Heptachlor	4.445	5.142	61201021	177.1E6	20.000	20.000
9)	A Endosulfan I	5.466	6.192	52030076	143.7E6	20.000	20.000
13)	MA Dieldrin	5.709	6.450	112.4E6	298.7E6	40.000	40.000
14)	MA Endrin	5.965	6.669	86178357	218.8E6	40.000	40.000
16)	A 4,4'-DDD	6.091	6.796	78988999	234.6E6	40.000	40.000
17)	MA 4,4'-DDT	6.329	7.093	81098922	232.5E6	40.000	40.000
20)	A Methoxychlor	6.877	7.555	174.1E6	548.7E6	200.000	200.000


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD122921\
Data File : PD067548.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Dec 2021 11:49
Operator : AR\AJ
Sample : INDA301
Misc :
ALS Vial : 35 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 28 13:49:54 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD122921CLP.M
Quant Title : GC Extractables
QLast Update : Tue Dec 28 13:49:05 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

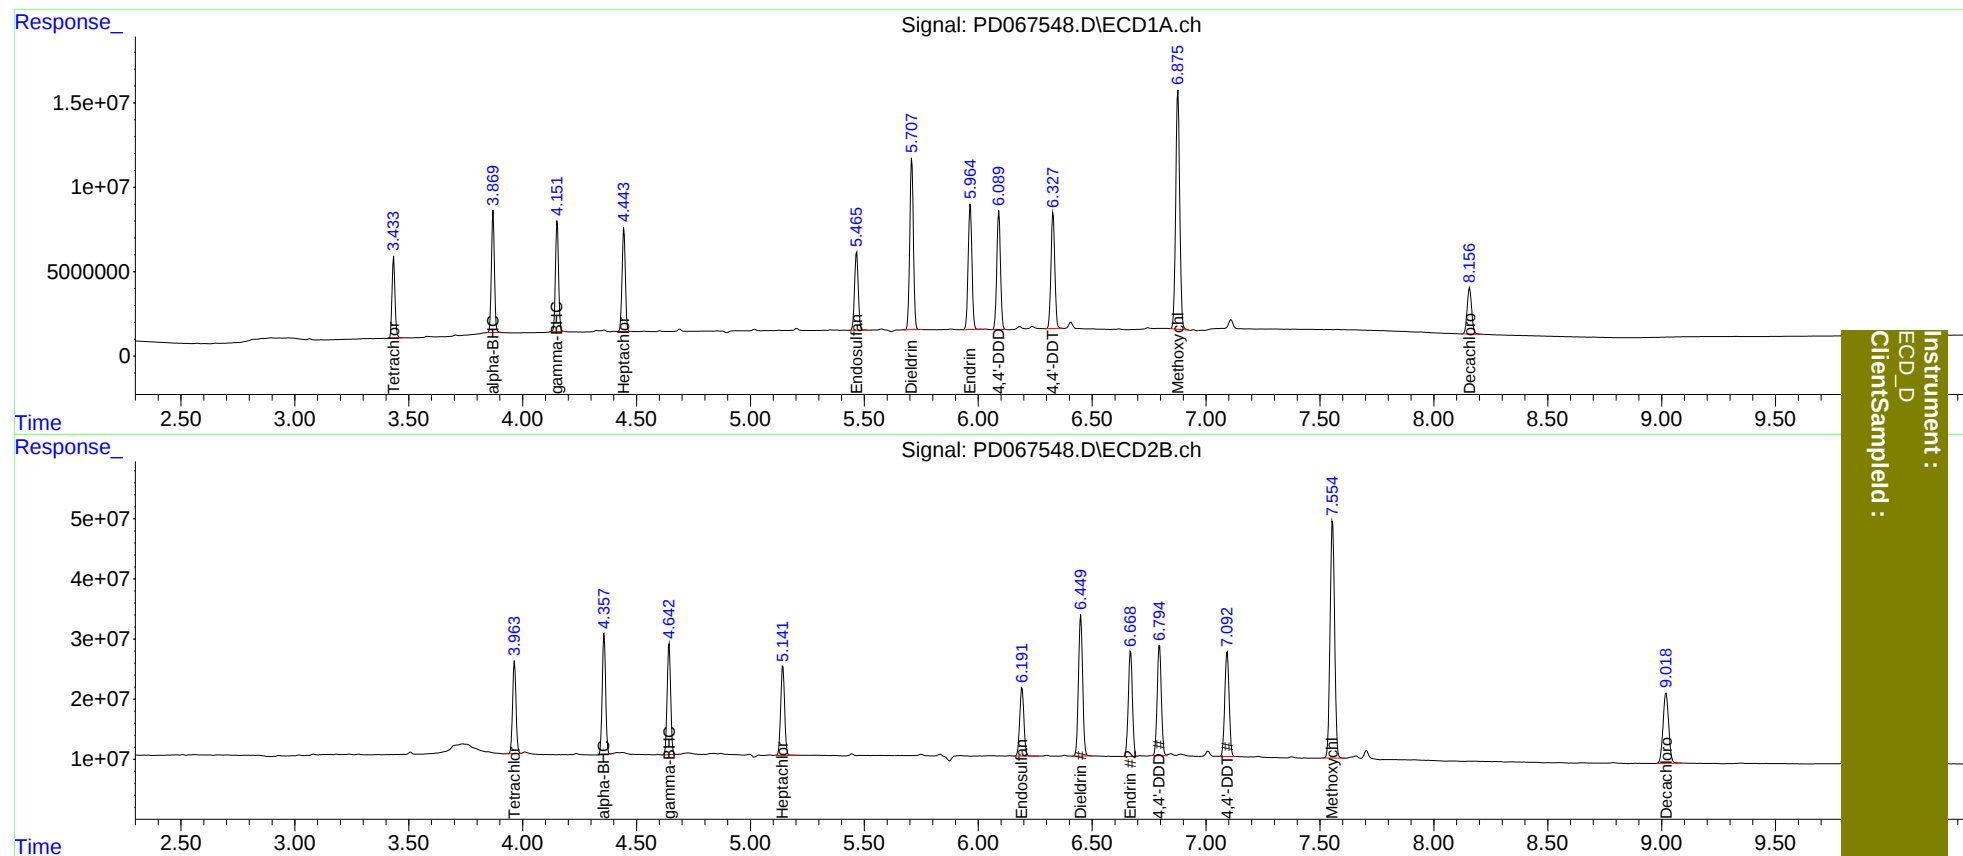


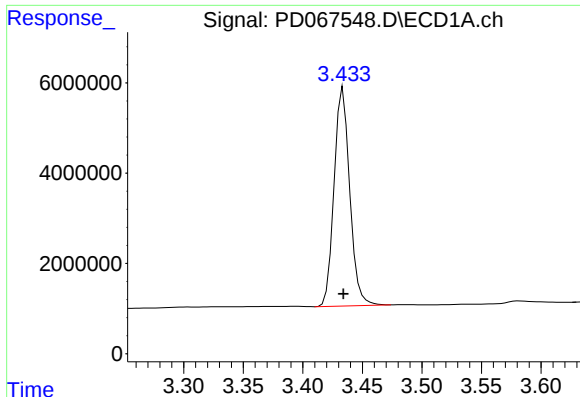

#1 Tetrachloro-m-xylene


R.T.: 3.434 min
Delta R.T.: 0.000 min
Response: 44099414
Conc: 20.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

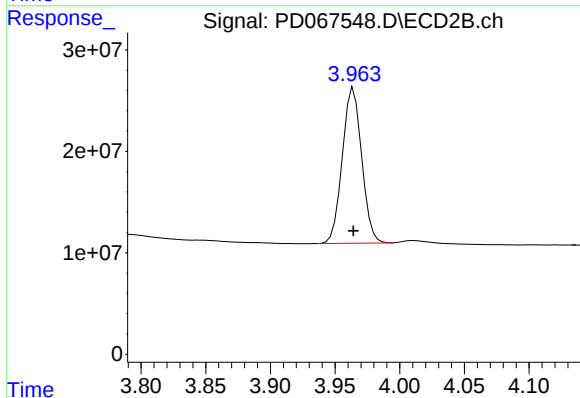


#1 Tetrachloro-m-xylene

R.T.: 3.964 min
Delta R.T.: 0.000 min
Response: 159413628
Conc: 20.00 ng/ml

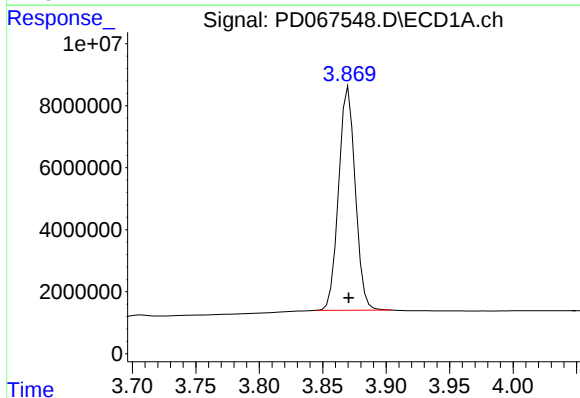


#2 alpha-BHC

R.T.: 3.870 min
Delta R.T.: 0.000 min
Response: 65792164
Conc: 20.00 ng/ml

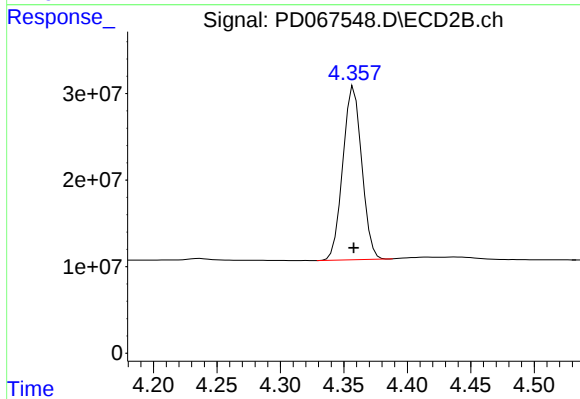

#2 alpha-BHC


R.T.: 4.358 min
Delta R.T.: 0.000 min
Response: 207769051
Conc: 20.00 ng/ml

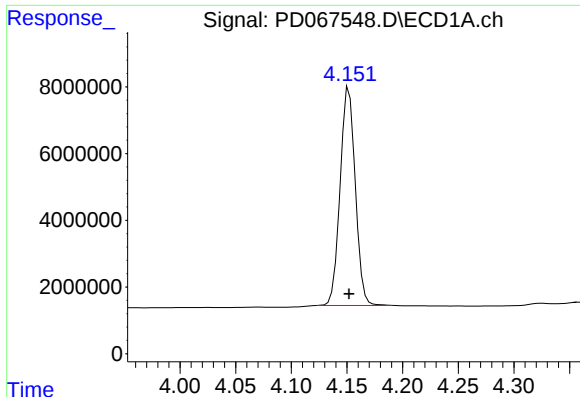

#3 gamma-BHC (Lindane)


R.T.: 4.152 min
Delta R.T.: 0.000 min
Response: 62003705
Conc: 20.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

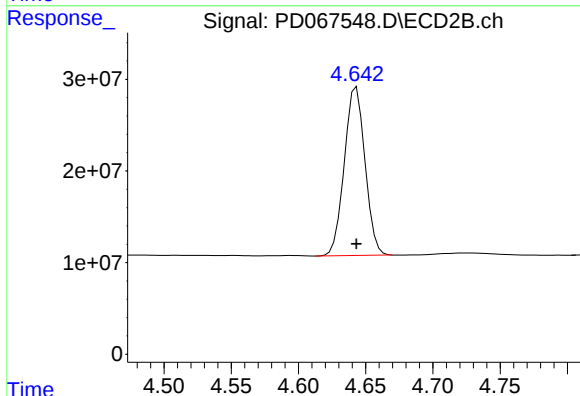


#3 gamma-BHC (Lindane)

R.T.: 4.643 min
Delta R.T.: 0.000 min
Response: 196484443
Conc: 20.00 ng/ml

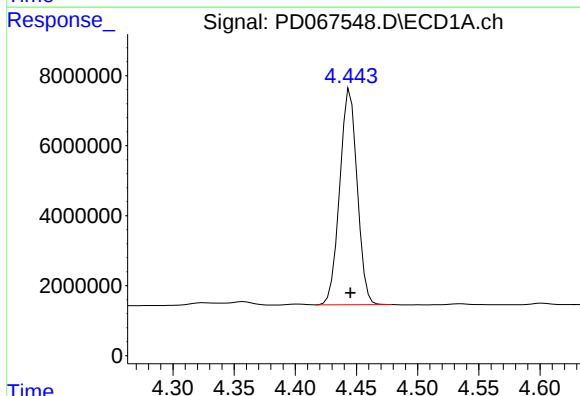


#4 Heptachlor

R.T.: 4.445 min
Delta R.T.: 0.000 min
Response: 61201021
Conc: 20.00 ng/ml

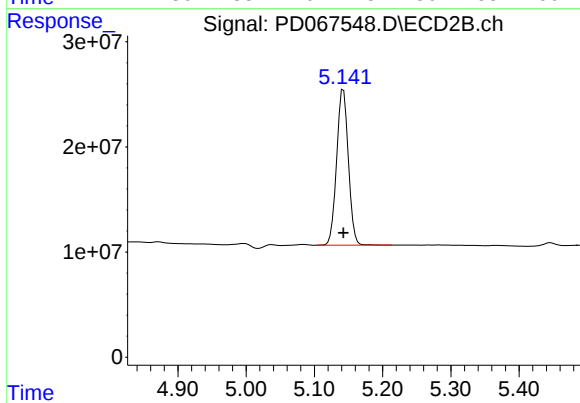

#4 Heptachlor


R.T.: 5.142 min
Delta R.T.: 0.000 min
Response: 177089091
Conc: 20.00 ng/ml

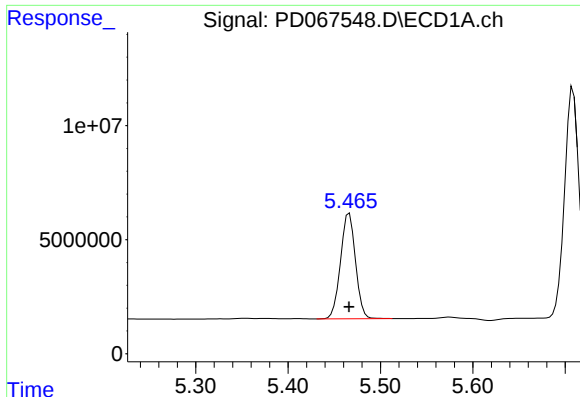

#9 Endosulfan I


R.T.: 5.466 min
Delta R.T.: 0.000 min
Response: 52030076
Conc: 20.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

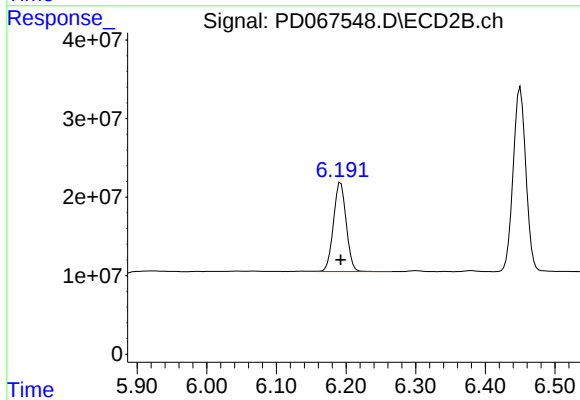


#9 Endosulfan I

R.T.: 6.192 min
Delta R.T.: 0.000 min
Response: 143654509
Conc: 20.00 ng/ml

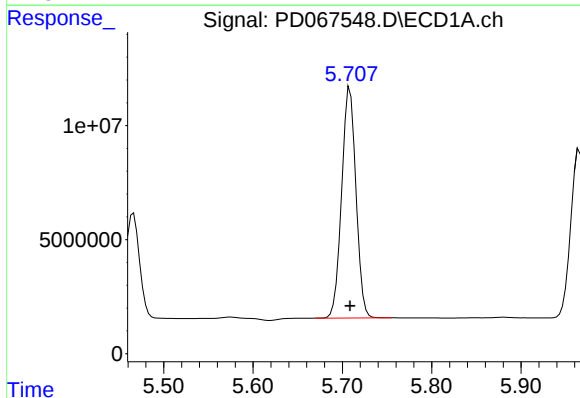


#13 Dieldrin

R.T.: 5.709 min
Delta R.T.: 0.000 min
Response: 112435513
Conc: 40.00 ng/ml

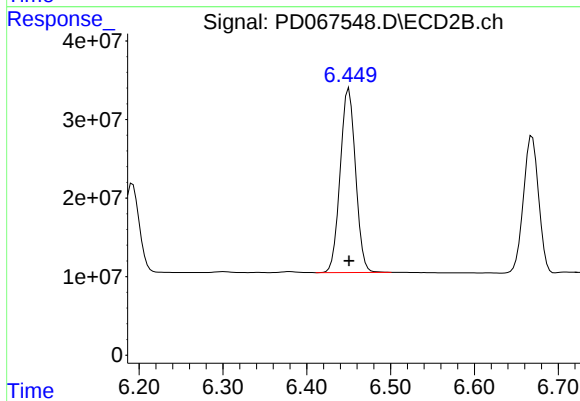

#13 Dieldrin


R.T.: 6.450 min
Delta R.T.: 0.000 min
Response: 298657528
Conc: 40.00 ng/ml

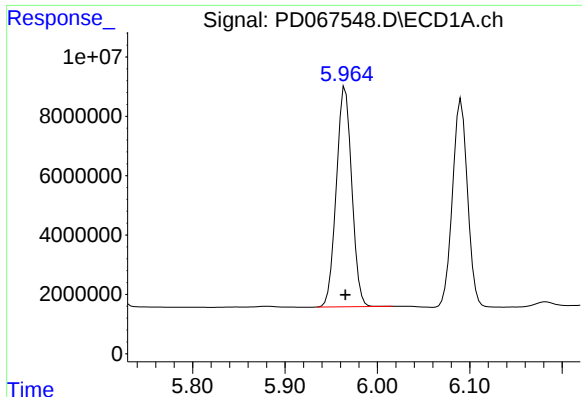

#14 Endrin


R.T.: 5.965 min
Delta R.T.: 0.000 min
Response: 86178357
Conc: 40.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

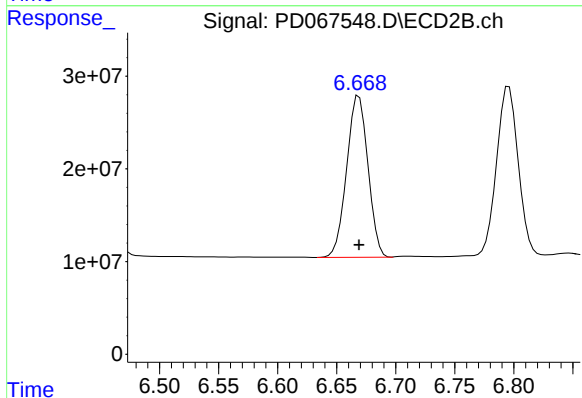


#14 Endrin

R.T.: 6.669 min
Delta R.T.: 0.000 min
Response: 218770875
Conc: 40.00 ng/ml

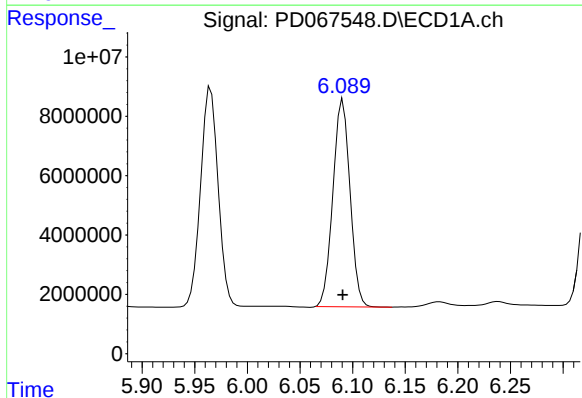


#16 4,4'-DDD

R.T.: 6.091 min
Delta R.T.: 0.000 min
Response: 78988999
Conc: 40.00 ng/ml

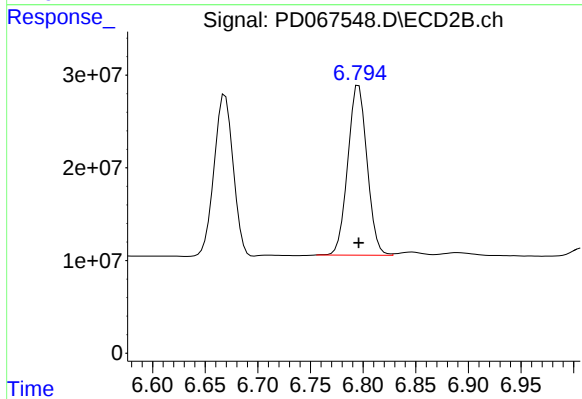

#16 4,4'-DDD


R.T.: 6.796 min
Delta R.T.: 0.000 min
Response: 234642428
Conc: 40.00 ng/ml

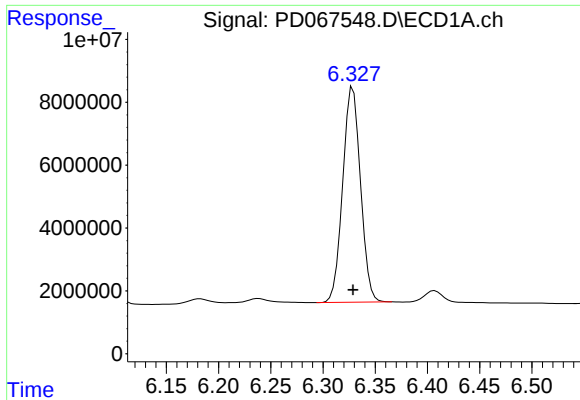

#17 4,4'-DDT


R.T.: 6.329 min
Delta R.T.: 0.000 min
Response: 81098922
Conc: 40.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

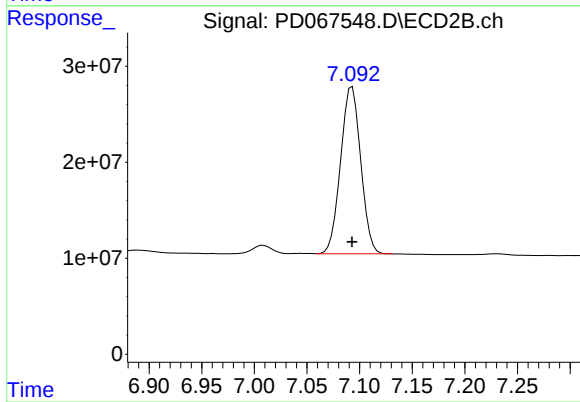


#17 4,4'-DDT

R.T.: 7.093 min
Delta R.T.: 0.000 min
Response: 232483835
Conc: 40.00 ng/ml

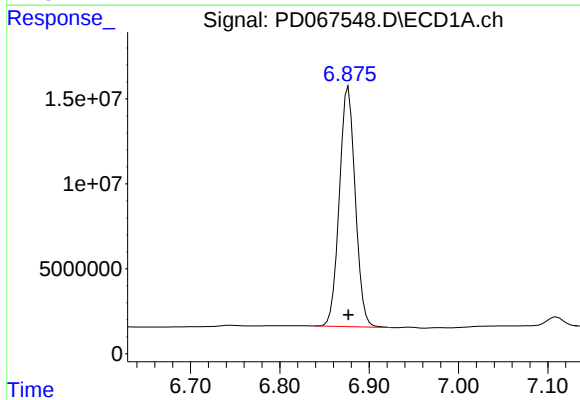


#20 Methoxychlor

R.T.: 6.877 min
Delta R.T.: 0.000 min
Response: 174102140
Conc: 200.00 ng/ml

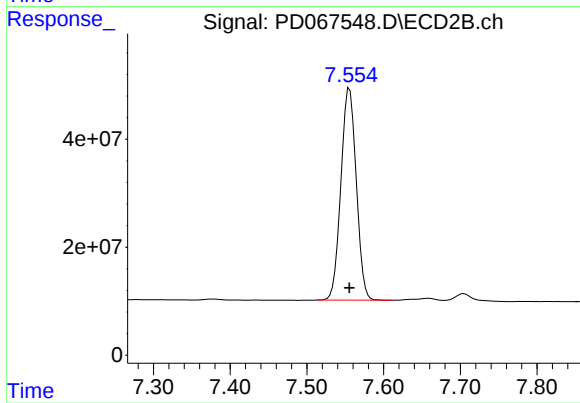

#20 Methoxychlor


R.T.: 7.555 min
Delta R.T.: 0.000 min
Response: 548748917
Conc: 200.00 ng/ml

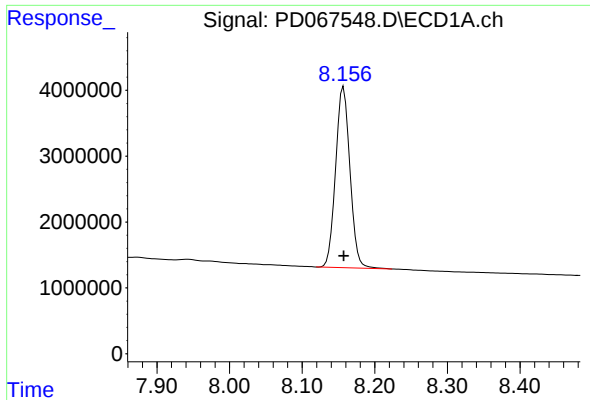

#27 Decachlorobiphenyl

R.T.: 8.157 min
Delta R.T.: 0.000 min
Response: 37680086
Conc: 40.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

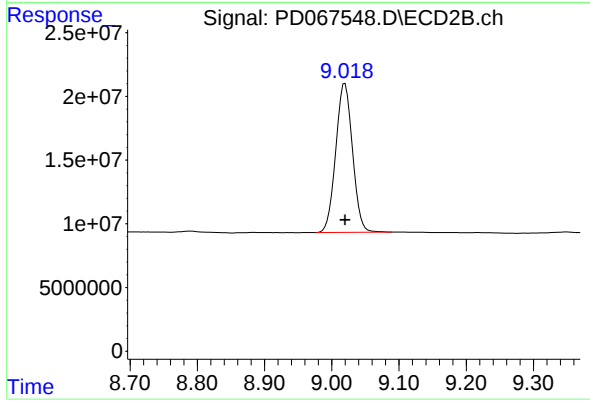

#27 Decachlorobiphenyl

R.T.: 9.020 min
Delta R.T.: 0.000 min
Response: 201191631
Conc: 40.00 ng/ml