

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD122921\
 Data File : PD067550.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Dec 2021 12:17
 Operator : AR\AJ
 Sample : INDA401
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 28 13:50:01 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD122921CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 28 13:49:05 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.434	3.964	89419000	308.4E6	40.553	38.689
27)	SA Decachlor...	8.158	9.020	72252510	389.1E6	76.701	77.350
Target Compounds							
2)	A alpha-BHC	3.870	4.358	138.7E6	418.0E6	42.148	40.236
3)	MA gamma-BHC...	4.152	4.642	129.7E6	391.2E6	41.839	39.818
4)	MA Heptachlor	4.445	5.143	128.2E6	350.0E6	41.894	39.529
9)	A Endosulfan I	5.466	6.192	107.2E6	283.5E6	41.198	39.475
13)	MA Dieldrin	5.708	6.450	237.3E6	599.7E6	84.414	80.324
14)	MA Endrin	5.966	6.669	177.7E6	449.3E6	82.467	82.156
16)	A 4,4'-DDD	6.091	6.796	165.5E6	470.9E6	83.816	80.279
17)	MA 4,4'-DDT	6.329	7.093	170.9E6	467.9E6	84.310	80.505
20)	A Methoxychlor	6.877	7.555	351.9E6	1065.1E6	404.272	388.191


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD122921\
Data File : PD067550.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Dec 2021 12:17
Operator : AR\AJ
Sample : INDA401
Misc :
ALS Vial : 37 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 28 13:50:01 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD122921CLP.M
Quant Title : GC Extractables
QLast Update : Tue Dec 28 13:49:05 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

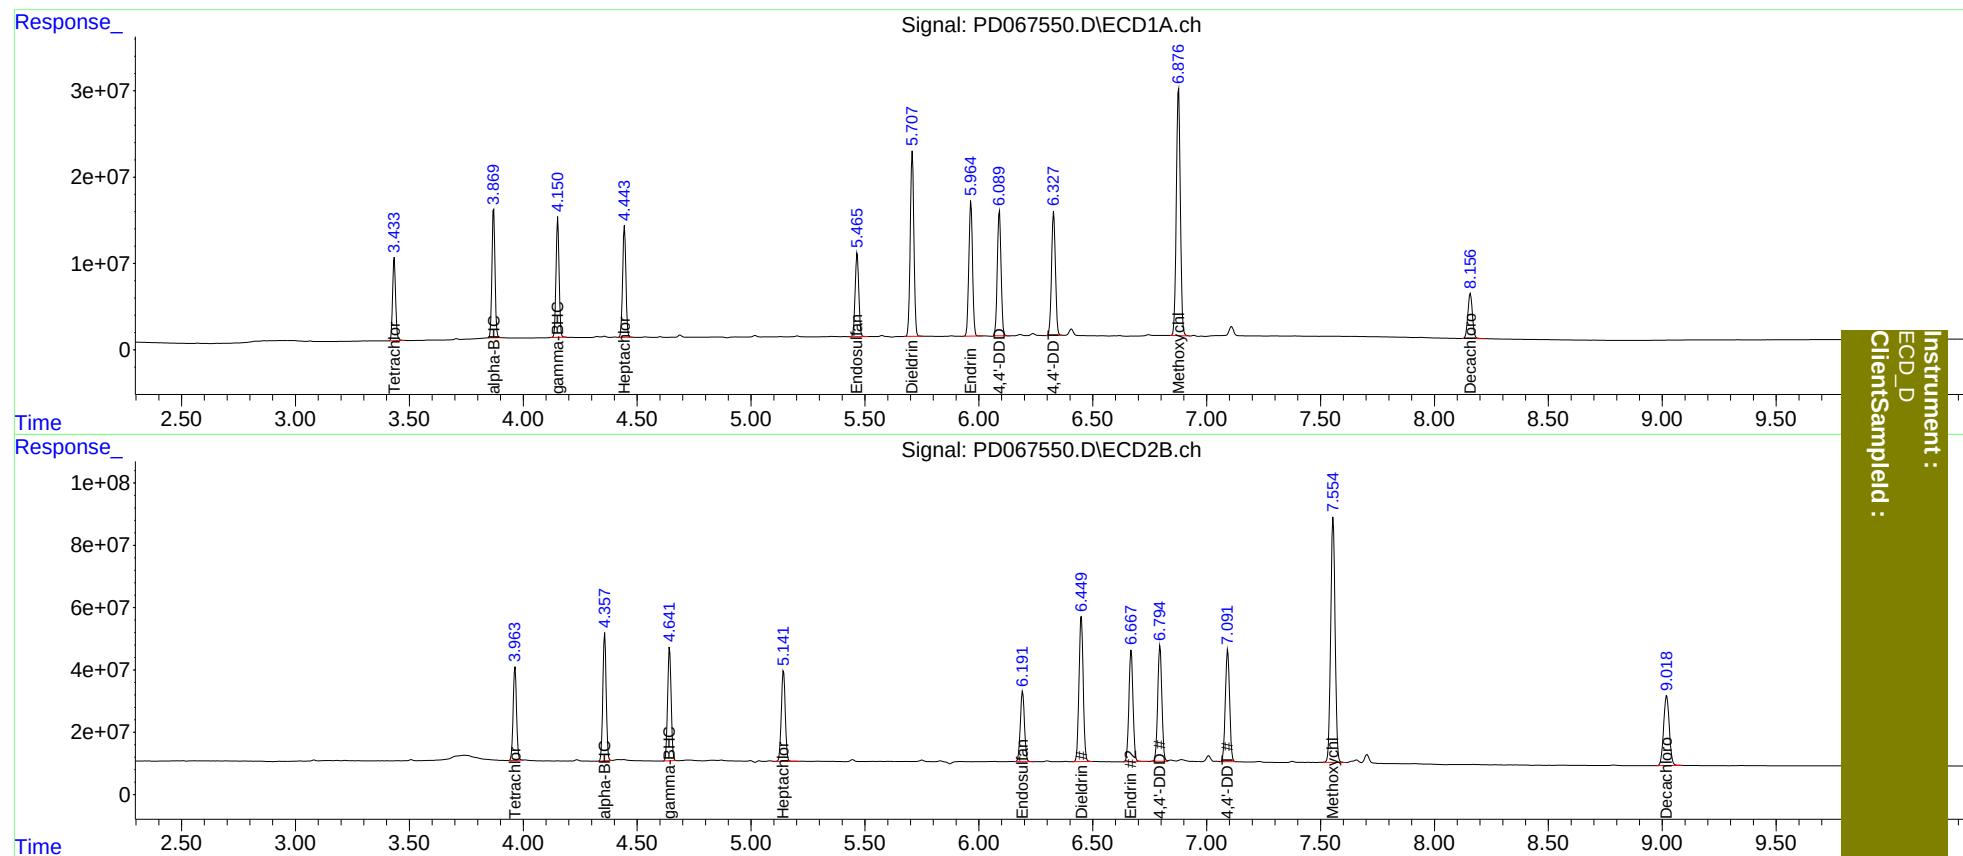


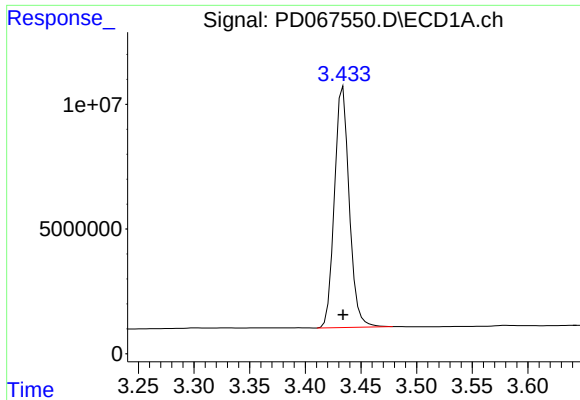

#1 Tetrachloro-m-xylene


R.T.: 3.434 min
Delta R.T.: 0.000 min
Response: 89419000
Conc: 40.55 ng/ml

Instrument :
ECD_D
ClientSampleId :

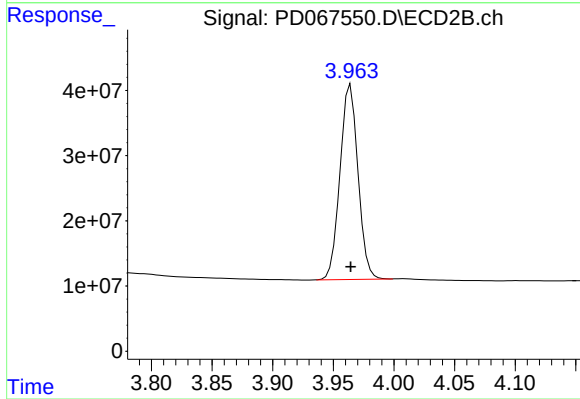


#1 Tetrachloro-m-xylene

R.T.: 3.964 min
Delta R.T.: 0.000 min
Response: 308376686
Conc: 38.69 ng/ml

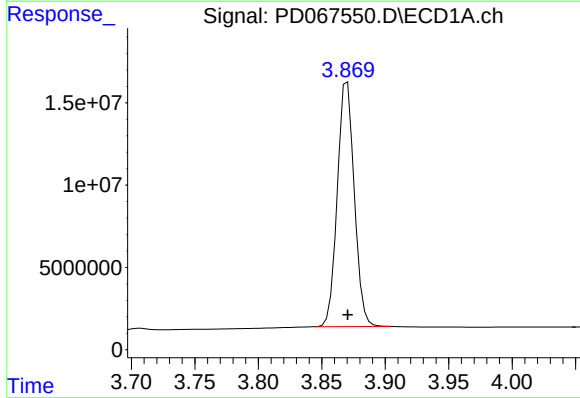


#2 alpha-BHC

R.T.: 3.870 min
Delta R.T.: 0.000 min
Response: 138651671
Conc: 42.15 ng/ml

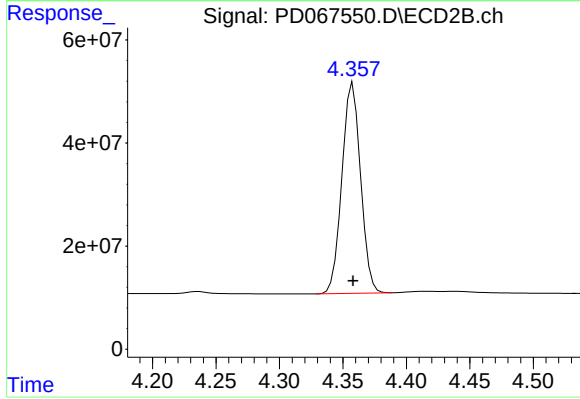

#2 alpha-BHC


R.T.: 4.358 min
Delta R.T.: 0.000 min
Response: 417989852
Conc: 40.24 ng/ml

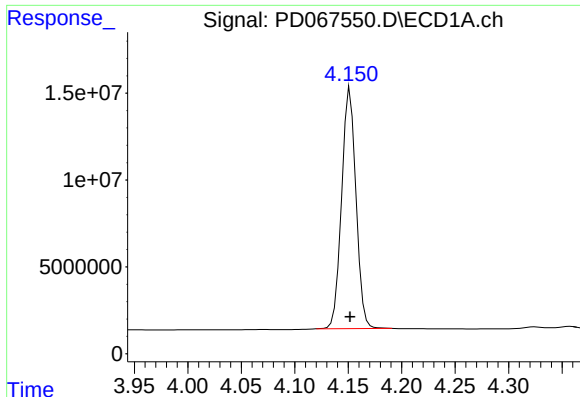

#3 gamma-BHC (Lindane)


R.T.: 4.152 min
Delta R.T.: 0.000 min
Response: 129707321
Conc: 41.84 ng/ml

Instrument :
ECD_D
ClientSampleId :

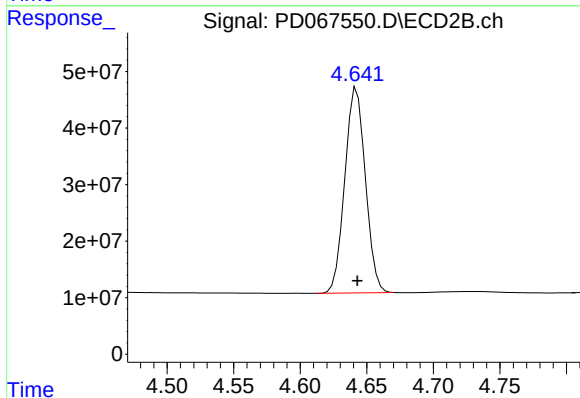


#3 gamma-BHC (Lindane)

R.T.: 4.642 min
Delta R.T.: 0.000 min
Response: 391184164
Conc: 39.82 ng/ml

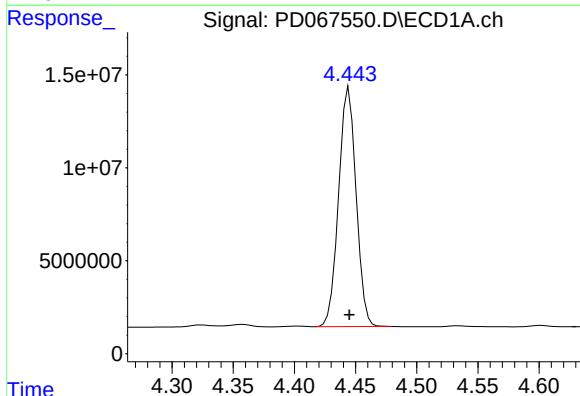


#4 Heptachlor

R.T.: 4.445 min
Delta R.T.: 0.000 min
Response: 128198727
Conc: 41.89 ng/ml

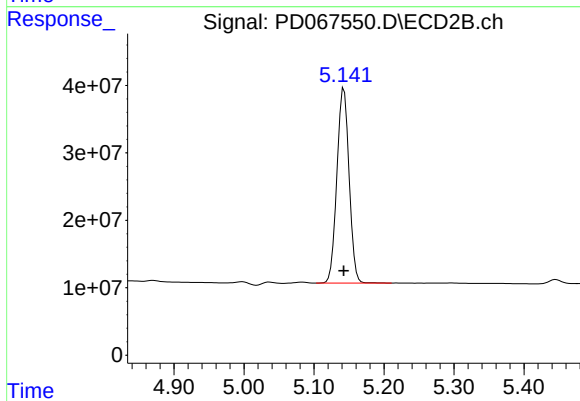

#4 Heptachlor


R.T.: 5.143 min
Delta R.T.: 0.000 min
Response: 350003961
Conc: 39.53 ng/ml

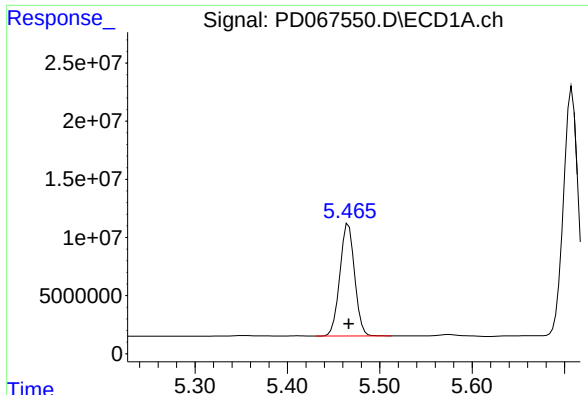

#9 Endosulfan I


R.T.: 5.466 min
Delta R.T.: 0.000 min
Response: 107175503
Conc: 41.20 ng/ml

Instrument :
ECD_D
ClientSampleId :

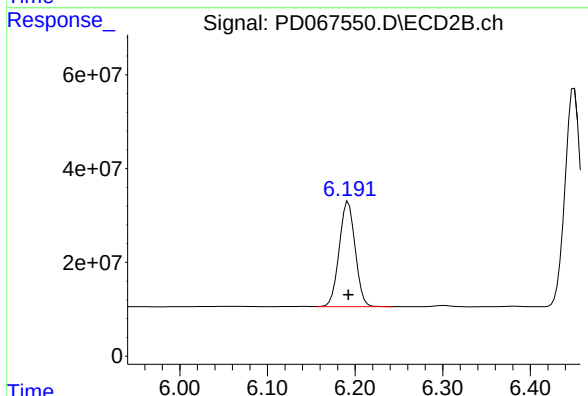


#9 Endosulfan I

R.T.: 6.192 min
Delta R.T.: 0.000 min
Response: 283540450
Conc: 39.48 ng/ml

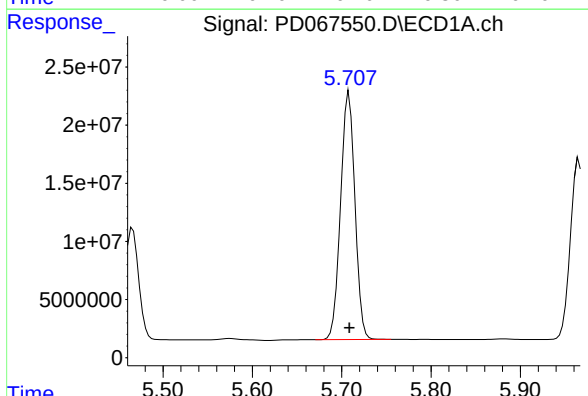


#13 Dieldrin

R.T.: 5.708 min
Delta R.T.: 0.000 min
Response: 237279338
Conc: 84.41 ng/ml

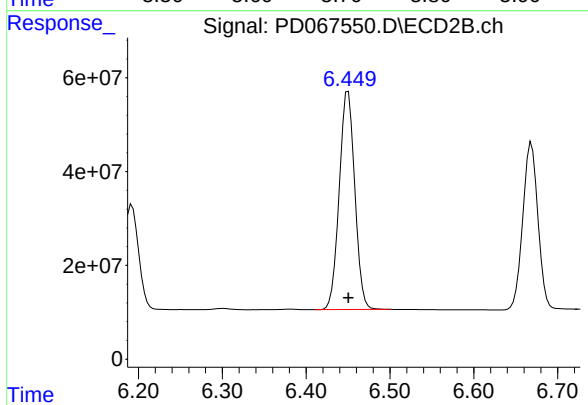

#13 Dieldrin


R.T.: 6.450 min
Delta R.T.: 0.000 min
Response: 599731355
Conc: 80.32 ng/ml

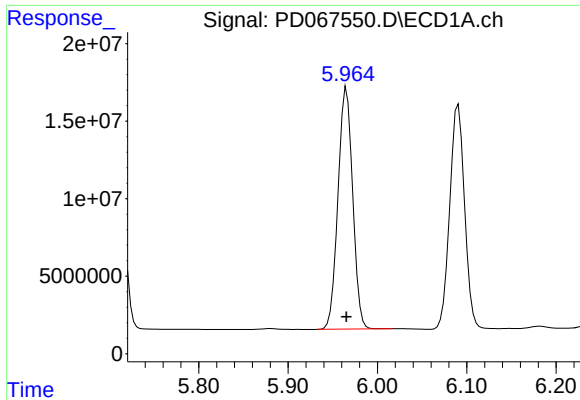

#14 Endrin


R.T.: 5.966 min
Delta R.T.: 0.000 min
Response: 177670752
Conc: 82.47 ng/ml

Instrument :
ECD_D
ClientSampleId :

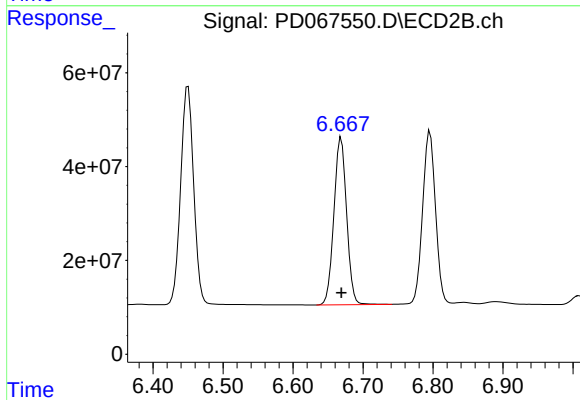


#14 Endrin

R.T.: 6.669 min
Delta R.T.: 0.000 min
Response: 449331836
Conc: 82.16 ng/ml

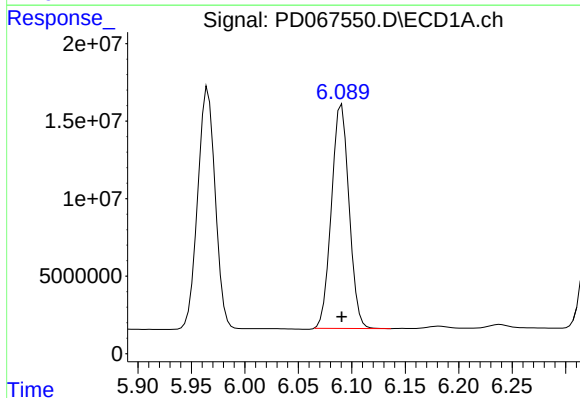


#16 4,4'-DDD

R.T.: 6.091 min
Delta R.T.: 0.000 min
Response: 165514257
Conc: 83.82 ng/ml

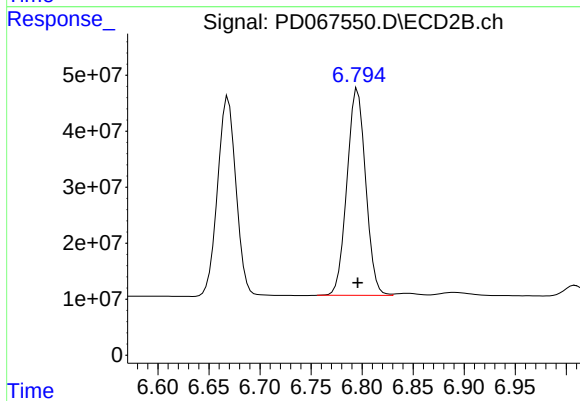

#16 4,4'-DDD


R.T.: 6.796 min
Delta R.T.: 0.000 min
Response: 470918567
Conc: 80.28 ng/ml

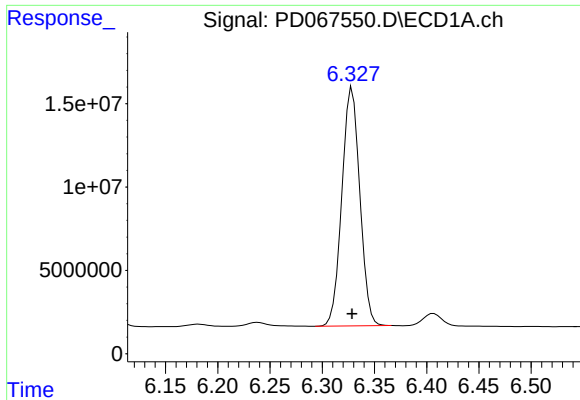

#17 4,4'-DDT


R.T.: 6.329 min
Delta R.T.: 0.000 min
Response: 170935340
Conc: 84.31 ng/ml

Instrument :
ECD_D
ClientSampleId :

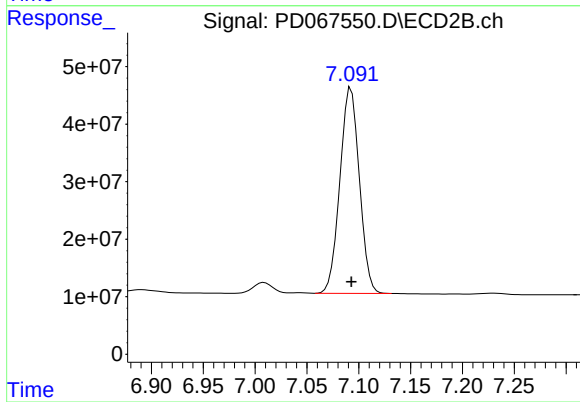


#17 4,4'-DDT

R.T.: 7.093 min
Delta R.T.: 0.000 min
Response: 467904339
Conc: 80.51 ng/ml

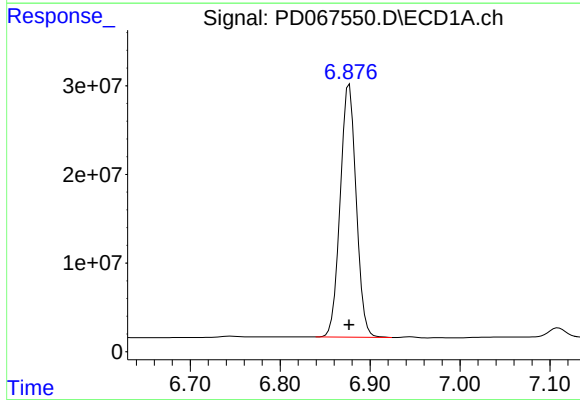


#20 Methoxychlor

R.T.: 6.877 min
Delta R.T.: 0.000 min
Response: 351923406
Conc: 404.27 ng/ml

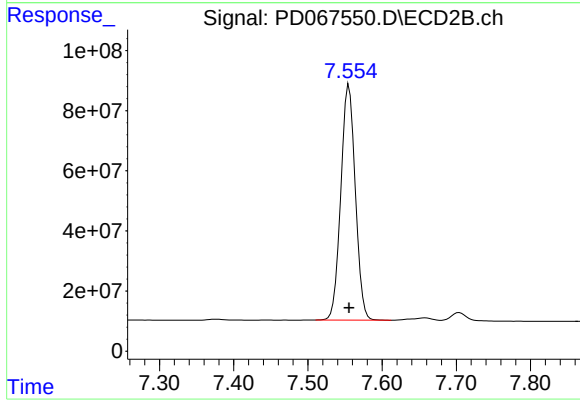

#20 Methoxychlor


R.T.: 7.555 min
Delta R.T.: 0.000 min
Response: 1065097703
Conc: 388.19 ng/ml

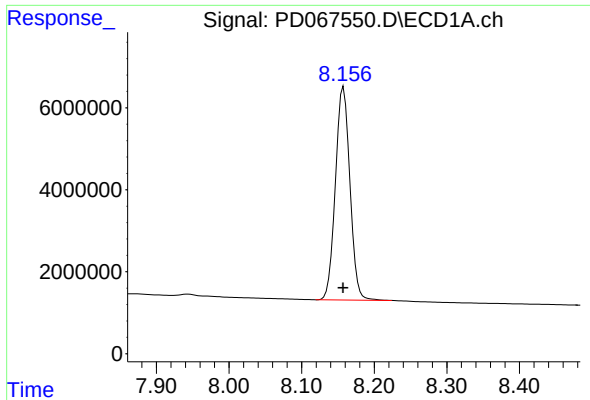

#27 Decachlorobiphenyl

R.T.: 8.158 min
Delta R.T.: 0.000 min
Response: 72252510
Conc: 76.70 ng/ml

Instrument :
ECD_D
ClientSampleId :

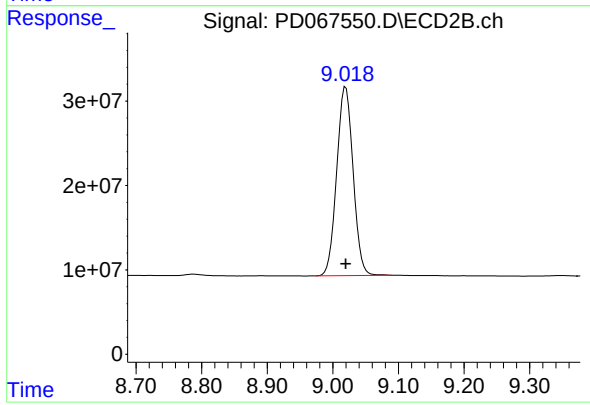

#27 Decachlorobiphenyl

R.T.: 9.020 min
Delta R.T.: 0.000 min
Response: 389052906
Conc: 77.35 ng/ml