

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD122921\
 Data File : PD067552.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Dec 2021 12:44
 Operator : AR\AJ
 Sample : INDA501
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 28 13:50:08 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD122921CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 28 13:49:05 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.434	3.964	161.9E6	540.0E6	73.421	67.746
27)	SA Decachlor...	8.158	9.020	124.8E6	671.6E6	132.476	133.516
Target Compounds							
2)	A alpha-BHC	3.870	4.358	258.1E6	752.8E6	78.455	72.463
3)	MA gamma-BHC...	4.151	4.643	238.8E6	698.5E6	77.034	71.098
4)	MA Heptachlor	4.444	5.142	235.0E6	613.7E6	76.781	69.313
9)	A Endosulfan I	5.466	6.192	193.0E6	494.7E6	74.172	68.874
13)	MA Dieldrin	5.708	6.450	431.4E6	1058.5E6	153.492	141.769
14)	MA Endrin	5.965	6.668	329.3E6	759.6E6	152.835	138.888
16)	A 4,4'-DDD	6.091	6.795	300.7E6	829.2E6	152.300	141.354
17)	MA 4,4'-DDT	6.329	7.093	310.5E6	826.0E6	153.160	142.114
20)	A Methoxychlor	6.877	7.555	623.9E6	1817.8E6	716.757	662.508


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD122921\
Data File : PD067552.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Dec 2021 12:44
Operator : AR\AJ
Sample : INDA501
Misc :
ALS Vial : 39 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 28 13:50:08 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD122921CLP.M
Quant Title : GC Extractables
QLast Update : Tue Dec 28 13:49:05 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

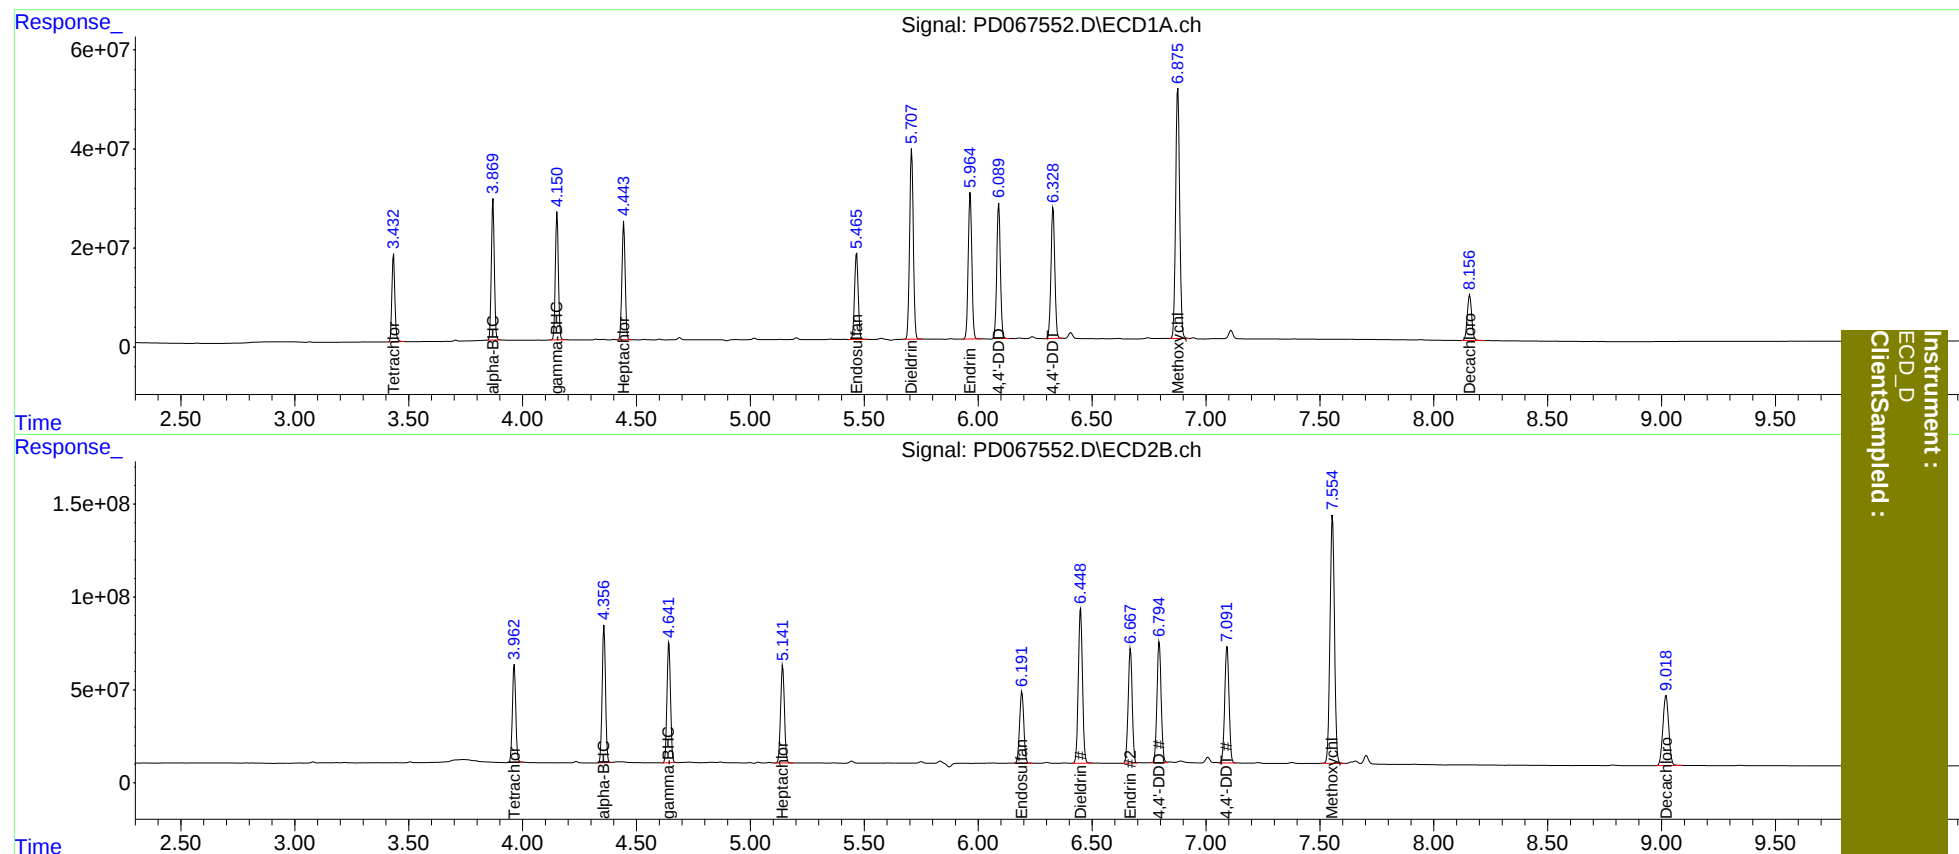


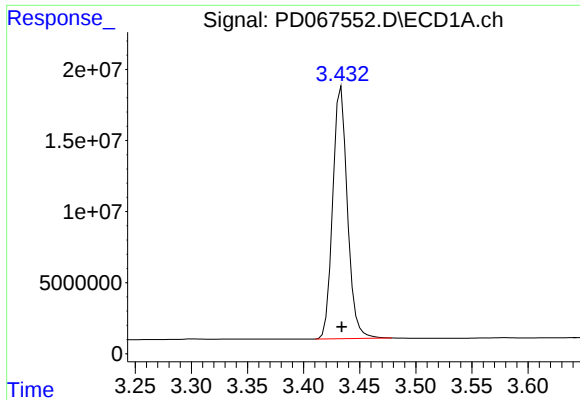

#1 Tetrachloro-m-xylene


R.T.: 3.434 min
Delta R.T.: 0.000 min
Response: 161891907
Conc: 73.42 ng/ml

Instrument :
ECD_D
ClientSampleId :

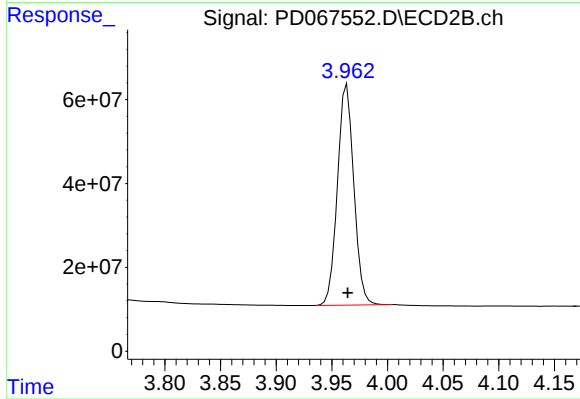


#1 Tetrachloro-m-xylene

R.T.: 3.964 min
Delta R.T.: 0.000 min
Response: 539979436
Conc: 67.75 ng/ml

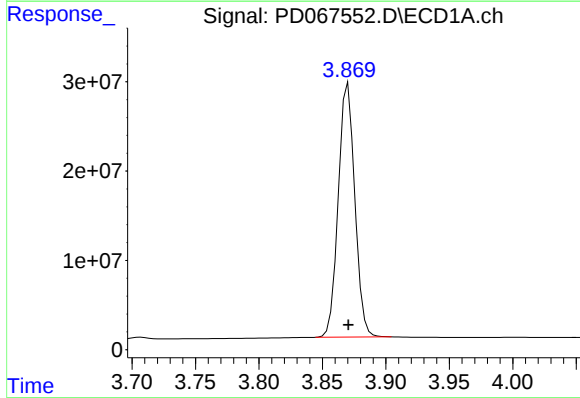


#2 alpha-BHC

R.T.: 3.870 min
Delta R.T.: 0.000 min
Response: 258084589
Conc: 78.45 ng/ml

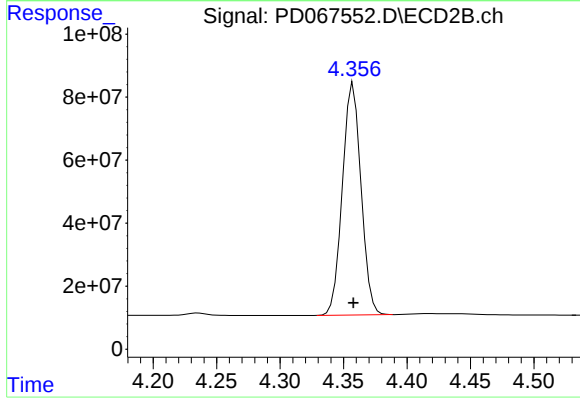

#2 alpha-BHC


R.T.: 4.358 min
Delta R.T.: 0.000 min
Response: 752779553
Conc: 72.46 ng/ml

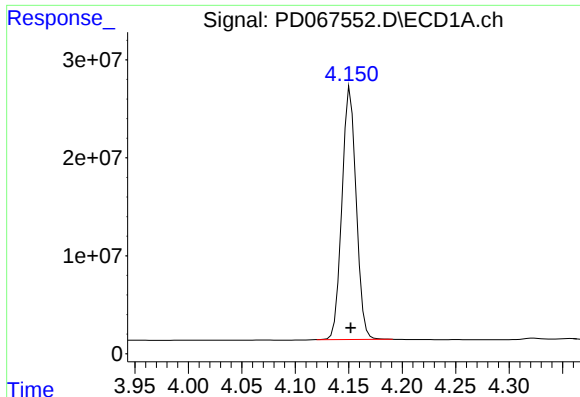

#3 gamma-BHC (Lindane)


R.T.: 4.151 min
Delta R.T.: 0.000 min
Response: 238820510
Conc: 77.03 ng/ml

Instrument :
ECD_D
ClientSampleId :

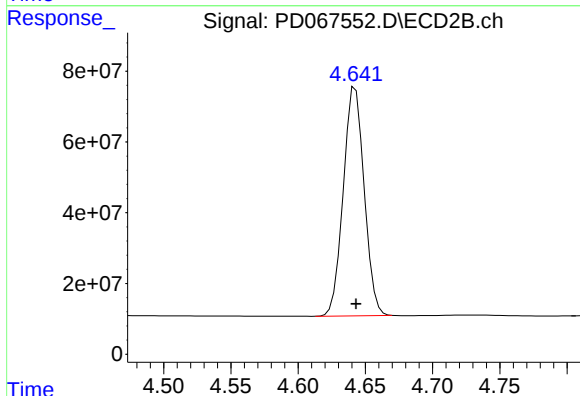


#3 gamma-BHC (Lindane)

R.T.: 4.643 min
Delta R.T.: 0.000 min
Response: 698483315
Conc: 71.10 ng/ml

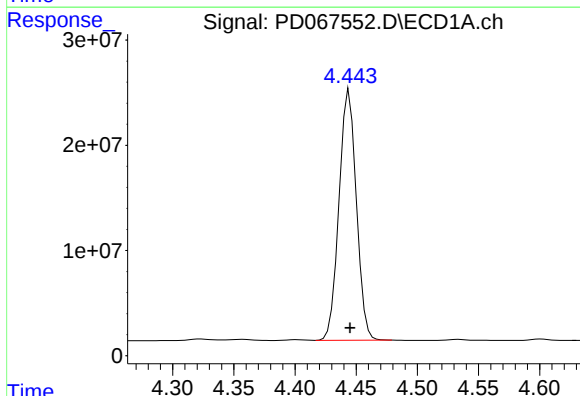


#4 Heptachlor

R.T.: 4.444 min
Delta R.T.: 0.000 min
Response: 234952621
Conc: 76.78 ng/ml

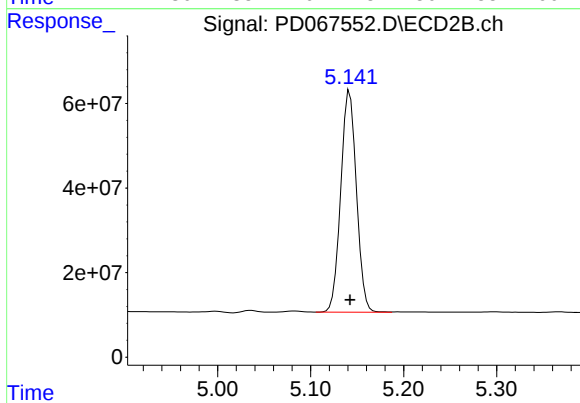

#4 Heptachlor


R.T.: 5.142 min
Delta R.T.: 0.000 min
Response: 613725984
Conc: 69.31 ng/ml

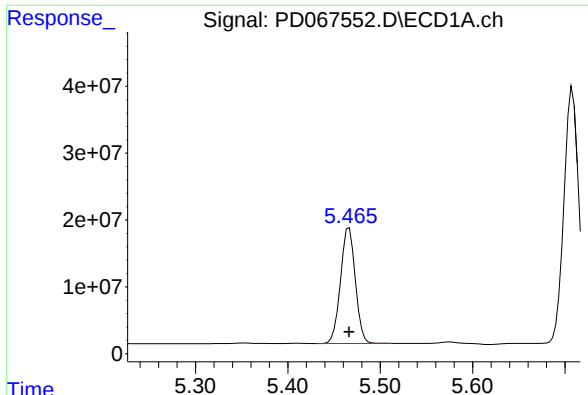

#9 Endosulfan I


R.T.: 5.466 min
Delta R.T.: 0.000 min
Response: 192957550
Conc: 74.17 ng/ml

Instrument :
ECD_D
ClientSampleId :

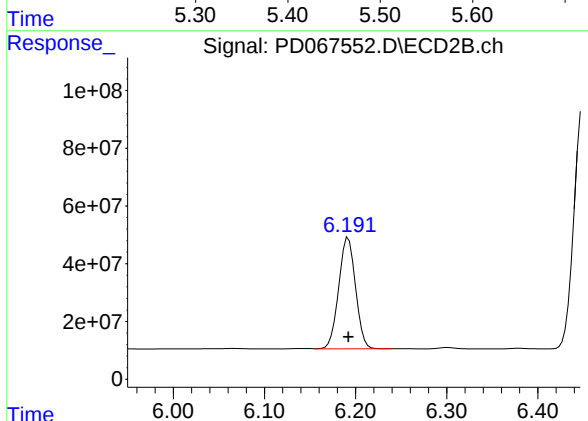


#9 Endosulfan I

R.T.: 6.192 min
Delta R.T.: 0.000 min
Response: 494701098
Conc: 68.87 ng/ml

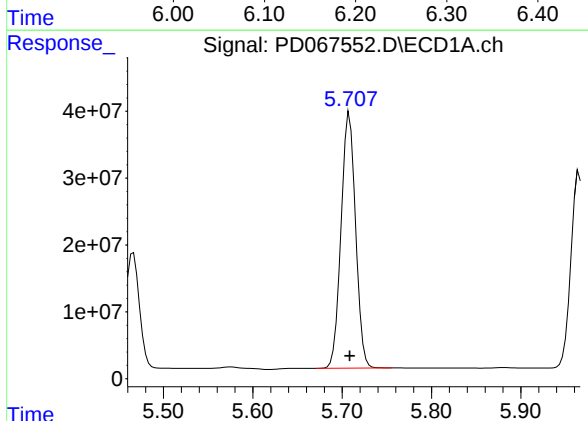


#13 Dieldrin

R.T.: 5.708 min
Delta R.T.: 0.000 min
Response: 431448045
Conc: 153.49 ng/ml

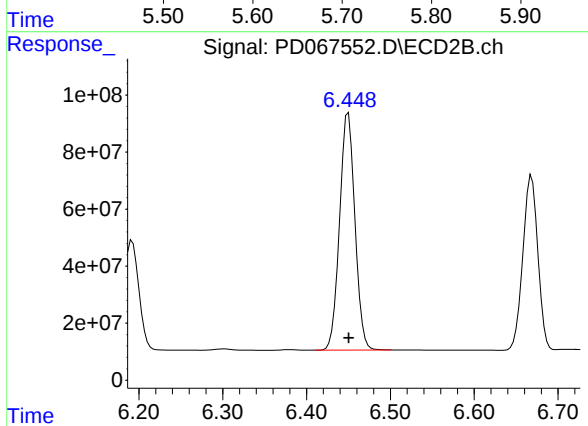

#13 Dieldrin


R.T.: 6.450 min
Delta R.T.: 0.000 min
Response: 1058508029
Conc: 141.77 ng/ml

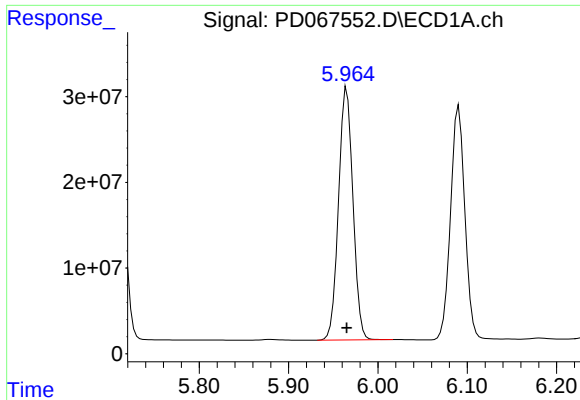

#14 Endrin


R.T.: 5.965 min
Delta R.T.: 0.000 min
Response: 329277460
Conc: 152.84 ng/ml

Instrument :
ECD_D
ClientSampleId :

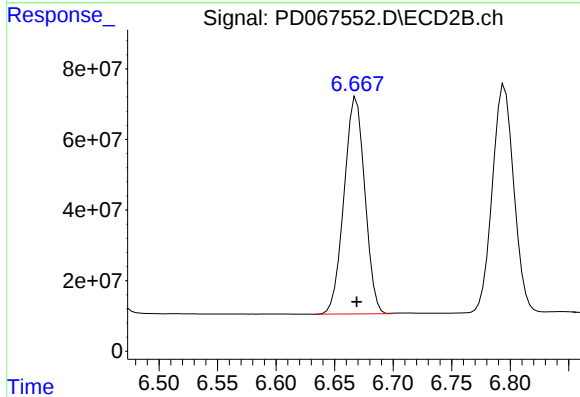


#14 Endrin

R.T.: 6.668 min
Delta R.T.: 0.000 min
Response: 759618573
Conc: 138.89 ng/ml

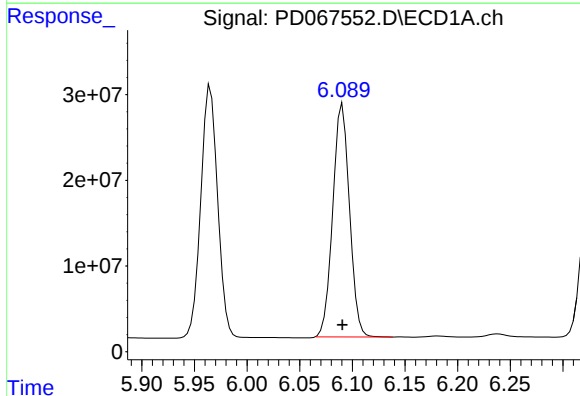


#16 4,4'-DDD

R.T.: 6.091 min
Delta R.T.: 0.000 min
Response: 300749979
Conc: 152.30 ng/ml

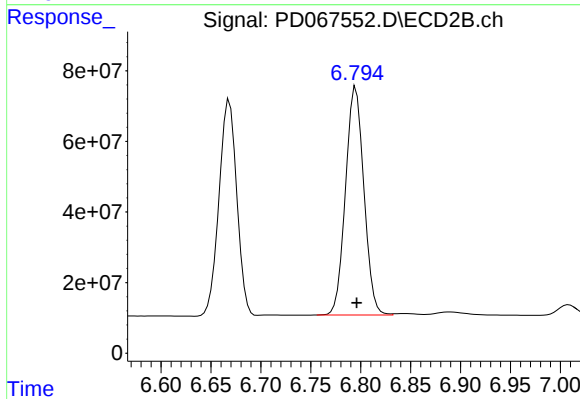

#16 4,4'-DDD


R.T.: 6.795 min
Delta R.T.: 0.000 min
Response: 829193872
Conc: 141.35 ng/ml

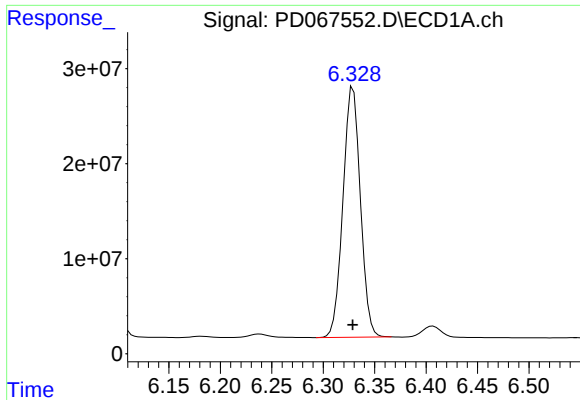

#17 4,4'-DDT


R.T.: 6.329 min
Delta R.T.: 0.000 min
Response: 310526953
Conc: 153.16 ng/ml

Instrument :
ECD_D
ClientSampleId :

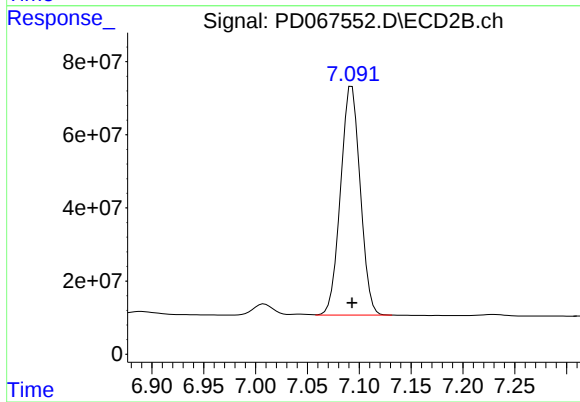


#17 4,4'-DDT

R.T.: 7.093 min
Delta R.T.: 0.000 min
Response: 825980611
Conc: 142.11 ng/ml

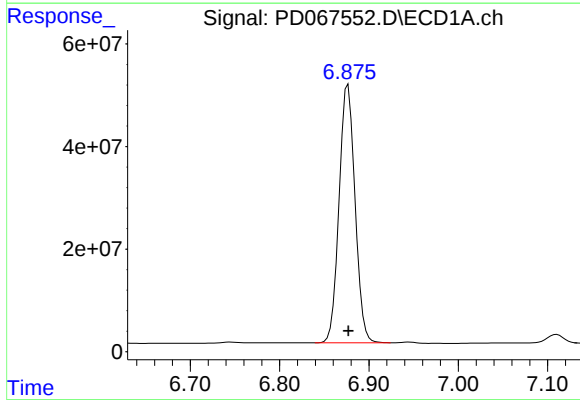


#20 Methoxychlor

R.T.: 6.877 min
Delta R.T.: 0.000 min
Response: 623944541
Conc: 716.76 ng/ml

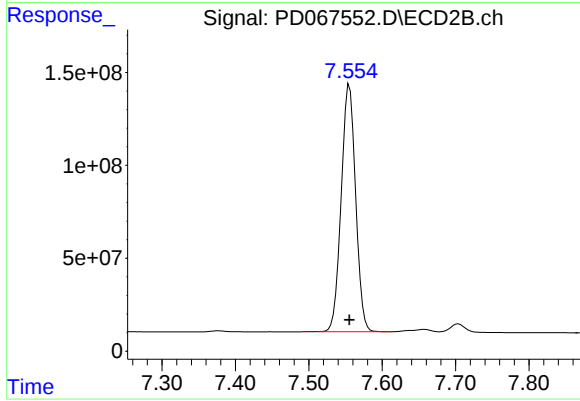

#20 Methoxychlor


R.T.: 7.555 min
Delta R.T.: 0.000 min
Response: 1817753749
Conc: 662.51 ng/ml

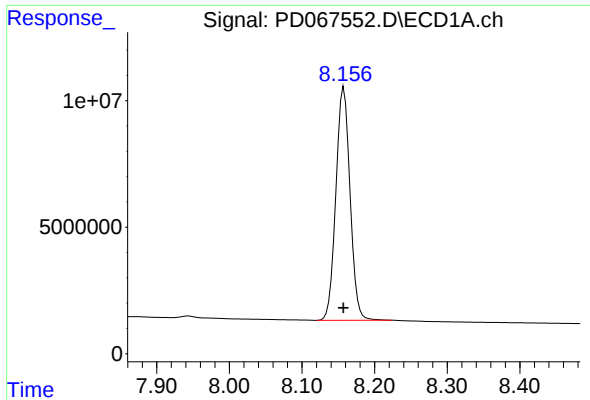

#27 Decachlorobiphenyl

R.T.: 8.158 min
Delta R.T.: 0.000 min
Response: 124793142
Conc: 132.48 ng/ml

Instrument :
ECD_D
ClientSampleId :

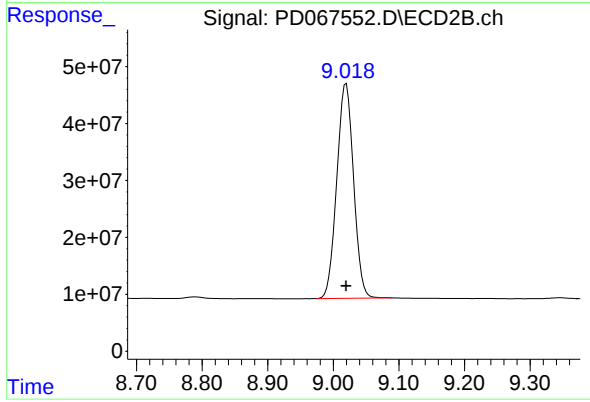

#27 Decachlorobiphenyl

R.T.: 9.020 min
Delta R.T.: 0.000 min
Response: 671557849
Conc: 133.52 ng/ml