

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD122921\
 Data File : PD067537.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Dec 2021 09:18
 Operator : AR\AJ
 Sample : RESC008
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 RESC016

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 28 14:48:07 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD122921CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 28 14:32:50 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.434	3.963	43987468	152.1E6	19.415	18.770
2)	SA Decachlor...	8.159	9.018	35979509	189.8E6	37.566	37.562
Target Compounds							
2)	A alpha-BHC	3.871	4.357	32731484	102.8E6	9.876	9.813
3)	MA gamma-BHC...	4.152	4.642	31392331	97419304	9.924	9.874
4)	MA Heptachlor	4.445	5.142	30375077	88929541	9.800	9.945
5)	MB Aldrin	4.690	5.445	32283689	85482118	10.326	10.193
6)	B beta-BHC	4.401	4.820	14419471	48421765	10.729	10.472
7)	B delta-BHC	4.603	5.035	30805249	95995466	10.415	10.239
8)	B Heptachlo...	5.131	5.834	28516503	81434904	10.258	9.707
9)	A Endosulfan I	5.467	6.191	26685979	71713663	10.082	9.981
10)	B trans-Chl...	5.355	6.068	28781417	74821948	10.195	10.005
11)	B cis-Chlor...	5.413	6.139	28205129	73775622	10.290	10.011
12)	B 4,4'-DDE	5.577	6.300	50671221	135.3E6	20.174	20.038
13)	MA Dieldrin	5.709	6.449	55552277	148.3E6	19.709	19.717
14)	MA Endrin	5.966	6.667	45207115	111.6E6	20.292	20.004
15)	B Endosulfa...	6.240	6.883	44234409	128.6E6	20.448	20.353
16)	A 4,4'-DDD	6.091	6.794	39412298	115.3E6	19.783	19.621
17)	MA 4,4'-DDT	6.330	7.092	39205745	115.0E6	19.039	19.794
18)	B Endrin al...	6.408	7.008	33558804	100.2E6	21.546	21.192
19)	B Endosulfa...	6.620	7.231	37360610	120.4E6	20.563	20.632
20)	A Methoxychlor	6.878	7.554	85802745	273.5E6	97.285	99.210
21)	B Endrin ke...	7.112	7.703	41407676	139.7E6	21.762	21.103

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD122921\
Data File : PD067537.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Dec 2021 09:18
Operator : AR\AJ
Sample : RESC008
Misc :
ALS Vial : 24 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 28 14:48:07 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD122921CLP.M
Quant Title : GC Extractables
QLast Update : Tue Dec 28 14:32:50 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

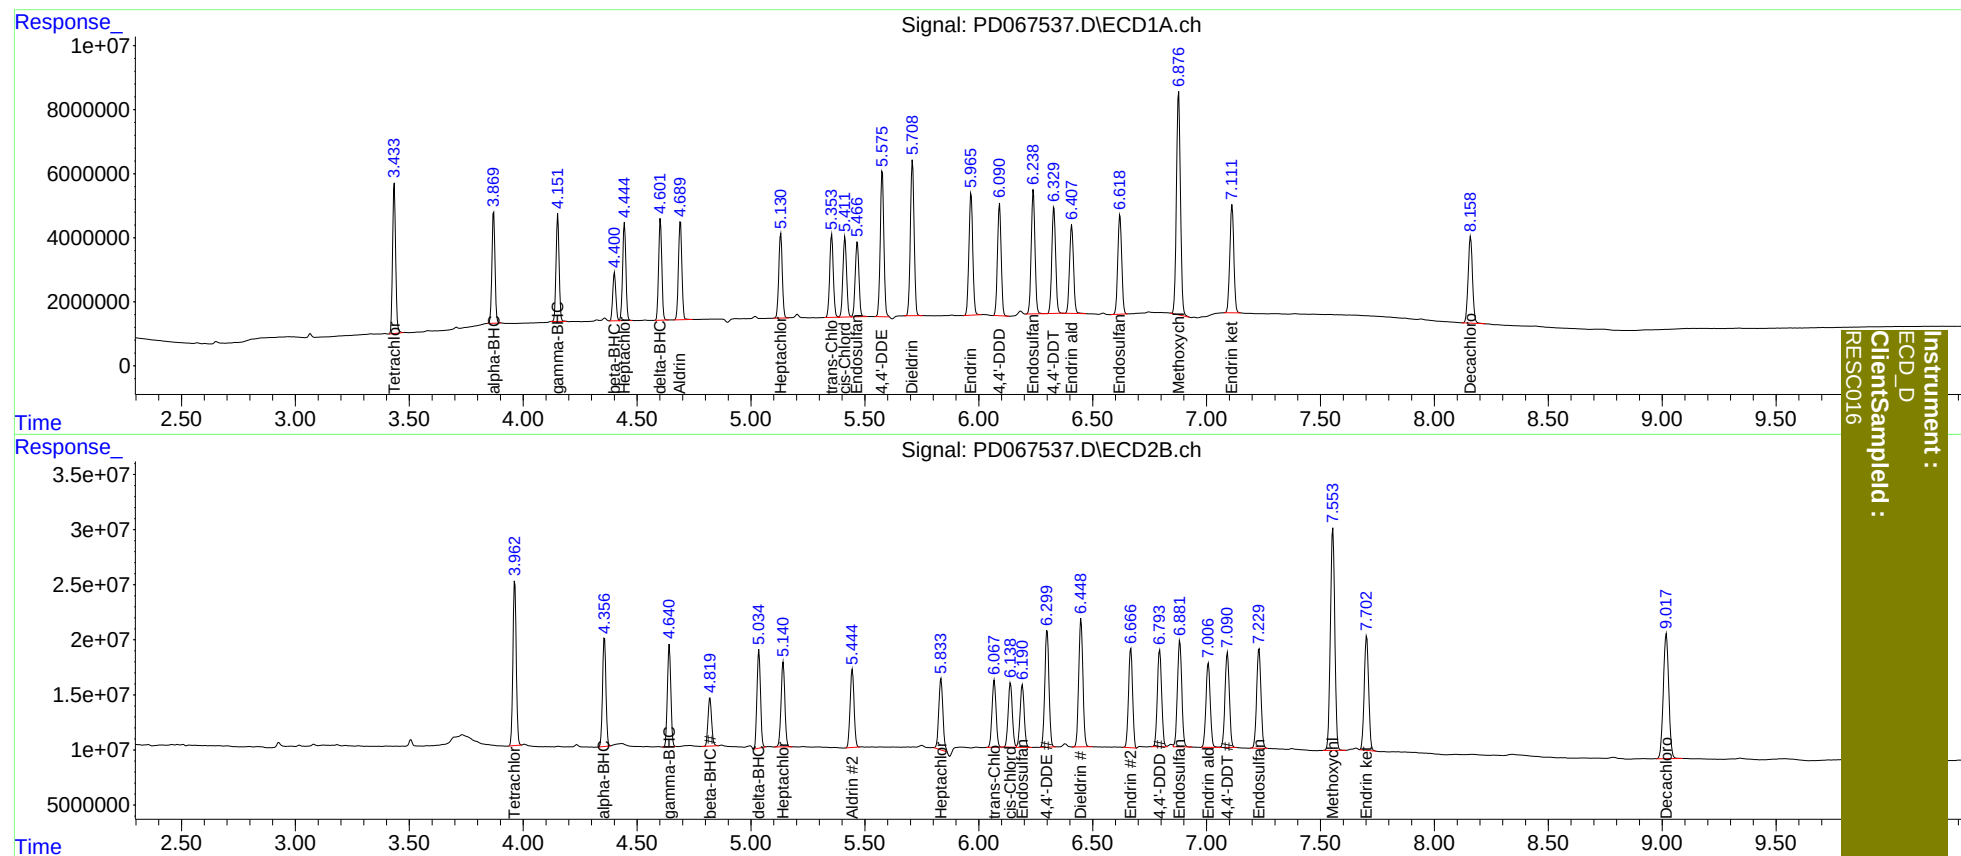

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD122921\
Data File : PD067537.D
Acq On : 28 Dec 2021 09:18
Operator : AR\AJ
Sample : RESC008
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESC016

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e

Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD122921CLP.M
Title : GC Extractables
Last Update : Tue Dec 28 14:32:50 2021
Integrator: ChemStation

RT#1	RT#2	Resolution
3.434	3.871	100.00%
3.871	4.152	100.00%
4.152	4.401	100.00%
4.401	4.445	99.92%
4.445	4.603	100.00%
4.603	4.690	100.00%
4.690	5.131	100.00%
5.131	5.355	100.00%
5.355	5.413	100.00%
5.413	5.467	98.88%
5.467	5.577	100.00%
5.577	5.709	100.00%
5.709	5.966	100.00%
5.966	6.091	100.00%
6.091	6.240	100.00%
6.240	6.330	100.00%
6.330	6.408	100.00%
6.408	6.620	100.00%
6.620	6.878	100.00%
6.878	7.112	100.00%
7.112	8.159	100.00%

Signal #2


3.963	4.357	100.00%
4.357	4.642	100.00%
4.642	4.820	100.00%
4.820	5.035	100.00%
5.035	5.142	100.00%
5.142	5.445	100.00%
5.445	5.834	100.00%
5.834	6.068	100.00%
6.068	6.139	100.00%
6.139	6.191	98.97%
6.191	6.300	100.00%
6.300	6.449	100.00%
6.449	6.667	100.00%
6.667	6.794	100.00%
6.794	6.883	100.00%
6.883	7.008	100.00%
7.008	7.092	100.00%
7.092	7.231	100.00%
7.231	7.554	100.00%
7.554	7.703	100.00%
7.703	9.018	100.00%

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD122921\
Data File : PD067537.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Dec 2021 09:18
Operator : AR\AJ
Sample : RESC008
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESC016

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 28 14:48:07 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD122921CLP.M
Quant Title : GC Extractables
QLast Update : Tue Dec 28 14:32:50 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

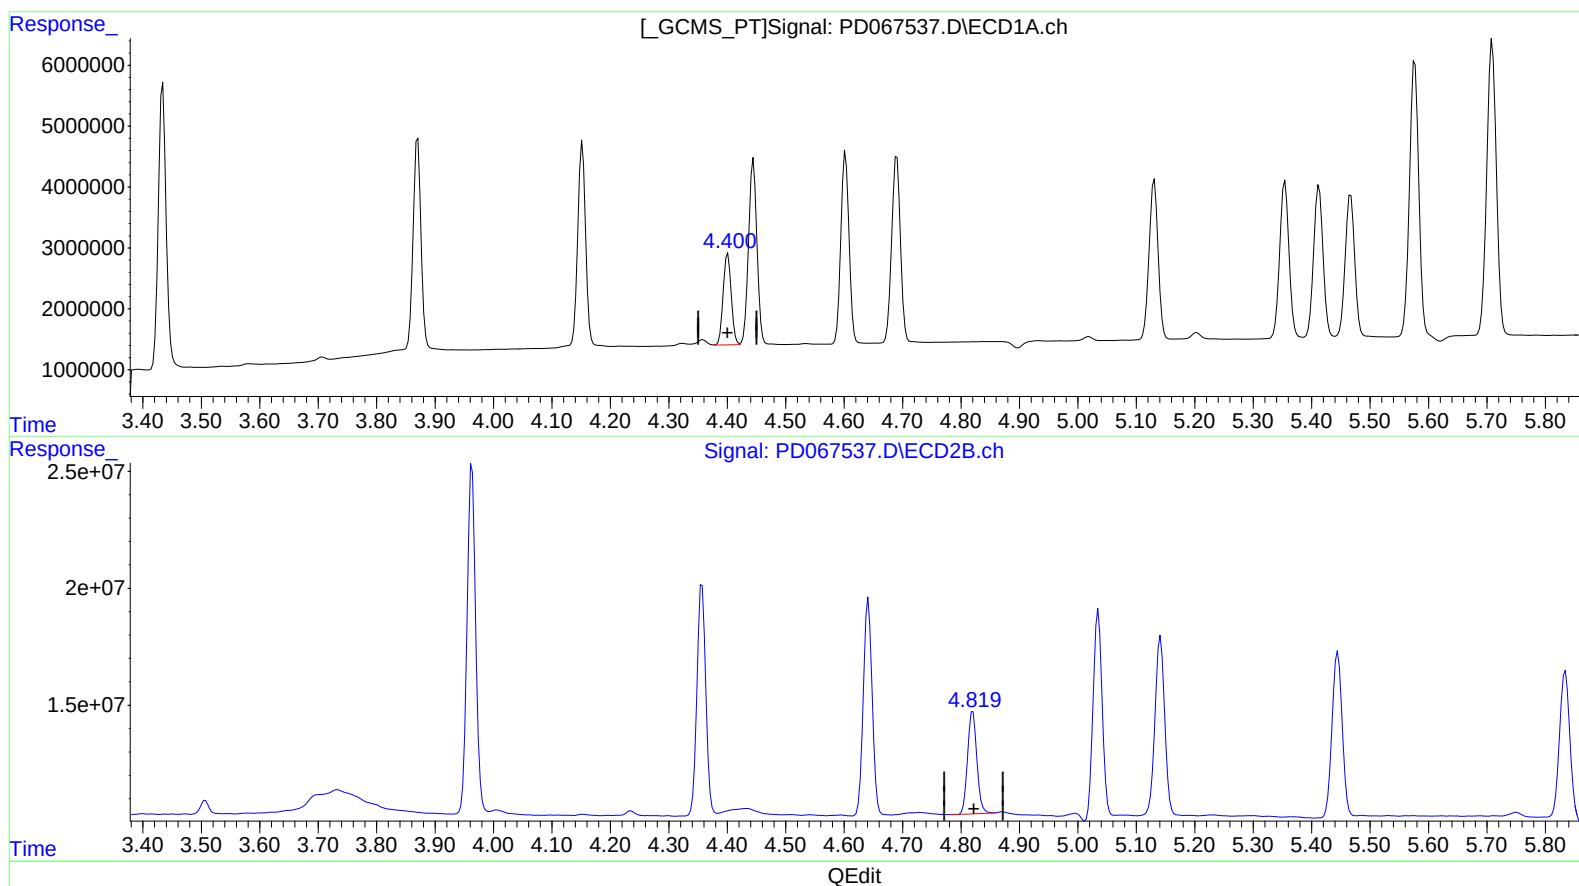

(6) beta-BHC (B)

4.401min 10.729 ng/ml

response 14419471

(6) beta-BHC #2 (B)

4.820min 10.472 ng/ml


response 48421765

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD122921\
Data File : PD067537.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Dec 2021 09:18
Operator : AR\AJ
Sample : RESC008
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESC016

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 28 14:48:07 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD122921CLP.M
Quant Title : GC Extractables
QLast Update : Tue Dec 28 14:32:50 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

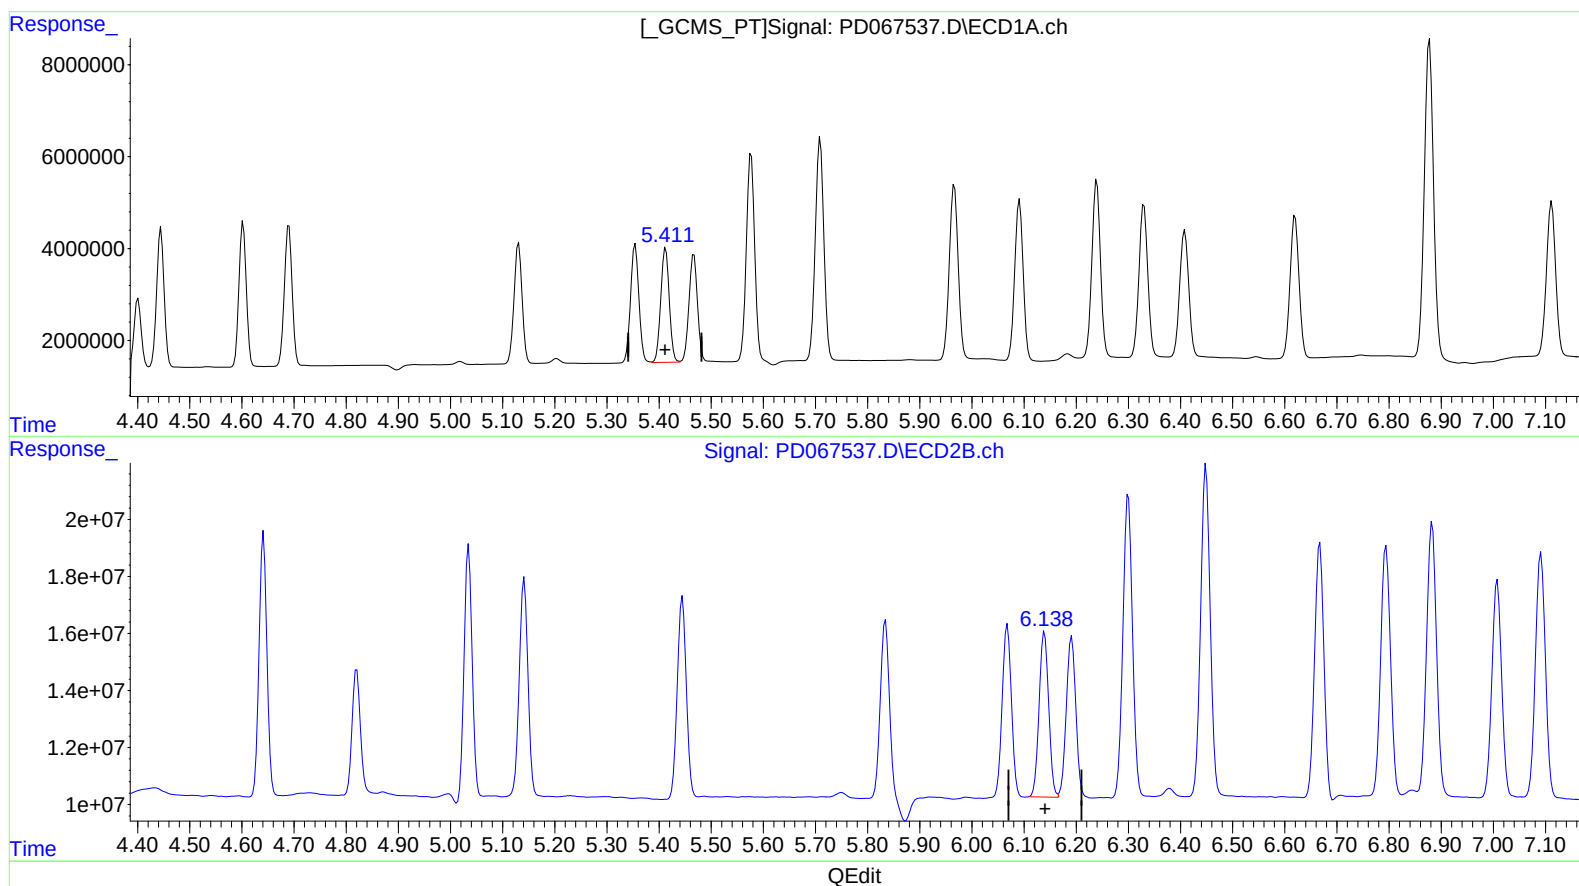

(11) cis-Chlordane (B)

5.413min 10.290 ng/ml

response 28205129

(11) cis-Chlordane #2 (B)

6.139min 10.011 ng/ml

response 73775622