Quantitation Report (QT Reviewed)

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD122923\
Data File : PD080597.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Dec 2023 17:02
Operator : AR\AJ
Sample : 05936-20
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
BGS51

Manual Integrations APPROVED

Reviewed By :Abdul Mirza 12/29/2023
Supervised By :Ankita Jodhani 12/29/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 29 04:56:30 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD121623CLP.M
Quant Title : GC Extractables
QLast Update : Thu Dec 21 13:52:23 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
	System Monitoring Compounds						
1)	SA Tetrachlo...	3.567	2.799	26205359	45464571	20.524	20.447
27)	SA Decachlor...	9.112	7.941	57736779	58213306	35.911m	24.253 #
	Target Compounds						
4)	MA Heptachlor	4.934	3.951	17443328	13691036	8.353m	4.275m#
7)	B delta-BHC	4.782	4.148	99132199	15206196	43.161m	3.911m#
13)	MA Dieldrin	6.383	5.388	45945901	87234036	24.688m	29.107m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Quantitation Report (QT Reviewed)

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD122923\
Data File : PD080597.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Dec 2023 17:02
Operator : AR\AJ
Sample : 05936-20
Misc :
ALS Vial : 27 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 29 04:56:30 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD121623CLP.M
Quant Title : GC Extractables
QLast Update : Thu Dec 21 13:52:23 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

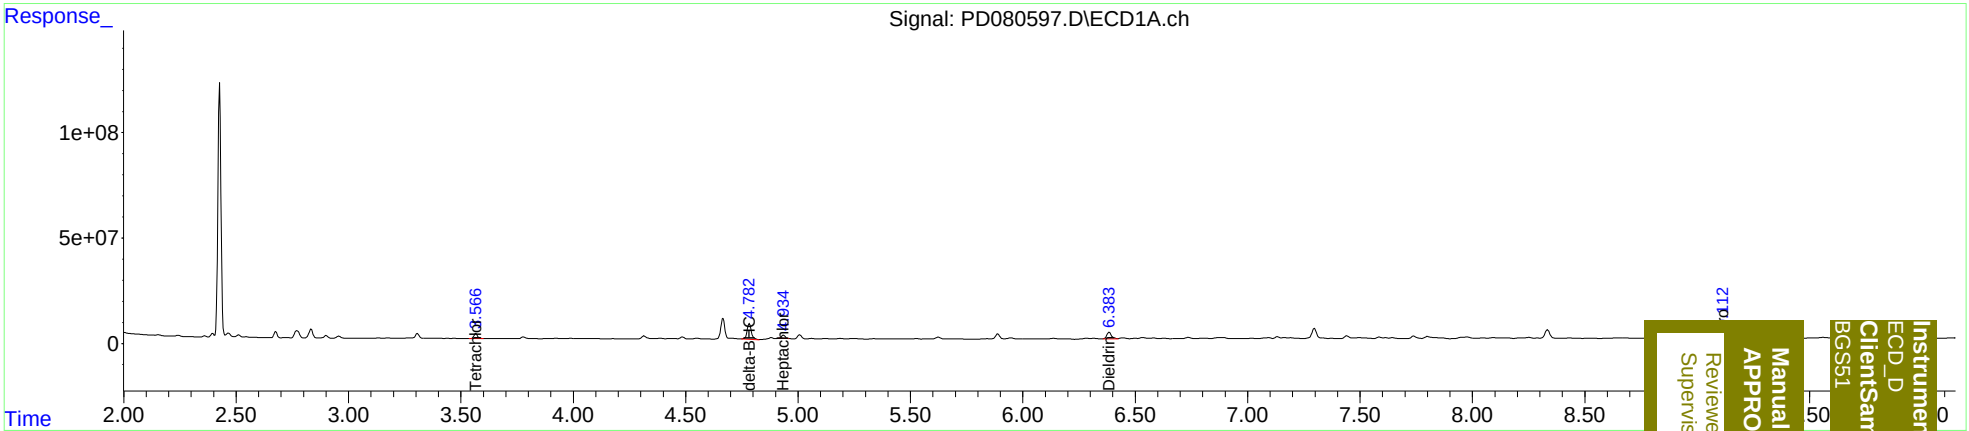

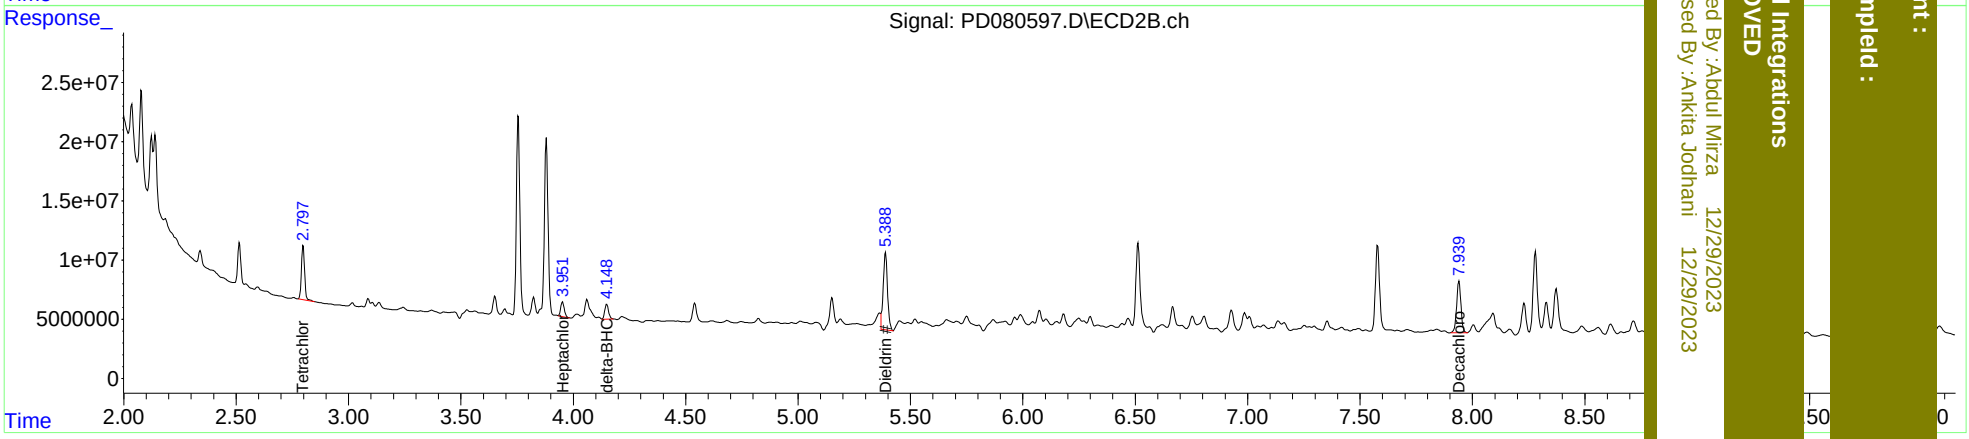

Manual Integrations APPROVED
Reviewed By :Abdul Mirza 12/29/2023
Supervised By :Ankita Jodhani 12/29/2023

Instrument :
ECD_D
ClientSampleId :
BGS51