

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Data\PD123020\  
 Data File : PD060878.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 30 Dec 2020 12:14  
 Operator : DD\AJ  
 Sample : INDA347  
 Misc :  
 ALS Vial : 10 Sample Multiplier: 1

Instrument :  
 ECD\_D  
 ClientSampleId :  
 INDA3047

Manual Integrations  
 APPROVED

Ankita  
 1/4/2021 8:40:51 AM

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Dec 31 01:30:33 2020  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Method\PD122920CLP.M  
 Quant Title : GC Extractables  
 QLast Update : Wed Dec 30 01:06:43 2020  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1 µl  
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1  
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm


|                             | Compound        | RT#1  | RT#2  | Resp#1   | Resp#2  | ng/ml   | ng/ml   |
|-----------------------------|-----------------|-------|-------|----------|---------|---------|---------|
| -----                       |                 |       |       |          |         |         |         |
| System Monitoring Compounds |                 |       |       |          |         |         |         |
| 1)                          | SA Tetrachlo... | 3.505 | 4.021 | 23002053 | 105.0E6 | 20.376  | 21.314  |
| 27)                         | SA Decachlor... | 8.292 | 9.106 | 56659586 | 167.9E6 | 41.076  | 42.478  |
| Target Compounds            |                 |       |       |          |         |         |         |
| 2)                          | A alpha-BHC     | 3.946 | 4.410 | 33082454 | 155.3E6 | 20.272  | 21.279m |
| 3)                          | MA gamma-BHC... | 4.232 | 4.697 | 31226949 | 146.2E6 | 20.129  | 22.093  |
| 4)                          | MA Heptachlor   | 4.539 | 5.209 | 33263968 | 142.8E6 | 20.167  | 21.491  |
| 9)                          | A Endosulfan I  | 5.576 | 6.260 | 28224474 | 114.5E6 | 20.205  | 21.388  |
| 13)                         | MA Dieldrin     | 5.821 | 6.518 | 61973596 | 245.2E6 | 40.532  | 42.605  |
| 14)                         | MA Endrin       | 6.080 | 6.736 | 51185187 | 181.1E6 | 39.548  | 39.120  |
| 16)                         | A 4,4'-DDD      | 6.204 | 6.855 | 49417586 | 187.8E6 | 40.674  | 41.617  |
| 17)                         | MA 4,4'-DDT     | 6.447 | 7.155 | 51873781 | 191.0E6 | 40.399  | 42.073  |
| 20)                         | A Methoxychlor  | 6.993 | 7.612 | 133.8E6  | 458.9E6 | 200.623 | 205.885 |
| -----                       |                 |       |       |          |         |         |         |

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Data\PD123020\  
Data File : PD060878.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 30 Dec 2020 12:14  
Operator : DD\AJ  
Sample : INDA347  
Misc :  
ALS Vial : 10 Sample Multiplier: 1

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Dec 31 01:30:33 2020  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Method\PD122920CLP.M  
Quant Title : GC Extractables  
QLast Update : Wed Dec 30 01:06:43 2020  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 µl  
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1  
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

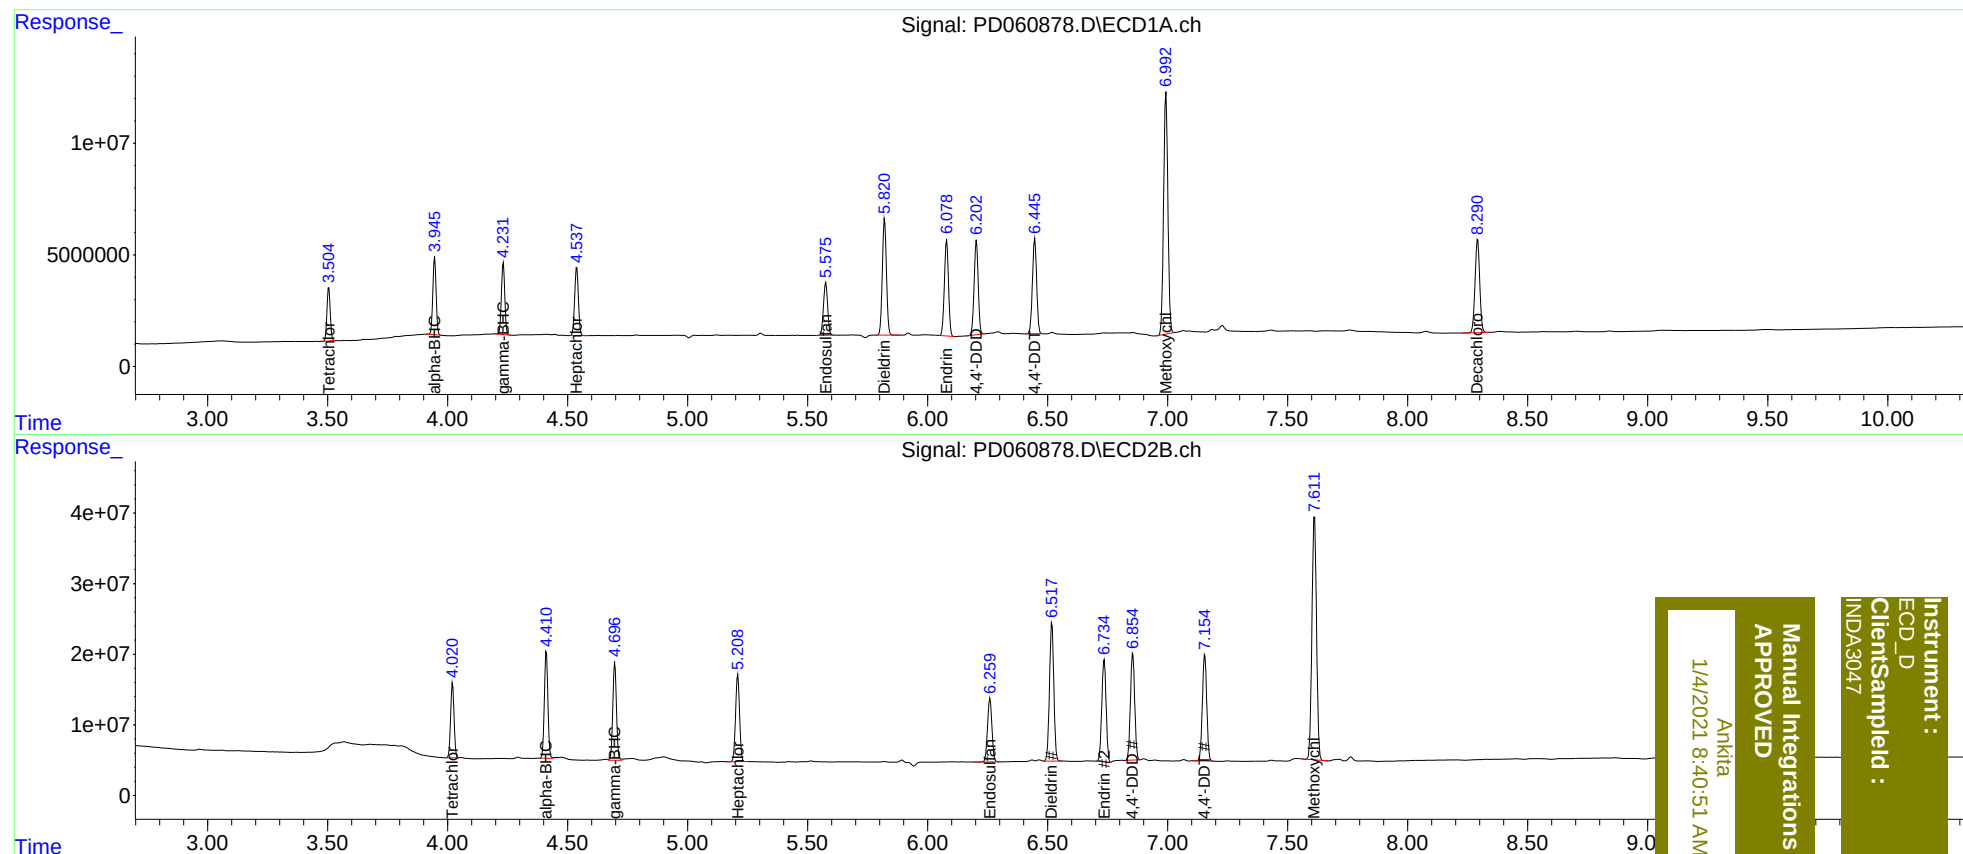

Manual Integrations  
APPROVED

Ankita  
1/4/2021 8:40:51 AM

Instrument :  
ECD\_D  
ClientSampled :  
INDA3047