

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD123020\
 Data File : PD060884.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Dec 2020 14:00
 Operator : DD\AJ
 Sample : L5195-03
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C0AC4

Manual Integrations
 APPROVED

Ankita
 1/4/2021 8:40:56 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 31 00:50:26 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD122920CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Dec 30 01:06:43 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.512	3.992f	5903.2E6	27889.7E6	5229.412m	5662.541m
2)	SA Decachlor...	8.284	9.104	43817507	130.6E6	31.766	33.052
Target Compounds							
13)	MA Dieldrin	5.814	6.516	12077415	52122928	7.899	9.057
14)	MA Endrin	6.087	6.743	5195232	13575420	4.014	2.932m#
17)	MA 4,4'-DDT	6.440	7.126	3799784	9788213	2.959	2.156 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD123020\
Data File : PD060884.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Dec 2020 14:00
Operator : DD\AJ
Sample : L5195-03
Misc :
ALS Vial : 16 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 31 00:50:26 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD122920CLP.M
Quant Title : GC Extractables
QLast Update : Wed Dec 30 01:06:43 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

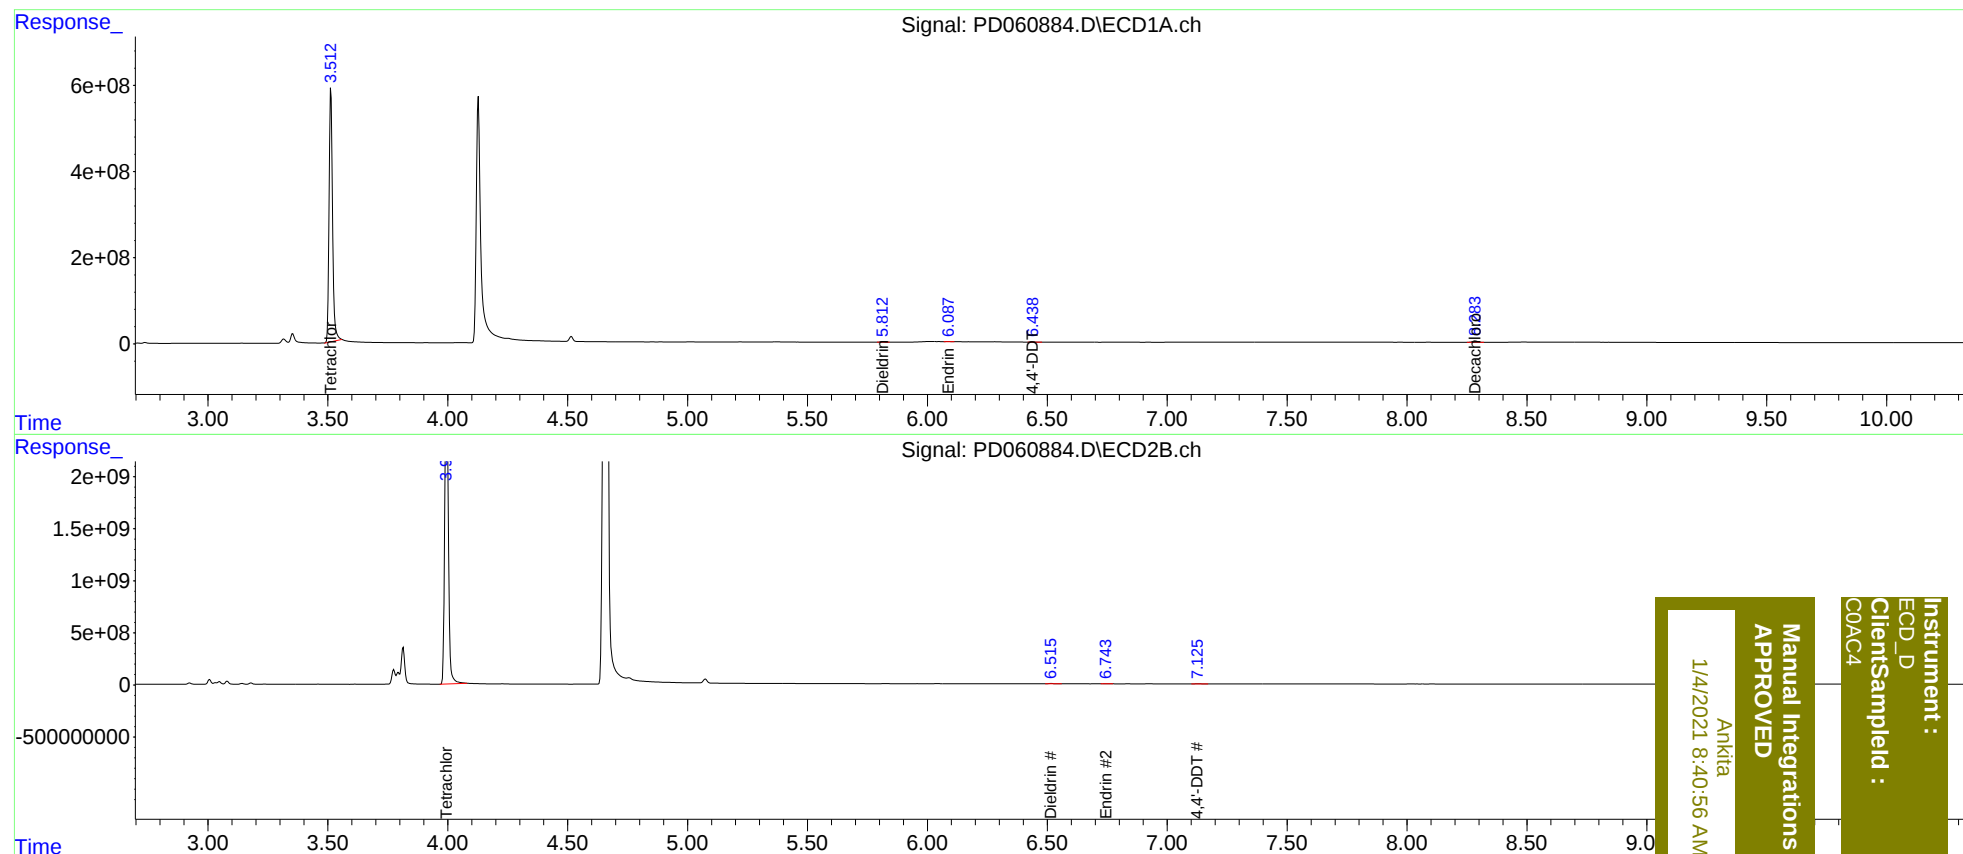

Manual Integrations
APPROVED

Ankita

1/4/2021 8:40:56 AM

Instrument :
ECD_D
ClientSampleId :
C0AC4