

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD123020\
 Data File : PD060887.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Dec 2020 14:41
 Operator : DD\AJ
 Sample : L5195-06
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C0AC7

Manual Integrations
 APPROVED

Ankita
 1/4/2021 8:41:01 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 31 00:51:29 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD122920CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Dec 30 01:06:43 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.500	4.020	24159245	101.9E6	21.402	20.682m
27)	SA Decachlor...	8.284	9.104	27408258	81345976	19.870	20.582
Target Compounds							
10)	B trans-Chl...	5.463	6.133	1655493	9116312	1.092m	1.583m#
11)	B cis-Chlor...	5.500	6.211	5466960	10734801	3.671	1.925 #
12)	B 4,4'-DDE	5.678	6.364	774178	2911900	0.529	0.535m
13)	MA Dieldrin	5.814	6.517	3636664	12613391	2.378	2.192

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD123020\
Data File : PD060887.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Dec 2020 14:41
Operator : DD\AJ
Sample : L5195-06
Misc :
ALS Vial : 19 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 31 00:51:29 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD122920CLP.M
Quant Title : GC Extractables
QLast Update : Wed Dec 30 01:06:43 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

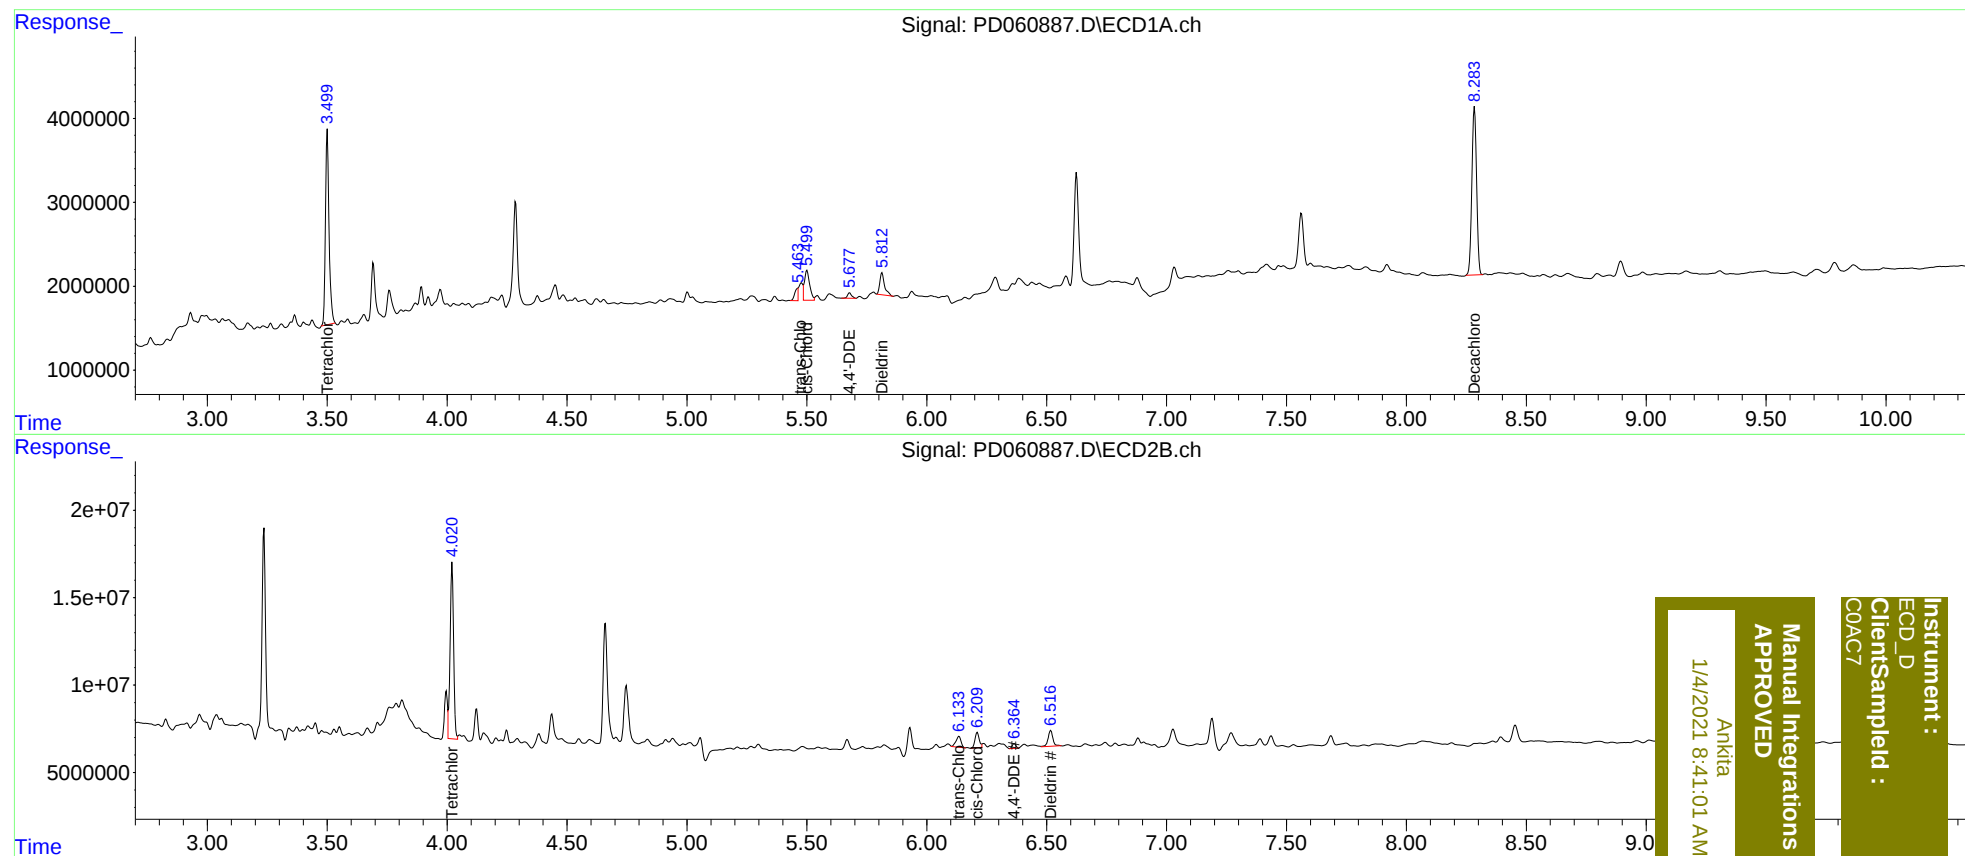

Manual Integrations
APPROVED

Ankita
1/4/2021 8:41:01 AM

Instrument :
ECD_D
ClientSampled :
C0AC7