

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD123020\
 Data File : PD060889.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Dec 2020 15:17
 Operator : DD\AJ
 Sample : L5195-03
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C0AC4

Manual Integrations
 APPROVED

Ankita
 1/4/2021 8:41:09 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 31 00:52:05 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD122920CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Dec 30 01:06:43 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.513	3.994f	5688.8E6	27048.1E6	5039.492m	5491.669m
27)	SA Decachlor...	8.286	9.106	43555012	127.9E6	31.576	32.365
Target Compounds							
13)	MA Dieldrin	5.815	6.517	11835474	52163713	7.741	9.064
14)	MA Endrin	6.088	6.744	2790132	7931279	2.156	1.713
17)	MA 4,4'-DDT	6.441	7.139	2459920	4458670	1.916	0.982 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD123020\
Data File : PD060889.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Dec 2020 15:17
Operator : DD\AJ
Sample : L5195-03
Misc :
ALS Vial : 21 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 31 00:52:05 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD122920CLP.M
Quant Title : GC Extractables
QLast Update : Wed Dec 30 01:06:43 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

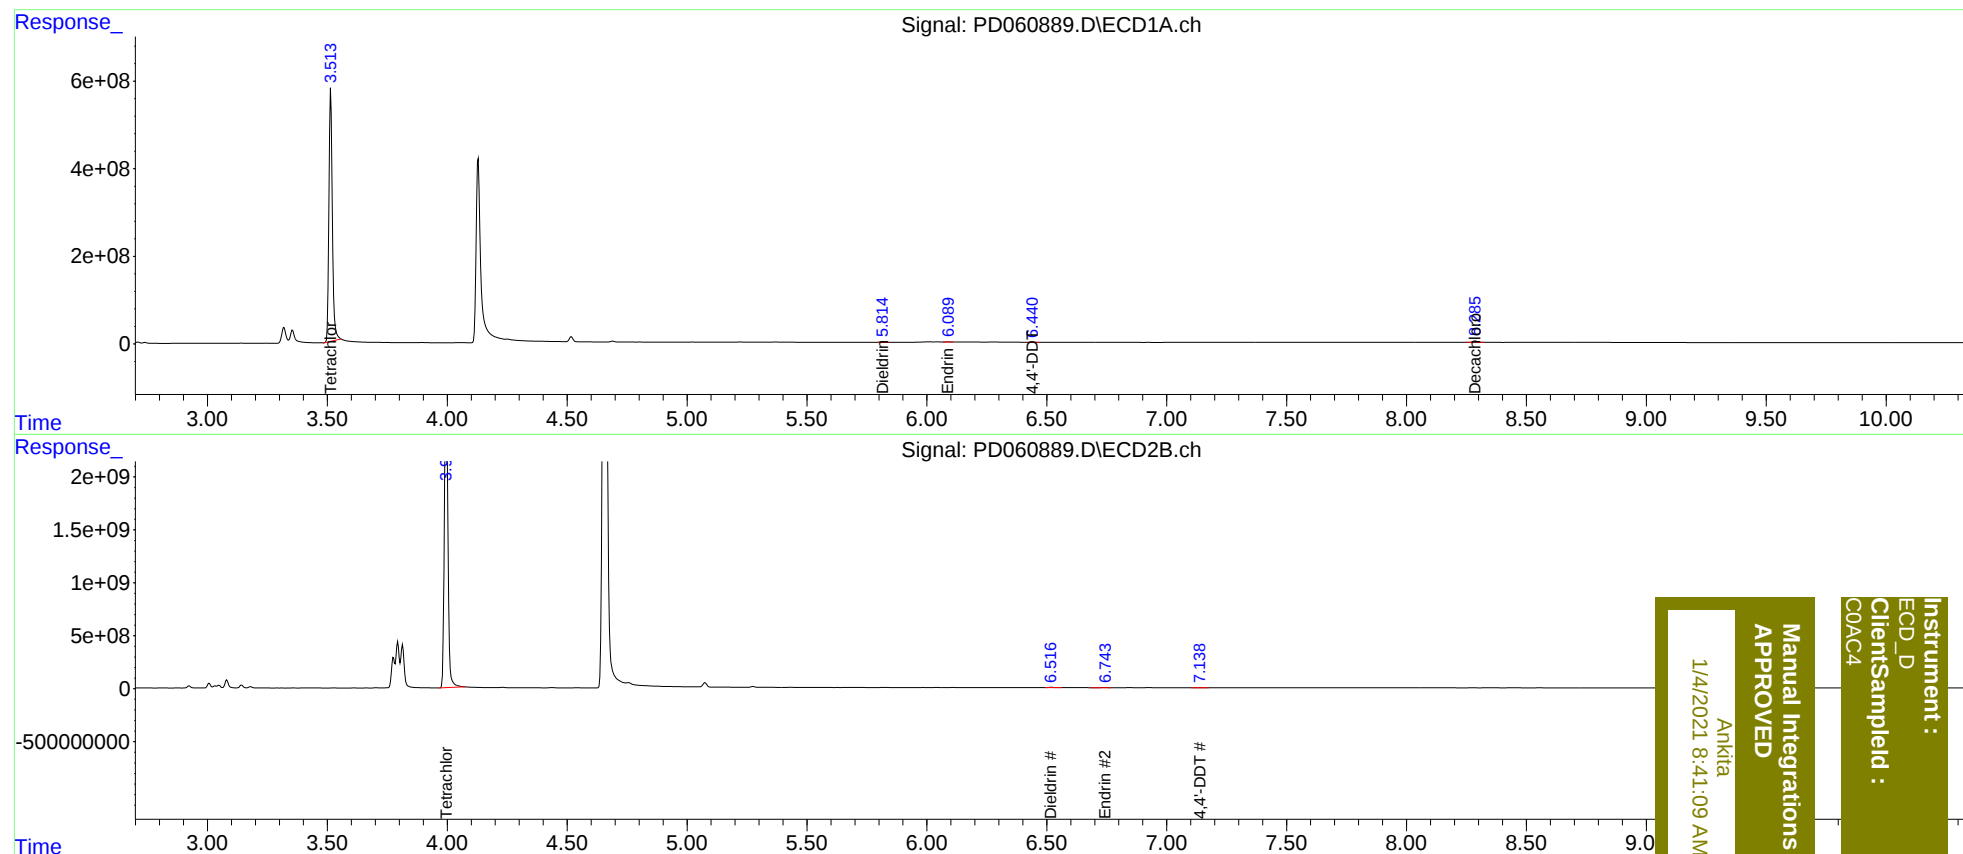

Manual Integrations
APPROVED

Ankita

1/4/2021 8:41:09 AM

Instrument :
ECD_D
ClientSampleId :
C0AC4