

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD123023\
 Data File : PD080605.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Dec 2023 12:36
 Operator : AR\AJ
 Sample : PIBLK148
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 30 01:15:36 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD121623CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Dec 21 13:52:23 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.567	2.797	34346449	59783811	26.901	26.887
27) SA Decachlor...	9.120	7.942	51139916	67433114	31.808	28.094
Target Compounds						
2) A alpha-BHC	0.000	3.286	0	121010	N.D.	<MDL
3) MA gamma-BHC...	0.000	3.648	0	88291	N.D.	<MDL
4) MA Heptachlor	0.000	3.962	0	57595	N.D.	<MDL
5) MB Aldrin	0.000	4.267	0	9169266	N.D.	2.595
6) B beta-BHC	0.000	3.937	0	26373	N.D.	<MDL
8) B Heptachlo...	5.715	4.778	3545764	121673	1.651	<MDL #
12) B 4,4'-DDE	6.291f	5.210f	2708249	427553	1.402	0.136 #
14) MA Endrin	0.000	5.681	0	4147119	N.D.	1.576
17) MA 4,4'-DDT	0.000	6.061	0	152754	N.D.	<MDL
18) B Endrin al...	0.000	6.153	0	161378	N.D.	<MDL


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD123023\
Data File : PD080605.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Dec 2023 12:36
Operator : AR\AJ
Sample : PIBLK148
Misc :
ALS Vial : 2 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 30 01:15:36 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD121623CLP.M
Quant Title : GC Extractables
QLast Update : Thu Dec 21 13:52:23 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

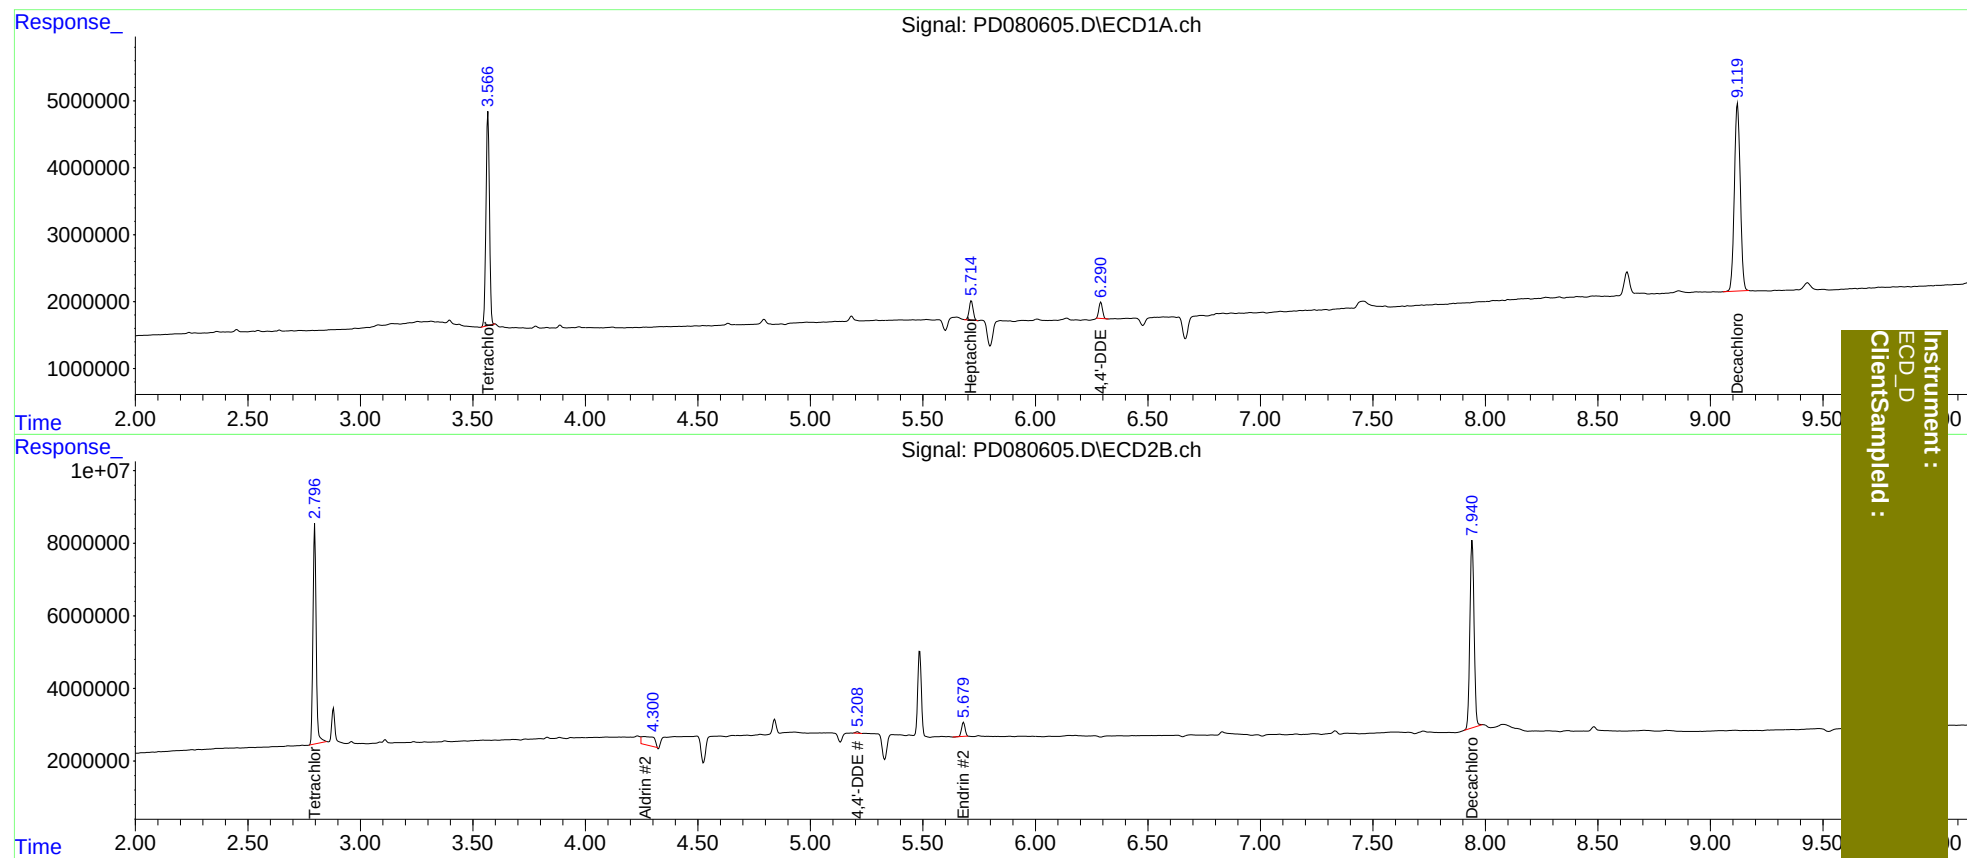


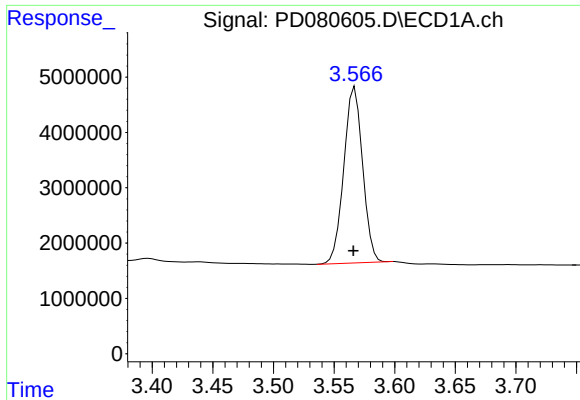

#1 Tetrachloro-m-xylene


R.T.: 3.567 min
Delta R.T.: 0.001 min
Response: 34346449
Conc: 26.90 ng/ml

Instrument :
ECD_D
ClientSampleId :

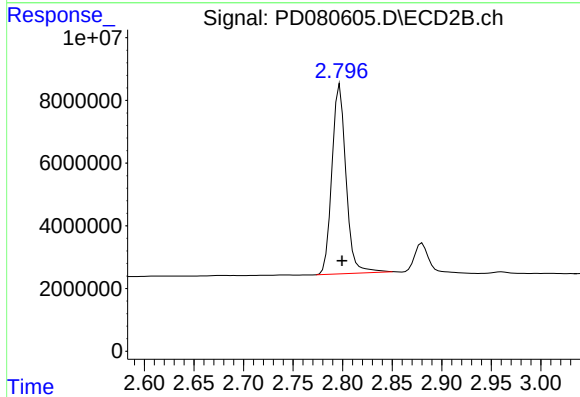


#1 Tetrachloro-m-xylene

R.T.: 2.797 min
Delta R.T.: -0.002 min
Response: 59783811
Conc: 26.89 ng/ml

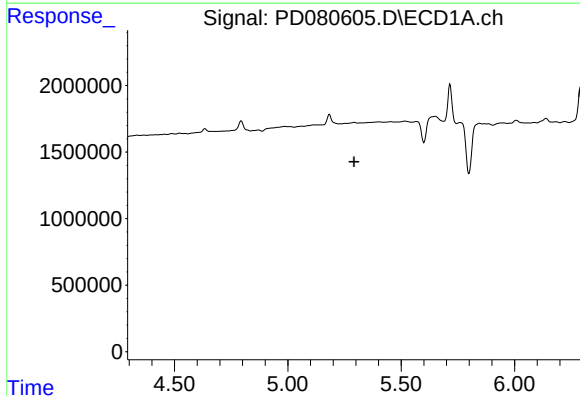


#5 Aldrin

R.T.: 0.000 min
Exp R.T. : 5.292 min
Response: 0
Conc: N.D.

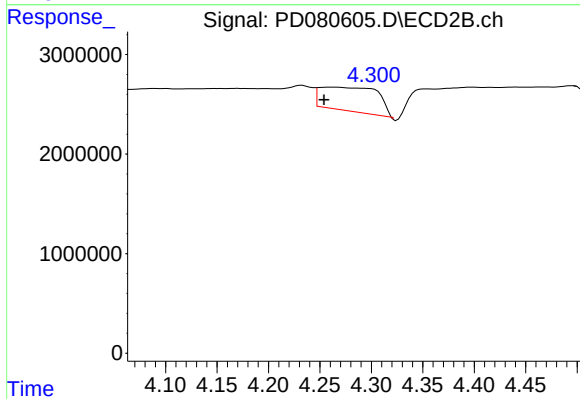

#5 Aldrin


R.T.: 4.267 min
Delta R.T.: 0.013 min
Response: 9169266
Conc: 2.60 ng/ml

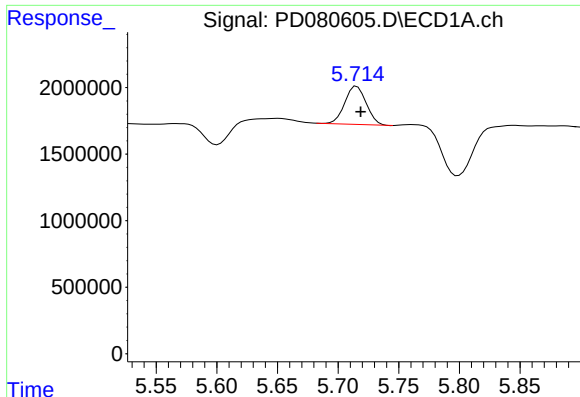

#8 Heptachlor epoxide


R.T.: 5.715 min
Delta R.T.: -0.003 min
Response: 3545764
Conc: 1.65 ng/ml

Instrument :
ECD_D
ClientSampleId :

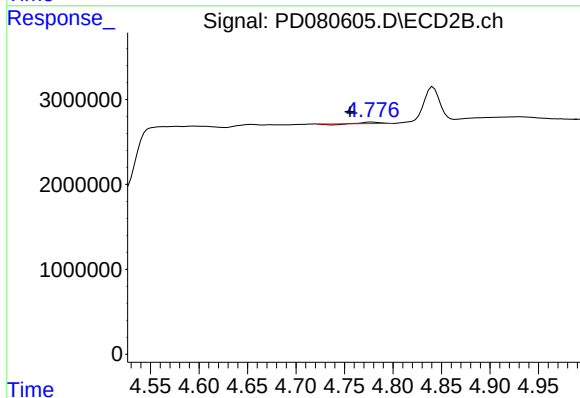


#8 Heptachlor epoxide

R.T.: 4.778 min
Delta R.T.: 0.022 min
Response: 121673
Conc: N.D.

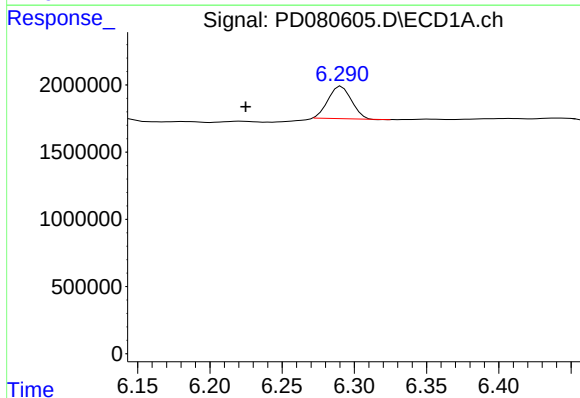


#12 4,4'-DDE

R.T.: 6.291 min
Delta R.T.: 0.066 min
Response: 2708249
Conc: 1.40 ng/ml

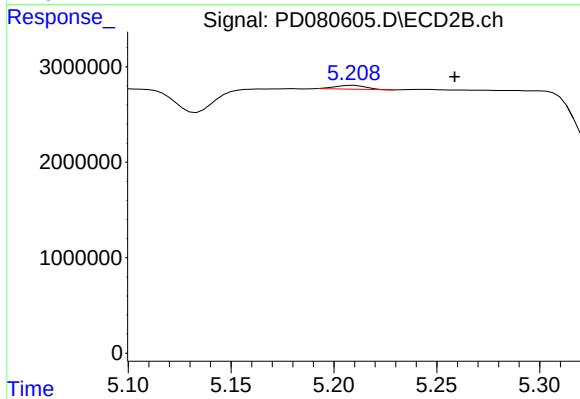

#12 4,4'-DDE


R.T.: 5.210 min
Delta R.T.: -0.049 min
Response: 427553
Conc: 0.14 ng/ml

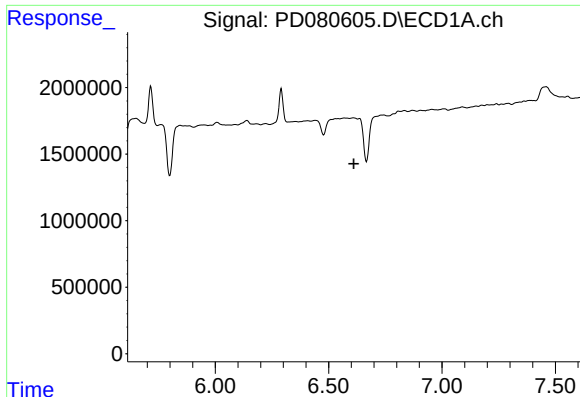

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 6.612 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

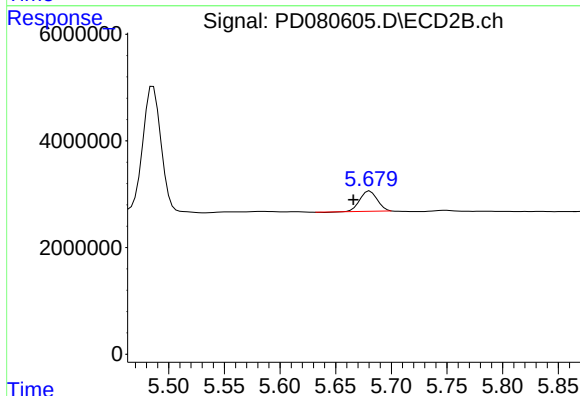


#14 Endrin

R.T.: 5.681 min
Delta R.T.: 0.015 min
Response: 4147119
Conc: 1.58 ng/ml

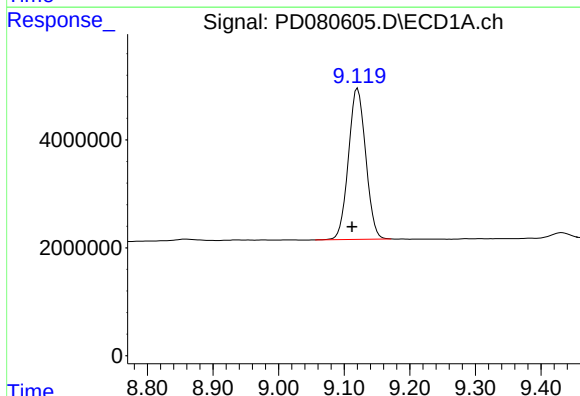

#27 Decachlorobiphenyl

R.T.: 9.120 min
Delta R.T.: 0.009 min
Response: 51139916
Conc: 31.81 ng/ml

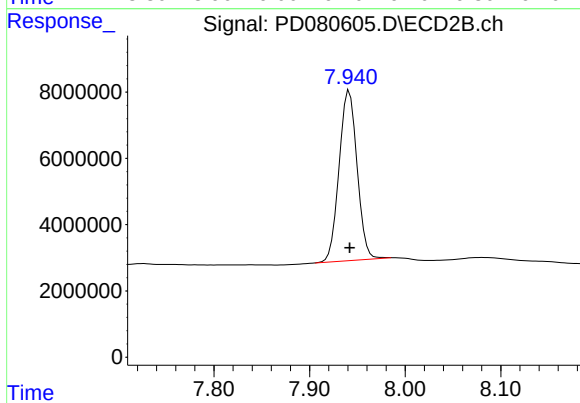

#27 Decachlorobiphenyl

R.T.: 7.942 min
Delta R.T.: 0.000 min
Response: 67433114
Conc: 28.09 ng/ml