

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD042825\
 Data File : PD088308.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Apr 2025 16:22
 Operator : AR\AJ
 Sample : Q1874-05
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 HT3727

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 04/29/2025
 Supervised By : mohammad ahmed 05/02/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 29 02:21:52 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD041825.M
 Quant Title : GC Extractables
 QLast Update : Sat Apr 19 06:32:27 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.549	2.880	35199587	284.8E6	17.623m	19.477m
28)	SA Decachlor...	9.073	8.075	53119947	252.3E6	16.057	13.652
Target Compounds							
14)	MA Endrin	6.575	5.781	1392524	7411277	0.467m	0.407m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD042825\
Data File : PD088308.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Apr 2025 16:22
Operator : AR\AJ
Sample : Q1874-05
Misc :
ALS Vial : 20 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
HT3727


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 04/29/2025
Supervised By : mohammad ahmed 05/02/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 29 02:21:52 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD041825.M
Quant Title : GC Extractables
QLast Update : Sat Apr 19 06:32:27 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

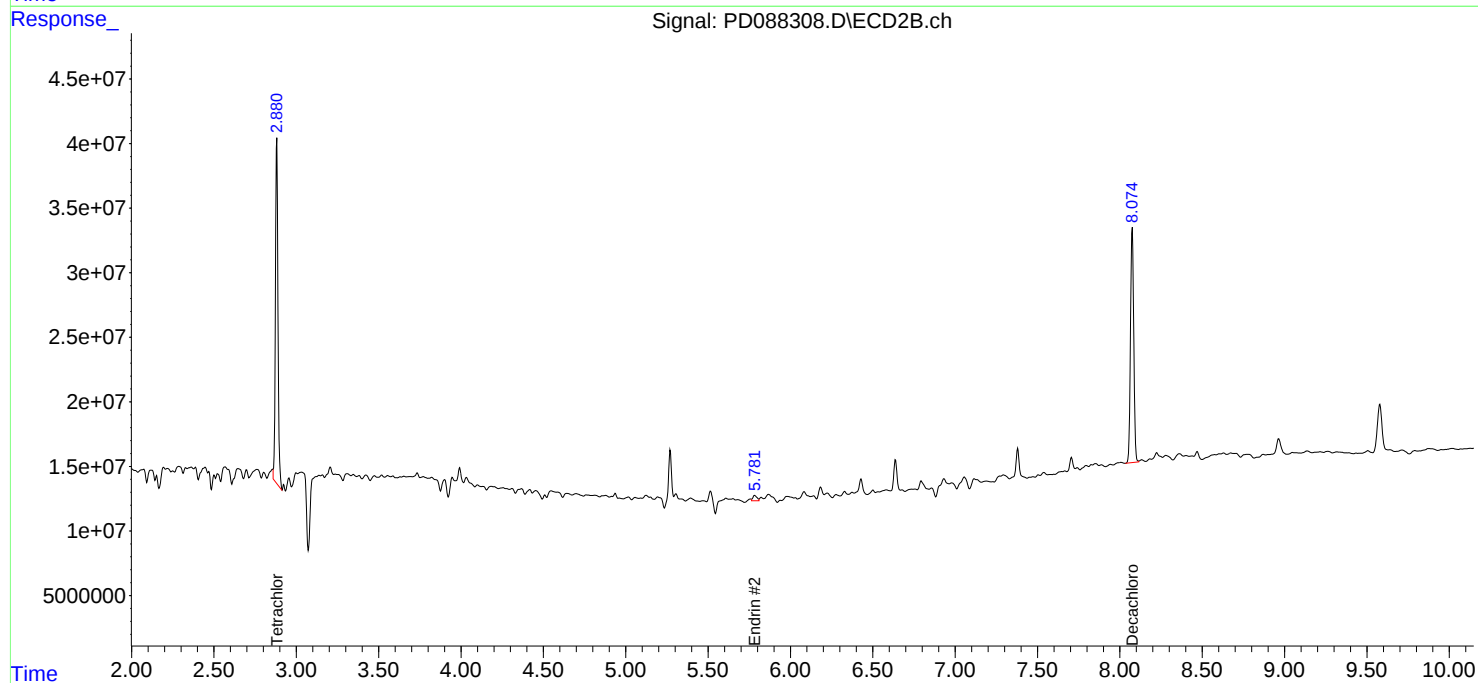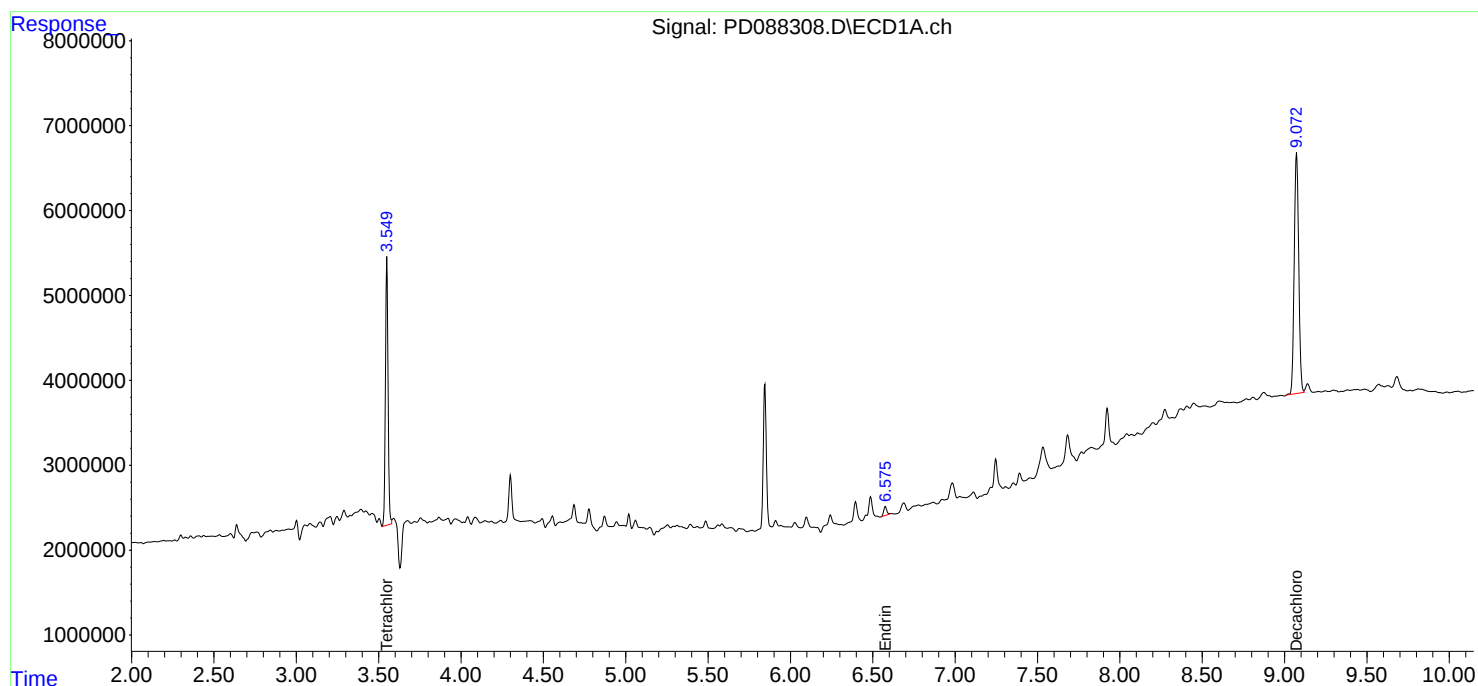

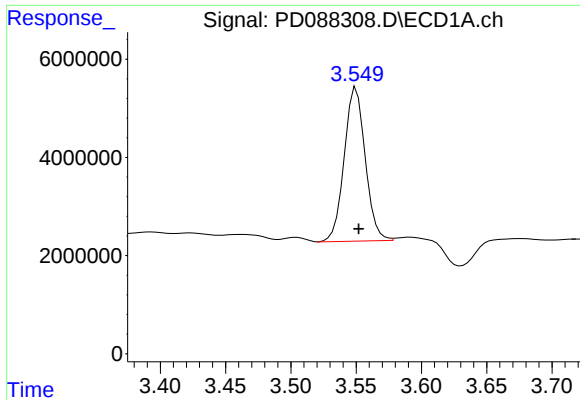


#1 Tetrachloro-m-xylene

R.T.: 3.549 min
Delta R.T.: -0.003 min
Response: 35199587
Conc: 17.62 ng/ml

Instrument :
ECD_D
ClientSampleId :
HT3727


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 04/29/2025
Supervised By :mohammad ahmed 05/02/2025

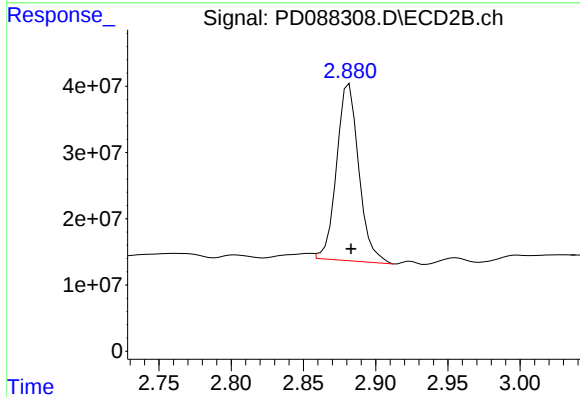


#1 Tetrachloro-m-xylene

R.T.: 2.880 min
Delta R.T.: -0.003 min
Response: 284788737
Conc: 19.48 ng/ml m

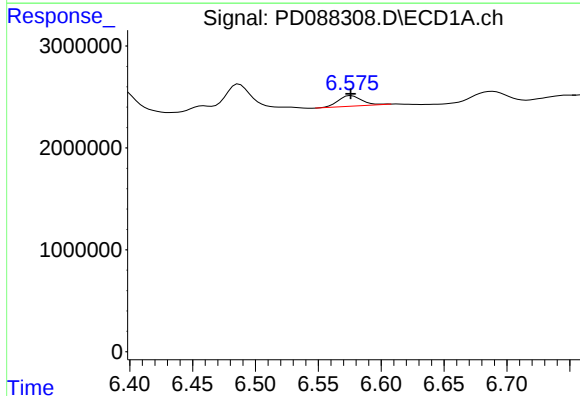


#14 Endrin

R.T.: 6.575 min
Delta R.T.: 0.000 min
Response: 1392524
Conc: 0.47 ng/ml m

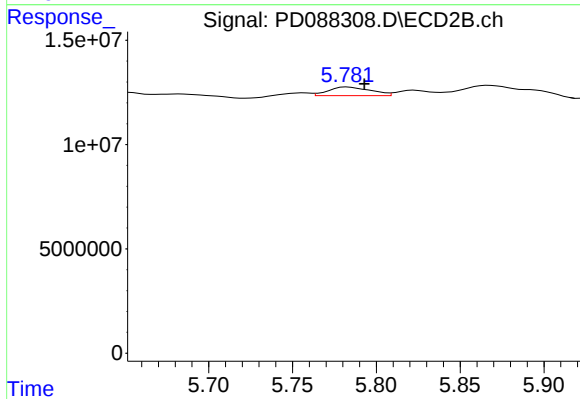

#14 Endrin

R.T.: 5.781 min
Delta R.T.: -0.012 min
Response: 7411277
Conc: 0.41 ng/ml m

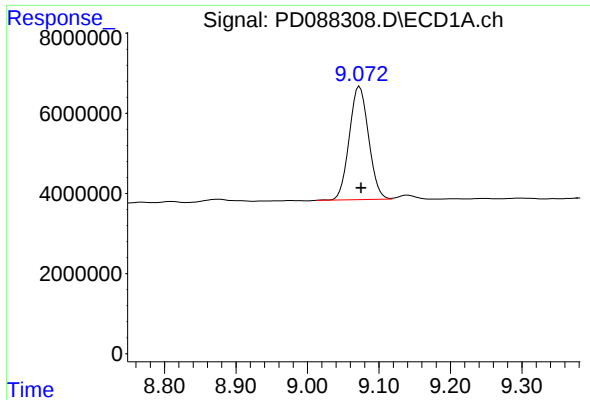


#28 Decachlorobiphenyl

R.T.: 9.073 min
Delta R.T.: -0.002 min
Response: 53119947
Conc: 16.06 ng/ml

Instrument :
ECD_D
ClientSampleId :
HT3727

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 04/29/2025
Supervised By :mohammad ahmed 05/02/2025

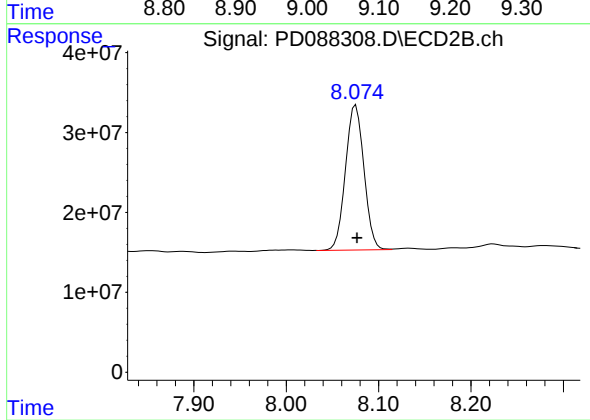

#28 Decachlorobiphenyl

R.T.: 8.075 min
Delta R.T.: -0.002 min
Response: 252284116
Conc: 13.65 ng/ml