

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111224\
 Data File : PD086545.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Nov 2024 21:49
 Operator : AR\AJ
 Sample : P4761-02
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 A0AL2

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 11/12/2024
 Supervised By :Ankita Jodhani 11/12/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 12 02:19:05 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102524CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 25 14:36:38 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.559	2.887	25140929	151.3E6	19.096	16.309
27)	SA Decachlor...	9.096	8.094	36653883	189.7E6	20.445	20.061
Target Compounds							
4)	MA Heptachlor	4.965	4.086	960517	12438650	0.389m	0.910m#
10)	B trans-Chl...	5.978	5.125	909102	9554755	0.412m	0.726m#
20)	A Methoxychlor	7.505	6.771	1915641	2864811	2.036m	0.603m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111224\
Data File : PD086545.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Nov 2024 21:49
Operator : AR\AJ
Sample : P4761-02
Misc :
ALS Vial : 19 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 12 02:19:05 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102524CLP.M
Quant Title : GC Extractables
QLast Update : Fri Oct 25 14:36:38 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

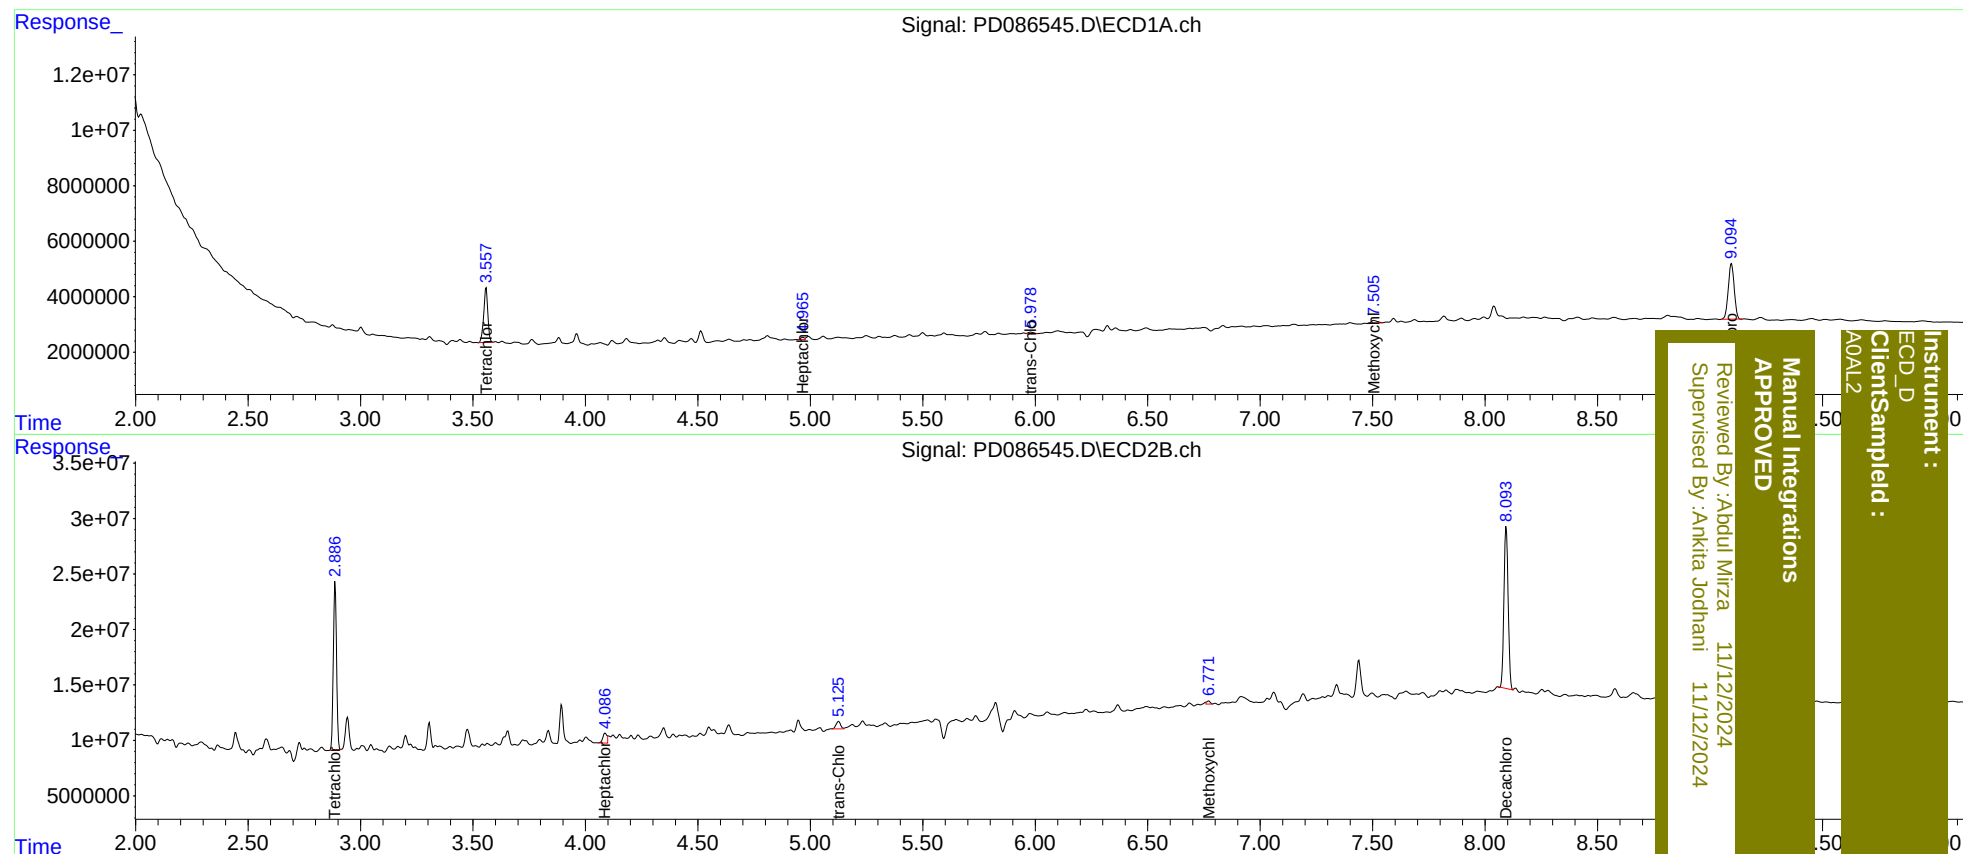

Instrument :
ECD_D
ClientSampled :
A0AL2

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 11/12/2024
Supervised By :Ankita Jodhani 11/12/2024