

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111224\
 Data File : PD086547.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Nov 2024 22:17
 Operator : AR\AJ
 Sample : P4761-05
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 A0AL7

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 11/12/2024
 Supervised By :Ankita Jodhani 11/12/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 12 02:19:47 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102524CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 25 14:36:38 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.559	2.887	23620236	142.9E6	17.941	15.401
27)	SA Decachlor...	9.096	8.095	33856555	172.7E6	18.885	18.264
Target Compounds							
10)	B trans-Chl...	5.980	5.125	1240026	10033318	0.562m	0.763m#
15)	B Endosulfa...	6.835	6.130	1621585	7016432	0.809m	0.636m
20)	A Methoxychlor	7.518	6.789	2750057	7566365	2.922m	1.592m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111224\
Data File : PD086547.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Nov 2024 22:17
Operator : AR\AJ
Sample : P4761-05
Misc :
ALS Vial : 21 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 12 02:19:47 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102524CLP.M
Quant Title : GC Extractables
QLast Update : Fri Oct 25 14:36:38 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

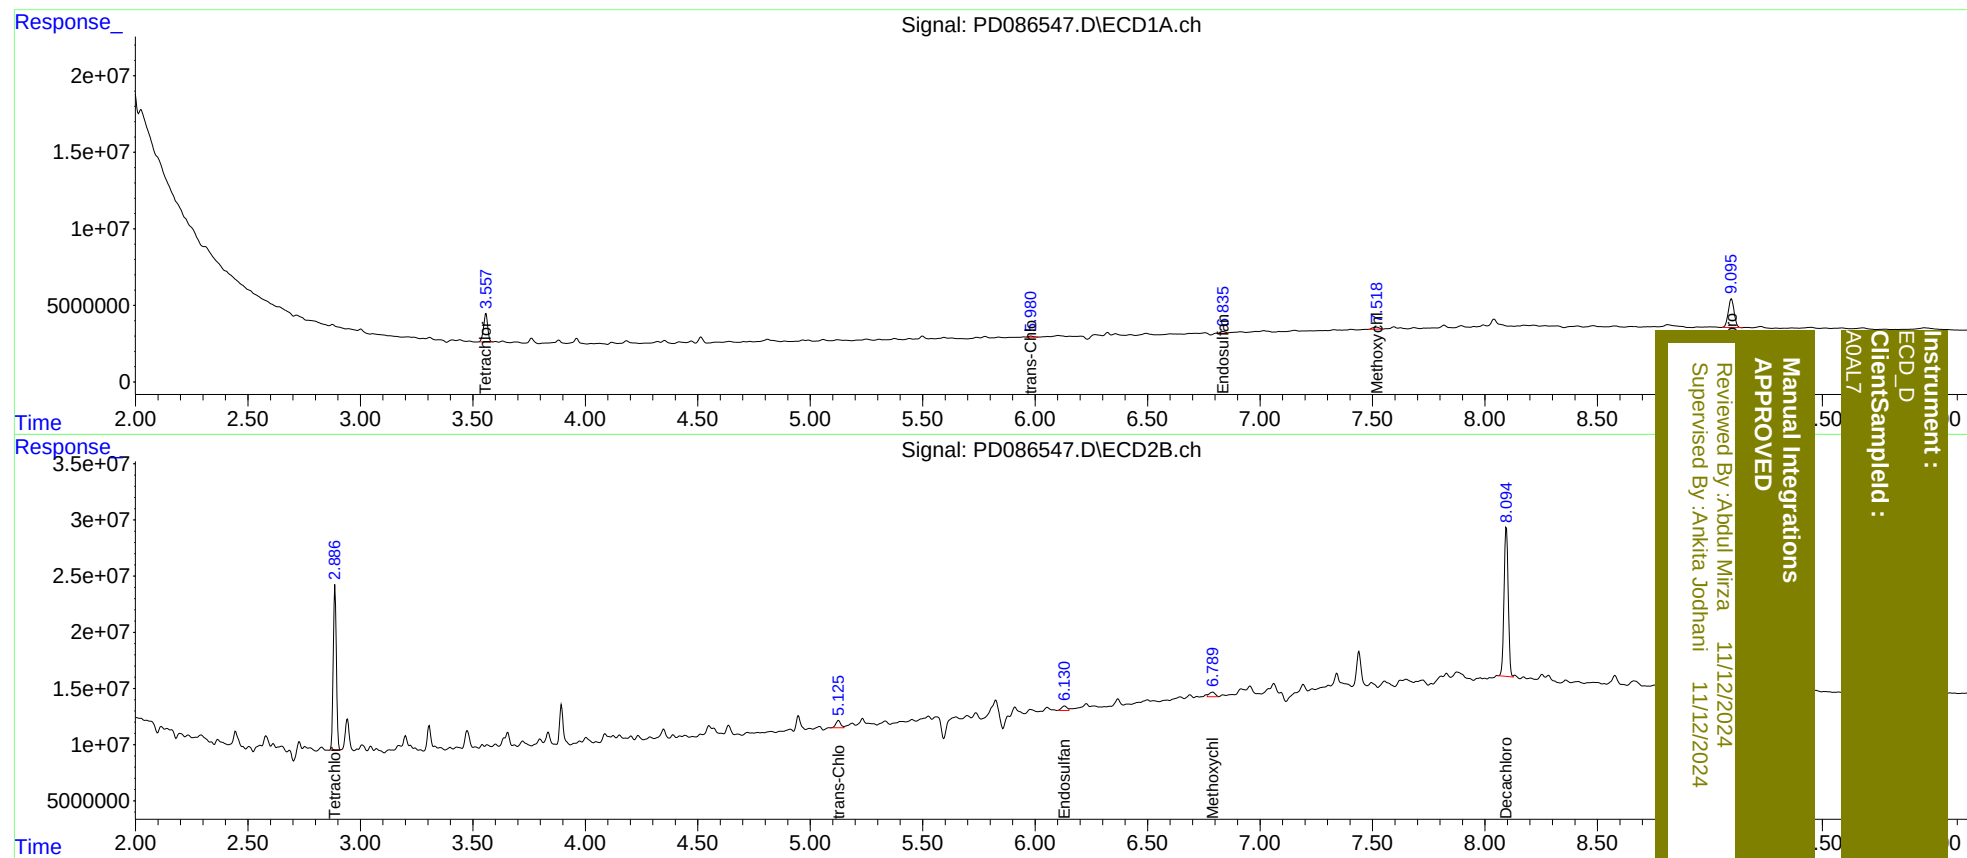

Instrument :
ECD_D
ClientSampled :
A0AL7

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 11/12/2024
Supervised By :Ankita Jodhani 11/12/2024