

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111224\
 Data File : PD086551.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Nov 2024 23:13
 Operator : AR\AJ
 Sample : P4761-10MS
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 A0ANOMS

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 11/12/2024
 Supervised By : Ankita Jodhani 11/12/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 12 02:21:04 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102524CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 25 14:36:38 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.558	2.887	22407839	159.8E6	17.020m	17.223
27)	SA Decachlor...	9.095	8.095	34761537	187.7E6	19.390	19.855
Target Compounds							
2)	A alpha-BHC	4.009	3.402	138.8E6	726.4E6	55.759	50.556
3)	MA gamma-BHC...	4.339	3.739	138.9E6	674.9E6	55.810m	50.036
4)	MA Heptachlor	4.941	4.095	127.2E6	637.1E6	51.452	46.635
5)	MB Aldrin	5.284	4.382	115.8E6	594.6E6	47.796	43.828
6)	B beta-BHC	4.524	4.034	48218956	283.6E6	43.418	45.239
7)	B delta-BHC	4.773	4.271	91968601	471.4E6	35.528	33.598
8)	B Heptachlo...	5.704	4.885	120.3E6	613.1E6	52.626	48.890m
9)	A Endosulfan I	6.087	5.262	112.0E6	533.2E6	55.284	46.444
10)	B trans-Chl...	5.958	5.141	114.1E6	628.1E6	51.721	47.745
11)	B cis-Chlor...	6.040	5.205	119.0E6	619.4E6	53.805	48.770
12)	B 4,4'-DDE	6.209	5.391	210.8E6	1118.5E6	98.691	91.224
13)	MA Dieldrin	6.361	5.528	256.5E6	1204.1E6	112.459	97.600
14)	MA Endrin	6.589	5.804	216.7E6	1128.8E6	115.264	100.442
15)	B Endosulfa...	6.798	6.096	203.9E6	1033.6E6	101.691m	93.683
16)	A 4,4'-DDD	6.718	5.946	176.6E6	829.4E6	108.974	84.490
17)	MA 4,4'-DDT	7.033	6.199	183.7E6	997.7E6	110.170m	97.222m
18)	B Endrin al...	6.928	6.274	150.7E6	735.0E6	101.026	88.546
19)	B Endosulfa...	7.162	6.498	191.9E6	940.5E6	104.129	89.217
20)	A Methoxychlor	7.508	6.773	495.0E6	2174.4E6	526.009	457.449
21)	B Endrin ke...	7.644	7.008	228.9E6	1082.0E6	111.100	94.555

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111224\
Data File : PD086551.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Nov 2024 23:13
Operator : AR\AJ
Sample : P4761-10MS
Misc :
ALS Vial : 25 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 12 02:21:04 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102524CLP.M
Quant Title : GC Extractables
QLast Update : Fri Oct 25 14:36:38 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

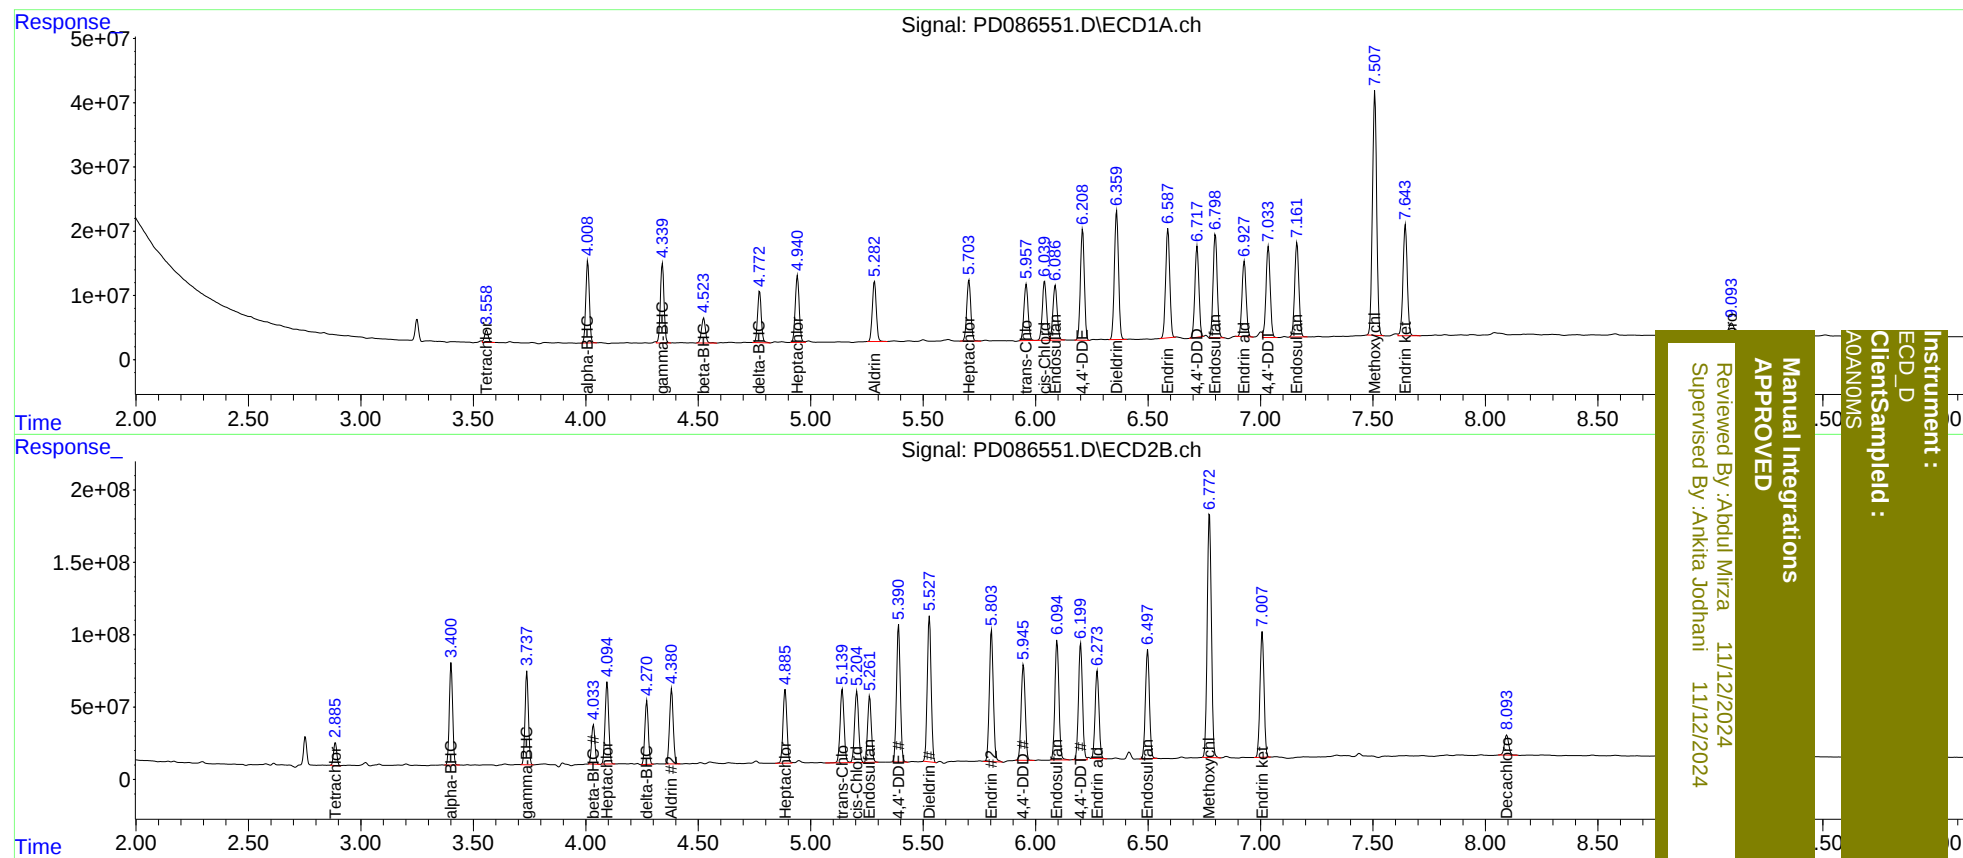

Instrument :
ECD_D
ClientSampled :
A0AN0MS

Manual Integrations
APPROVED

Reviewed By: Abdul Miza 11/12/2024
Supervised By: Ankita Jodhani 11/12/2024