

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111224\
 Data File : PD086552.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Nov 2024 23:27
 Operator : AR\AJ
 Sample : P4761-11MSD
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 A0AN0MSD

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 11/12/2024
 Supervised By : Ankita Jodhani 11/12/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 12 02:21:25 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102524CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 25 14:36:38 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.558	2.887	22554604	162.0E6	17.131m	17.464
27)	SA Decachlor...	9.095	8.095	35170542	191.8E6	19.618	20.284
Target Compounds							
2)	A alpha-BHC	4.009	3.402	140.8E6	740.2E6	56.558	51.517
3)	MA gamma-BHC...	4.340	3.739	141.4E6	689.0E6	56.853m	51.080
4)	MA Heptachlor	4.942	4.095	129.5E6	652.1E6	52.403	47.731
5)	MB Aldrin	5.284	4.382	117.8E6	607.6E6	48.624	44.788
6)	B beta-BHC	4.524	4.034	49006485	289.6E6	44.128	46.190
7)	B delta-BHC	4.773	4.272	93694379	482.5E6	36.195	34.387
8)	B Heptachlo...	5.704	4.885	121.9E6	624.5E6	53.360	49.801m
9)	A Endosulfan I	6.088	5.262	113.9E6	544.2E6	56.226	47.394
10)	B trans-Chl...	5.959	5.140	116.5E6	644.0E6	52.775	48.956
11)	B cis-Chlor...	6.041	5.205	120.9E6	632.8E6	54.693	49.820
12)	B 4,4'-DDE	6.210	5.391	215.0E6	1147.2E6	100.662	93.562
13)	MA Dieldrin	6.361	5.528	262.2E6	1234.6E6	114.943	100.065
14)	MA Endrin	6.589	5.804	221.5E6	1157.8E6	117.821	103.029
15)	B Endosulfa...	6.798	6.096	206.4E6	1056.9E6	102.938m	95.794
16)	A 4,4'-DDD	6.719	5.946	180.6E6	845.9E6	111.464	86.175
17)	MA 4,4'-DDT	7.034	6.199	188.8E6	1014.6E6	113.233m	98.872m
18)	B Endrin al...	6.928	6.275	153.2E6	752.4E6	102.717	90.642
19)	B Endosulfa...	7.163	6.498	195.6E6	963.4E6	106.094	91.391
20)	A Methoxychlor	7.508	6.773	504.1E6	2225.6E6	535.657	468.212
21)	B Endrin ke...	7.644	7.007	232.9E6	1103.7E6	113.040	96.455

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111224\
Data File : PD086552.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Nov 2024 23:27
Operator : AR\AJ
Sample : P4761-11MSD
Misc :
ALS Vial : 26 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 12 02:21:25 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102524CLP.M
Quant Title : GC Extractables
QLast Update : Fri Oct 25 14:36:38 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

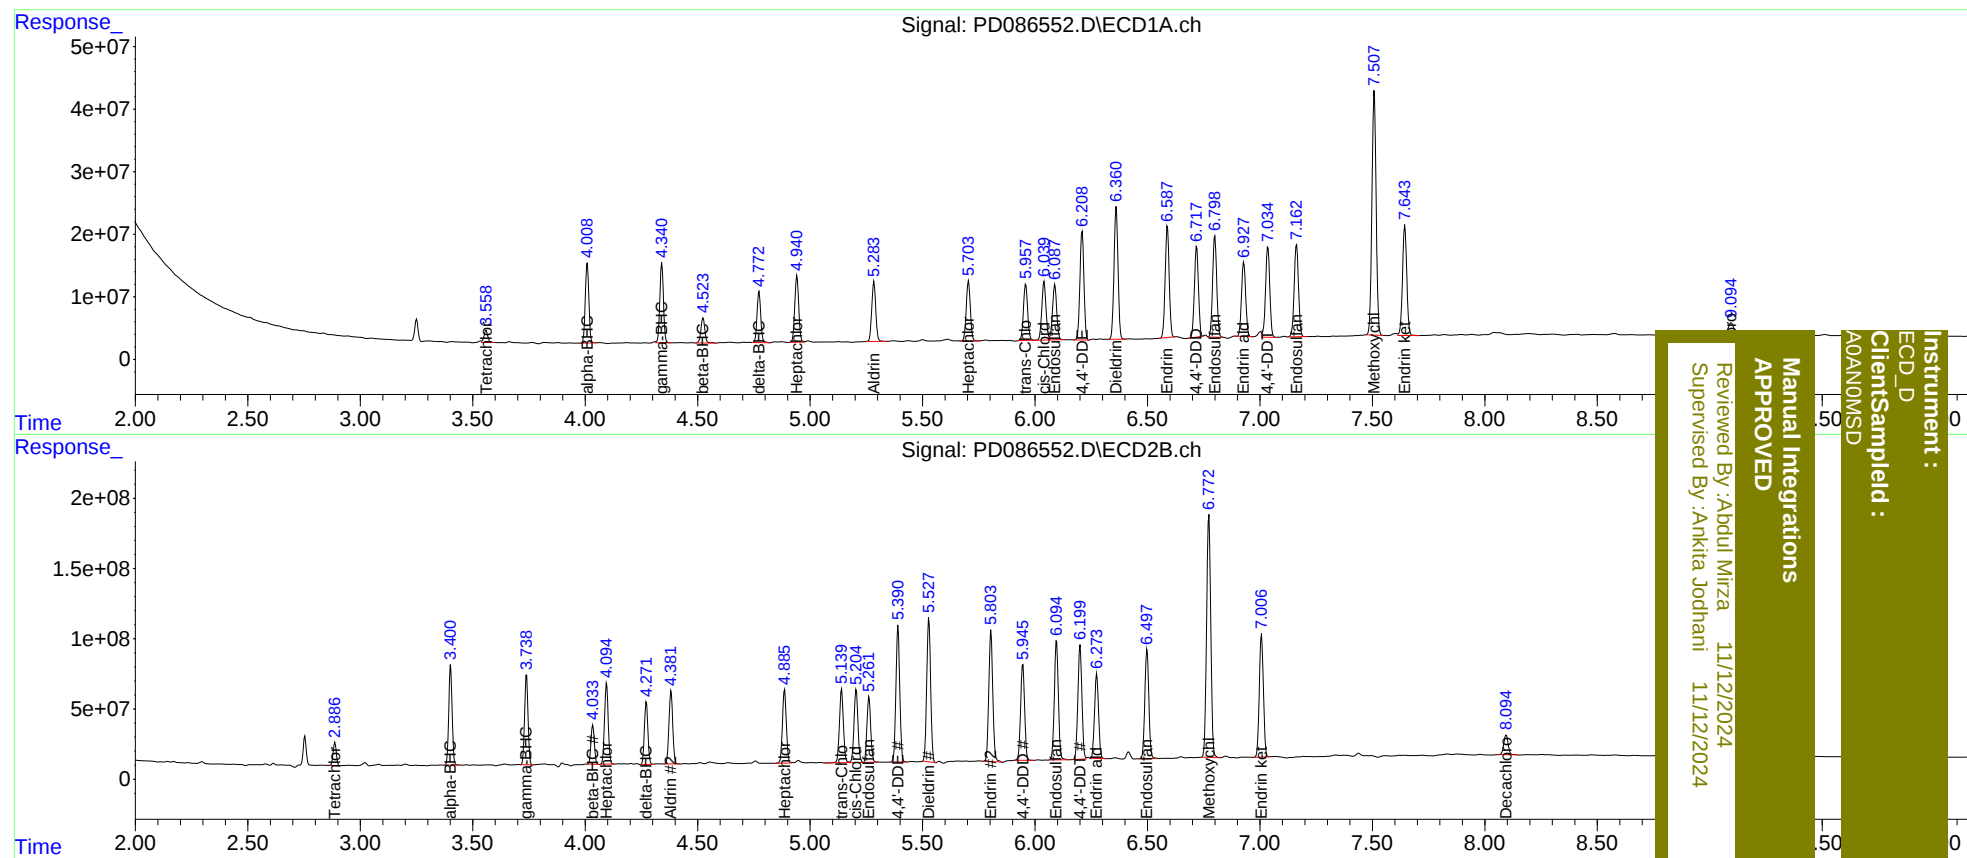

Instrument :
ECD_D
Client Sampled :
A0AN0MSD

Manual Integrations
APPROVED

Reviewed By: Abdul Miza 11/12/2024
Supervised By: Ankita Jodhani 11/12/2024