

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD022122\
 Data File : PD068119.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Feb 2022 12:53
 Operator : AR\AJ
 Sample : N1331-02
 Misc : PEST MDL
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 MDL-WATER-QT1-2022-02

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 02/22/2022
 Supervised By :Ankita Jodhani 02/22/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 22 06:30:13 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD021822CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Feb 18 23:15:19 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.450	4.176	26415580	171.4E6	18.589	17.307
27)	SA Decachlor...	8.214	9.371	52049882	181.1E6	42.591	39.955
Target Compounds							
2)	A alpha-BHC	3.890	4.572	2133616	16629541	1.077	1.221
3)	MA gamma-BHC...	4.173	4.863	1975400	15318333	1.047	1.225
4)	MA Heptachlor	4.473	5.390	2066072	13026891	1.192	1.248
5)	MB Aldrin	4.721	5.703	2190529	15562753	1.153	1.323
6)	B beta-BHC	4.423	5.025	1015605	7199989	1.154	1.275
7)	B delta-BHC	4.627	5.251	1992633	15574986	1.078	1.249
8)	B Heptachlo...	5.165	6.091	2181542	14162556	1.261	1.381
9)	A Endosulfan I	5.504	6.453	2001512	12290690	1.230	1.348
10)	B trans-Chl...	5.392	6.327	2229981	13133328	1.264	1.316
11)	B cis-Chlor...	5.451	6.402	2210685	13046653	1.273	1.357
12)	B 4,4'-DDE	5.617	6.551	1860079	11866898	1.164	1.371
13)	MA Dieldrin	5.748	6.712	2184398	12623057	1.228	1.354
14)	MA Endrin	6.006	6.932	1751648	8432784	1.267	1.281
15)	B Endosulfa...	6.280	7.135	1949082	9990169	1.296	1.381m
16)	A 4,4'-DDD	6.135	7.041	1716107	8343237	1.233	1.224m
17)	MA 4,4'-DDT	6.375	7.346	1043454	5434343	0.894	1.089
18)	B Endrin al...	6.451	7.261	1594721	7976522	1.456	1.521
19)	B Endosulfa...	6.662	7.485	1771729	8854308	1.294m	1.408
20)	A Methoxychlor	6.928	7.798	747184	2654451	1.160	1.190
21)	B Endrin ke...	7.156	7.961	1926652	9383123	1.311	1.529

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD022122\
Data File : PD068119.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Feb 2022 12:53
Operator : AR\AJ
Sample : N1331-02
Misc : PEST MDL
ALS Vial : 9 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 22 06:30:13 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD021822CLP.M
Quant Title : GC Extractables
QLast Update : Fri Feb 18 23:15:19 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

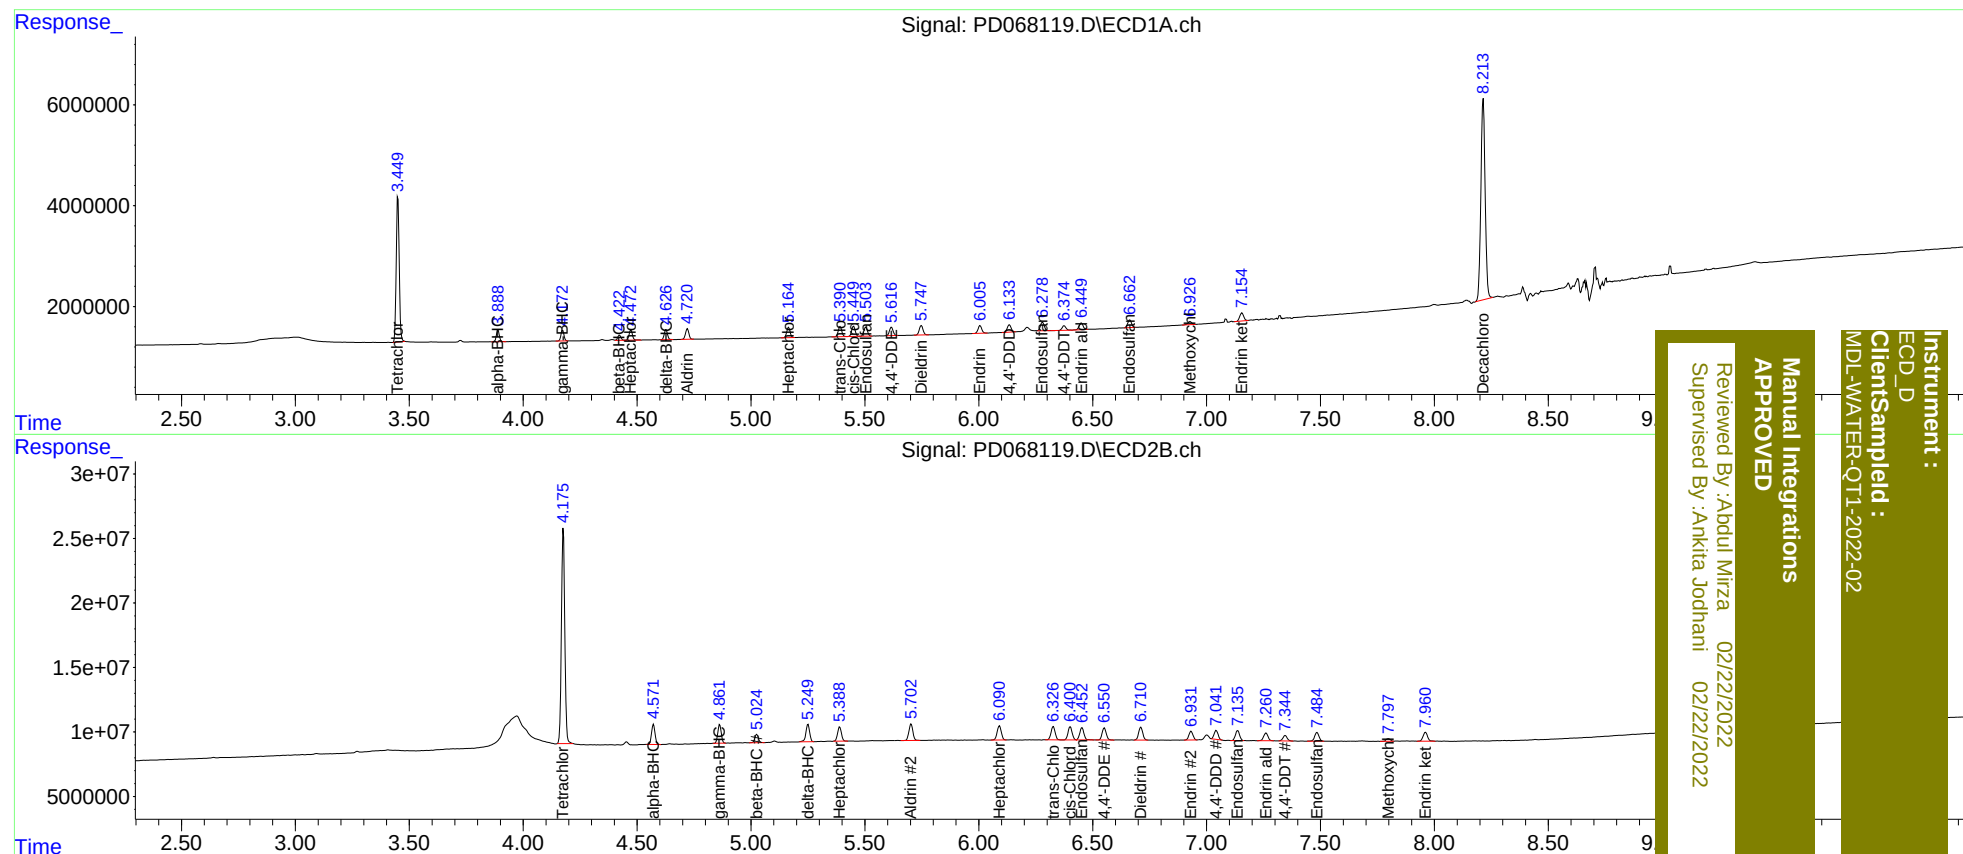

Manual Integrations
APPROVED
Reviewed By: Abdul Mirza 02/22/2022
Supervised By: Ankita Jodhani 02/22/2022

Instrument :
ECD_D
Client Sample :
MDL-WATER-QT1-2022-02