

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD022822\
 Data File : PD068234.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Feb 2022 12:58
 Operator : AR\AJ
 Sample : INDA201
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 28 14:26:24 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD022822CLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Feb 28 14:24:43 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.450	4.176	10651981	95720439	9.886	10.554
27)	SA Decachlor...	8.213	9.372	26374043	128.2E6	22.224	22.526
Target Compounds							
2)	A alpha-BHC	3.890	4.572	12870219	122.1E6	9.228	10.237
3)	MA gamma-BHC...	4.173	4.863	12596136	113.7E6	9.386	10.302
4)	MA Heptachlor	4.473	5.390	12918905	105.6E6	9.902	10.414
9)	A Endosulfan I	5.504	6.454	11676899	89502556	10.001	10.439
13)	MA Dieldrin	5.748	6.712	24518446	182.8E6	19.477	20.673
14)	MA Endrin	6.005	6.932	21669486	140.7E6	19.747	20.441
16)	A 4,4'-DDD	6.134	7.043	19427049	140.0E6	19.658	20.785
17)	MA 4,4'-DDT	6.374	7.347	18654228	116.5E6	19.440	20.445
20)	A Methoxychlor	6.926	7.799	55114474	269.5E6	102.691	104.335


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD022822\
Data File : PD068234.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Feb 2022 12:58
Operator : AR\AJ
Sample : INDA201
Misc :
ALS Vial : 11 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 28 14:26:24 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD022822CLP.M
Quant Title : GC Extractables
QLast Update : Mon Feb 28 14:24:43 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

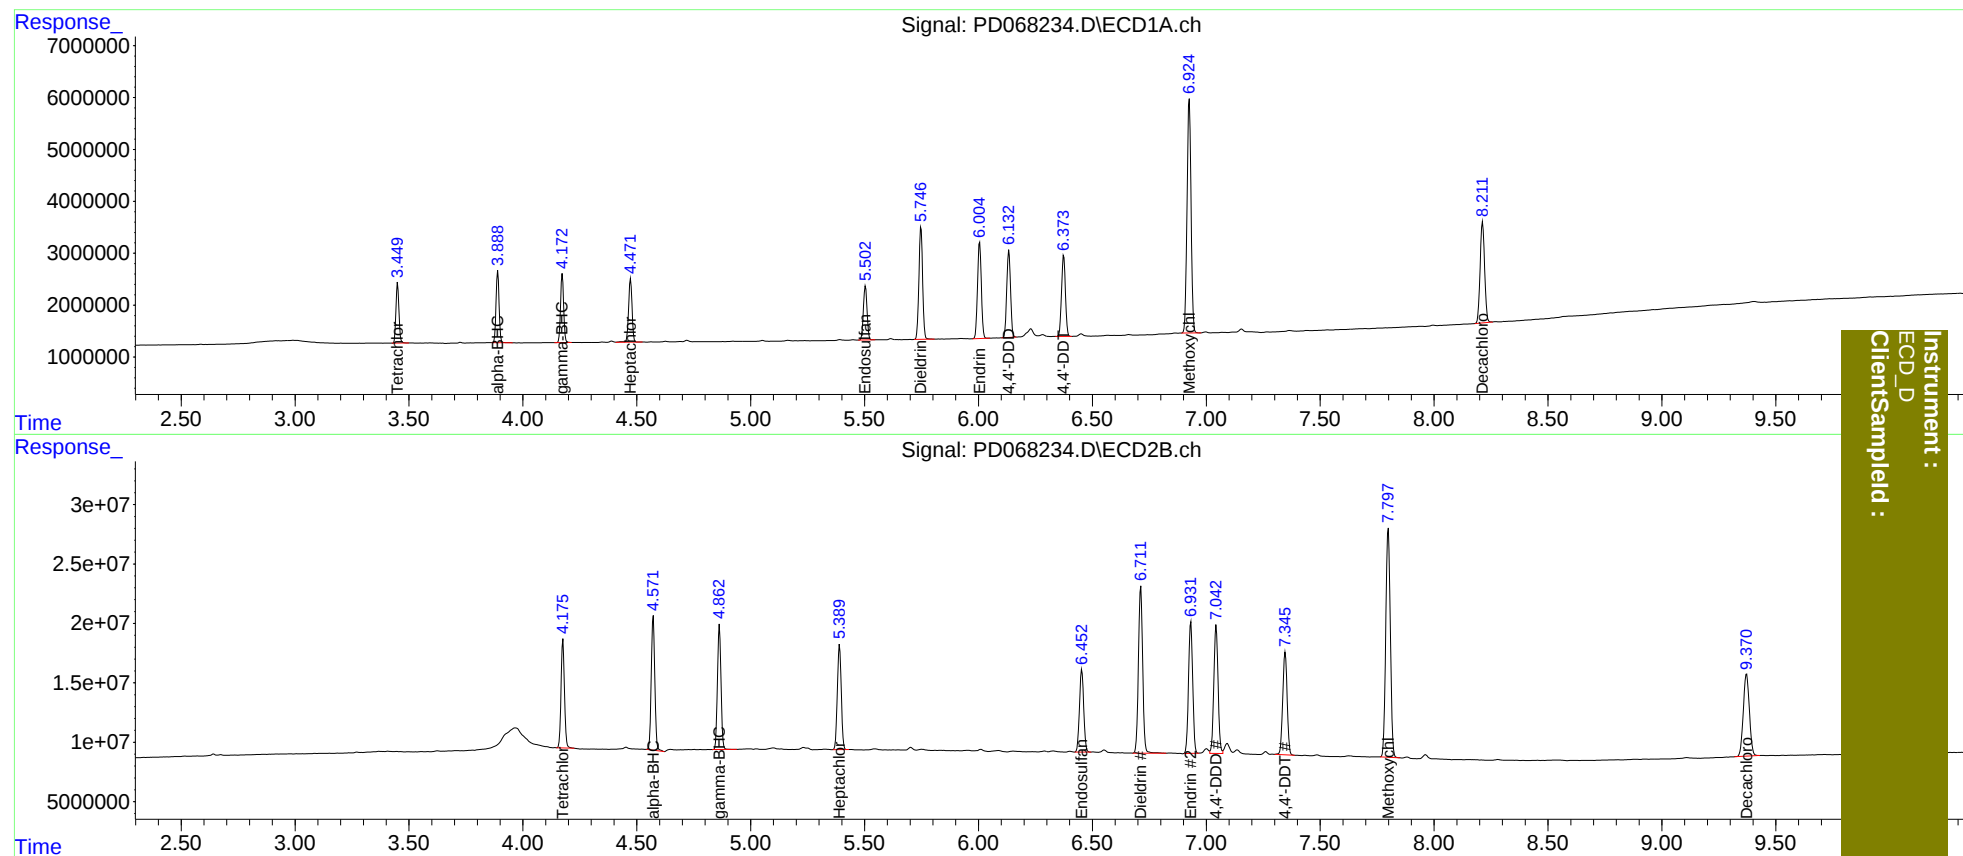


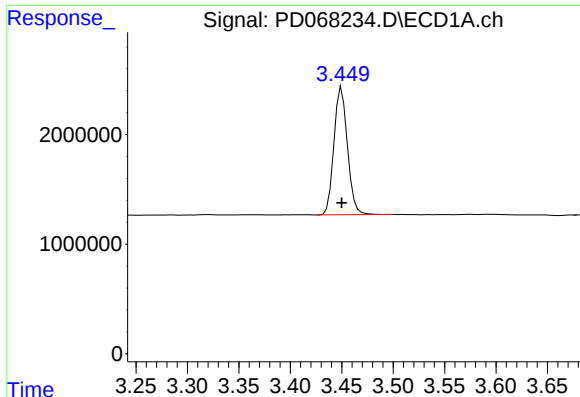

#1 Tetrachloro-m-xylene


R.T.: 3.450 min
Delta R.T.: 0.000 min
Response: 10651981
Conc: 9.89 ng/ml

Instrument :
ECD_D
ClientSampleId :

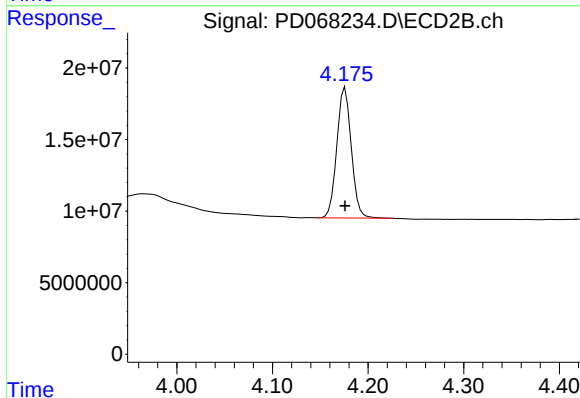


#1 Tetrachloro-m-xylene

R.T.: 4.176 min
Delta R.T.: 0.000 min
Response: 95720439
Conc: 10.55 ng/ml

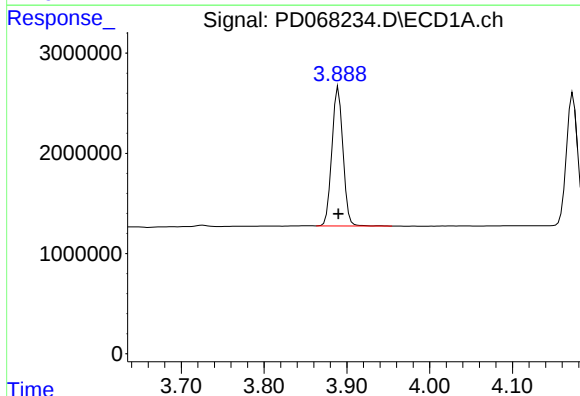


#2 alpha-BHC

R.T.: 3.890 min
Delta R.T.: 0.000 min
Response: 12870219
Conc: 9.23 ng/ml

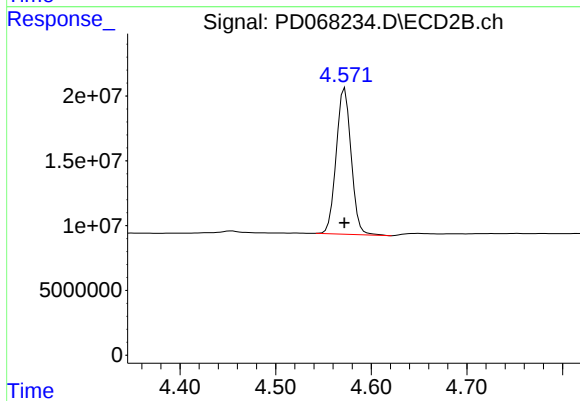

#2 alpha-BHC


R.T.: 4.572 min
Delta R.T.: 0.000 min
Response: 122061361
Conc: 10.24 ng/ml

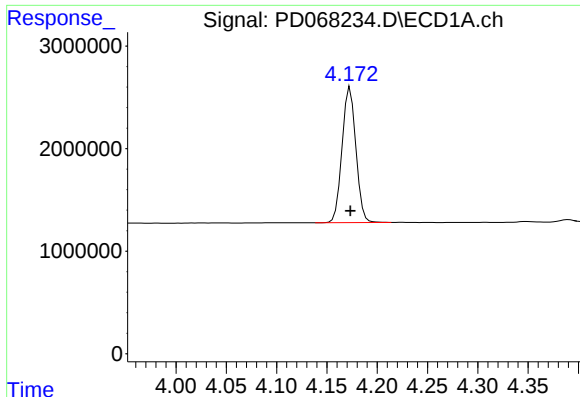

#3 gamma-BHC (Lindane)


R.T.: 4.173 min
Delta R.T.: 0.000 min
Response: 12596136
Conc: 9.39 ng/ml

Instrument :
ECD_D
ClientSampleId :

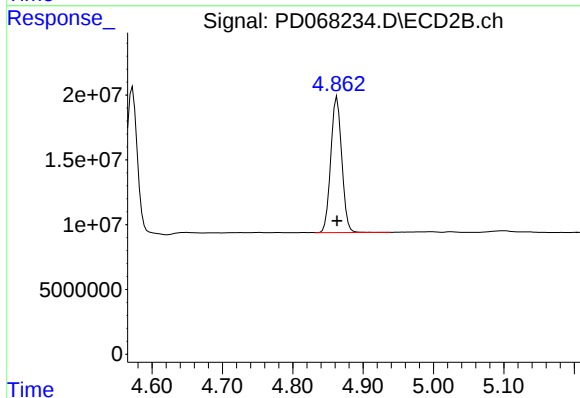


#3 gamma-BHC (Lindane)

R.T.: 4.863 min
Delta R.T.: 0.000 min
Response: 113742539
Conc: 10.30 ng/ml

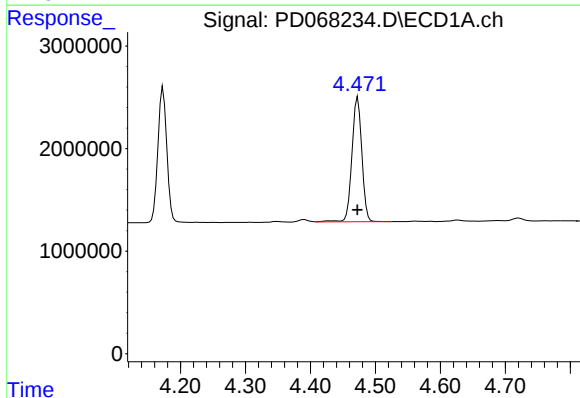


#4 Heptachlor

R.T.: 4.473 min
Delta R.T.: 0.000 min
Response: 12918905
Conc: 9.90 ng/ml

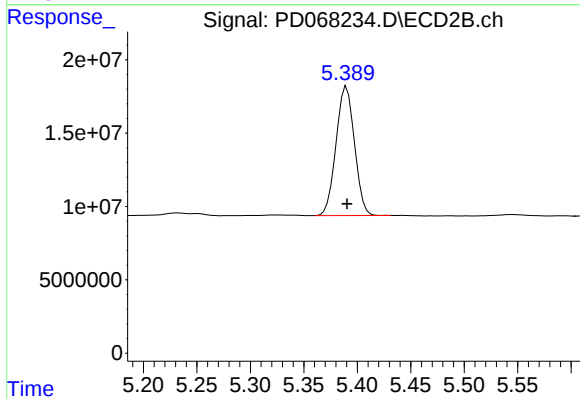

#4 Heptachlor


R.T.: 5.390 min
Delta R.T.: 0.000 min
Response: 105560491
Conc: 10.41 ng/ml

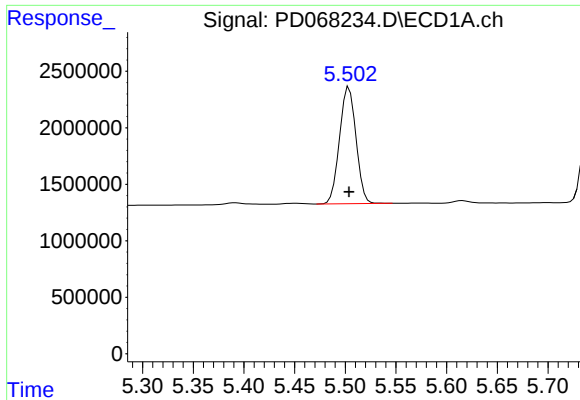

#9 Endosulfan I


R.T.: 5.504 min
Delta R.T.: 0.000 min
Response: 11676899
Conc: 10.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

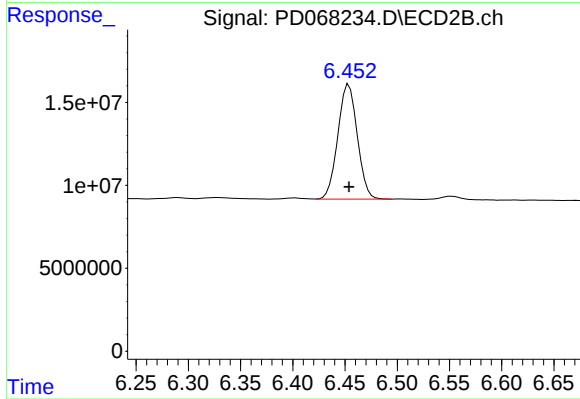


#9 Endosulfan I

R.T.: 6.454 min
Delta R.T.: 0.000 min
Response: 89502556
Conc: 10.44 ng/ml

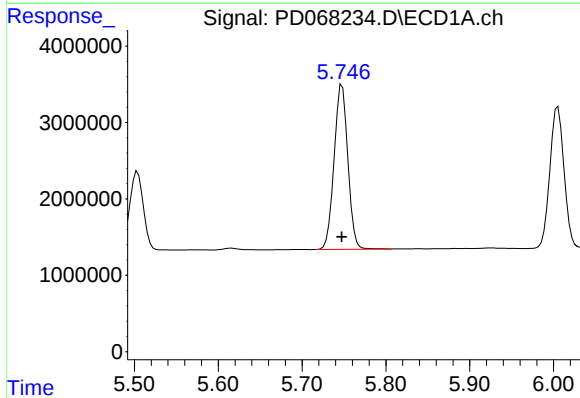


#13 Dieldrin

R.T.: 5.748 min
Delta R.T.: 0.000 min
Response: 24518446
Conc: 19.48 ng/ml

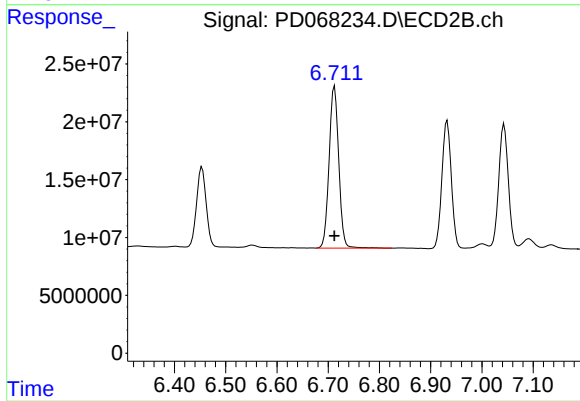

#13 Dieldrin


R.T.: 6.712 min
Delta R.T.: 0.000 min
Response: 182781203
Conc: 20.67 ng/ml

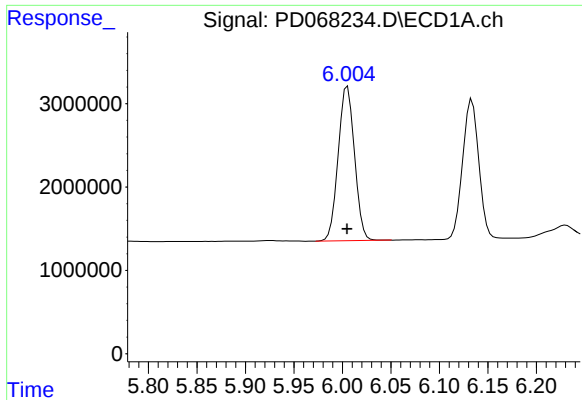

#14 Endrin


R.T.: 6.005 min
Delta R.T.: 0.000 min
Response: 21669486
Conc: 19.75 ng/ml

Instrument :
ECD_D
ClientSampleId :

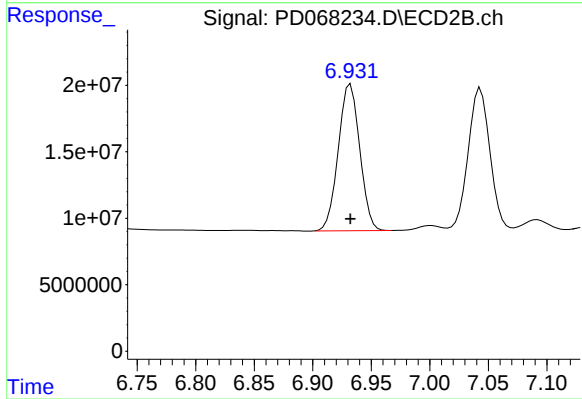


#14 Endrin

R.T.: 6.932 min
Delta R.T.: 0.000 min
Response: 140675209
Conc: 20.44 ng/ml

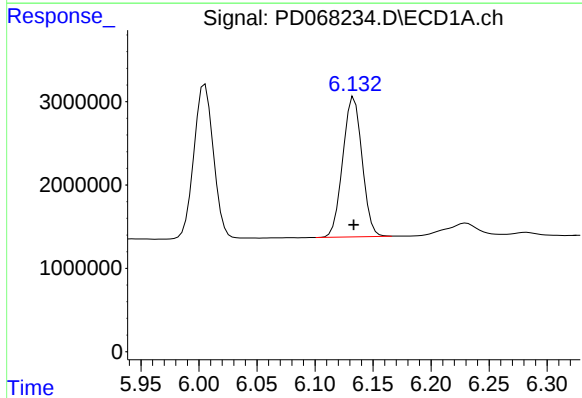


#16 4,4'-DDD

R.T.: 6.134 min
Delta R.T.: 0.000 min
Response: 19427049
Conc: 19.66 ng/ml

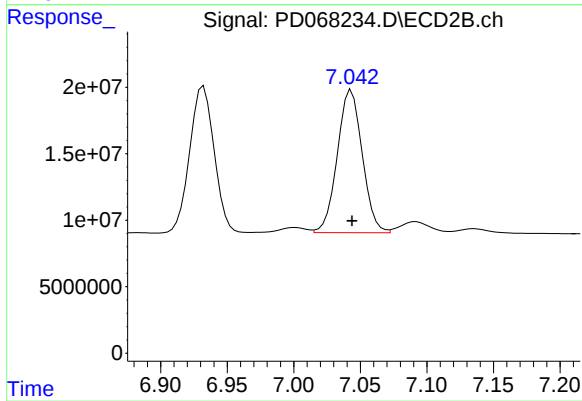

#16 4,4'-DDD


R.T.: 7.043 min
Delta R.T.: 0.000 min
Response: 139993555
Conc: 20.79 ng/ml

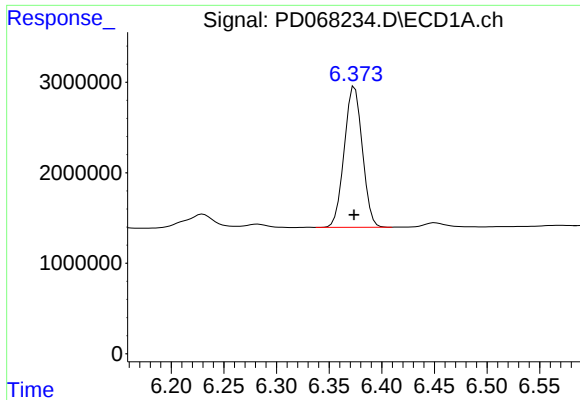

#17 4,4'-DDT


R.T.: 6.374 min
Delta R.T.: 0.000 min
Response: 18654228
Conc: 19.44 ng/ml

Instrument :
ECD_D
ClientSampleId :

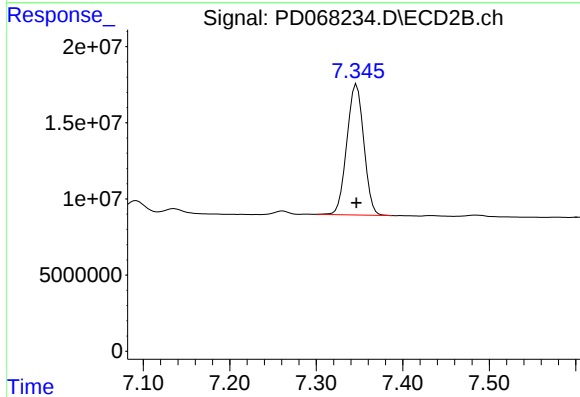


#17 4,4'-DDT

R.T.: 7.347 min
Delta R.T.: 0.000 min
Response: 116501478
Conc: 20.44 ng/ml

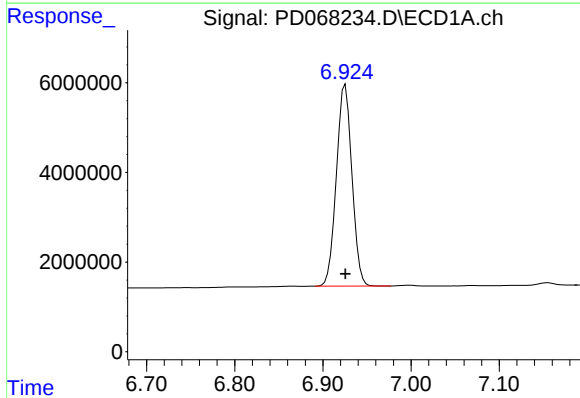


#20 Methoxychlor

R.T.: 6.926 min
Delta R.T.: 0.000 min
Response: 55114474
Conc: 102.69 ng/ml

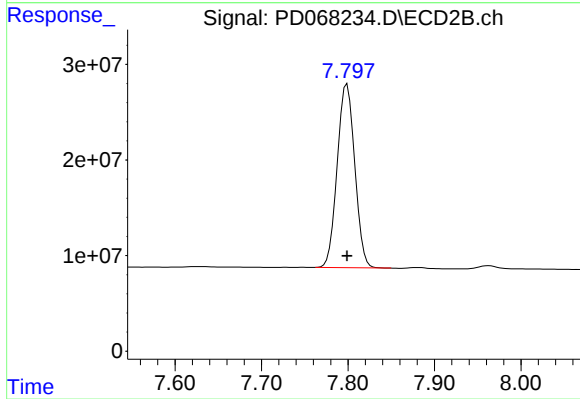

#20 Methoxychlor


R.T.: 7.799 min
Delta R.T.: 0.000 min
Response: 269470911
Conc: 104.34 ng/ml

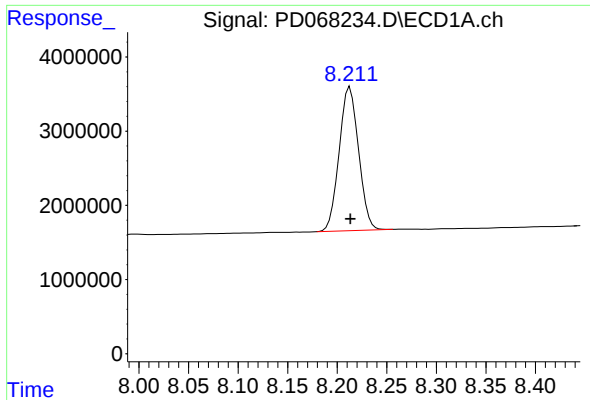

#27 Decachlorobiphenyl

R.T.: 8.213 min
Delta R.T.: 0.000 min
Response: 26374043
Conc: 22.22 ng/ml

Instrument :
ECD_D
ClientSampleId :

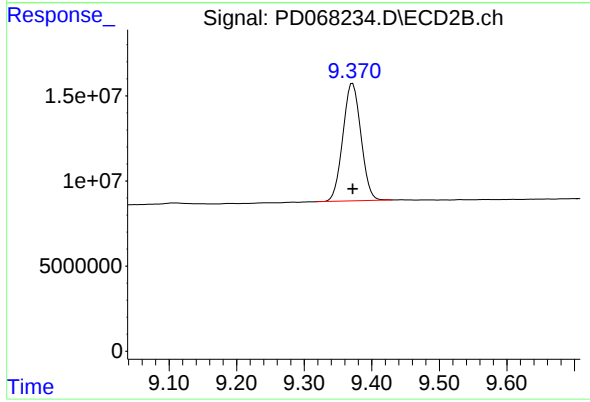

#27 Decachlorobiphenyl

R.T.: 9.372 min
Delta R.T.: 0.000 min
Response: 128185082
Conc: 22.53 ng/ml