

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD022822\
 Data File : PD068236.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Feb 2022 13:26
 Operator : AR\AJ
 Sample : INDA301
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 28 14:26:32 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD022822CLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Feb 28 14:24:43 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.450	4.176	21550438	181.4E6	20.000	20.000
27)	SA Decachlor...	8.213	9.372	47469570	227.6E6	40.000	40.000
Target Compounds							
2)	A alpha-BHC	3.890	4.572	27894412	238.5E6	20.000	20.000
3)	MA gamma-BHC...	4.173	4.863	26839188	220.8E6	20.000	20.000
4)	MA Heptachlor	4.472	5.390	26093849	202.7E6	20.000	20.000
9)	A Endosulfan I	5.504	6.454	23351519	171.5E6	20.000	20.000
13)	MA Dieldrin	5.747	6.712	50352969	353.7E6	40.000	40.000
14)	MA Endrin	6.005	6.932	43893973	275.3E6	40.000	40.000
16)	A 4,4'-DDD	6.133	7.044	39529658	269.4E6	40.000	40.000
17)	MA 4,4'-DDT	6.374	7.347	38383923	227.9E6	40.000	40.000
20)	A Methoxychlor	6.926	7.799	107.3E6	516.5E6	200.000	200.000


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD022822\
Data File : PD068236.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Feb 2022 13:26
Operator : AR\AJ
Sample : INDA301
Misc :
ALS Vial : 13 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 28 14:26:32 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD022822CLP.M
Quant Title : GC Extractables
QLast Update : Mon Feb 28 14:24:43 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

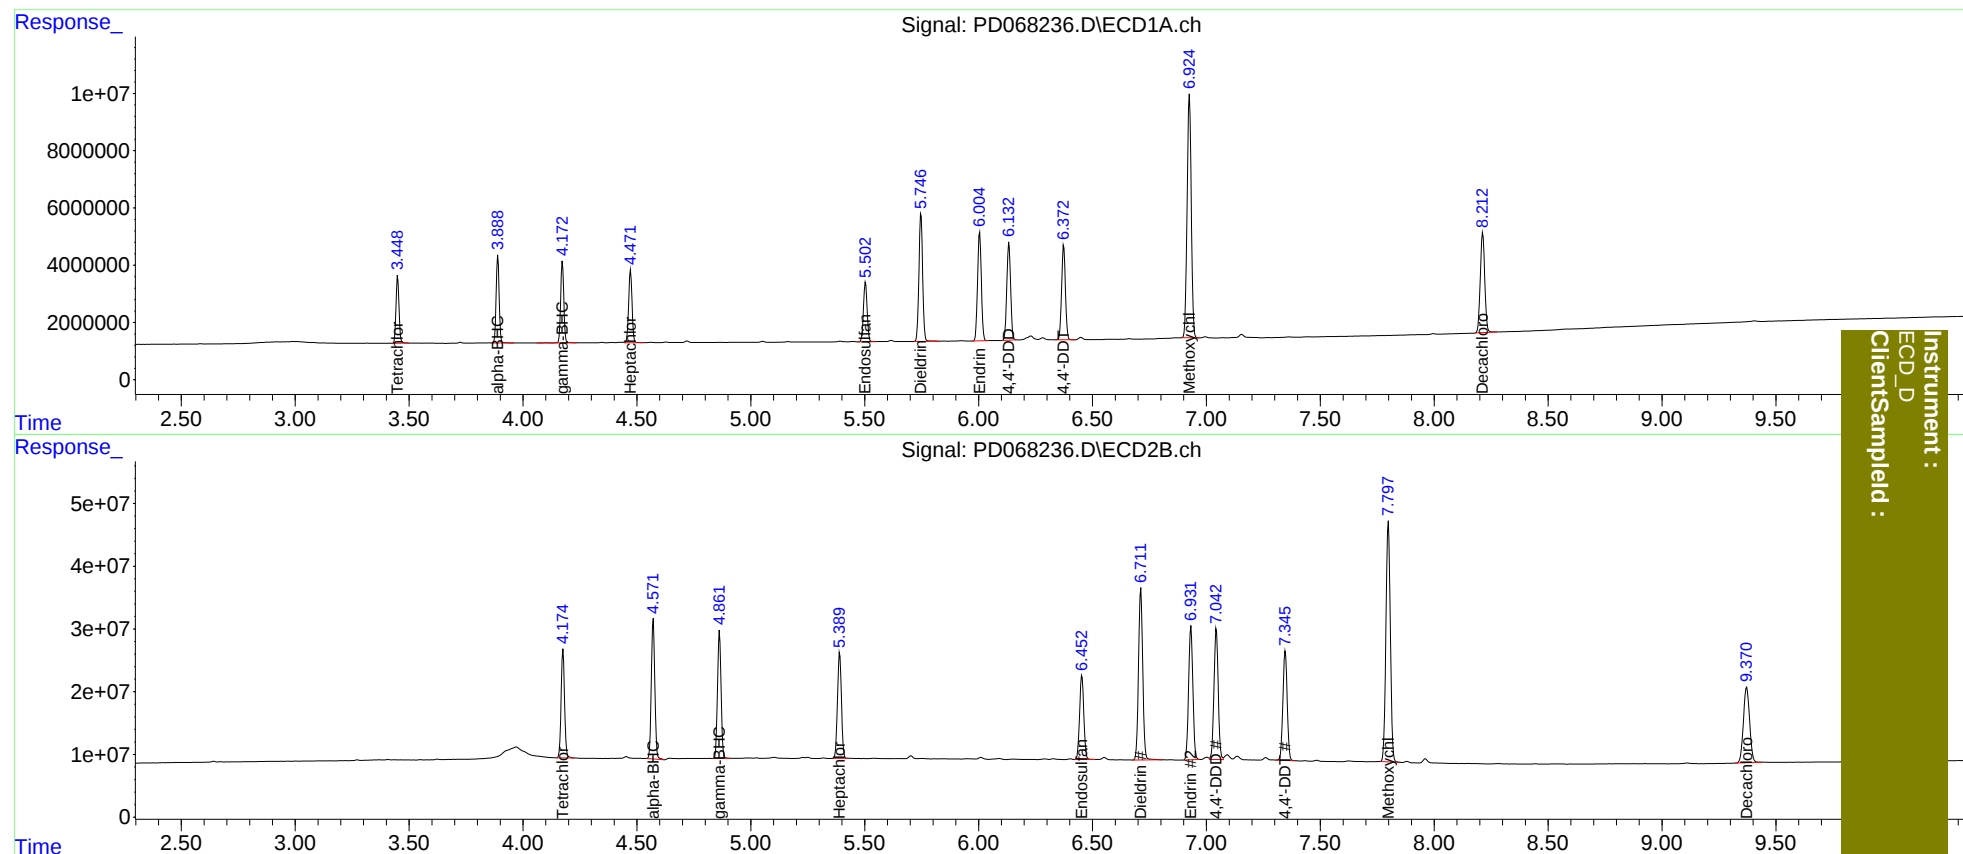


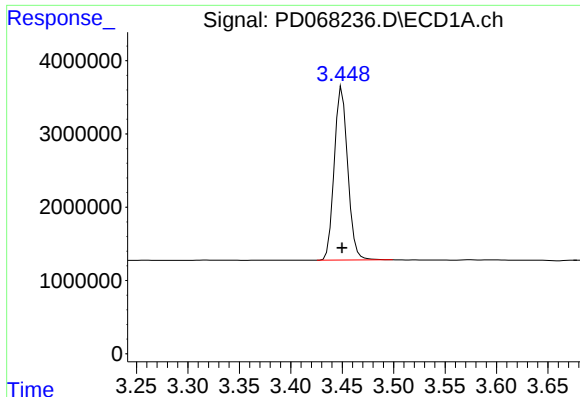

#1 Tetrachloro-m-xylene


R.T.: 3.450 min
Delta R.T.: 0.000 min
Response: 21550438
Conc: 20.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

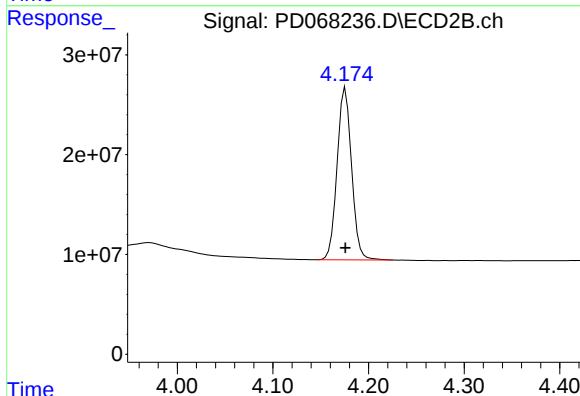


#1 Tetrachloro-m-xylene

R.T.: 4.176 min
Delta R.T.: 0.000 min
Response: 181392872
Conc: 20.00 ng/ml

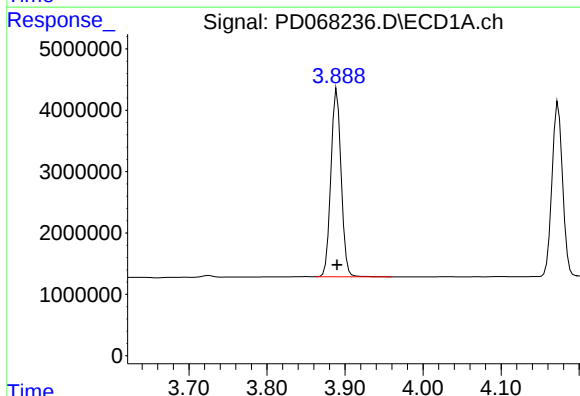


#2 alpha-BHC

R.T.: 3.890 min
Delta R.T.: 0.000 min
Response: 27894412
Conc: 20.00 ng/ml

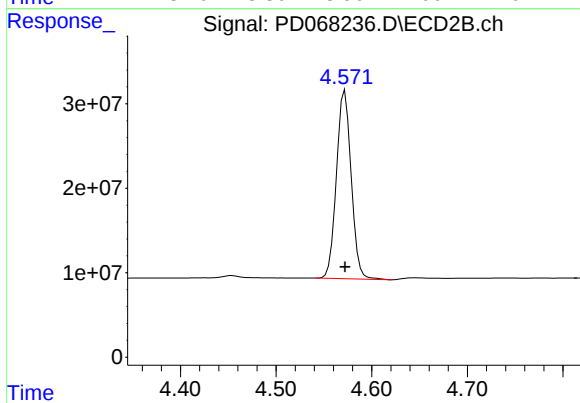

#2 alpha-BHC


R.T.: 4.572 min
Delta R.T.: 0.000 min
Response: 238476846
Conc: 20.00 ng/ml

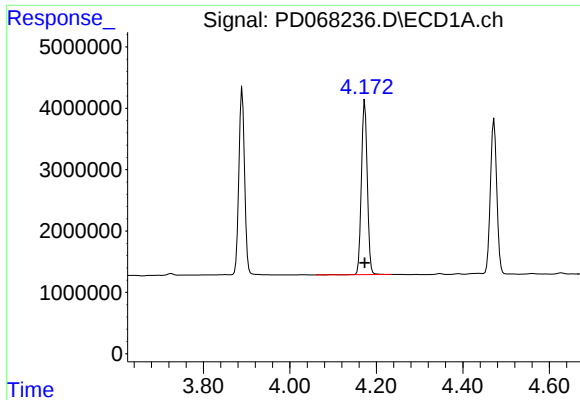

#3 gamma-BHC (Lindane)


R.T.: 4.173 min
Delta R.T.: 0.000 min
Response: 26839188
Conc: 20.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

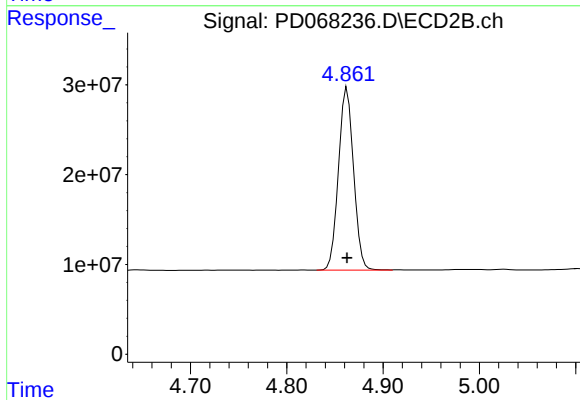


#3 gamma-BHC (Lindane)

R.T.: 4.863 min
Delta R.T.: 0.000 min
Response: 220816375
Conc: 20.00 ng/ml

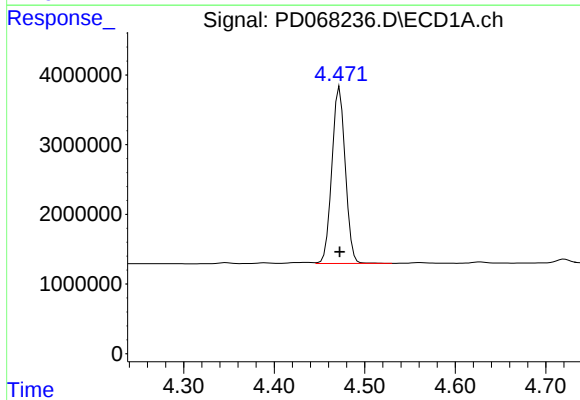


#4 Heptachlor

R.T.: 4.472 min
Delta R.T.: 0.000 min
Response: 26093849
Conc: 20.00 ng/ml

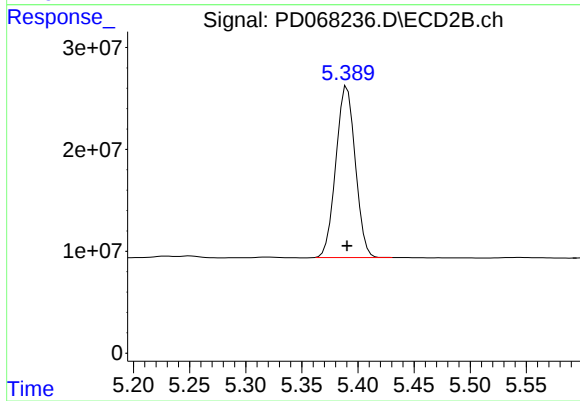

#4 Heptachlor


R.T.: 5.390 min
Delta R.T.: 0.000 min
Response: 202729719
Conc: 20.00 ng/ml

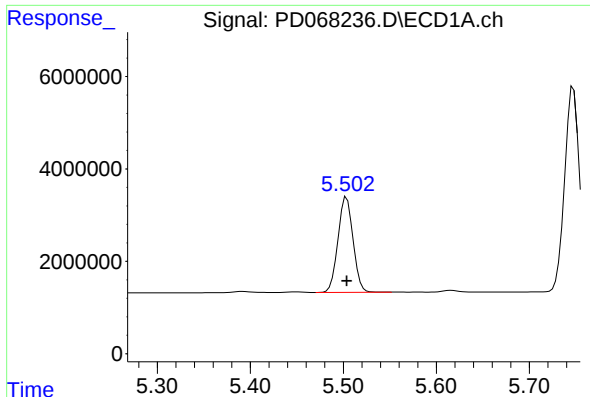

#9 Endosulfan I


R.T.: 5.504 min
Delta R.T.: 0.000 min
Response: 23351519
Conc: 20.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

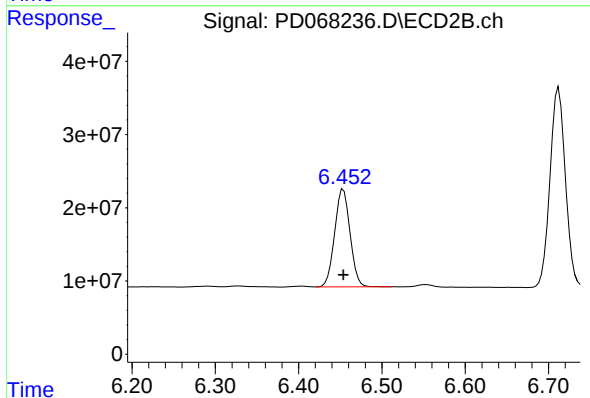


#9 Endosulfan I

R.T.: 6.454 min
Delta R.T.: 0.000 min
Response: 171484654
Conc: 20.00 ng/ml

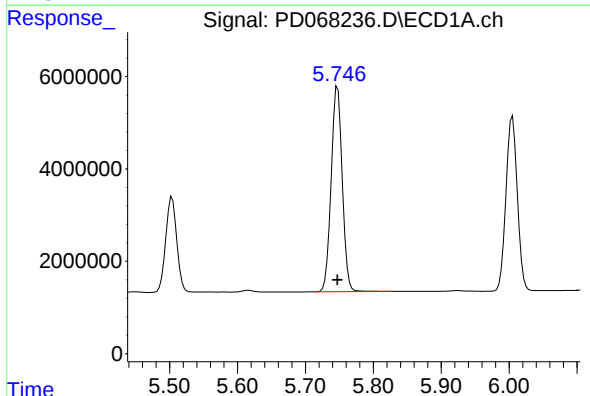


#13 Dieldrin

R.T.: 5.747 min
Delta R.T.: 0.000 min
Response: 50352969
Conc: 40.00 ng/ml

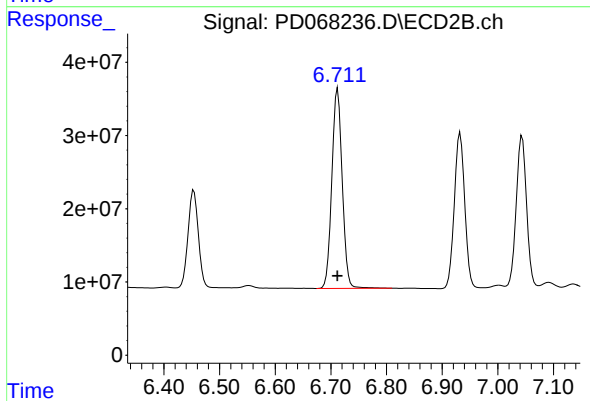

#13 Dieldrin


R.T.: 6.712 min
Delta R.T.: 0.000 min
Response: 353661009
Conc: 40.00 ng/ml

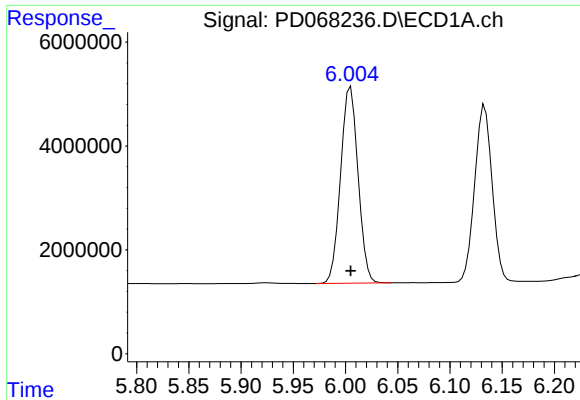

#14 Endrin


R.T.: 6.005 min
Delta R.T.: 0.000 min
Response: 43893973
Conc: 40.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

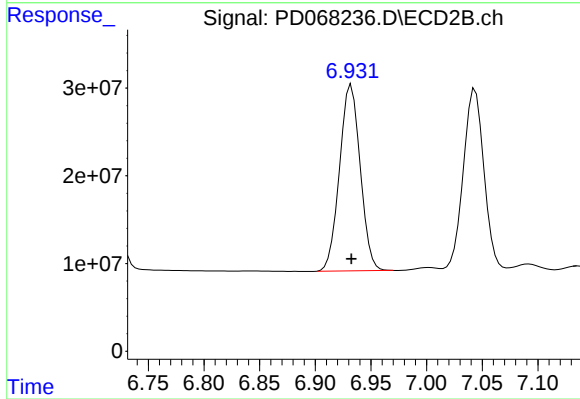


#14 Endrin

R.T.: 6.932 min
Delta R.T.: 0.000 min
Response: 275282698
Conc: 40.00 ng/ml

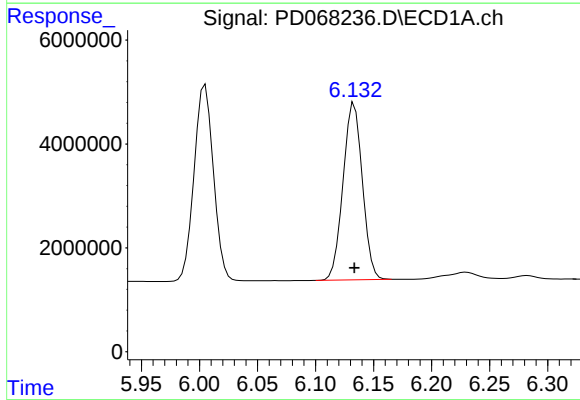


#16 4,4'-DDD

R.T.: 6.133 min
Delta R.T.: 0.000 min
Response: 39529658
Conc: 40.00 ng/ml

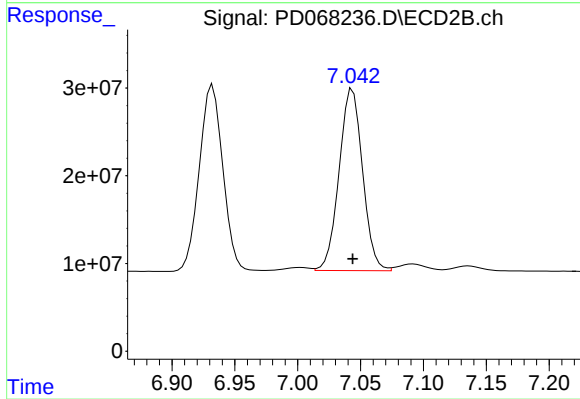

#16 4,4'-DDD


R.T.: 7.044 min
Delta R.T.: 0.000 min
Response: 269410632
Conc: 40.00 ng/ml

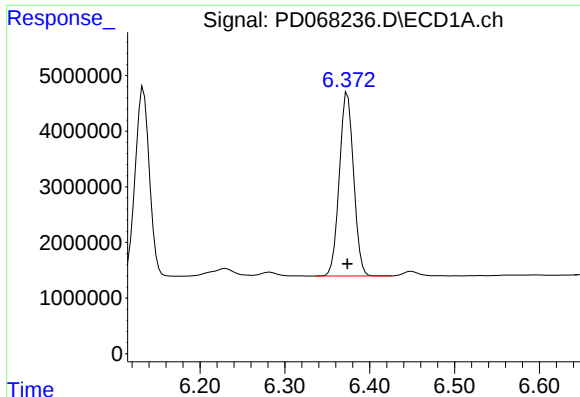

#17 4,4'-DDT


R.T.: 6.374 min
Delta R.T.: 0.000 min
Response: 38383923
Conc: 40.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

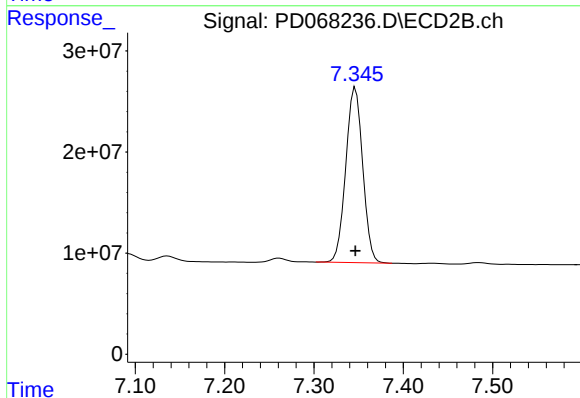


#17 4,4'-DDT

R.T.: 7.347 min
Delta R.T.: 0.000 min
Response: 227936142
Conc: 40.00 ng/ml

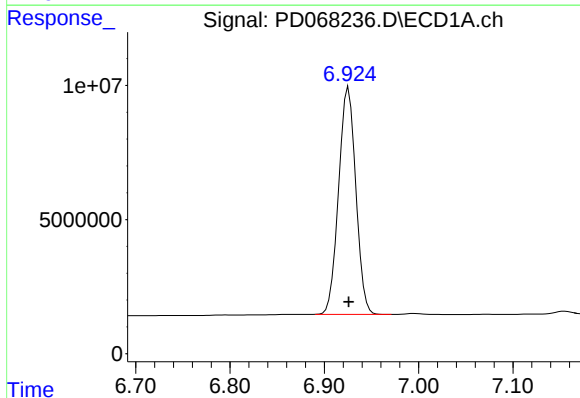


#20 Methoxychlor

R.T.: 6.926 min
Delta R.T.: 0.000 min
Response: 107340208
Conc: 200.00 ng/ml

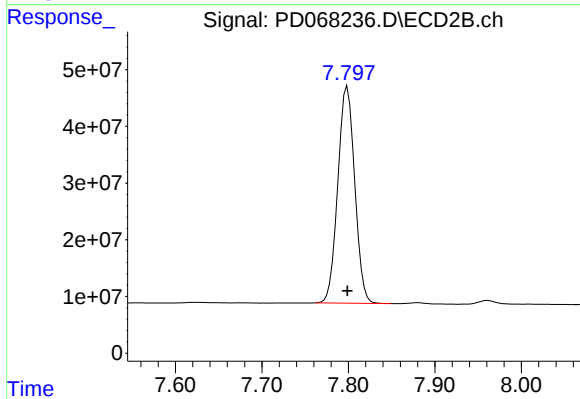

#20 Methoxychlor


R.T.: 7.799 min
Delta R.T.: 0.000 min
Response: 516547841
Conc: 200.00 ng/ml

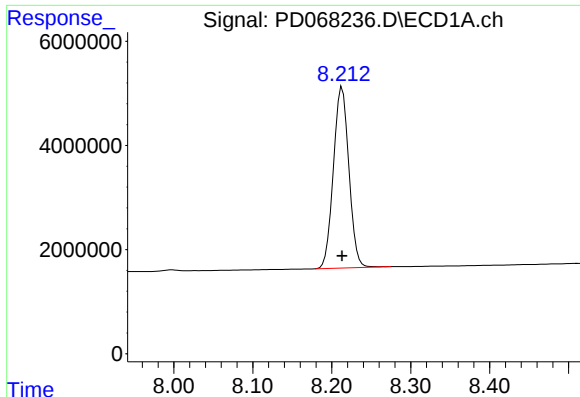

#27 Decachlorobiphenyl

R.T.: 8.213 min
Delta R.T.: 0.000 min
Response: 47469570
Conc: 40.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

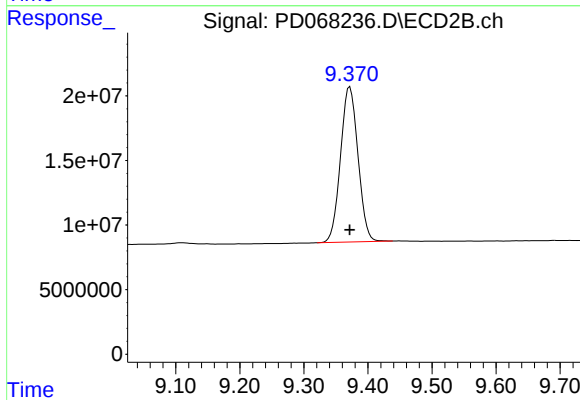

#27 Decachlorobiphenyl

R.T.: 9.372 min
Delta R.T.: 0.000 min
Response: 227617901
Conc: 40.00 ng/ml