

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD022822\
 Data File : PD068238.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Feb 2022 13:56
 Operator : AR\AJ
 Sample : INDA401
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 28 14:26:40 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD022822CLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Feb 28 14:24:43 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.450	4.176	45831935	373.0E6	42.535	41.124
27)	SA Decachlor...	8.214	9.372	88194738	419.9E6	74.317	73.797
Target Compounds							
2)	A alpha-BHC	3.890	4.572	65640437	522.9E6	47.064	43.856
3)	MA gamma-BHC...	4.173	4.863	61874600	484.2E6	46.108	43.853
4)	MA Heptachlor	4.473	5.390	58683830	440.0E6	44.979	43.410
9)	A Endosulfan I	5.504	6.454	51867836	370.4E6	44.424	43.196
13)	MA Dieldrin	5.748	6.712	117.4E6	778.4E6	93.296	88.044
14)	MA Endrin	6.006	6.933	101.7E6	603.3E6	92.692	87.668
16)	A 4,4'-DDD	6.134	7.044	91412718	583.0E6	92.500	86.566
17)	MA 4,4'-DDT	6.375	7.347	90583270	509.7E6	94.397	89.442
20)	A Methoxychlor	6.926	7.800	238.5E6	1130.4E6	444.319	437.660


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD022822\
Data File : PD068238.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Feb 2022 13:56
Operator : AR\AJ
Sample : INDA401
Misc :
ALS Vial : 15 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 28 14:26:40 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD022822CLP.M
Quant Title : GC Extractables
QLast Update : Mon Feb 28 14:24:43 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

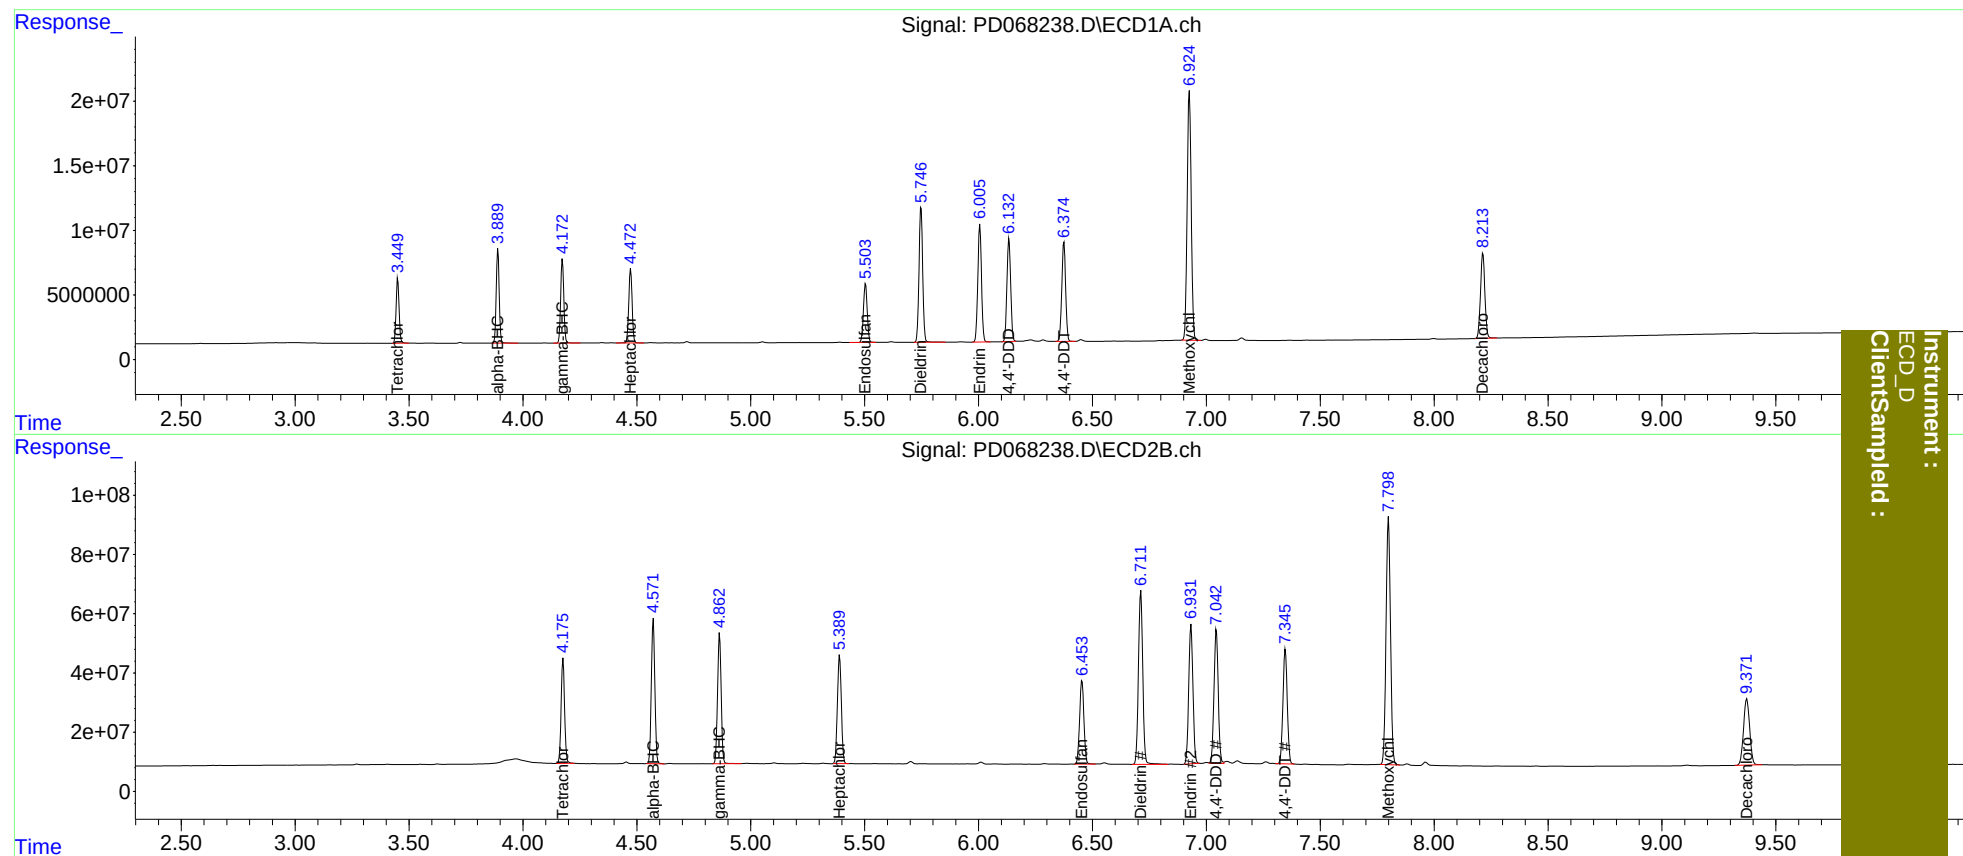


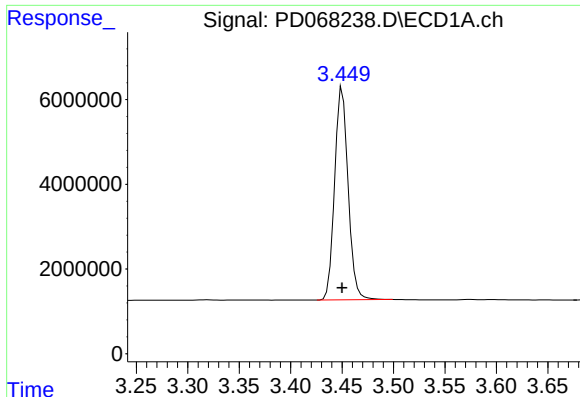

#1 Tetrachloro-m-xylene


R.T.: 3.450 min
Delta R.T.: 0.000 min
Response: 45831935
Conc: 42.53 ng/ml

Instrument :
ECD_D
ClientSampleId :

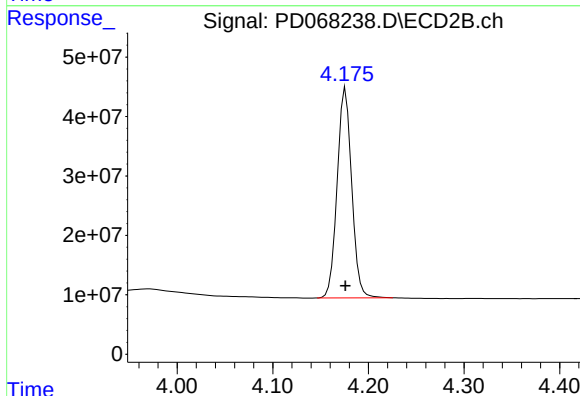


#1 Tetrachloro-m-xylene

R.T.: 4.176 min
Delta R.T.: 0.000 min
Response: 372980246
Conc: 41.12 ng/ml

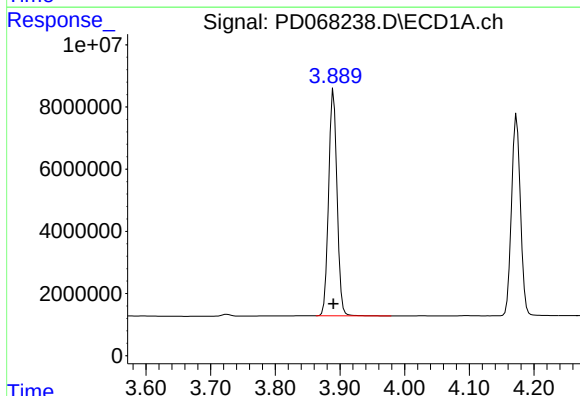


#2 alpha-BHC

R.T.: 3.890 min
Delta R.T.: 0.000 min
Response: 65640437
Conc: 47.06 ng/ml

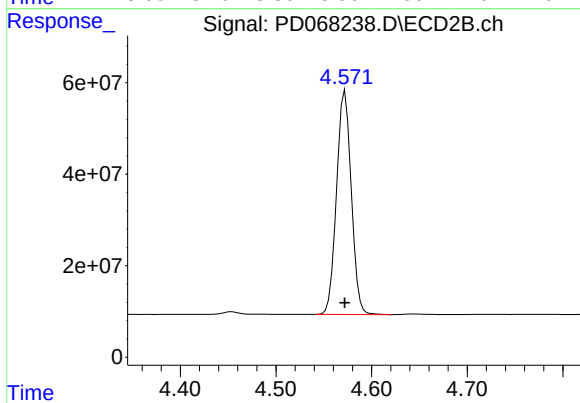

#2 alpha-BHC


R.T.: 4.572 min
Delta R.T.: 0.000 min
Response: 522929122
Conc: 43.86 ng/ml

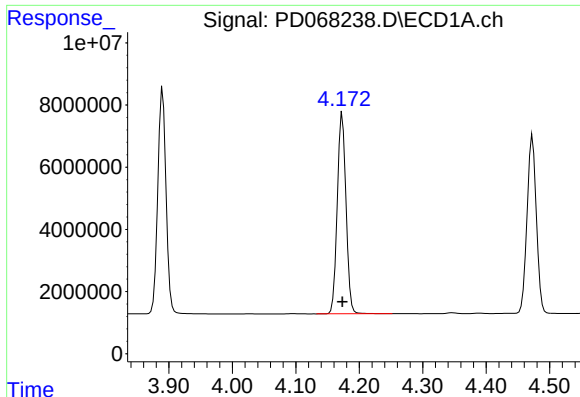

#3 gamma-BHC (Lindane)


R.T.: 4.173 min
Delta R.T.: 0.000 min
Response: 61874600
Conc: 46.11 ng/ml

Instrument :
ECD_D
ClientSampleId :

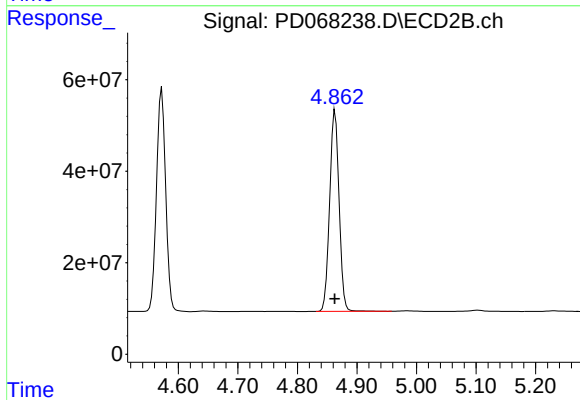


#3 gamma-BHC (Lindane)

R.T.: 4.863 min
Delta R.T.: 0.000 min
Response: 484174589
Conc: 43.85 ng/ml

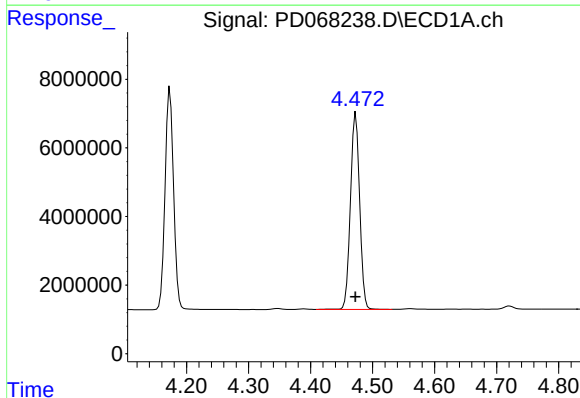


#4 Heptachlor

R.T.: 4.473 min
Delta R.T.: 0.000 min
Response: 58683830
Conc: 44.98 ng/ml

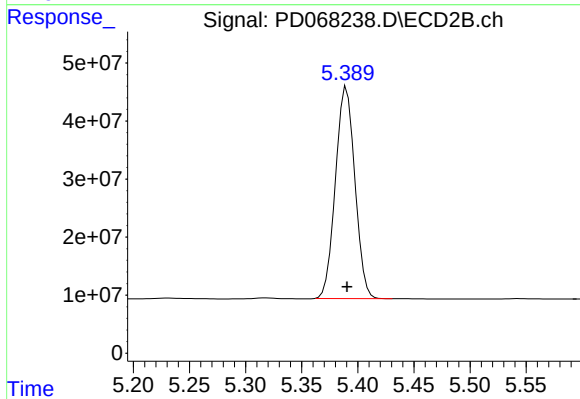

#4 Heptachlor


R.T.: 5.390 min
Delta R.T.: 0.000 min
Response: 440022830
Conc: 43.41 ng/ml

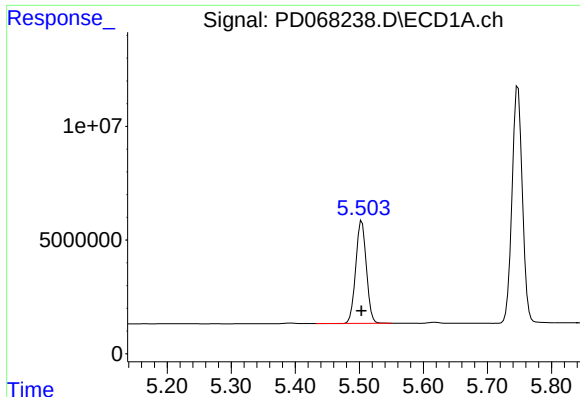

#9 Endosulfan I


R.T.: 5.504 min
Delta R.T.: 0.000 min
Response: 51867836
Conc: 44.42 ng/ml

Instrument :
ECD_D
ClientSampleId :

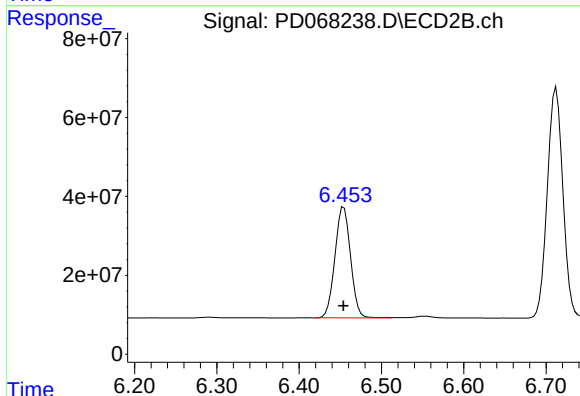


#9 Endosulfan I

R.T.: 6.454 min
Delta R.T.: 0.000 min
Response: 370376081
Conc: 43.20 ng/ml

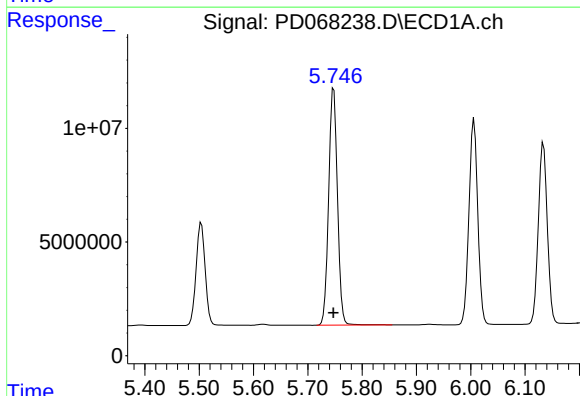


#13 Dieldrin

R.T.: 5.748 min
Delta R.T.: 0.000 min
Response: 117442932
Conc: 93.30 ng/ml

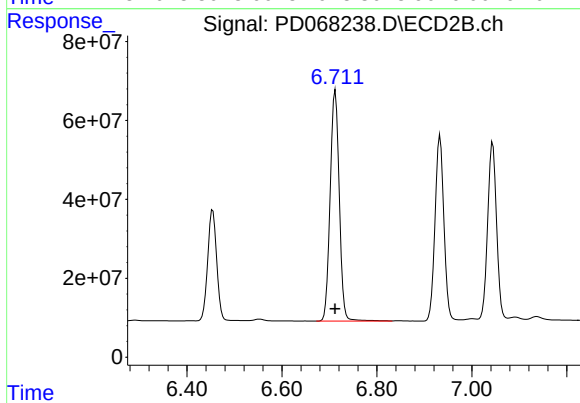

#13 Dieldrin


R.T.: 6.712 min
Delta R.T.: 0.000 min
Response: 778440735
Conc: 88.04 ng/ml

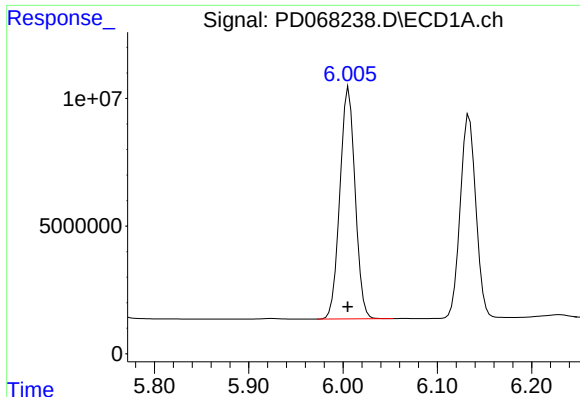

#14 Endrin


R.T.: 6.006 min
Delta R.T.: 0.001 min
Response: 101715083
Conc: 92.69 ng/ml

Instrument :
ECD_D
ClientSampleId :

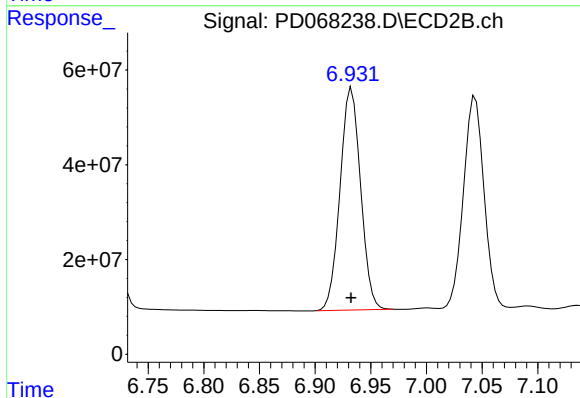


#14 Endrin

R.T.: 6.933 min
Delta R.T.: 0.000 min
Response: 603336361
Conc: 87.67 ng/ml

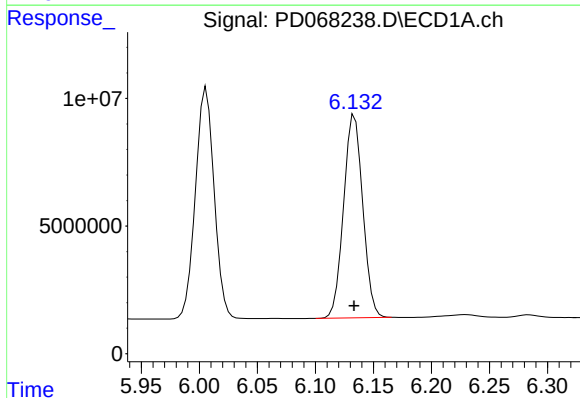


#16 4,4'-DDD

R.T.: 6.134 min
Delta R.T.: 0.000 min
Response: 91412718
Conc: 92.50 ng/ml

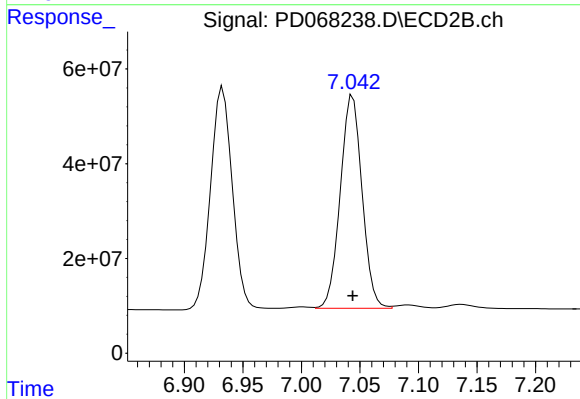

#16 4,4'-DDD


R.T.: 7.044 min
Delta R.T.: 0.000 min
Response: 583045191
Conc: 86.57 ng/ml

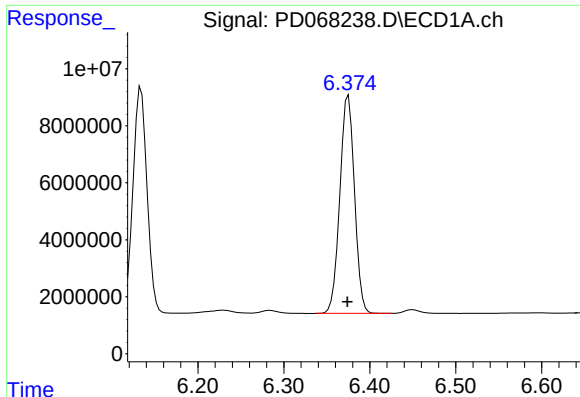

#17 4,4'-DDT


R.T.: 6.375 min
Delta R.T.: 0.001 min
Response: 90583270
Conc: 94.40 ng/ml

Instrument :
ECD_D
ClientSampleId :

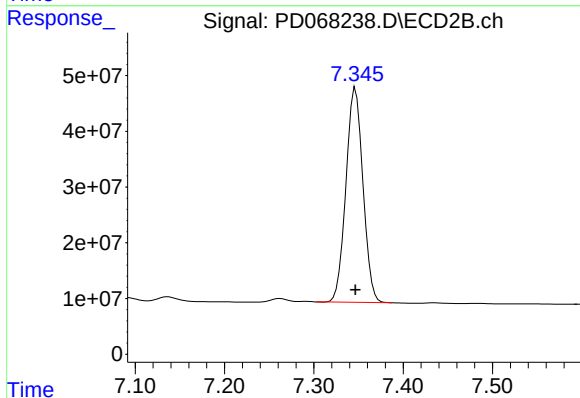


#17 4,4'-DDT

R.T.: 7.347 min
Delta R.T.: 0.000 min
Response: 509674662
Conc: 89.44 ng/ml

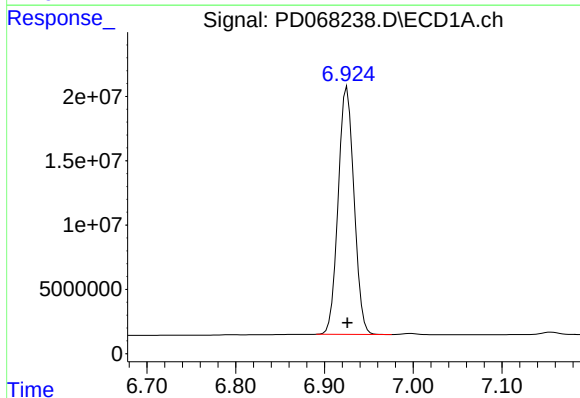


#20 Methoxychlor

R.T.: 6.926 min
Delta R.T.: 0.000 min
Response: 238466650
Conc: 444.32 ng/ml

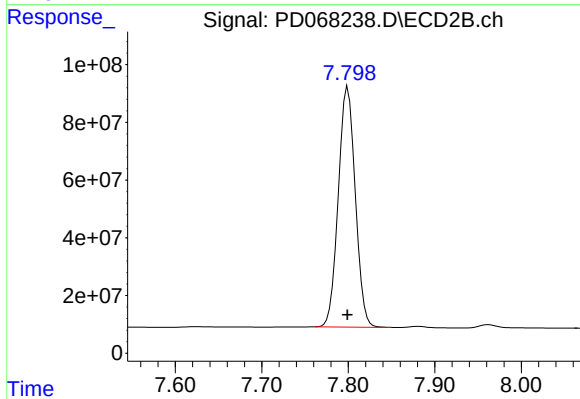

#20 Methoxychlor


R.T.: 7.800 min
Delta R.T.: 0.000 min
Response: 1130362852
Conc: 437.66 ng/ml

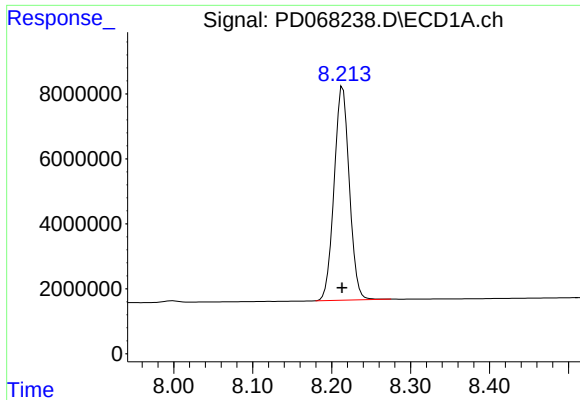

#27 Decachlorobiphenyl

R.T.: 8.214 min
Delta R.T.: 0.000 min
Response: 88194738
Conc: 74.32 ng/ml

Instrument :
ECD_D
ClientSampleId :

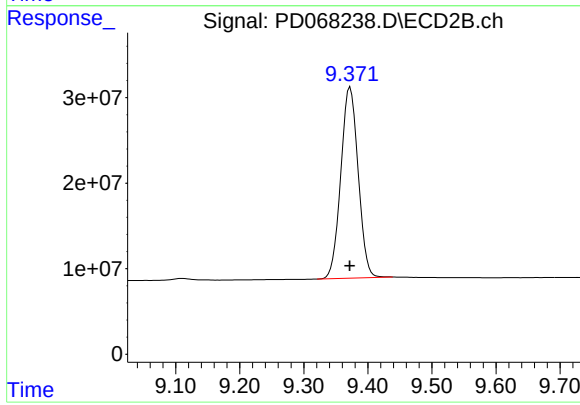

#27 Decachlorobiphenyl

R.T.: 9.372 min
Delta R.T.: 0.000 min
Response: 419935937
Conc: 73.80 ng/ml