

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD022822\
 Data File : PD068240.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Feb 2022 14:24
 Operator : AR\AJ
 Sample : INDA501
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 28 14:54:57 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD022822CLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Feb 28 14:24:43 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.450	4.176	91290491	697.0E6	84.723	76.851
27)	SA Decachlor...	8.214	9.372	170.3E6	788.8E6	143.529	138.621
Target Compounds							
2)	A alpha-BHC	3.890	4.572	139.0E6	1014.6E6	99.647	85.093
3)	MA gamma-BHC...	4.173	4.863	130.0E6	933.8E6	96.867	84.576
4)	MA Heptachlor	4.473	5.390	121.6E6	845.0E6	93.229	83.359
9)	A Endosulfan I	5.504	6.454	105.7E6	701.0E6	90.523	81.757
13)	MA Dieldrin	5.747	6.712	245.1E6	1504.9E6	194.669	170.213
14)	MA Endrin	6.006	6.932	211.2E6	1171.2E6	192.489	170.177
16)	A 4,4'-DDD	6.134	7.043	190.1E6	1120.6E6	192.318	166.385
17)	MA 4,4'-DDT	6.374	7.347	190.5E6	1001.9E6	198.557	175.813
20)	A Methoxychlor	6.926	7.799	467.8E6	2166.5E6	871.678	838.846


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD022822\
Data File : PD068240.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Feb 2022 14:24
Operator : AR\AJ
Sample : INDA501
Misc :
ALS Vial : 17 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 28 14:54:57 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD022822CLP.M
Quant Title : GC Extractables
QLast Update : Mon Feb 28 14:24:43 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

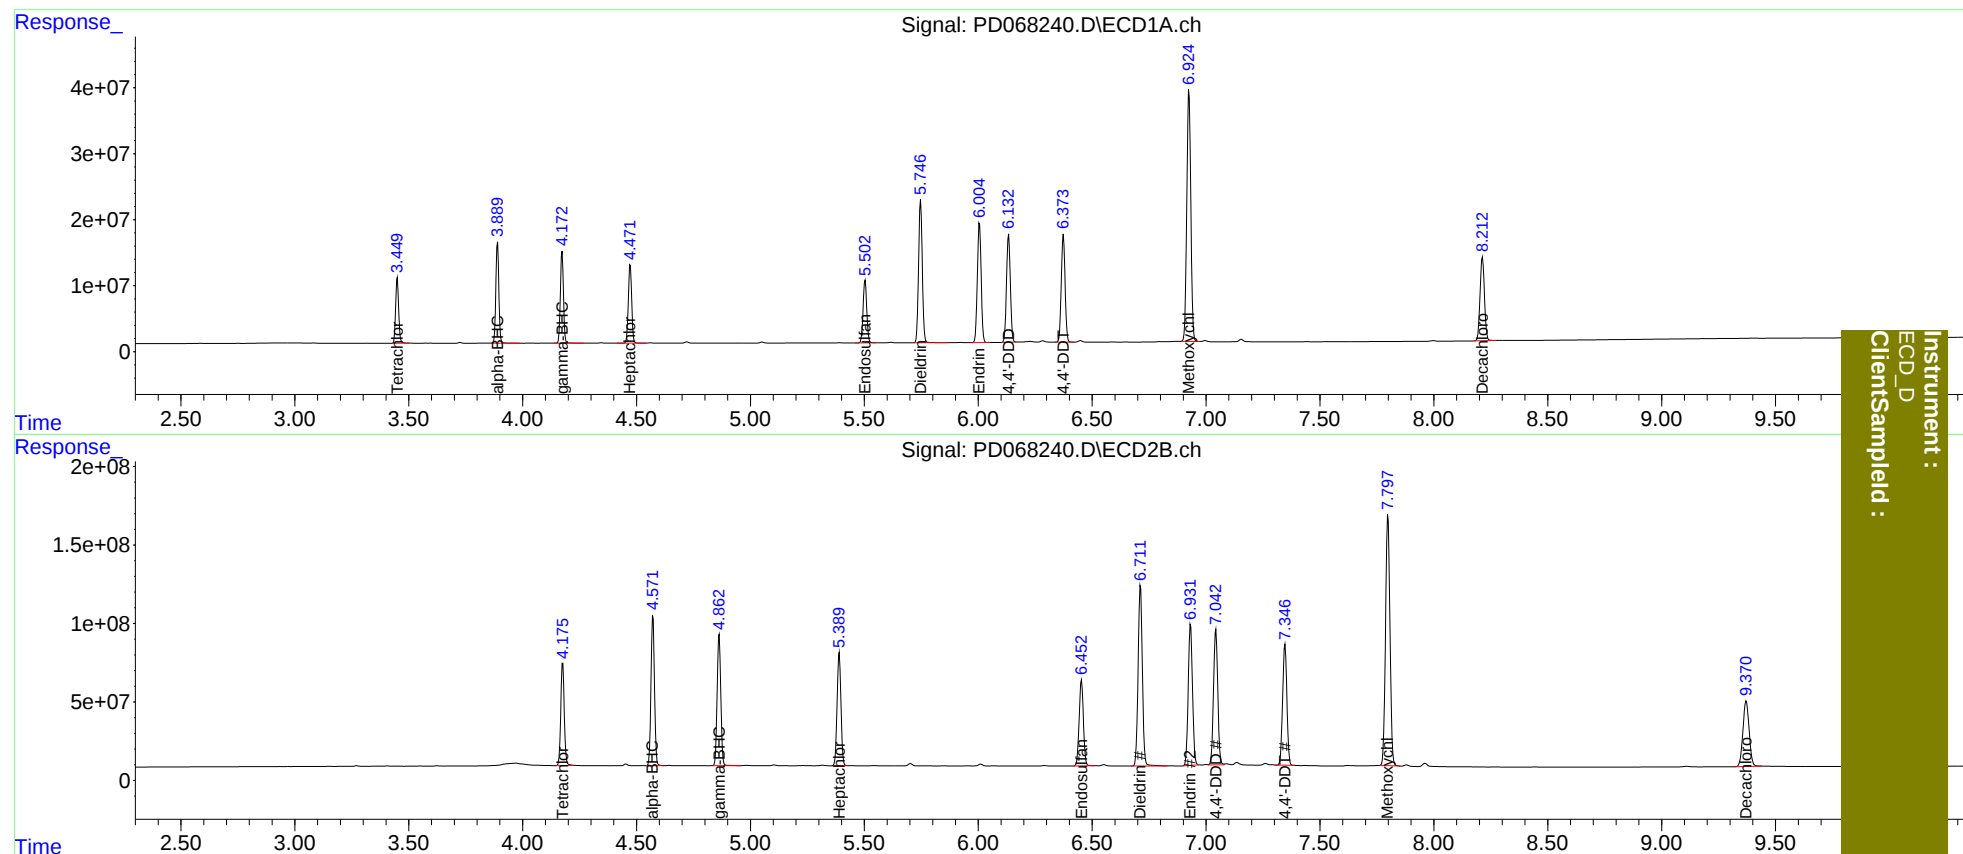


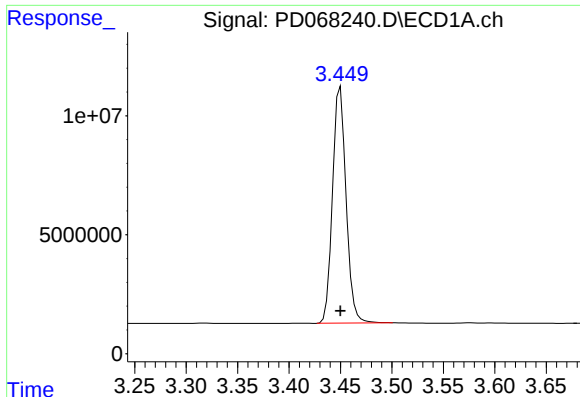

#1 Tetrachloro-m-xylene


R.T.: 3.450 min
Delta R.T.: 0.000 min
Response: 91290491
Conc: 84.72 ng/ml

Instrument :
ECD_D
ClientSampleId :

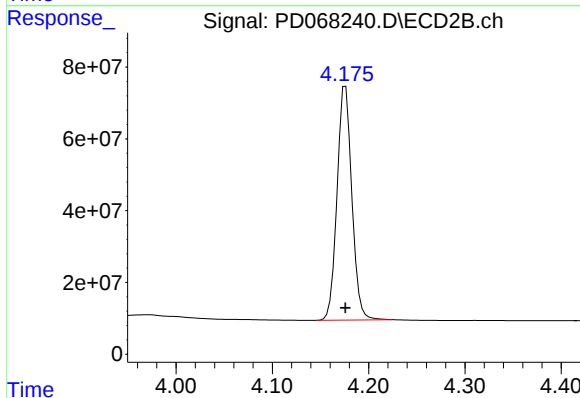


#1 Tetrachloro-m-xylene

R.T.: 4.176 min
Delta R.T.: 0.000 min
Response: 697007023
Conc: 76.85 ng/ml

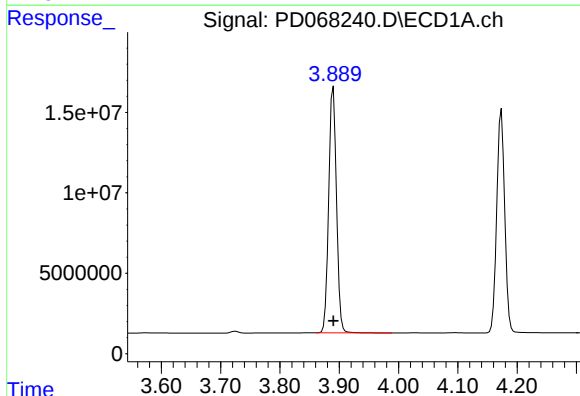


#2 alpha-BHC

R.T.: 3.890 min
Delta R.T.: 0.000 min
Response: 138979928
Conc: 99.65 ng/ml

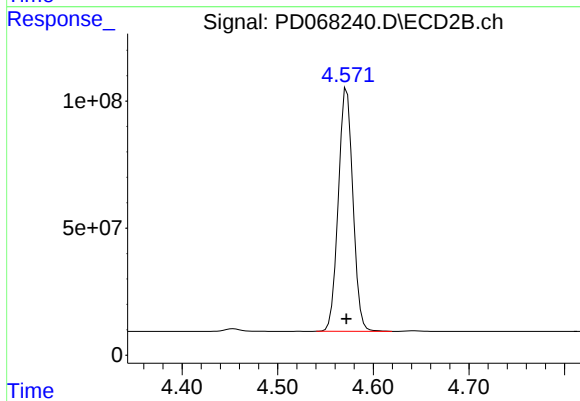

#2 alpha-BHC


R.T.: 4.572 min
Delta R.T.: 0.000 min
Response: 1014633636
Conc: 85.09 ng/ml

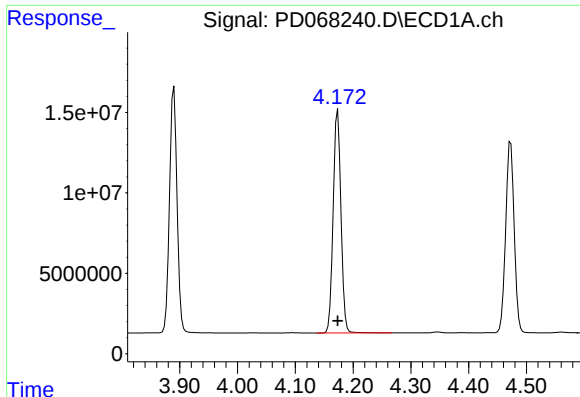

#3 gamma-BHC (Lindane)


R.T.: 4.173 min
Delta R.T.: 0.000 min
Response: 129991357
Conc: 96.87 ng/ml

Instrument :
ECD_D
ClientSampleId :

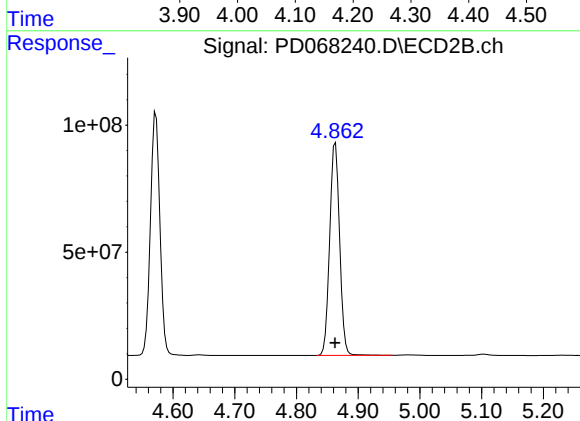


#3 gamma-BHC (Lindane)

R.T.: 4.863 min
Delta R.T.: 0.000 min
Response: 933788631
Conc: 84.58 ng/ml

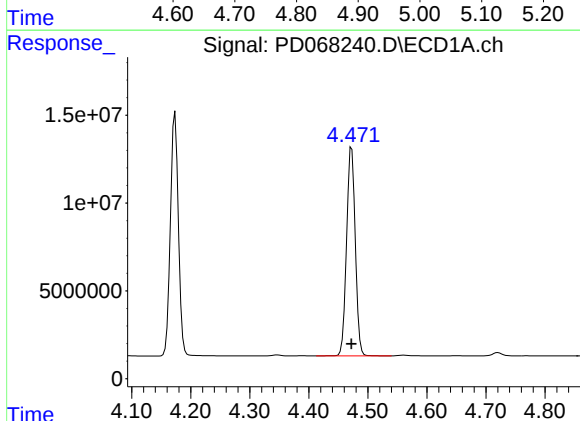


#4 Heptachlor

R.T.: 4.473 min
Delta R.T.: 0.000 min
Response: 121634961
Conc: 93.23 ng/ml

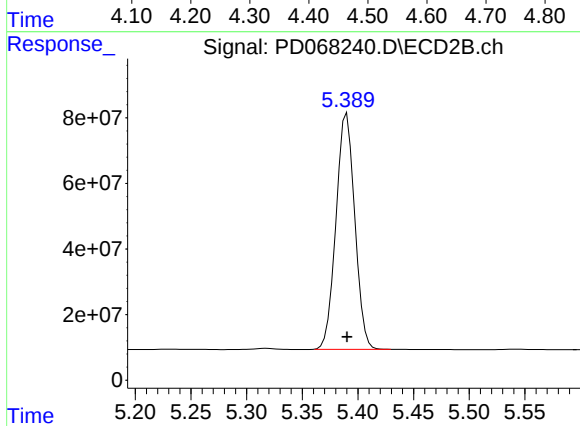

#4 Heptachlor


R.T.: 5.390 min
Delta R.T.: 0.000 min
Response: 844966603
Conc: 83.36 ng/ml

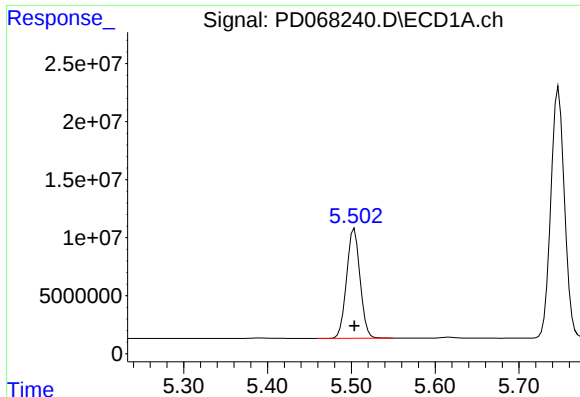

#9 Endosulfan I


R.T.: 5.504 min
Delta R.T.: 0.000 min
Response: 105692258
Conc: 90.52 ng/ml

Instrument :
ECD_D
ClientSampleId :

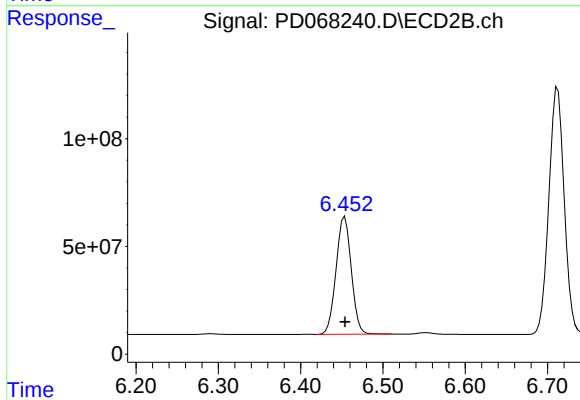


#9 Endosulfan I

R.T.: 6.454 min
Delta R.T.: 0.000 min
Response: 701003235
Conc: 81.76 ng/ml

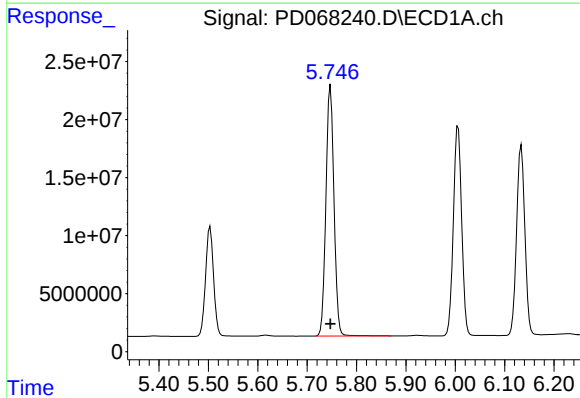


#13 Dieldrin

R.T.: 5.747 min
Delta R.T.: 0.000 min
Response: 245054668
Conc: 194.67 ng/ml

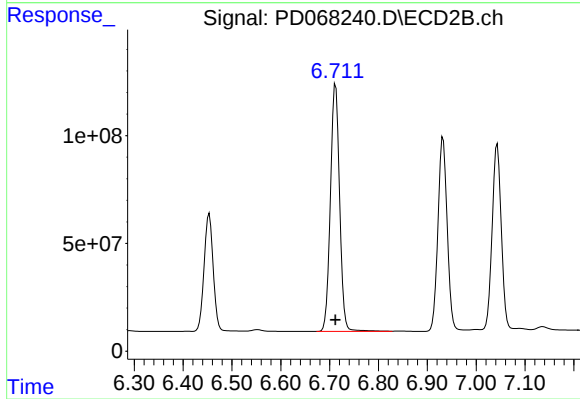

#13 Dieldrin


R.T.: 6.712 min
Delta R.T.: 0.000 min
Response: 1504946307
Conc: 170.21 ng/ml

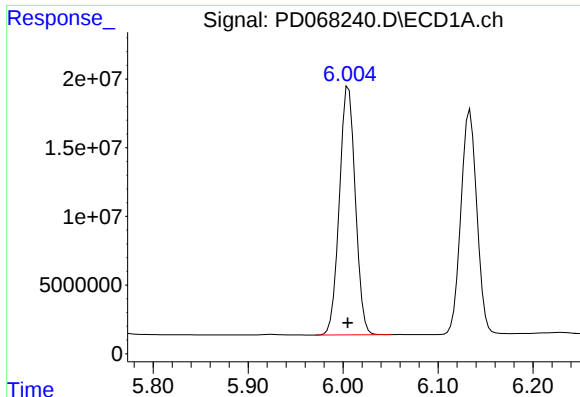

#14 Endrin


R.T.: 6.006 min
Delta R.T.: 0.000 min
Response: 211227305
Conc: 192.49 ng/ml

Instrument :
ECD_D
ClientSampleId :

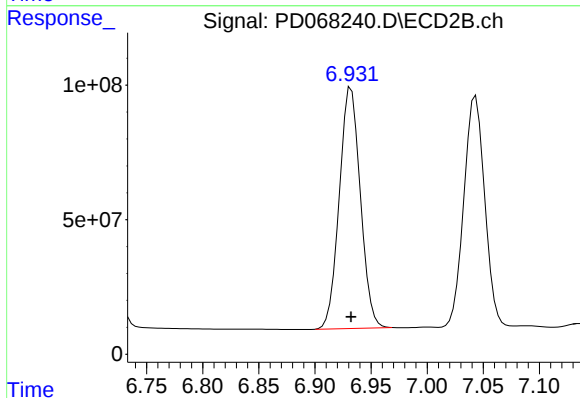


#14 Endrin

R.T.: 6.932 min
Delta R.T.: 0.000 min
Response: 1171172118
Conc: 170.18 ng/ml

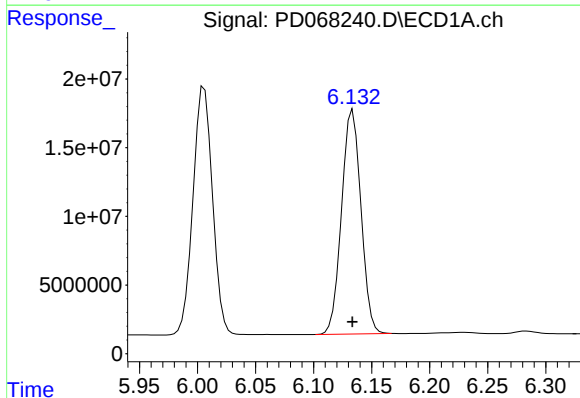


#16 4,4'-DDD

R.T.: 6.134 min
Delta R.T.: 0.000 min
Response: 190057028
Conc: 192.32 ng/ml

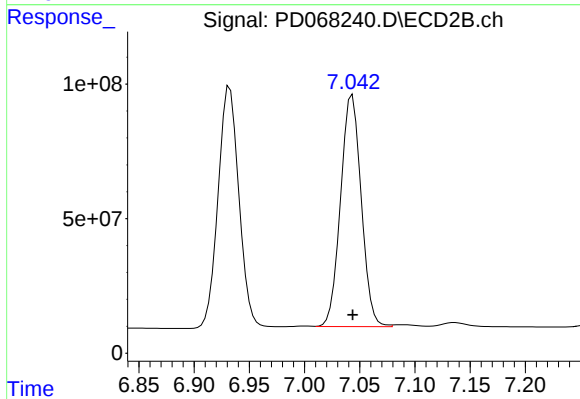

#16 4,4'-DDD


R.T.: 7.043 min
Delta R.T.: 0.000 min
Response: 1120647622
Conc: 166.39 ng/ml

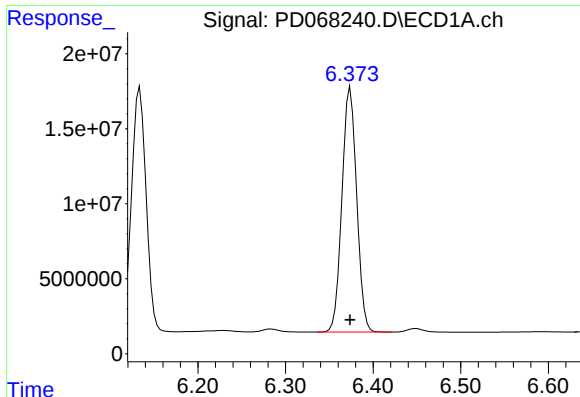

#17 4,4'-DDT


R.T.: 6.374 min
Delta R.T.: 0.000 min
Response: 190534941
Conc: 198.56 ng/ml

Instrument :
ECD_D
ClientSampleId :

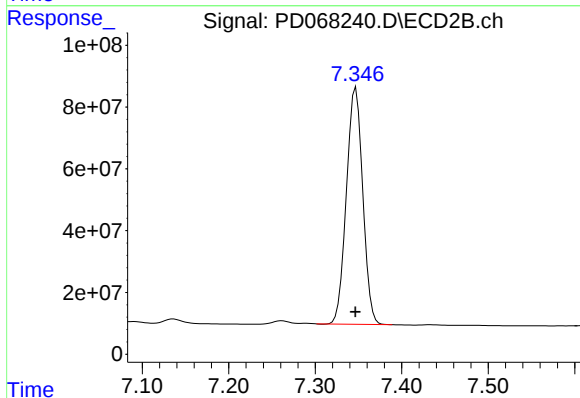


#17 4,4'-DDT

R.T.: 7.347 min
Delta R.T.: 0.000 min
Response: 1001854417
Conc: 175.81 ng/ml

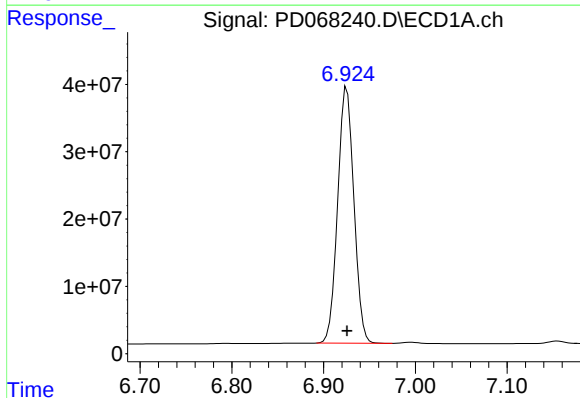


#20 Methoxychlor

R.T.: 6.926 min
Delta R.T.: 0.000 min
Response: 467830459
Conc: 871.68 ng/ml

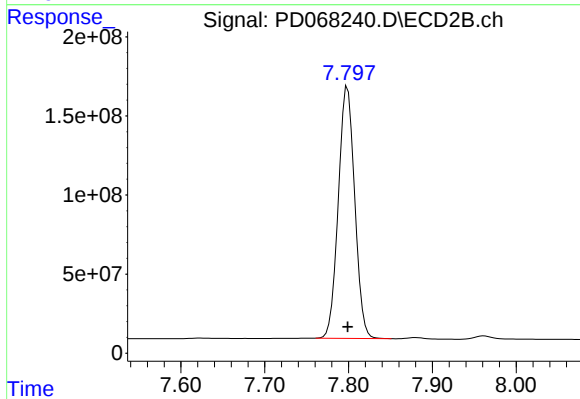

#20 Methoxychlor


R.T.: 7.799 min
Delta R.T.: 0.000 min
Response: 2166519697
Conc: 838.85 ng/ml

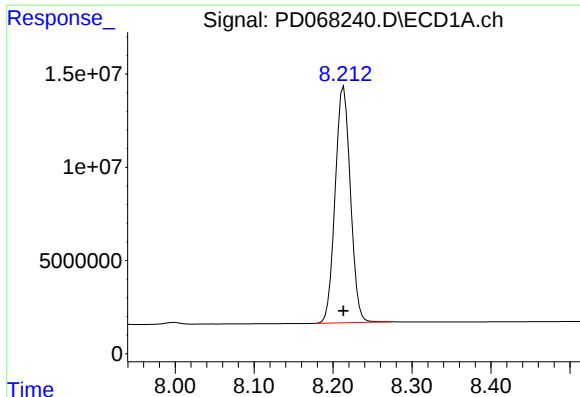

#27 Decachlorobiphenyl

R.T.: 8.214 min
Delta R.T.: 0.000 min
Response: 170331445
Conc: 143.53 ng/ml

Instrument :
ECD_D
ClientSampleId :

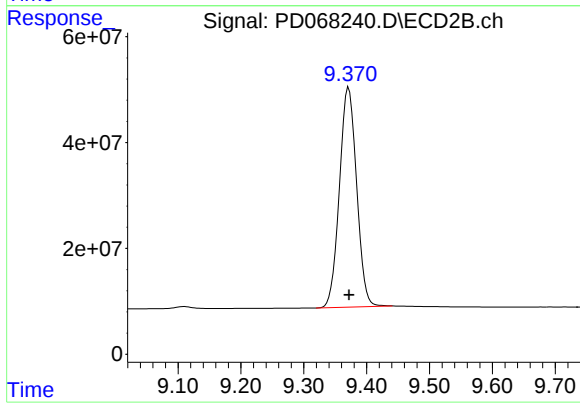

#27 Decachlorobiphenyl

R.T.: 9.372 min
Delta R.T.: 0.000 min
Response: 788815092
Conc: 138.62 ng/ml