

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD022822\
 Data File : PD068241.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Feb 2022 14:38
 Operator : AR\AJ
 Sample : INDB501
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 28 15:18:40 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD022822CLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Feb 28 15:12:42 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.450	4.176	89164999	679.6E6	85.403	76.474
27)	SA Decachlor...	8.213	9.373	166.6E6	772.9E6	154.620	143.190
Target Compounds							
5)	MB Aldrin	4.721	5.703	123.6E6	861.6E6	95.022	80.444
6)	B beta-BHC	4.423	5.025	53433616	393.7E6	81.438	76.325
7)	B delta-BHC	4.628	5.251	127.2E6	919.3E6	97.667	82.043
8)	B Heptachlo...	5.166	6.091	110.2E6	755.4E6	89.938	78.334
10)	B trans-Chl...	5.392	6.328	113.9E6	759.5E6	91.799	79.304
11)	B cis-Chlor...	5.450	6.403	112.0E6	734.8E6	91.034	79.052
12)	B 4,4'-DDE	5.617	6.553	218.4E6	1358.4E6	196.294	164.313
15)	B Endosulfa...	6.280	7.137	199.0E6	1163.8E6	181.200	157.703
18)	B Endrin al...	6.450	7.262	147.2E6	839.5E6	175.465	156.240
19)	B Endosulfa...	6.662	7.487	191.8E6	1044.8E6	182.419	157.139
21)	B Endrin ke...	7.156	7.962	214.4E6	1078.1E6	180.218	156.471


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD022822\
Data File : PD068241.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Feb 2022 14:38
Operator : AR\AJ
Sample : INDB501
Misc :
ALS Vial : 18 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 28 15:18:40 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD022822CLP.M
Quant Title : GC Extractables
QLast Update : Mon Feb 28 15:12:42 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

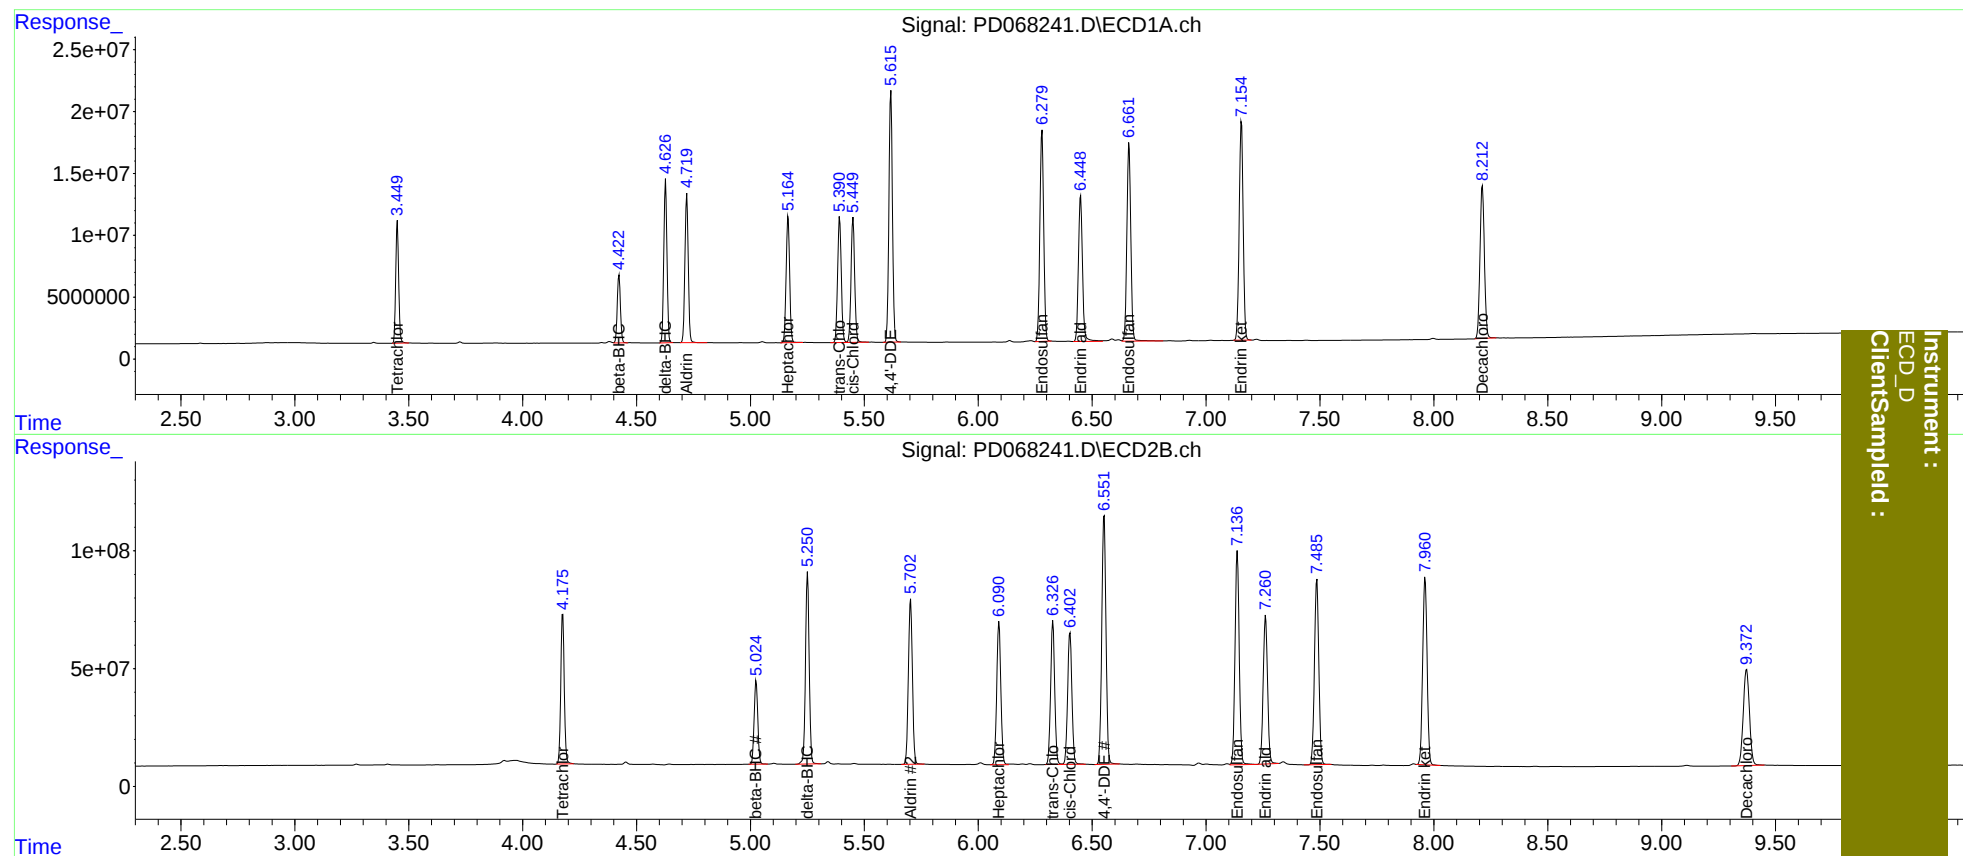


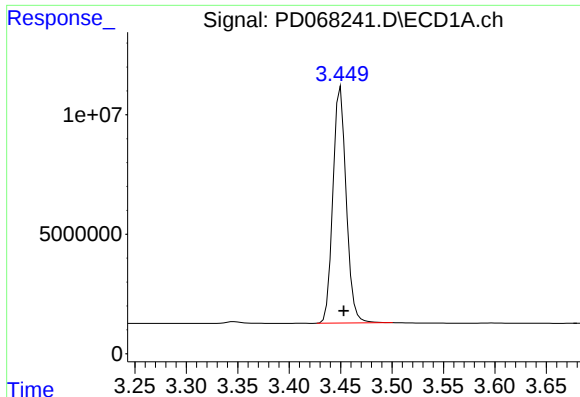

#1 Tetrachloro-m-xylene


R.T.: 3.450 min
Delta R.T.: -0.003 min
Response: 89164999
Conc: 85.40 ng/ml

Instrument :
ECD_D
ClientSampleId :

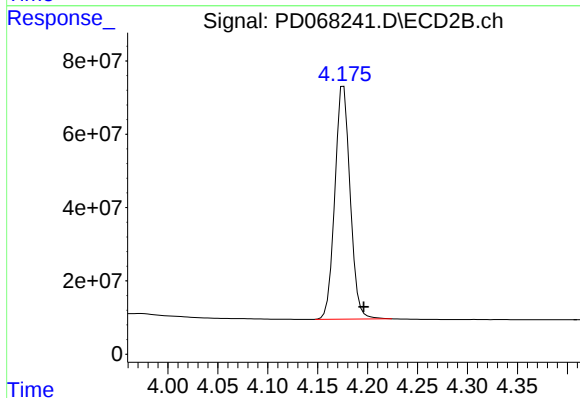


#1 Tetrachloro-m-xylene

R.T.: 4.176 min
Delta R.T.: -0.020 min
Response: 679613775
Conc: 76.47 ng/ml

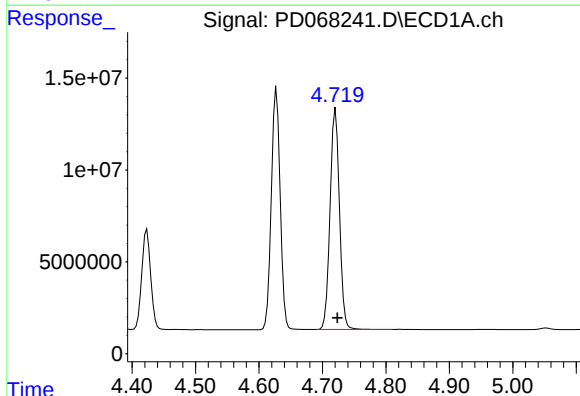


#5 Aldrin

R.T.: 4.721 min
Delta R.T.: -0.003 min
Response: 123609024
Conc: 95.02 ng/ml

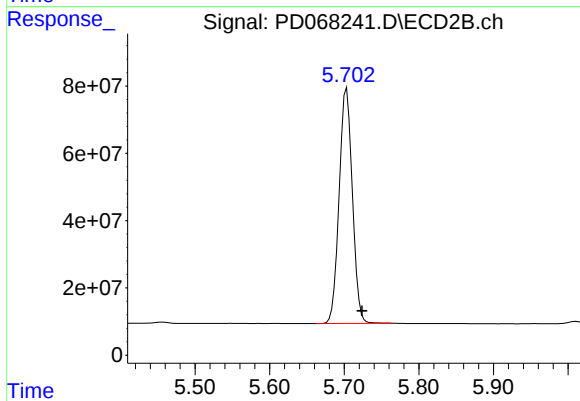

#5 Aldrin


R.T.: 5.703 min
Delta R.T.: -0.021 min
Response: 861559914
Conc: 80.44 ng/ml

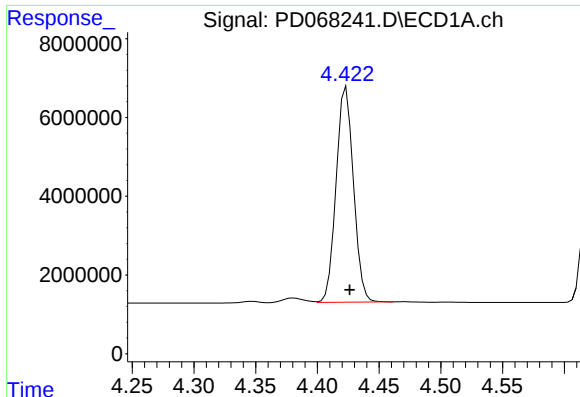

#6 beta-BHC


R.T.: 4.423 min
Delta R.T.: -0.003 min
Response: 53433616
Conc: 81.44 ng/ml

Instrument :
ECD_D
ClientSampleId :

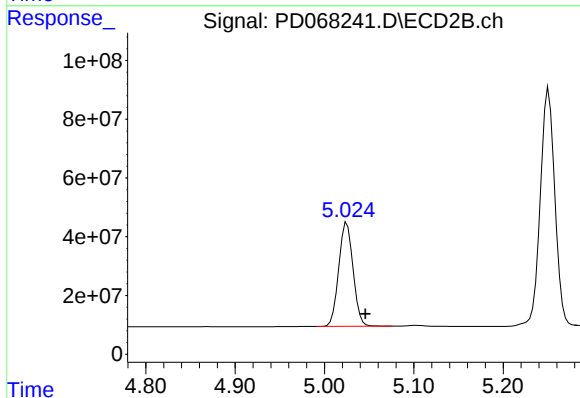


#6 beta-BHC

R.T.: 5.025 min
Delta R.T.: -0.021 min
Response: 393704853
Conc: 76.32 ng/ml

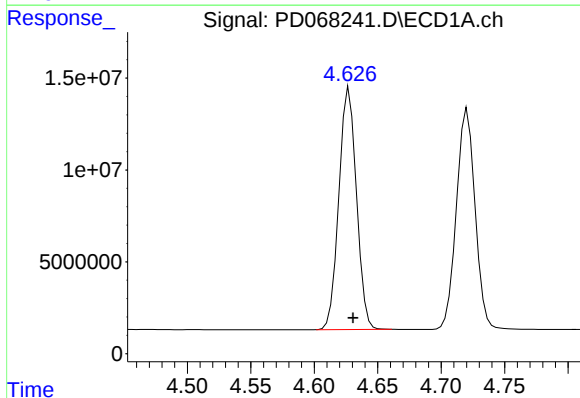


#7 delta-BHC

R.T.: 4.628 min
Delta R.T.: -0.003 min
Response: 127167225
Conc: 97.67 ng/ml

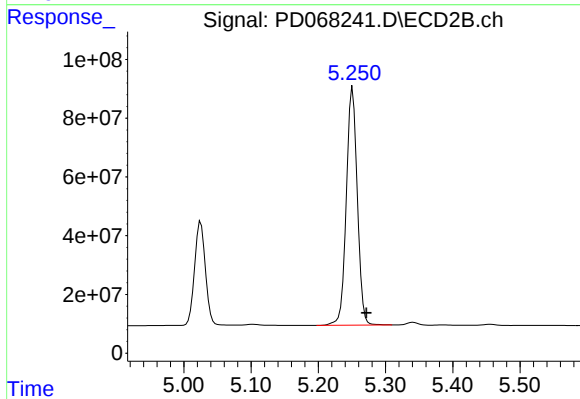

#7 delta-BHC


R.T.: 5.251 min
Delta R.T.: -0.021 min
Response: 919319054
Conc: 82.04 ng/ml

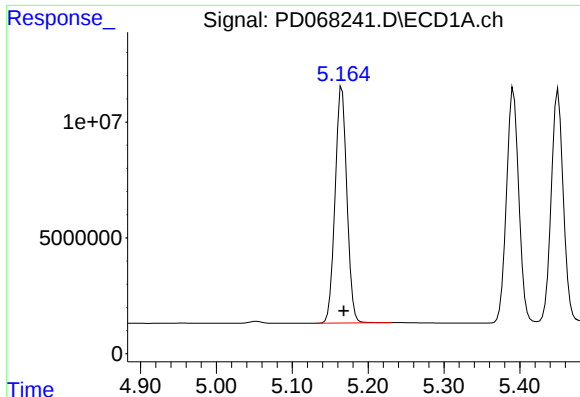

#8 Heptachlor epoxide


R.T.: 5.166 min
Delta R.T.: -0.003 min
Response: 110244936
Conc: 89.94 ng/ml

Instrument :
ECD_D
ClientSampleId :

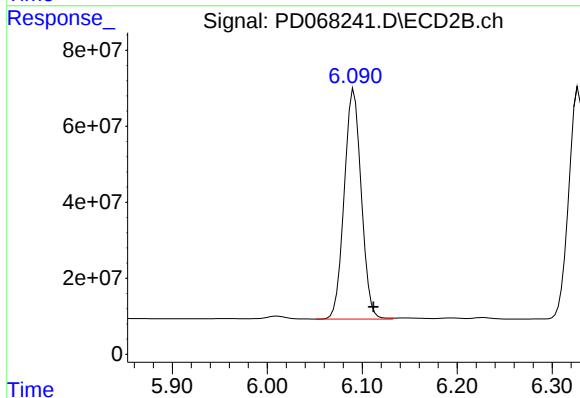


#8 Heptachlor epoxide

R.T.: 6.091 min
Delta R.T.: -0.021 min
Response: 755383764
Conc: 78.33 ng/ml

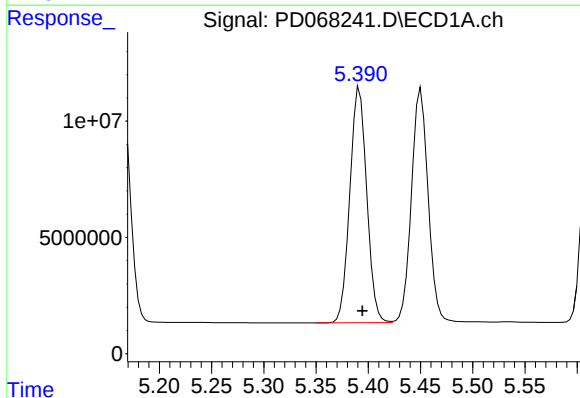


#10 trans-Chlordane

R.T.: 5.392 min
Delta R.T.: -0.003 min
Response: 113929503
Conc: 91.80 ng/ml

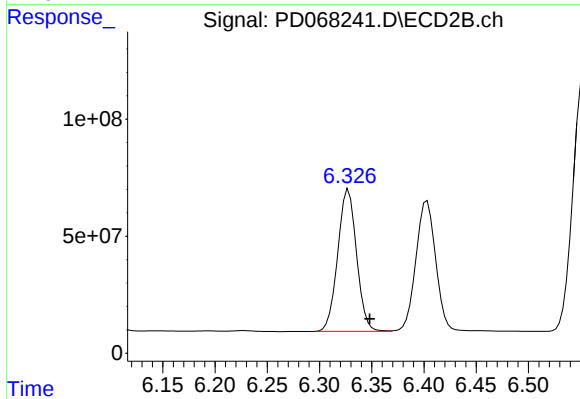

#10 trans-Chlordane


R.T.: 6.328 min
Delta R.T.: -0.020 min
Response: 759510627
Conc: 79.30 ng/ml

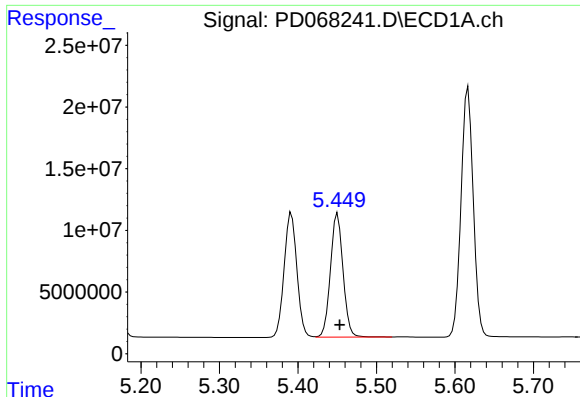

#11 cis-Chlordane


R.T.: 5.450 min
Delta R.T.: -0.003 min
Response: 111970734
Conc: 91.03 ng/ml

Instrument :
ECD_D
ClientSampleId :

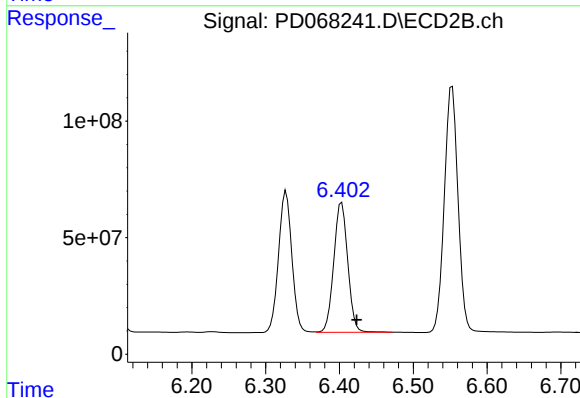


#11 cis-Chlordane

R.T.: 6.403 min
Delta R.T.: -0.020 min
Response: 734772502
Conc: 79.05 ng/ml

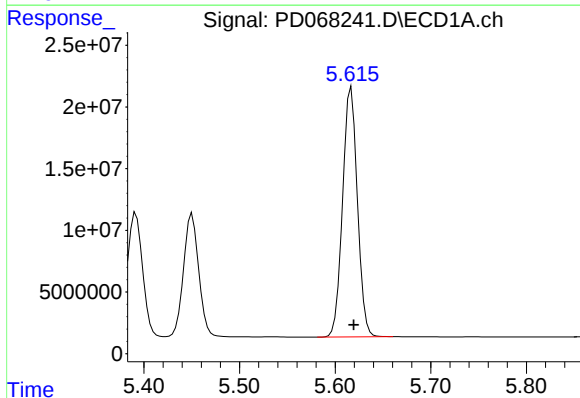


#12 4,4'-DDE

R.T.: 5.617 min
Delta R.T.: -0.003 min
Response: 218362325
Conc: 196.29 ng/ml

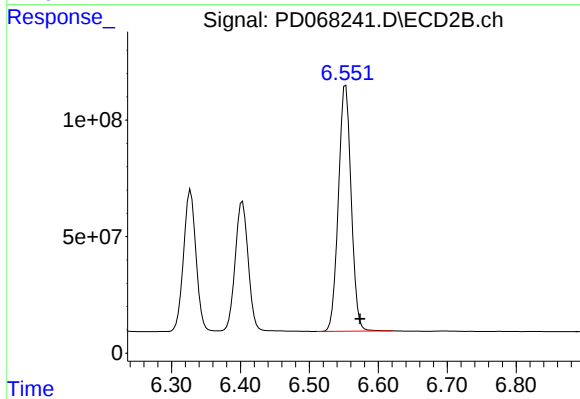

#12 4,4'-DDE


R.T.: 6.553 min
Delta R.T.: -0.021 min
Response: 1358431997
Conc: 164.31 ng/ml

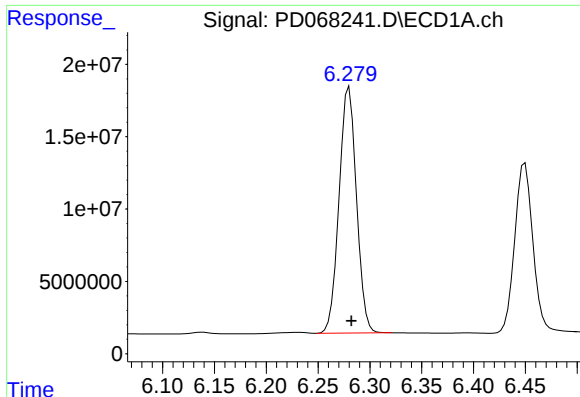

#15 Endosulfan II


R.T.: 6.280 min
Delta R.T.: -0.002 min
Response: 198957219
Conc: 181.20 ng/ml

Instrument :
ECD_D
ClientSampleId :

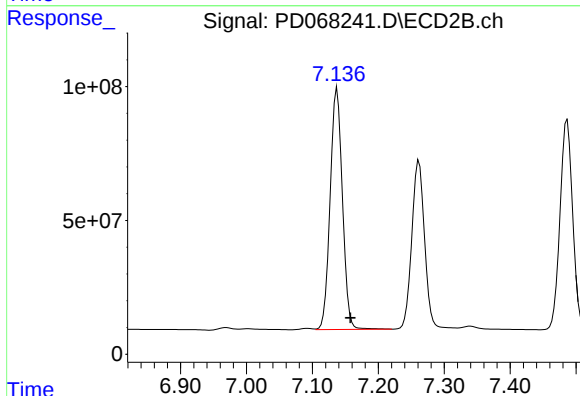


#15 Endosulfan II

R.T.: 7.137 min
Delta R.T.: -0.020 min
Response: 1163751926
Conc: 157.70 ng/ml

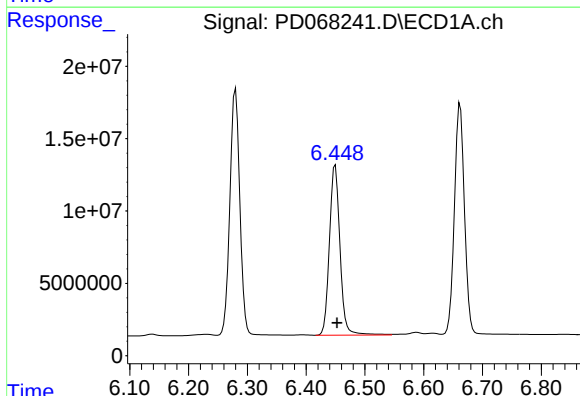


#18 Endrin aldehyde

R.T.: 6.450 min
Delta R.T.: -0.003 min
Response: 147202430
Conc: 175.47 ng/ml

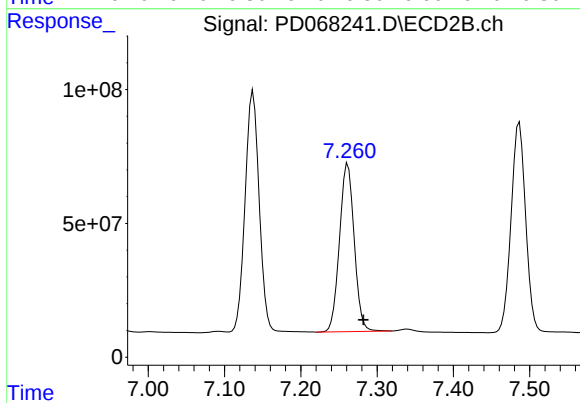

#18 Endrin aldehyde


R.T.: 7.262 min
Delta R.T.: -0.021 min
Response: 839490200
Conc: 156.24 ng/ml

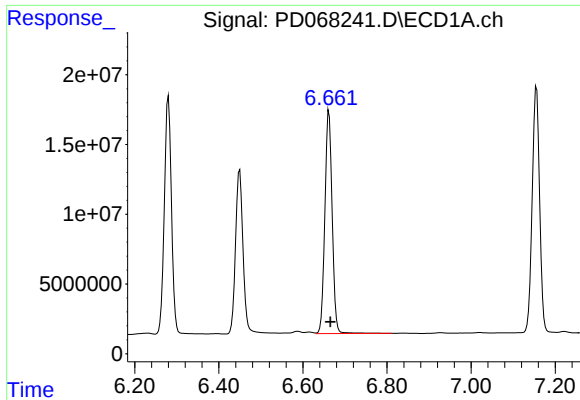

#19 Endosulfan Sulfate


R.T.: 6.662 min
Delta R.T.: -0.003 min
Response: 191789391
Conc: 182.42 ng/ml

Instrument :
ECD_D
ClientSampleId :

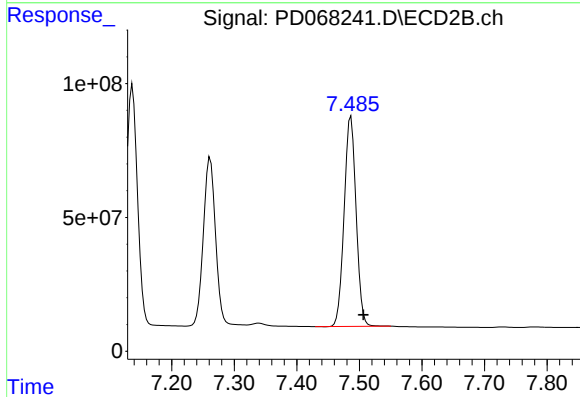


#19 Endosulfan Sulfate

R.T.: 7.487 min
Delta R.T.: -0.020 min
Response: 1044777587
Conc: 157.14 ng/ml

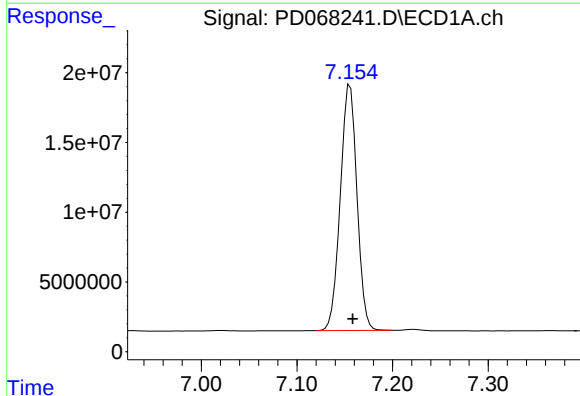


#21 Endrin ketone

R.T.: 7.156 min
Delta R.T.: -0.003 min
Response: 214356149
Conc: 180.22 ng/ml

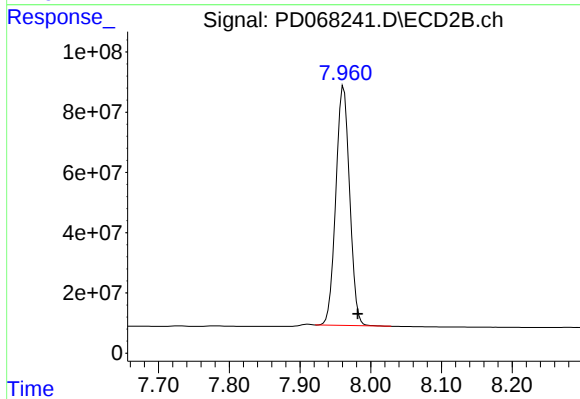

#21 Endrin ketone

R.T.: 7.962 min
Delta R.T.: -0.020 min
Response: 1078139994
Conc: 156.47 ng/ml

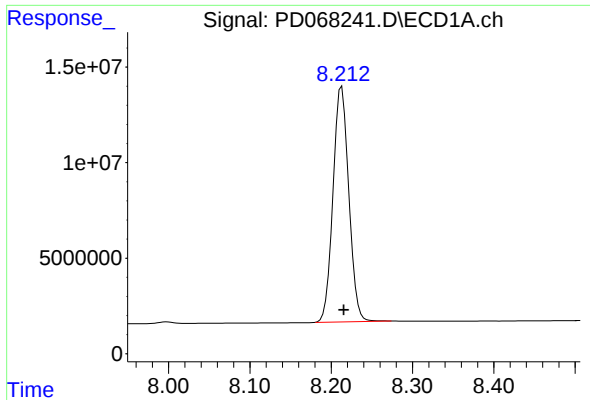

#27 Decachlorobiphenyl


R.T.: 8.213 min

Delta R.T.: -0.003 min

Response: 166638446

Conc: 154.62 ng/ml

Instrument :
ECD_D
ClientSampleId :

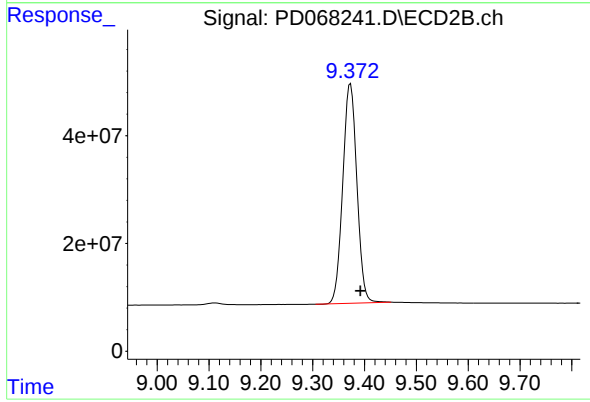

#27 Decachlorobiphenyl

R.T.: 9.373 min

Delta R.T.: -0.019 min

Response: 772872298

Conc: 143.19 ng/ml