

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031522\
 Data File : PD0684621.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Mar 2022 18:15
 Operator : AR\AJ
 Sample : N1883-03
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 16 06:34:17 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031322CLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Mar 14 07:24:04 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.449	4.175	16100337	134.7E6	11.823	12.308
27)	SA Decachlor...	8.210	9.372	27346973	130.3E6	19.666	20.662
Target Compounds							
2)	A alpha-BHC	0.000	4.599f	0	1967973	N.D.	0.126
3)	MA gamma-BHC...	0.000	4.827f	0	423648	N.D.	<MDL
4)	MA Heptachlor	4.436f	5.387	828708	1109468	0.463	<MDL #
5)	MB Aldrin	0.000	5.744f	0	107181	N.D.	<MDL
6)	B beta-BHC	4.436	5.001	828708	1243719	0.994	0.195 #
7)	B delta-BHC	0.000	5.228	0	5992410	N.D.	0.423
8)	B Heptachlo...	0.000	6.075	0	2223070	N.D.	0.185
9)	A Endosulfan I	0.000	6.401f	0	1611999	N.D.	0.148
10)	B trans-Chl...	0.000	6.326	0	2312580	N.D.	0.194
11)	B cis-Chlor...	0.000	6.401	0	1611999	N.D.	0.141
13)	MA Dieldrin	0.000	6.713	0	3099851	N.D.	0.279
14)	MA Endrin	0.000	7.000f	0	143169	N.D.	<MDL
15)	B Endosulfa...	6.227f	7.140	1122168	1844271	0.774	0.206 #
16)	A 4,4'-DDD	0.000	7.000f	0	143169	N.D.	<MDL
23)	Toxaphene-2	6.227f	0.000	1122168	0	104.638	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031522\
Data File : PD0684621.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Mar 2022 18:15
Operator : AR\AJ
Sample : N1883-03
Misc :
ALS Vial : 14 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 16 06:34:17 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031322CLP.M
Quant Title : GC Extractables
QLast Update : Mon Mar 14 07:24:04 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

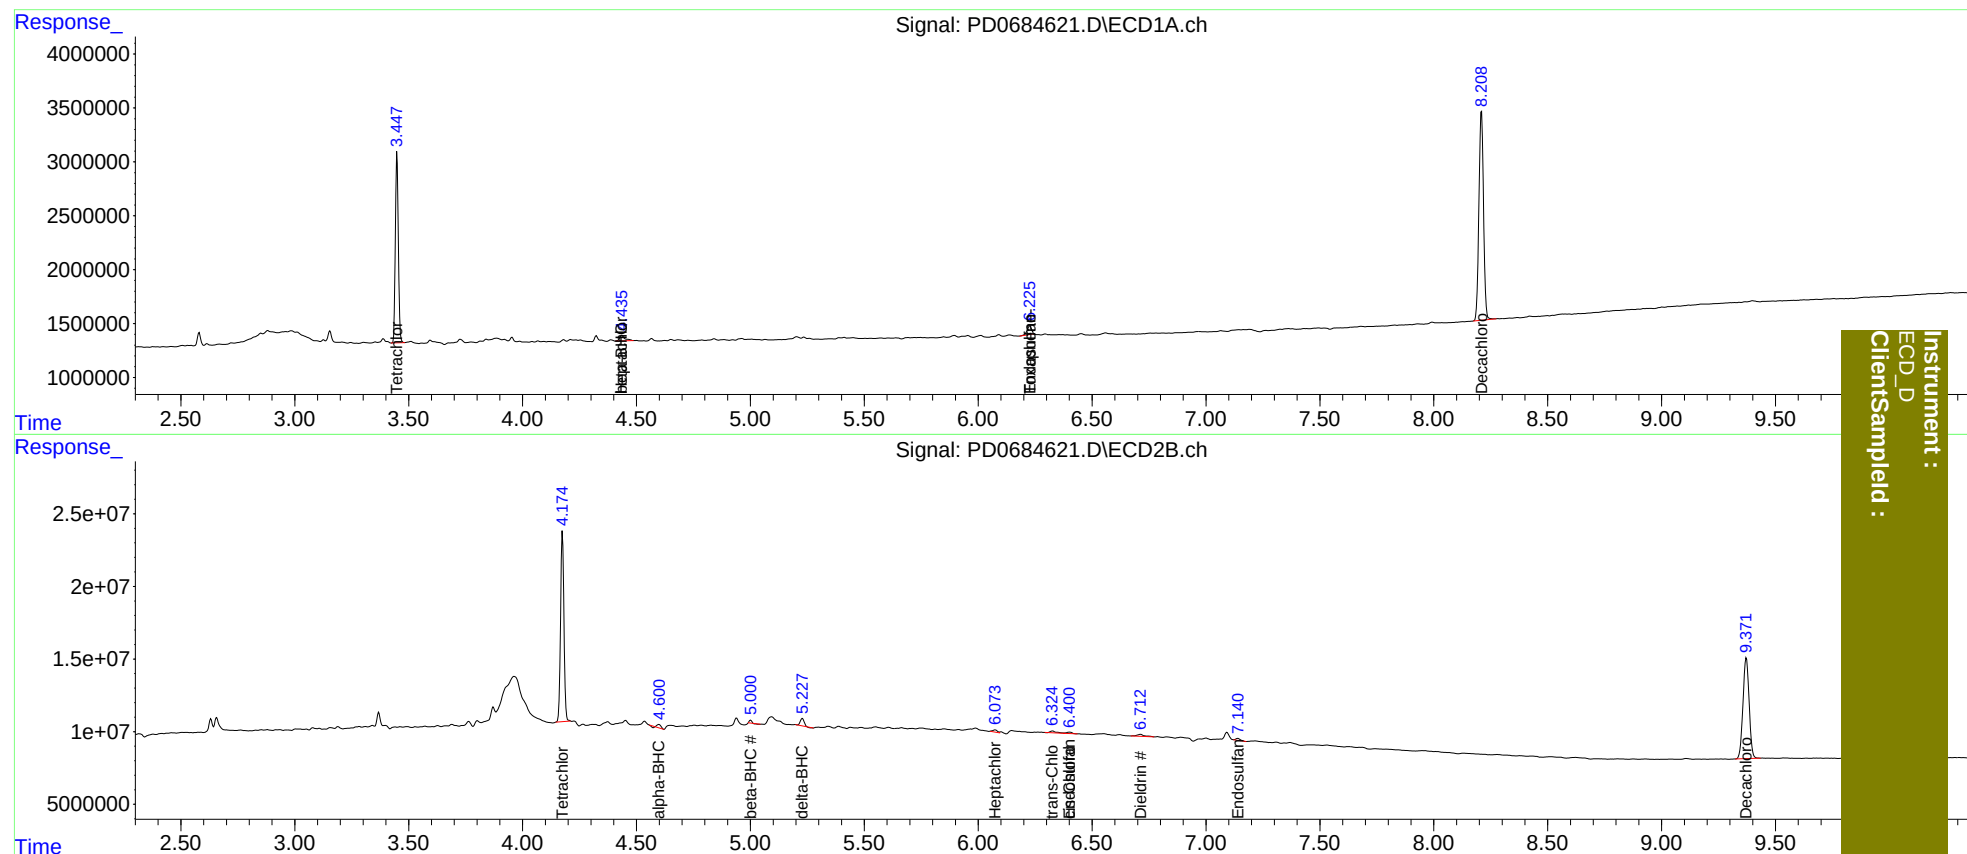


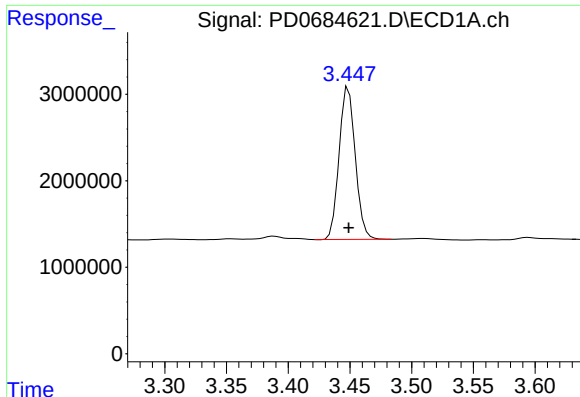

#1 Tetrachloro-m-xylene


R.T.: 3.449 min
Delta R.T.: 0.000 min
Response: 16100337
Conc: 11.82 ng/ml

Instrument :
ECD_D
ClientSampleId :

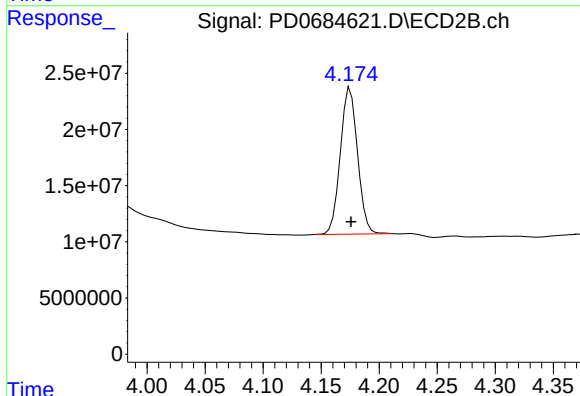


#1 Tetrachloro-m-xylene

R.T.: 4.175 min
Delta R.T.: 0.000 min
Response: 134719801
Conc: 12.31 ng/ml

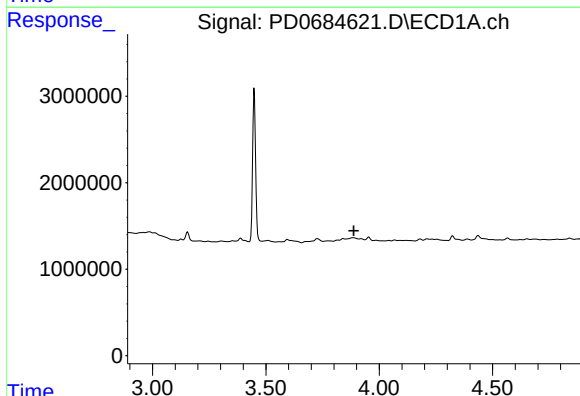


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 3.888 min
Response: 0
Conc: N.D.

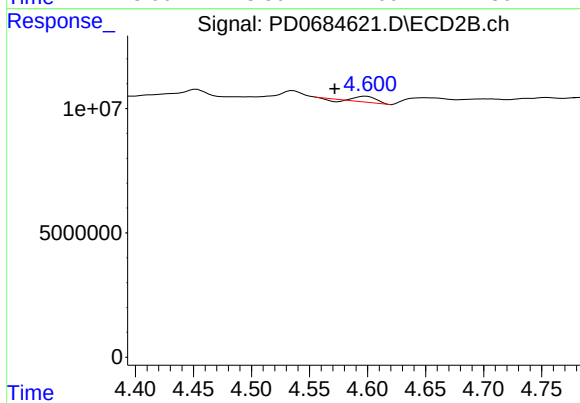

#2 alpha-BHC


R.T.: 4.599 min
Delta R.T.: 0.027 min
Response: 1967973
Conc: 0.13 ng/ml

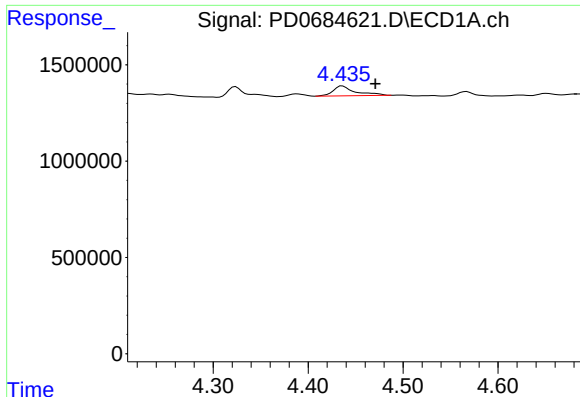

#4 Heptachlor


R.T.: 4.436 min
Delta R.T.: -0.035 min
Response: 828708
Conc: 0.46 ng/ml

Instrument :
ECD_D
ClientSampleId :

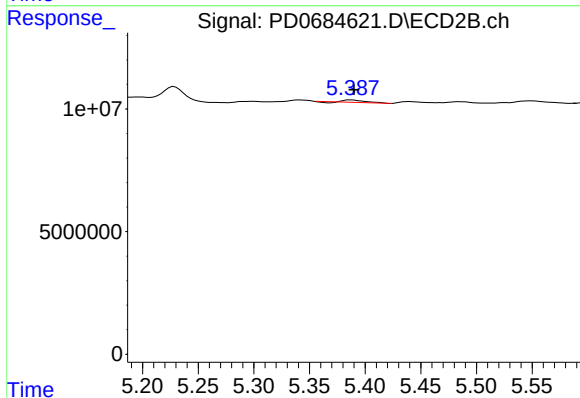


#4 Heptachlor

R.T.: 5.387 min
Delta R.T.: -0.003 min
Response: 1109468
Conc: N.D.

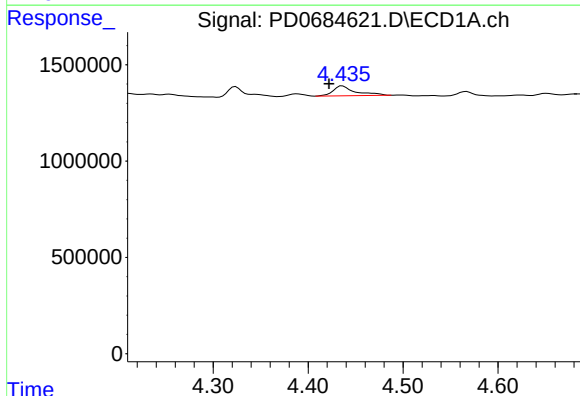


#6 beta-BHC

R.T.: 4.436 min
Delta R.T.: 0.014 min
Response: 828708
Conc: 0.99 ng/ml

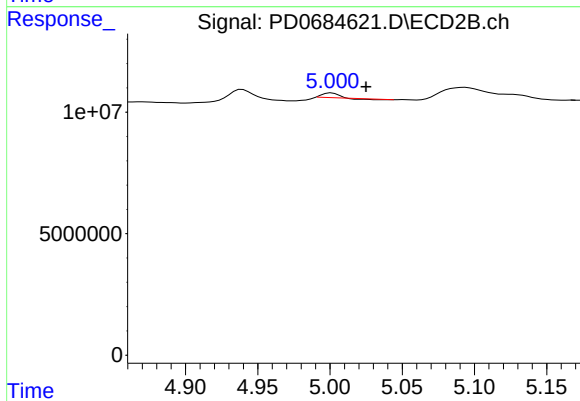

#6 beta-BHC


R.T.: 5.001 min
Delta R.T.: -0.024 min
Response: 1243719
Conc: 0.19 ng/ml

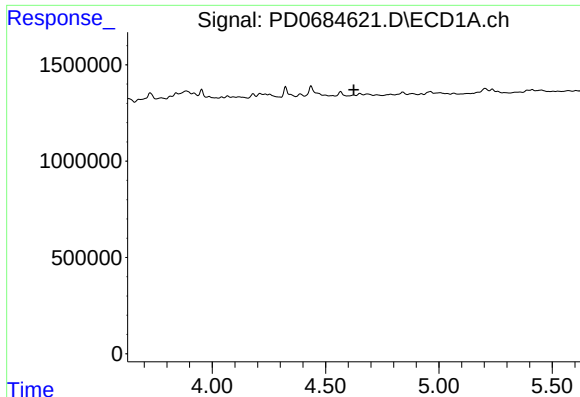

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 4.625 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

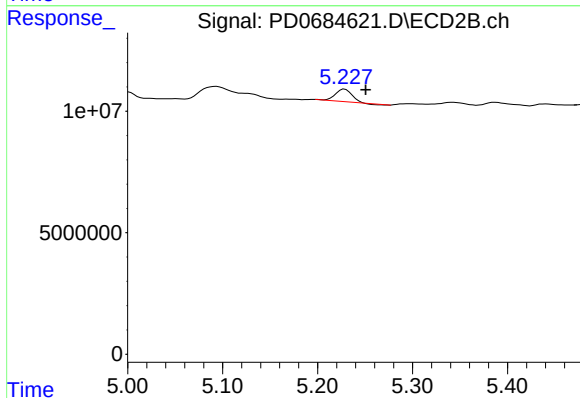


#7 delta-BHC

R.T.: 5.228 min
Delta R.T.: -0.022 min
Response: 5992410
Conc: 0.42 ng/ml

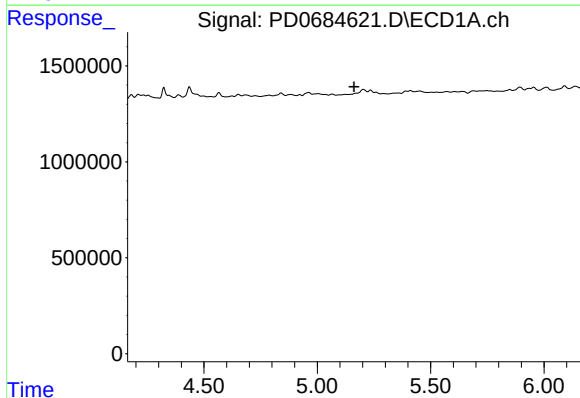


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T.: 5.163 min
Response: 0
Conc: N.D.

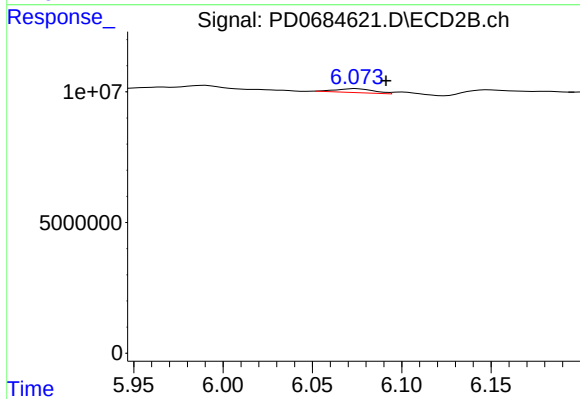

#8 Heptachlor epoxide


R.T.: 6.075 min
Delta R.T.: -0.017 min
Response: 2223070
Conc: 0.18 ng/ml

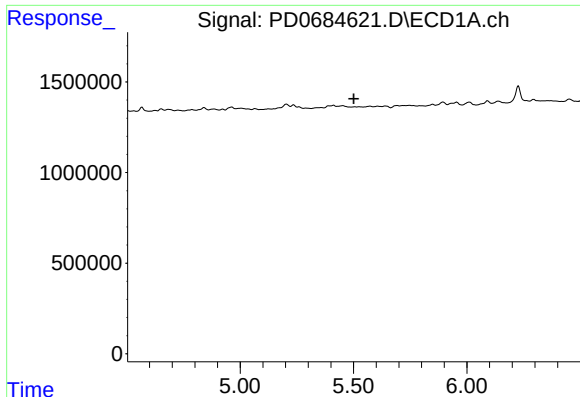

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 5.502 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

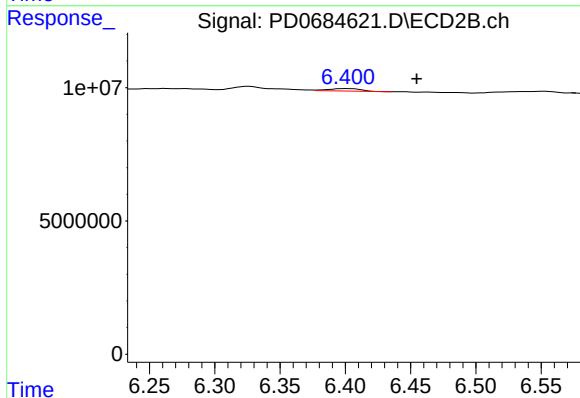


#9 Endosulfan I

R.T.: 6.401 min
Delta R.T.: -0.053 min
Response: 1611999
Conc: 0.15 ng/ml

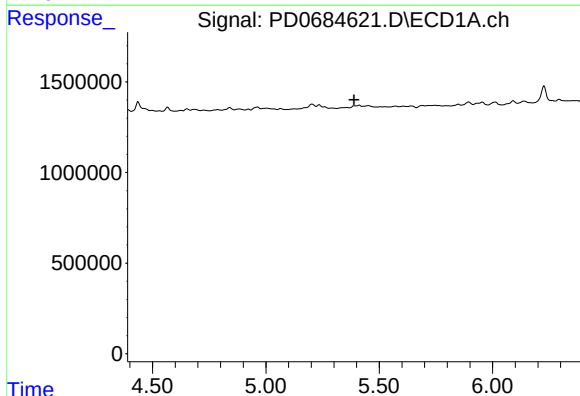


#10 trans-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.389 min
Response: 0
Conc: N.D.

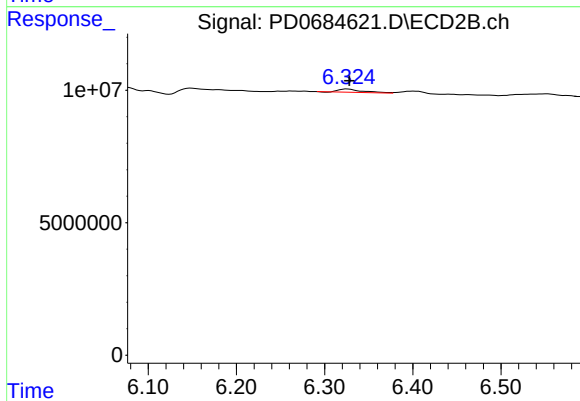

#10 trans-Chlordane


R.T.: 6.326 min
Delta R.T.: -0.002 min
Response: 2312580
Conc: 0.19 ng/ml

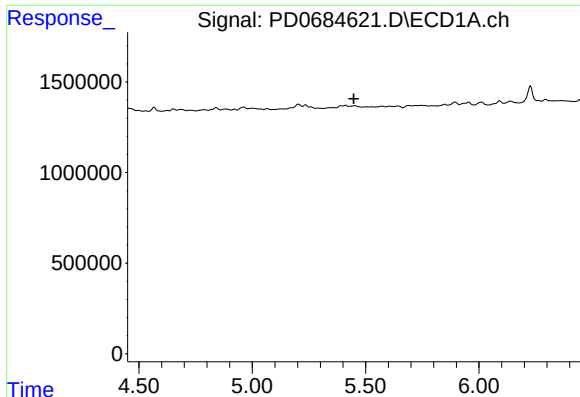

#11 cis-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.448 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

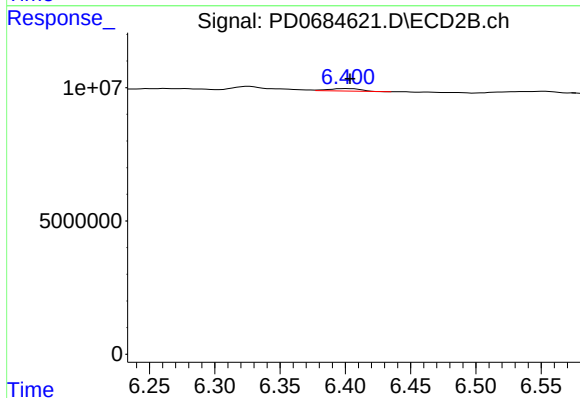


#11 cis-Chlordane

R.T.: 6.401 min
Delta R.T.: -0.002 min
Response: 1611999
Conc: 0.14 ng/ml

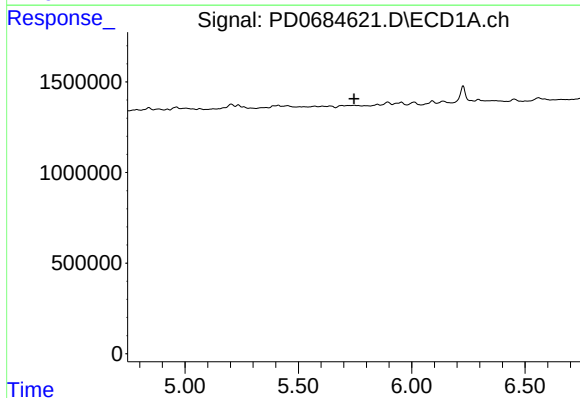


#13 Dieldrin

R.T.: 0.000 min
Exp R.T.: 5.746 min
Response: 0
Conc: N.D.

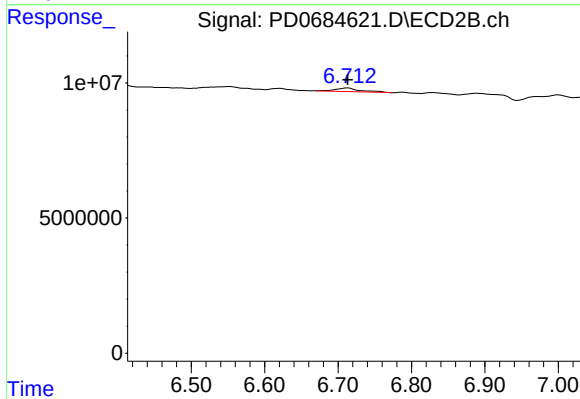

#13 Dieldrin


R.T.: 6.713 min
Delta R.T.: 0.000 min
Response: 3099851
Conc: 0.28 ng/ml

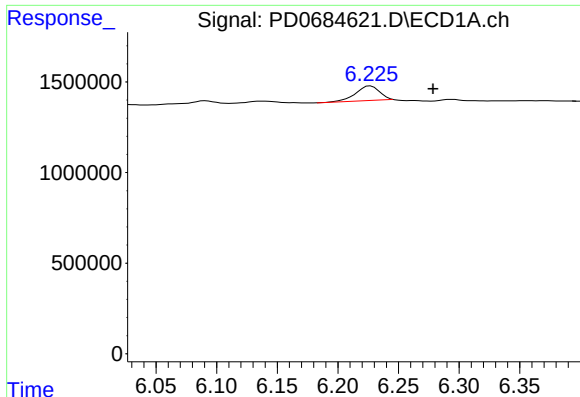

#15 Endosulfan II


R.T.: 6.227 min
Delta R.T.: -0.052 min
Response: 1122168
Conc: 0.77 ng/ml

Instrument :
ECD_D
ClientSampleId :

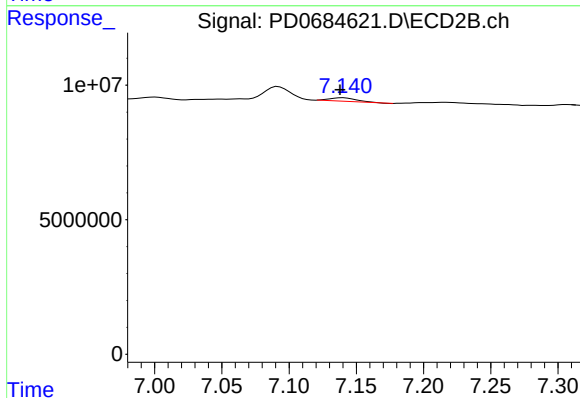


#15 Endosulfan II

R.T.: 7.140 min
Delta R.T.: 0.002 min
Response: 1844271
Conc: 0.21 ng/ml

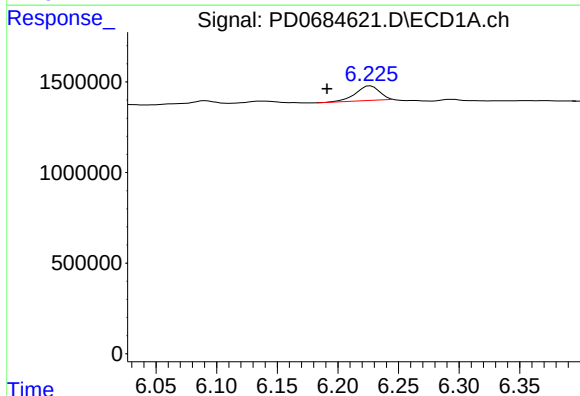


#23 Toxaphene-2

R.T.: 6.227 min
Delta R.T.: 0.036 min
Response: 1122168
Conc: 104.64 ng/ml

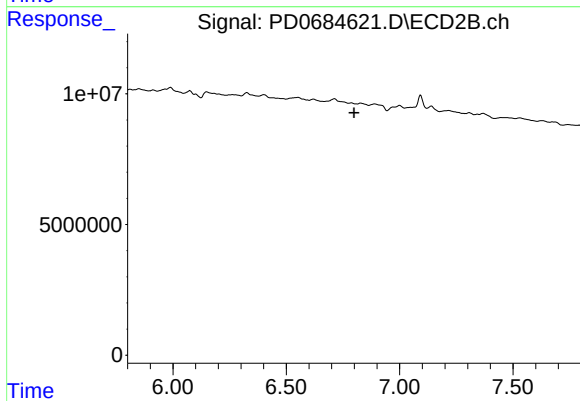

#23 Toxaphene-2


R.T.: 0.000 min
Exp R.T.: 6.799 min
Response: 0
Conc: N.D.

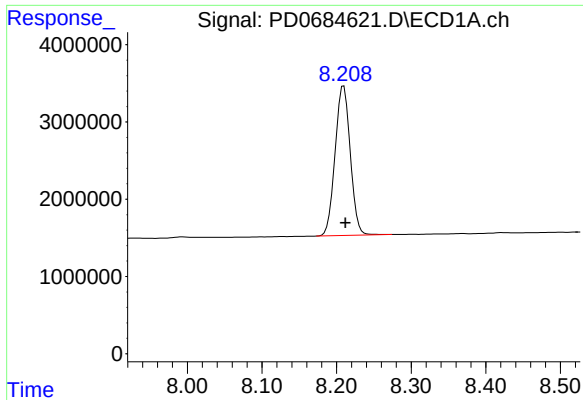

#27 Decachlorobiphenyl

R.T.: 8.210 min
Delta R.T.: -0.002 min
Response: 27346973
Conc: 19.67 ng/ml

Instrument :
ECD_D
ClientSampleId :

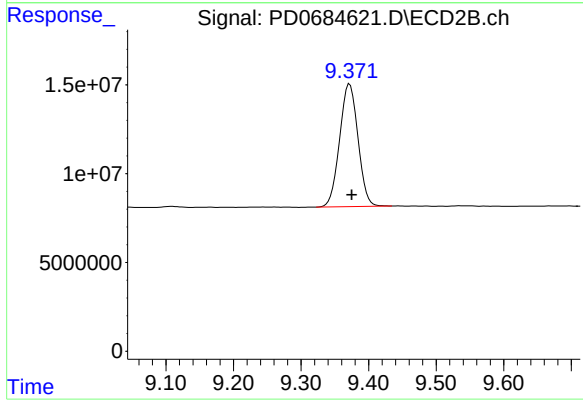

#27 Decachlorobiphenyl

R.T.: 9.372 min
Delta R.T.: -0.003 min
Response: 130315538
Conc: 20.66 ng/ml