

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031522\
 Data File : PD0684622.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Mar 2022 18:29
 Operator : AR\AJ
 Sample : N1883-04
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 16 06:34:37 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031322CLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Mar 14 07:24:04 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.449	4.175	16444985	135.6E6	12.076	12.388
27)	SA Decachlor...	8.209	9.371	29662824	141.5E6	21.332	22.442
Target Compounds							
2)	A alpha-BHC	0.000	4.600f	0	3052179	N.D.	0.195
3)	MA gamma-BHC...	0.000	4.824f	0	571967	N.D.	<MDL
4)	MA Heptachlor	0.000	5.388	0	350702	N.D.	<MDL
6)	B beta-BHC	0.000	5.003	0	3198058	N.D.	0.501
7)	B delta-BHC	0.000	5.228	0	6489667	N.D.	0.458
8)	B Heptachlo...	0.000	6.076	0	2681112	N.D.	0.223
9)	A Endosulfan I	0.000	6.403f	0	1730865	N.D.	0.159
10)	B trans-Chl...	0.000	6.324	0	1490422	N.D.	0.125
11)	B cis-Chlor...	0.000	6.403	0	1730865	N.D.	0.151
13)	MA Dieldrin	0.000	6.710	0	1431790	N.D.	0.129
14)	MA Endrin	0.000	6.997f	0	384123	N.D.	<MDL
15)	B Endosulfa...	6.226f	7.140	1130713	1535978	0.780	0.172 #
16)	A 4,4'-DDD	0.000	6.997f	0	384123	N.D.	<MDL
23)	Toxaphene-2	6.226f	6.788	1130713	945817	105.435	9.394 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031522\
Data File : PD0684622.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Mar 2022 18:29
Operator : AR\AJ
Sample : N1883-04
Misc :
ALS Vial : 15 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 16 06:34:37 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031322CLP.M
Quant Title : GC Extractables
QLast Update : Mon Mar 14 07:24:04 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

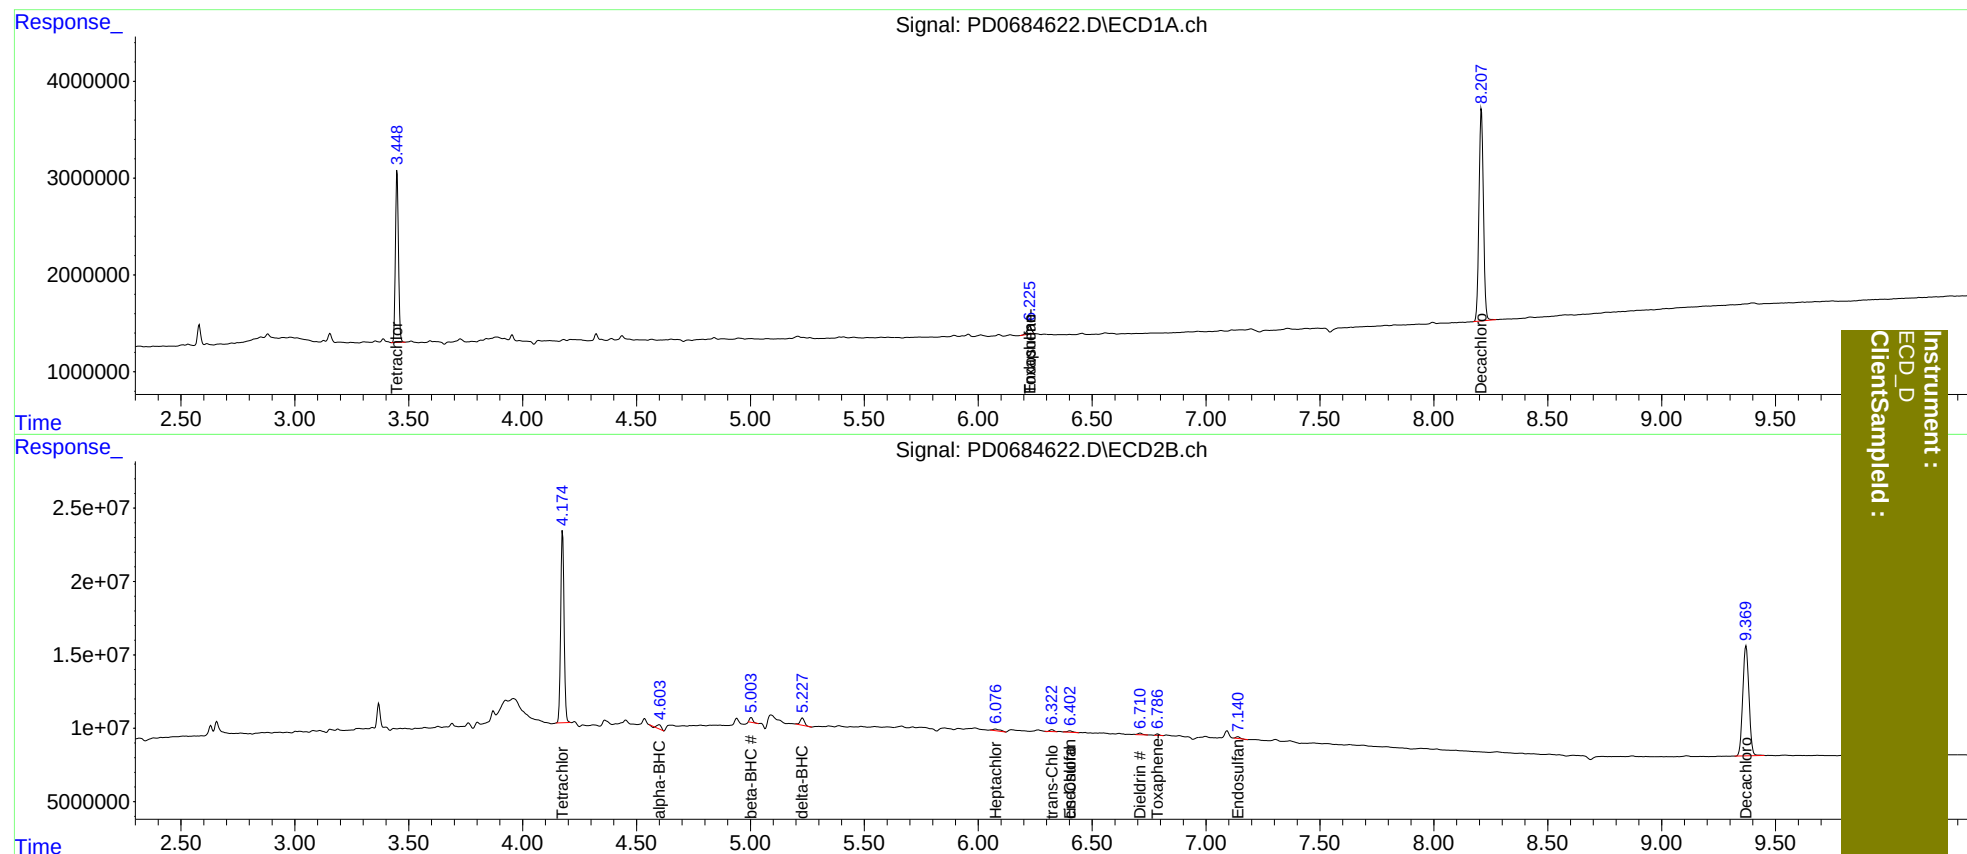


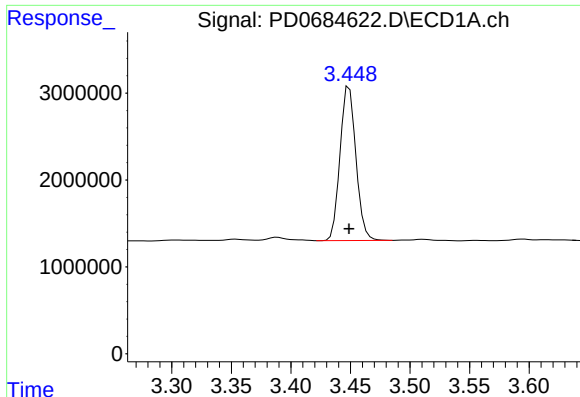

#1 Tetrachloro-m-xylene


R.T.: 3.449 min
Delta R.T.: 0.000 min
Response: 16444985
Conc: 12.08 ng/ml

Instrument :
ECD_D
ClientSampleId :

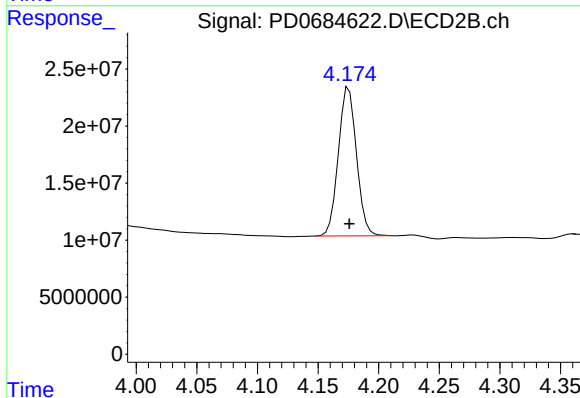


#1 Tetrachloro-m-xylene

R.T.: 4.175 min
Delta R.T.: 0.000 min
Response: 135590265
Conc: 12.39 ng/ml

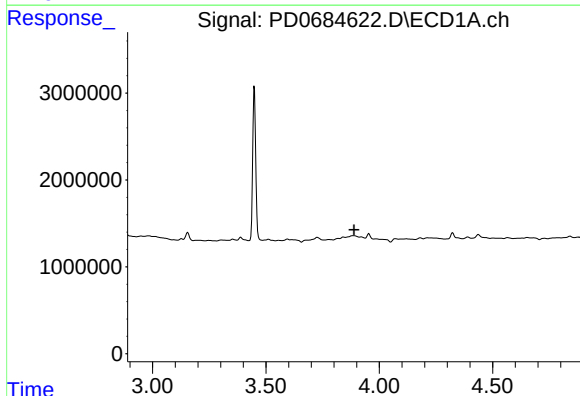


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 3.888 min
Response: 0
Conc: N.D.

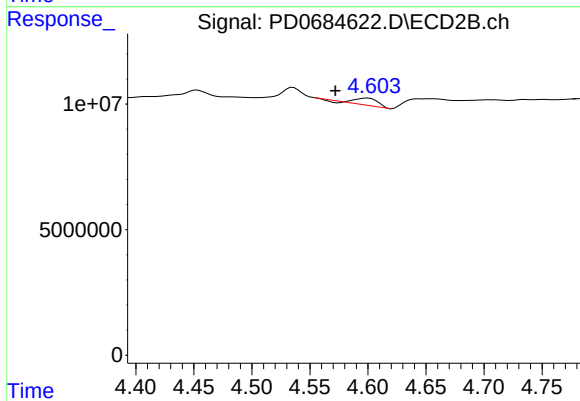

#2 alpha-BHC


R.T.: 4.600 min
Delta R.T.: 0.028 min
Response: 3052179
Conc: 0.20 ng/ml

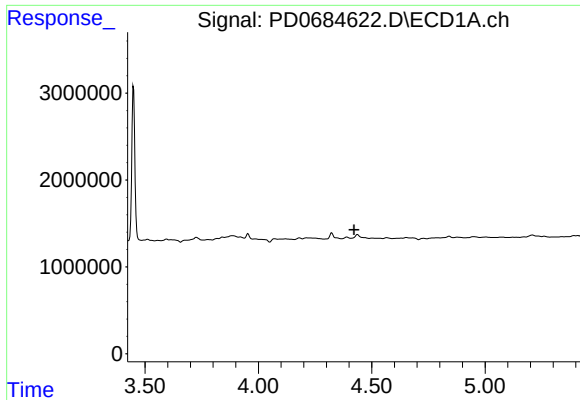

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 4.422 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

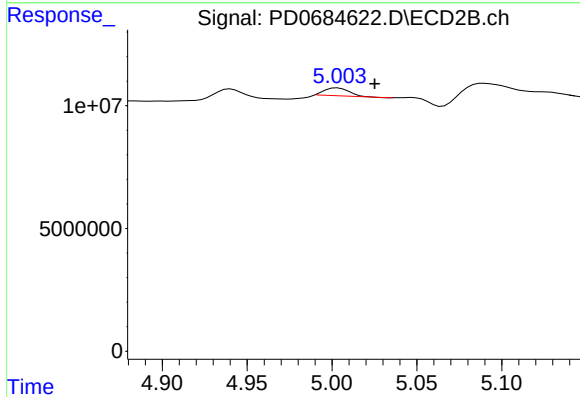


#6 beta-BHC

R.T.: 5.003 min
Delta R.T.: -0.022 min
Response: 3198058
Conc: 0.50 ng/ml

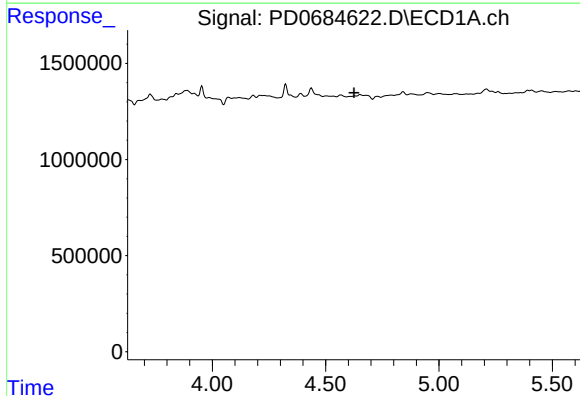


#7 delta-BHC

R.T.: 0.000 min
Exp R.T.: 4.625 min
Response: 0
Conc: N.D.

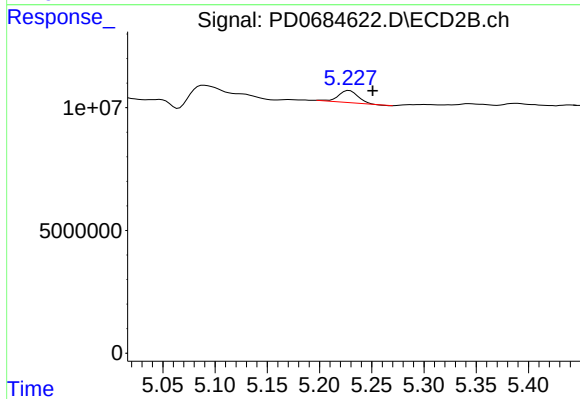

#7 delta-BHC


R.T.: 5.228 min
Delta R.T.: -0.022 min
Response: 6489667
Conc: 0.46 ng/ml

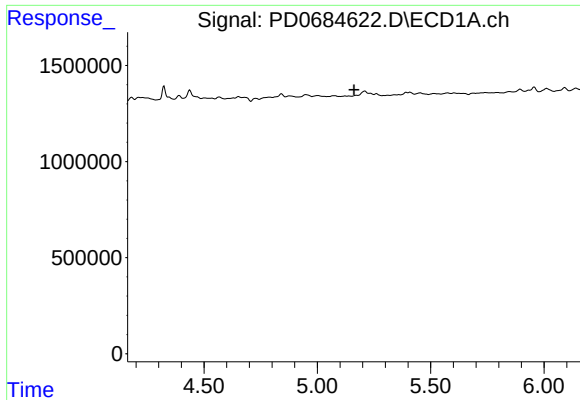

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 5.163 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

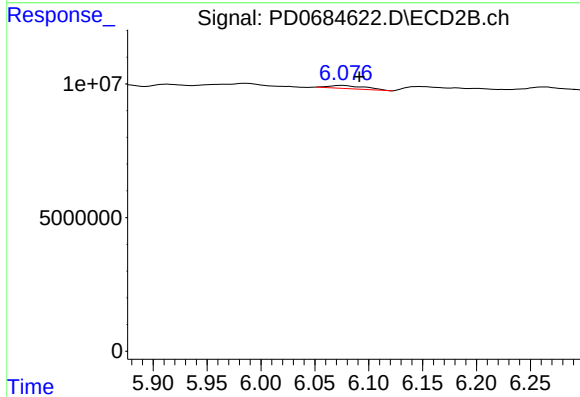


#8 Heptachlor epoxide

R.T.: 6.076 min
Delta R.T.: -0.015 min
Response: 2681112
Conc: 0.22 ng/ml

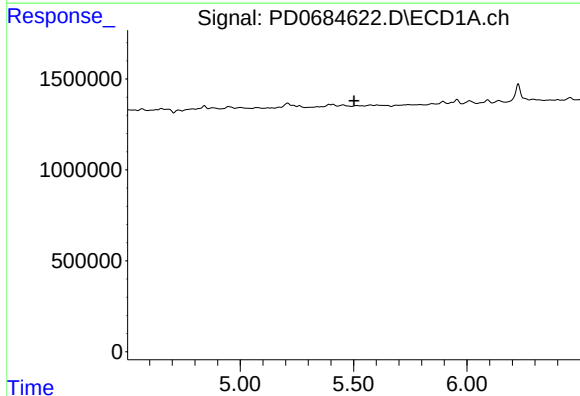


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T.: 5.502 min
Response: 0
Conc: N.D.

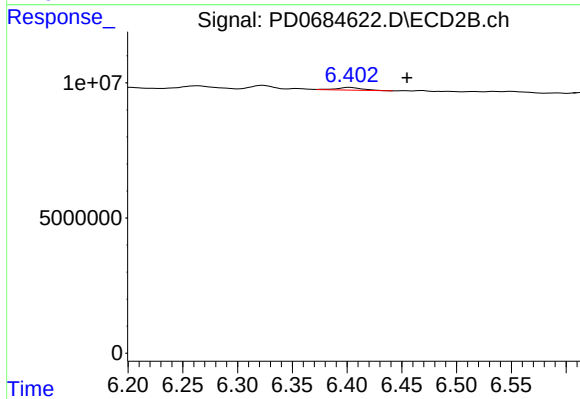

#9 Endosulfan I


R.T.: 6.403 min
Delta R.T.: -0.052 min
Response: 1730865
Conc: 0.16 ng/ml

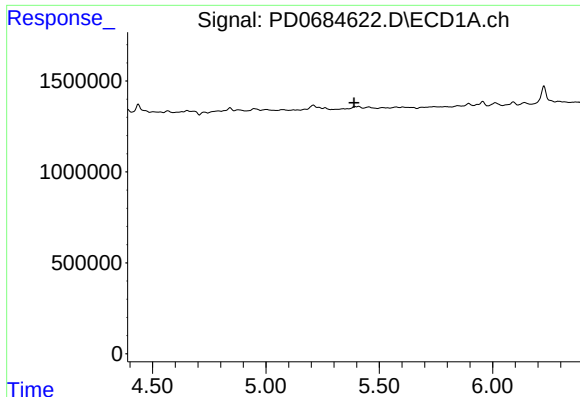

#10 trans-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.389 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

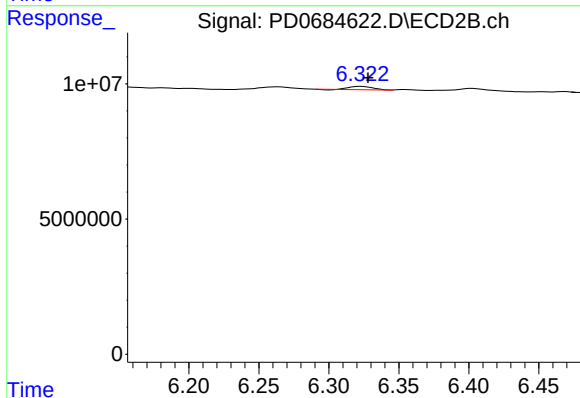


#10 trans-Chlordane

R.T.: 6.324 min
Delta R.T.: -0.004 min
Response: 1490422
Conc: 0.13 ng/ml

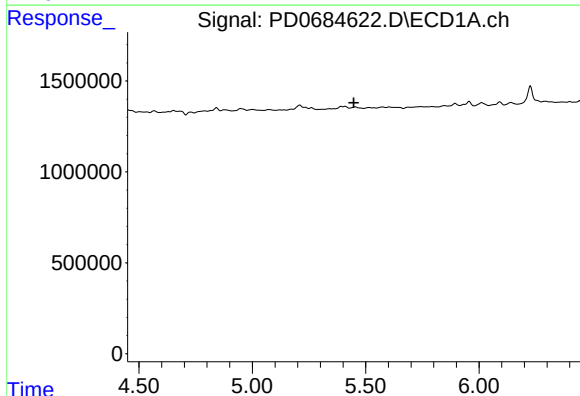


#11 cis-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.448 min
Response: 0
Conc: N.D.

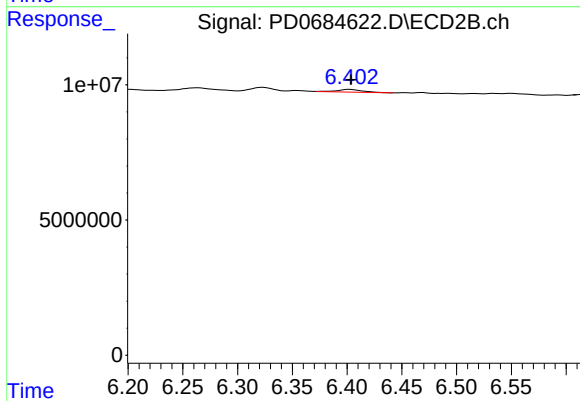

#11 cis-Chlordane


R.T.: 6.403 min
Delta R.T.: 0.000 min
Response: 1730865
Conc: 0.15 ng/ml

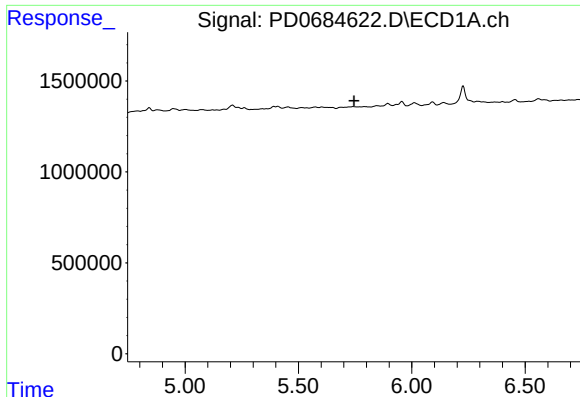

#13 Dieldrin


R.T.: 0.000 min
Exp R.T.: 5.746 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

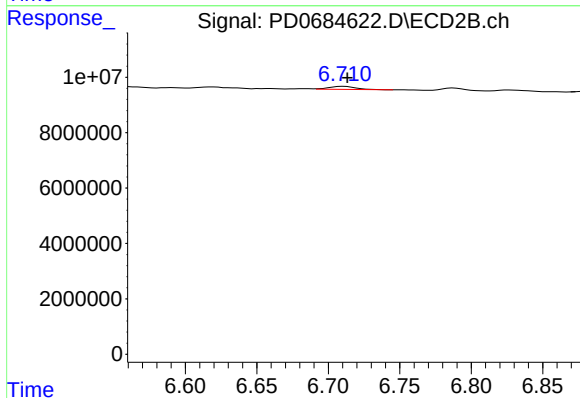


#13 Dieldrin

R.T.: 6.710 min
Delta R.T.: -0.003 min
Response: 1431790
Conc: 0.13 ng/ml

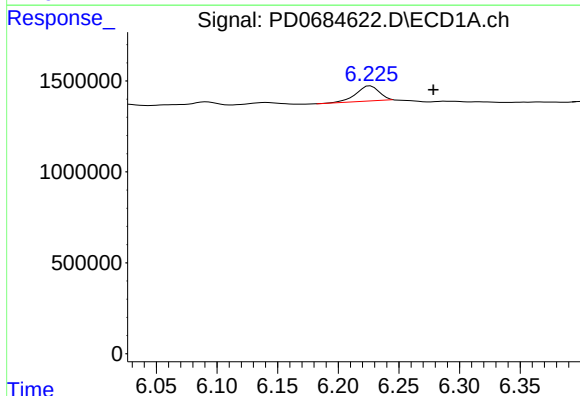


#15 Endosulfan II

R.T.: 6.226 min
Delta R.T.: -0.052 min
Response: 1130713
Conc: 0.78 ng/ml

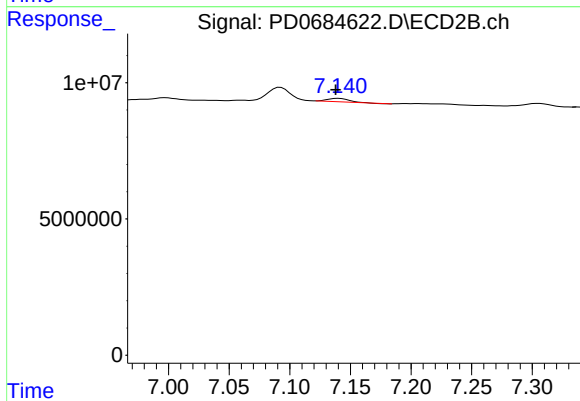

#15 Endosulfan II


R.T.: 7.140 min
Delta R.T.: 0.002 min
Response: 1535978
Conc: 0.17 ng/ml

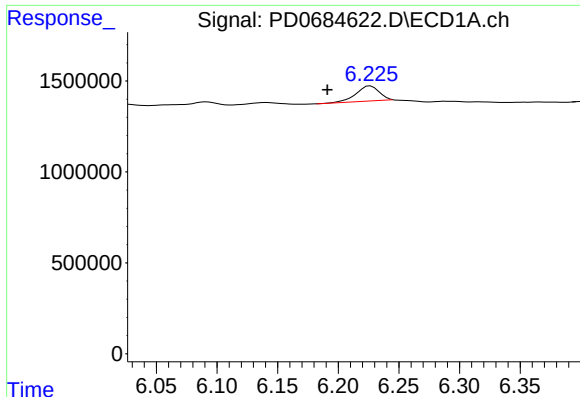

#23 Toxaphene-2


R.T.: 6.226 min
Delta R.T.: 0.035 min
Response: 1130713
Conc: 105.43 ng/ml

Instrument :
ECD_D
ClientSampleId :

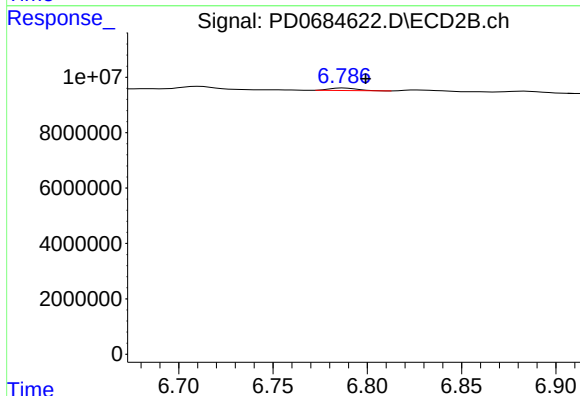


#23 Toxaphene-2

R.T.: 6.788 min
Delta R.T.: -0.011 min
Response: 945817
Conc: 9.39 ng/ml

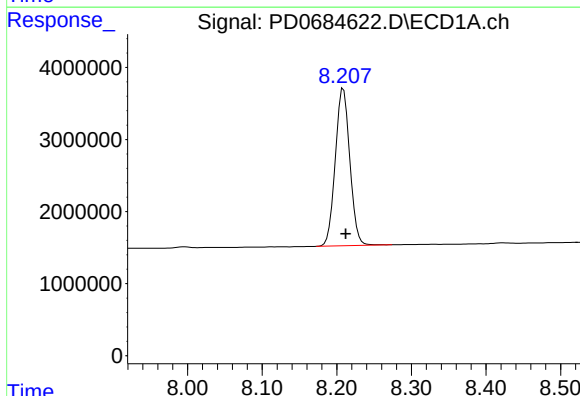

#27 Decachlorobiphenyl

R.T.: 8.209 min
Delta R.T.: -0.003 min
Response: 29662824
Conc: 21.33 ng/ml

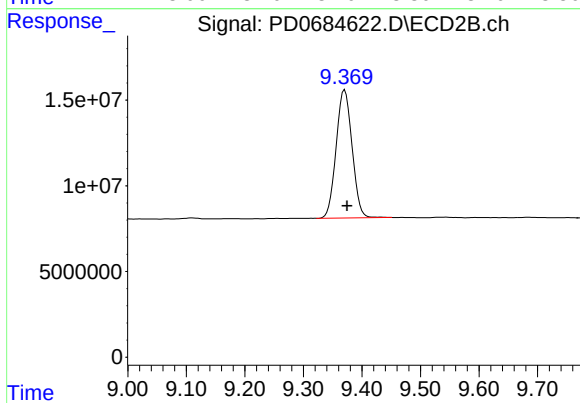

#27 Decachlorobiphenyl

R.T.: 9.371 min
Delta R.T.: -0.004 min
Response: 141543545
Conc: 22.44 ng/ml