

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031522\
 Data File : PD0684633.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Mar 2022 21:03
 Operator : AR\AJ
 Sample : N1883-15
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 16 06:38:15 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031322CLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Mar 14 07:24:04 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.449	4.175	17829412	148.1E6	13.093	13.530
27)	SA Decachlor...	8.208	9.371	36192531	169.2E6	26.027	26.823
Target Compounds							
2)	A alpha-BHC	0.000	4.599f	0	3057177	N.D.	0.196
3)	MA gamma-BHC...	0.000	4.822f	0	624602	N.D.	<MDL
4)	MA Heptachlor	4.436f	5.387	1082876	1121834	0.605	<MDL #
6)	B beta-BHC	4.436	5.002	1082876	7463713	1.299	1.169
7)	B delta-BHC	0.000	5.228	0	7935575	N.D.	0.561
8)	B Heptachlo...	0.000	6.070	0	2344870	N.D.	0.195
9)	A Endosulfan I	0.000	6.402f	0	1961142	N.D.	0.180
10)	B trans-Chl...	0.000	6.324	0	3343655	N.D.	0.281
11)	B cis-Chlor...	0.000	6.402	0	1961142	N.D.	0.171
13)	MA Dieldrin	0.000	6.710	0	2808033	N.D.	0.253
14)	MA Endrin	0.000	6.998f	0	388805	N.D.	<MDL
15)	B Endosulfa...	6.225f	7.138	1132404	1558135	0.781	0.174 #
16)	A 4,4'-DDD	0.000	6.998f	0	388805	N.D.	<MDL
21)	B Endrin ke...	0.000	7.944	0	534777	N.D.	<MDL
23)	Toxaphene-2	6.225	6.789	1132404	997203	105.593	9.905 #
26)	Toxaphene-5	0.000	7.944f	0	534777	N.D.	6.103


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031522\
Data File : PD0684633.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Mar 2022 21:03
Operator : AR\AJ
Sample : N1883-15
Misc :
ALS Vial : 26 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 16 06:38:15 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031322CLP.M
Quant Title : GC Extractables
QLast Update : Mon Mar 14 07:24:04 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

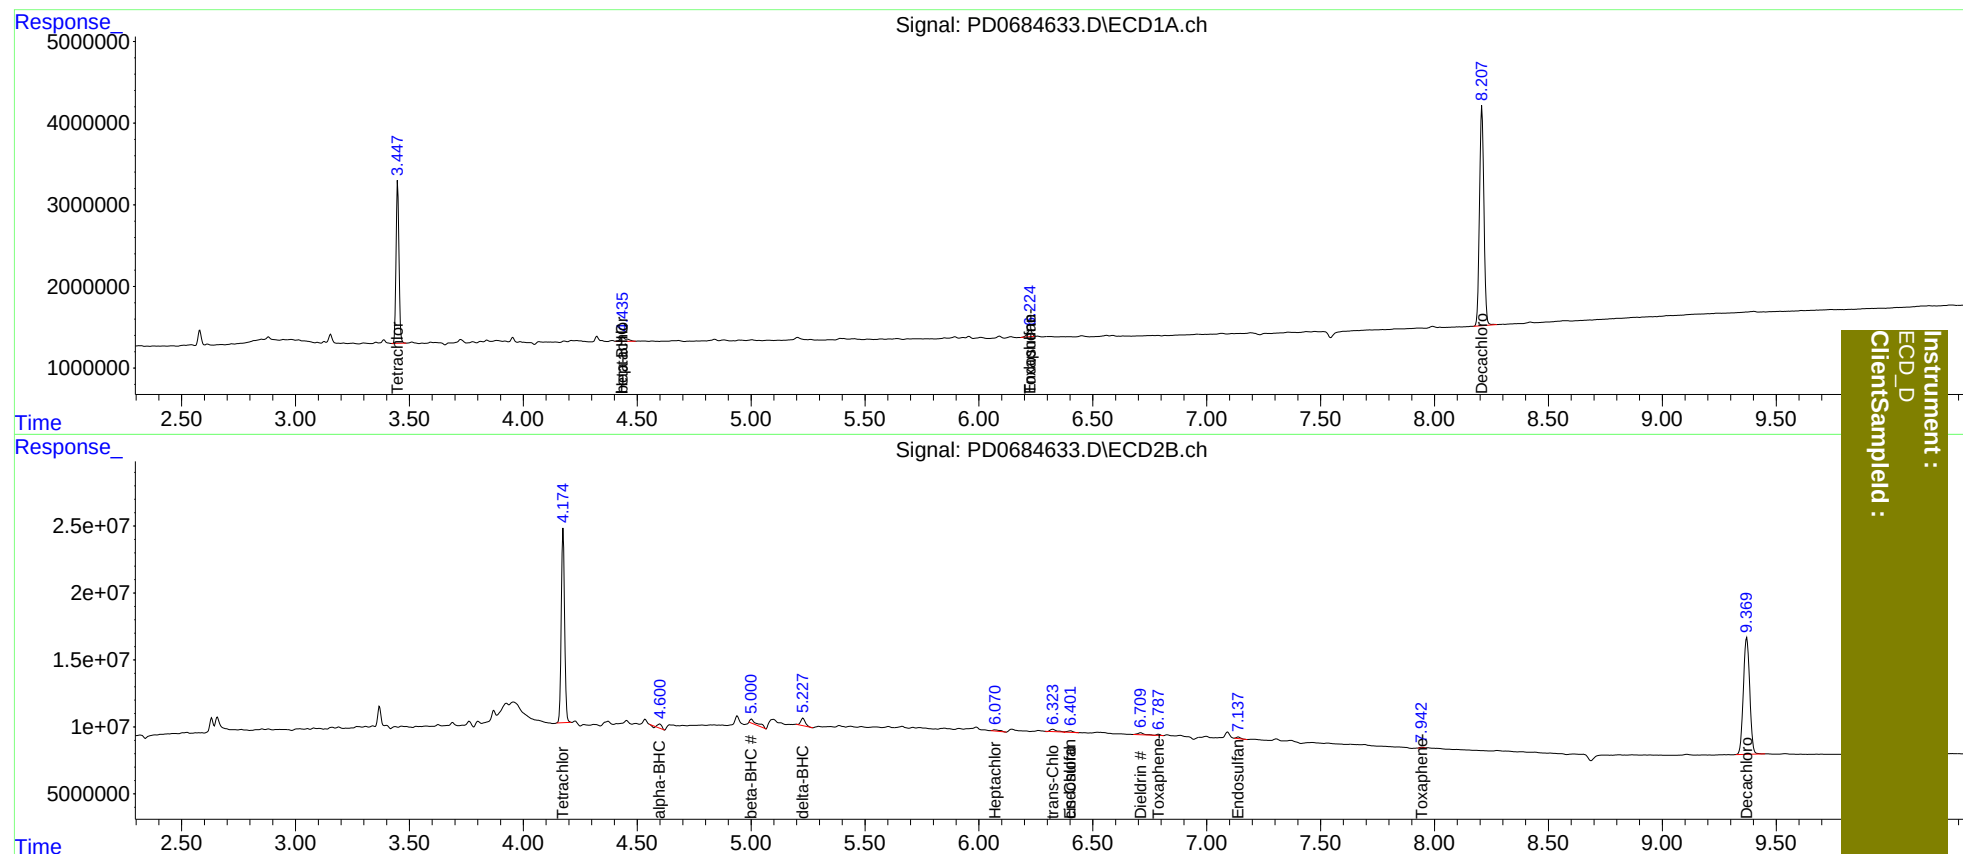


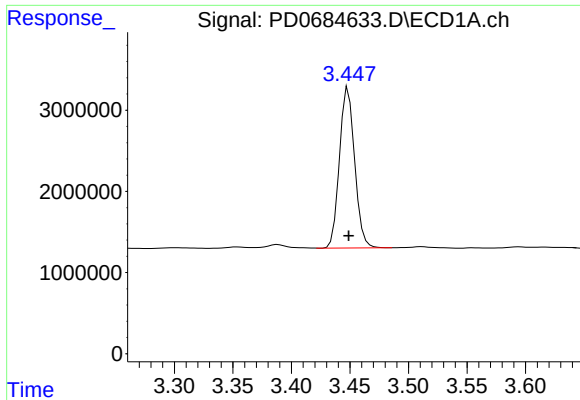

#1 Tetrachloro-m-xylene


R.T.: 3.449 min
Delta R.T.: 0.000 min
Response: 17829412
Conc: 13.09 ng/ml

Instrument :
ECD_D
ClientSampleId :

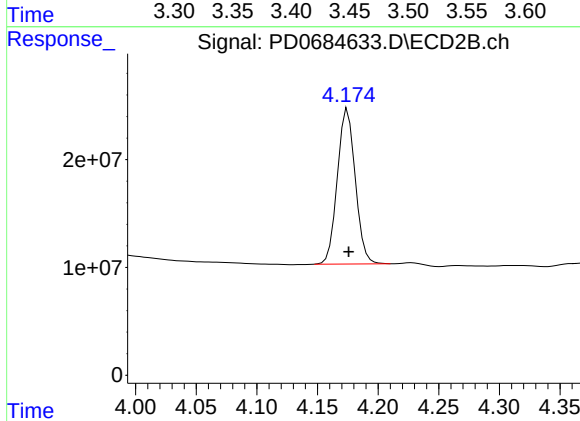


#1 Tetrachloro-m-xylene

R.T.: 4.175 min
Delta R.T.: 0.000 min
Response: 148091445
Conc: 13.53 ng/ml

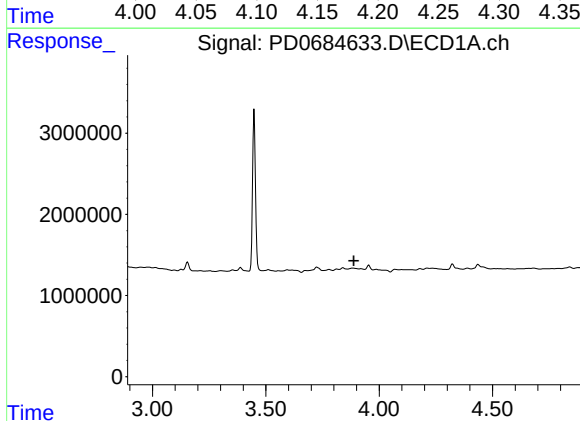


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 3.888 min
Response: 0
Conc: N.D.

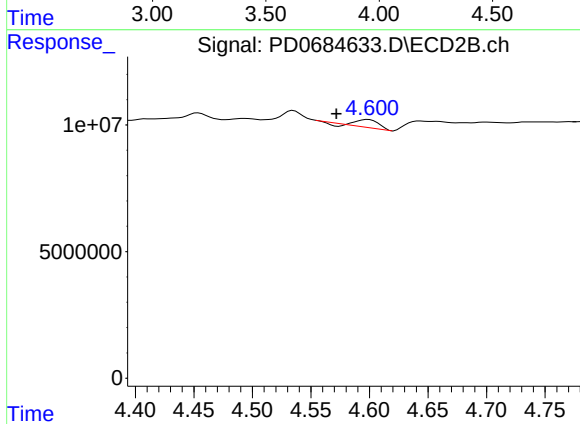

#2 alpha-BHC


R.T.: 4.599 min
Delta R.T.: 0.027 min
Response: 3057177
Conc: 0.20 ng/ml

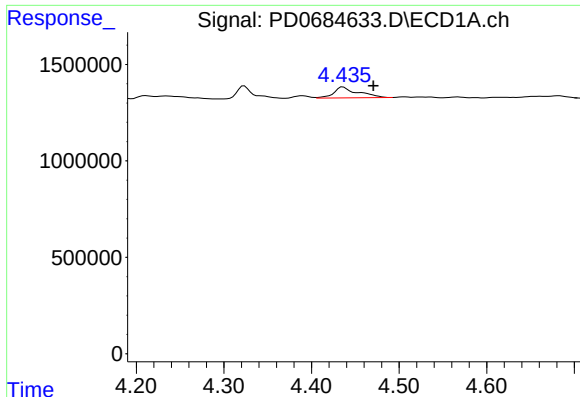

#4 Heptachlor


R.T.: 4.436 min
Delta R.T.: -0.035 min
Response: 1082876
Conc: 0.60 ng/ml

Instrument :
ECD_D
ClientSampleId :

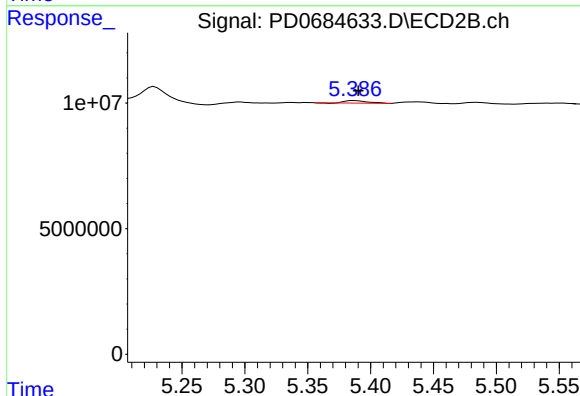


#4 Heptachlor

R.T.: 5.387 min
Delta R.T.: -0.003 min
Response: 1121834
Conc: N.D.

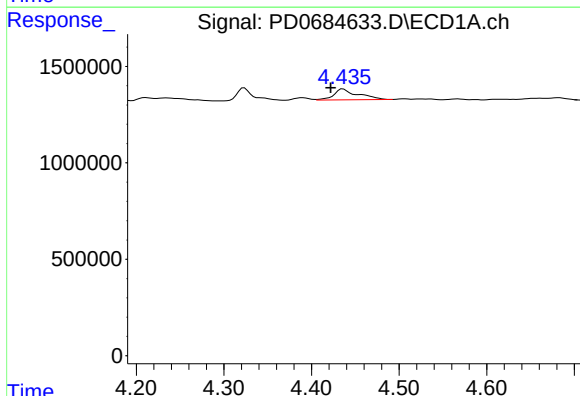


#6 beta-BHC

R.T.: 4.436 min
Delta R.T.: 0.014 min
Response: 1082876
Conc: 1.30 ng/ml

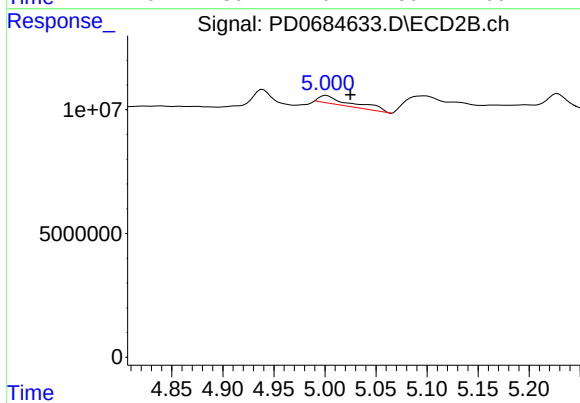

#6 beta-BHC


R.T.: 5.002 min
Delta R.T.: -0.023 min
Response: 7463713
Conc: 1.17 ng/ml

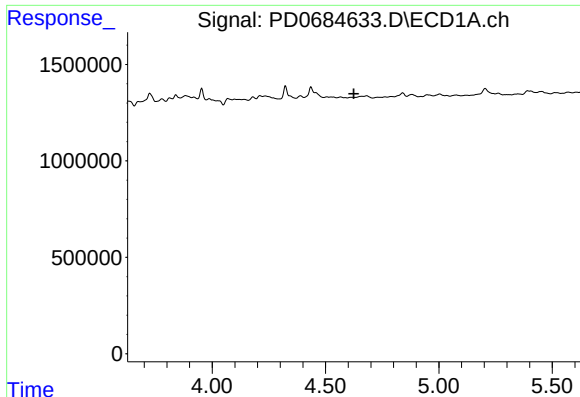

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 4.625 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

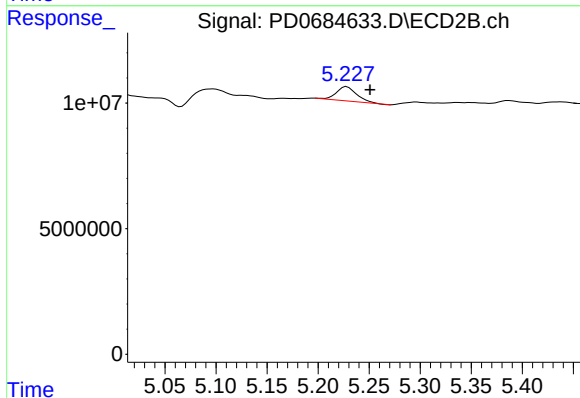


#7 delta-BHC

R.T.: 5.228 min
Delta R.T.: -0.023 min
Response: 7935575
Conc: 0.56 ng/ml

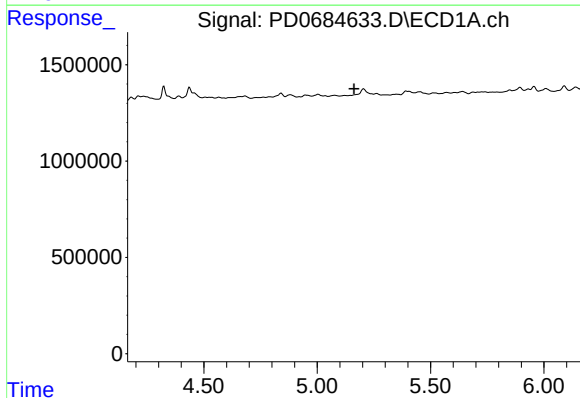


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.163 min
Response: 0
Conc: N.D.

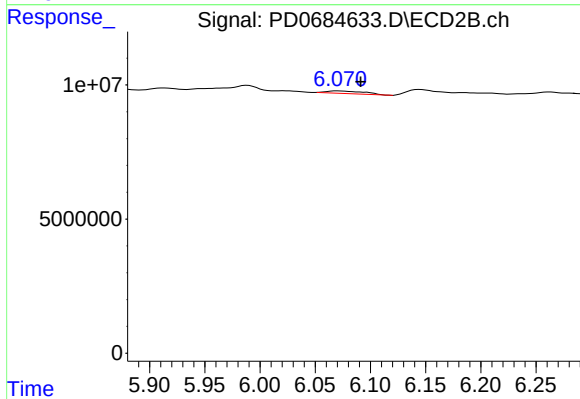

#8 Heptachlor epoxide


R.T.: 6.070 min
Delta R.T.: -0.021 min
Response: 2344870
Conc: 0.19 ng/ml

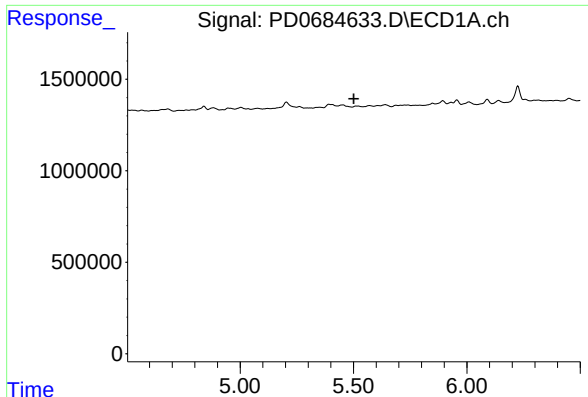

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 5.502 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

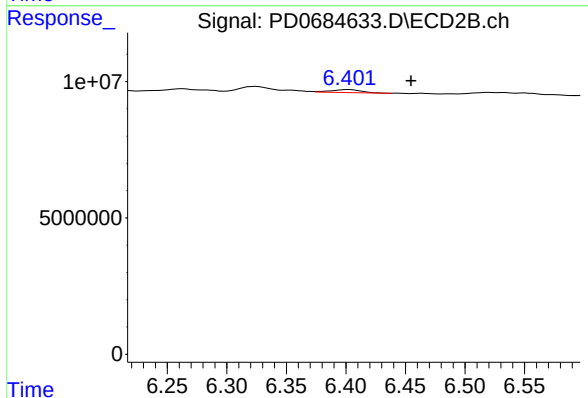


#9 Endosulfan I

R.T.: 6.402 min
Delta R.T.: -0.052 min
Response: 1961142
Conc: 0.18 ng/ml

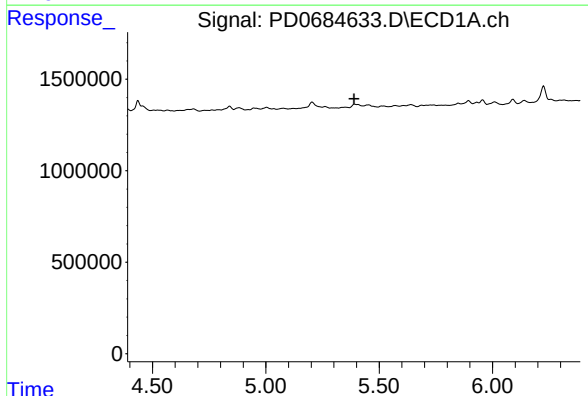


#10 trans-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.389 min
Response: 0
Conc: N.D.

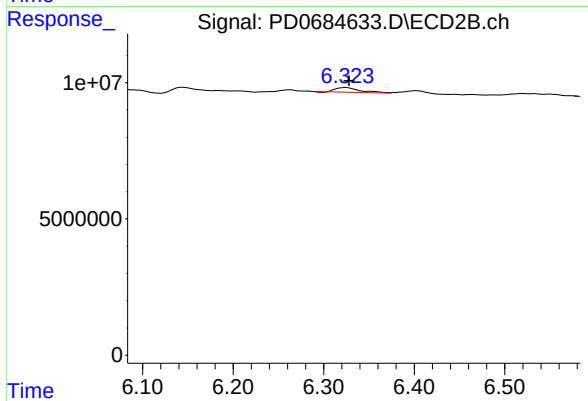

#10 trans-Chlordane


R.T.: 6.324 min
Delta R.T.: -0.004 min
Response: 3343655
Conc: 0.28 ng/ml

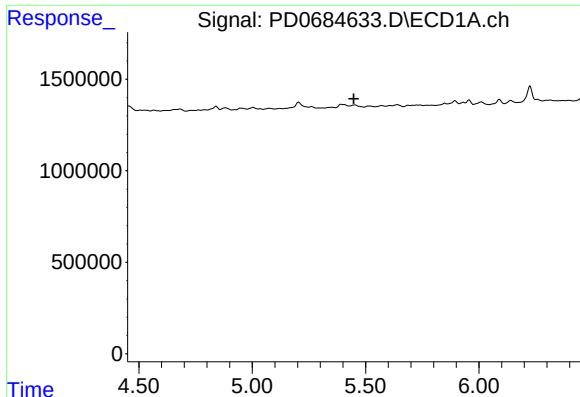

#11 cis-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.448 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

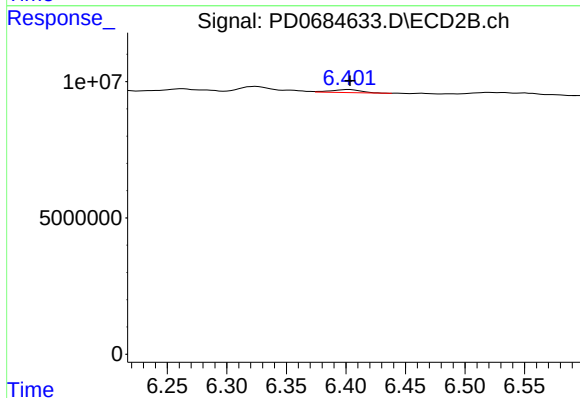


#11 cis-Chlordane

R.T.: 6.402 min
Delta R.T.: -0.001 min
Response: 1961142
Conc: 0.17 ng/ml

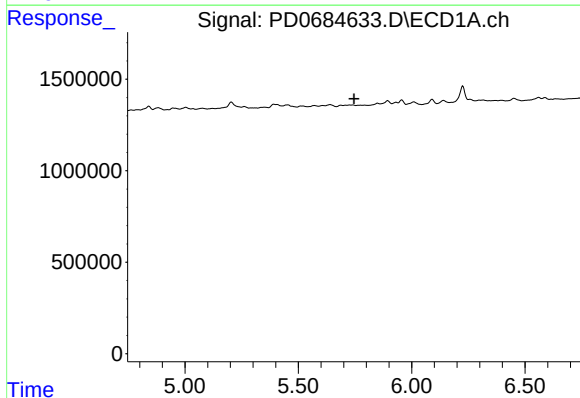


#13 Dieldrin

R.T.: 0.000 min
Exp R.T.: 5.746 min
Response: 0
Conc: N.D.

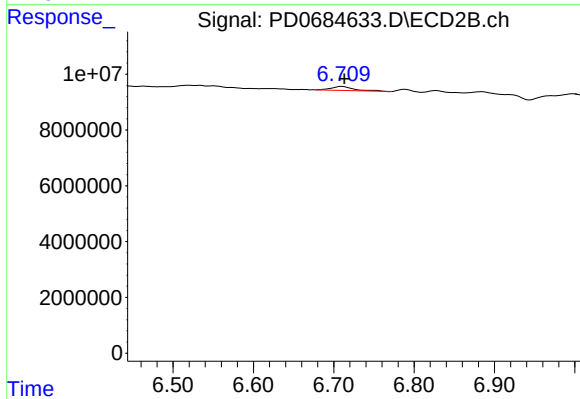

#13 Dieldrin


R.T.: 6.710 min
Delta R.T.: -0.003 min
Response: 2808033
Conc: 0.25 ng/ml

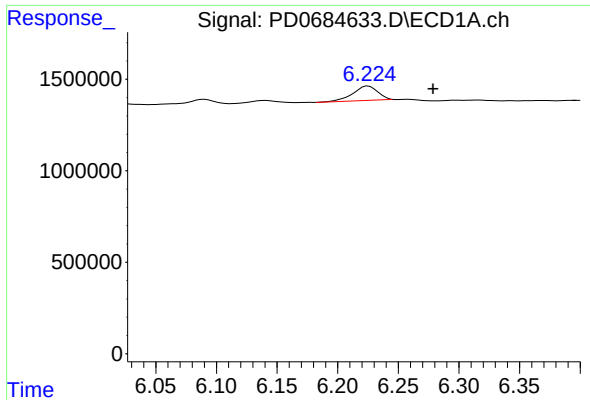

#15 Endosulfan II


R.T.: 6.225 min
Delta R.T.: -0.053 min
Response: 1132404
Conc: 0.78 ng/ml

Instrument :
ECD_D
ClientSampleId :

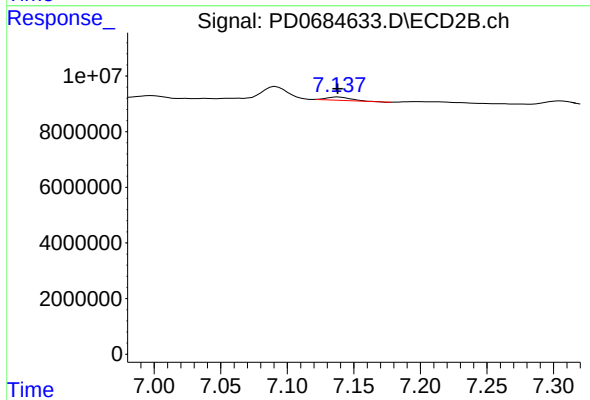


#15 Endosulfan II

R.T.: 7.138 min
Delta R.T.: 0.000 min
Response: 1558135
Conc: 0.17 ng/ml

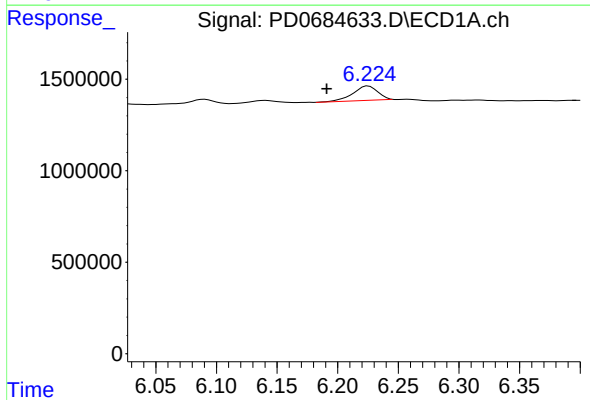


#23 Toxaphene-2

R.T.: 6.225 min
Delta R.T.: 0.034 min
Response: 1132404
Conc: 105.59 ng/ml

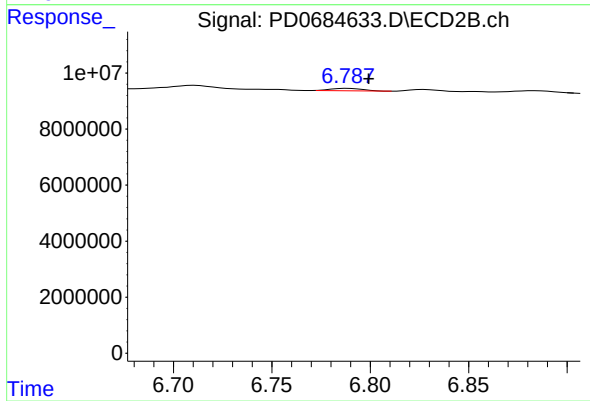

#23 Toxaphene-2


R.T.: 6.789 min
Delta R.T.: -0.010 min
Response: 997203
Conc: 9.90 ng/ml

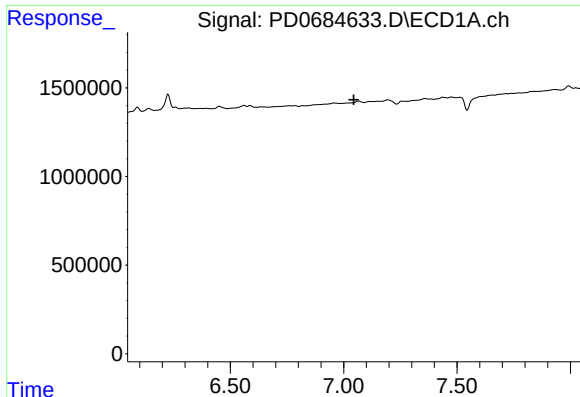

#26 Toxaphene-5


R.T.: 0.000 min
Exp R.T.: 7.045 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

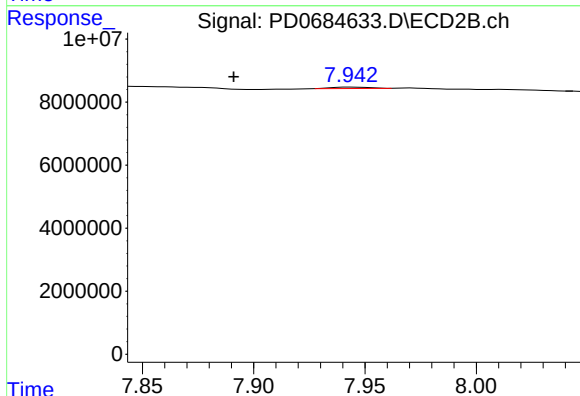


#26 Toxaphene-5

R.T.: 7.944 min
Delta R.T.: 0.053 min
Response: 534777
Conc: 6.10 ng/ml

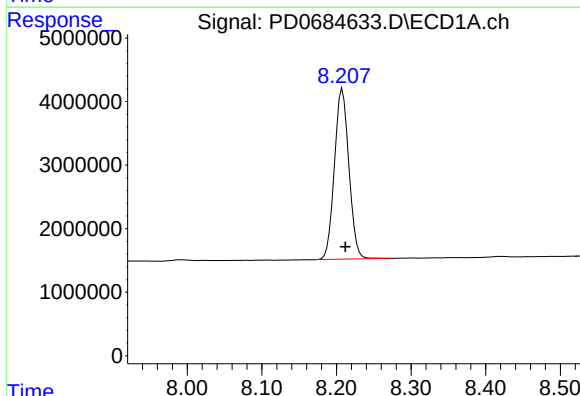

#27 Decachlorobiphenyl

R.T.: 8.208 min
Delta R.T.: -0.004 min
Response: 36192531
Conc: 26.03 ng/ml

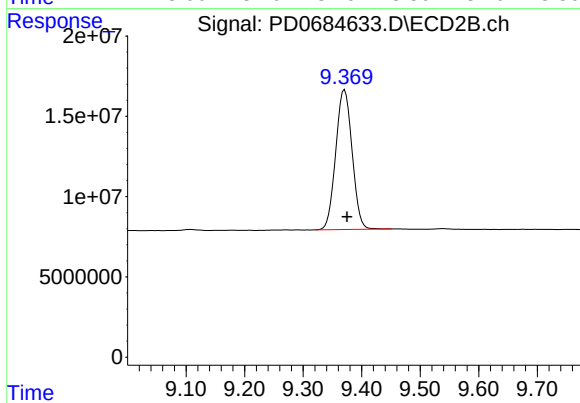

#27 Decachlorobiphenyl

R.T.: 9.371 min
Delta R.T.: -0.004 min
Response: 169178489
Conc: 26.82 ng/ml