

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031522\
 Data File : PD068628.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Mar 2022 19:53
 Operator : AR\AJ
 Sample : N1883-10MS
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 DBSA8MS

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 03/17/2022
 Supervised By : Ankita Jodhani 03/18/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 16 06:36:34 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031322CLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Mar 14 07:24:04 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.449	4.175	23413047	193.3E6	17.193	17.663
27)	SA Decachlor...	8.208	9.372	45623630	212.5E6	32.810	33.694
Target Compounds							
2)	A alpha-BHC	3.888	4.571	92652547	660.7E6	48.401	42.256
3)	MA gamma-BHC...	4.172	4.862	87082539	628.8E6	47.973	43.369
4)	MA Heptachlor	4.470	5.389	85382671	588.7E6	47.664	42.771
5)	MB Aldrin	4.718	5.702	85139333	587.9E6	48.409	43.568
6)	B beta-BHC	4.422	5.025	38956999	282.4E6	46.750	44.223
7)	B delta-BHC	4.626	5.250	73531049	519.9E6	41.586	36.729
8)	B Heptachlo...	5.162	6.090	78891806	523.3E6	48.578	43.444
9)	A Endosulfan I	5.501	6.453	73915748	472.3E6	48.010	43.398
10)	B trans-Chl...	5.388	6.325	81247007	519.7E6	48.683	43.695m
11)	B cis-Chlor...	5.447	6.401	79440362	502.0E6	48.393	43.770
12)	B 4,4'-DDE	5.613	6.551	156.0E6	948.4E6	104.867	92.828
13)	MA Dieldrin	5.745	6.712	169.4E6	1005.3E6	101.437	90.474
14)	MA Endrin	6.003	6.932	147.9E6	804.4E6	104.643	95.145
15)	B Endosulfa...	6.276	7.136	142.2E6	792.5E6	98.023	88.555
16)	A 4,4'-DDD	6.130	7.043	128.8E6	741.1E6	97.995	88.332
17)	MA 4,4'-DDT	6.371	7.345	138.5E6	773.7E6	103.700	98.171
18)	B Endrin al...	6.446	7.260	105.7E6	586.2E6	96.358	88.273
19)	B Endosulfa...	6.659	7.485	129.7E6	708.3E6	92.810	86.478
20)	A Methoxychlor	6.922	7.798	360.3E6	1670.8E6	508.998	476.965
21)	B Endrin ke...	7.152	7.960	162.7E6	790.7E6	101.985	92.598

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031522\
Data File : PD068628.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Mar 2022 19:53
Operator : AR\AJ
Sample : N1883-10MS
Misc :
ALS Vial : 21 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 16 06:36:34 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031322CLP.M
Quant Title : GC Extractables
QLast Update : Mon Mar 14 07:24:04 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

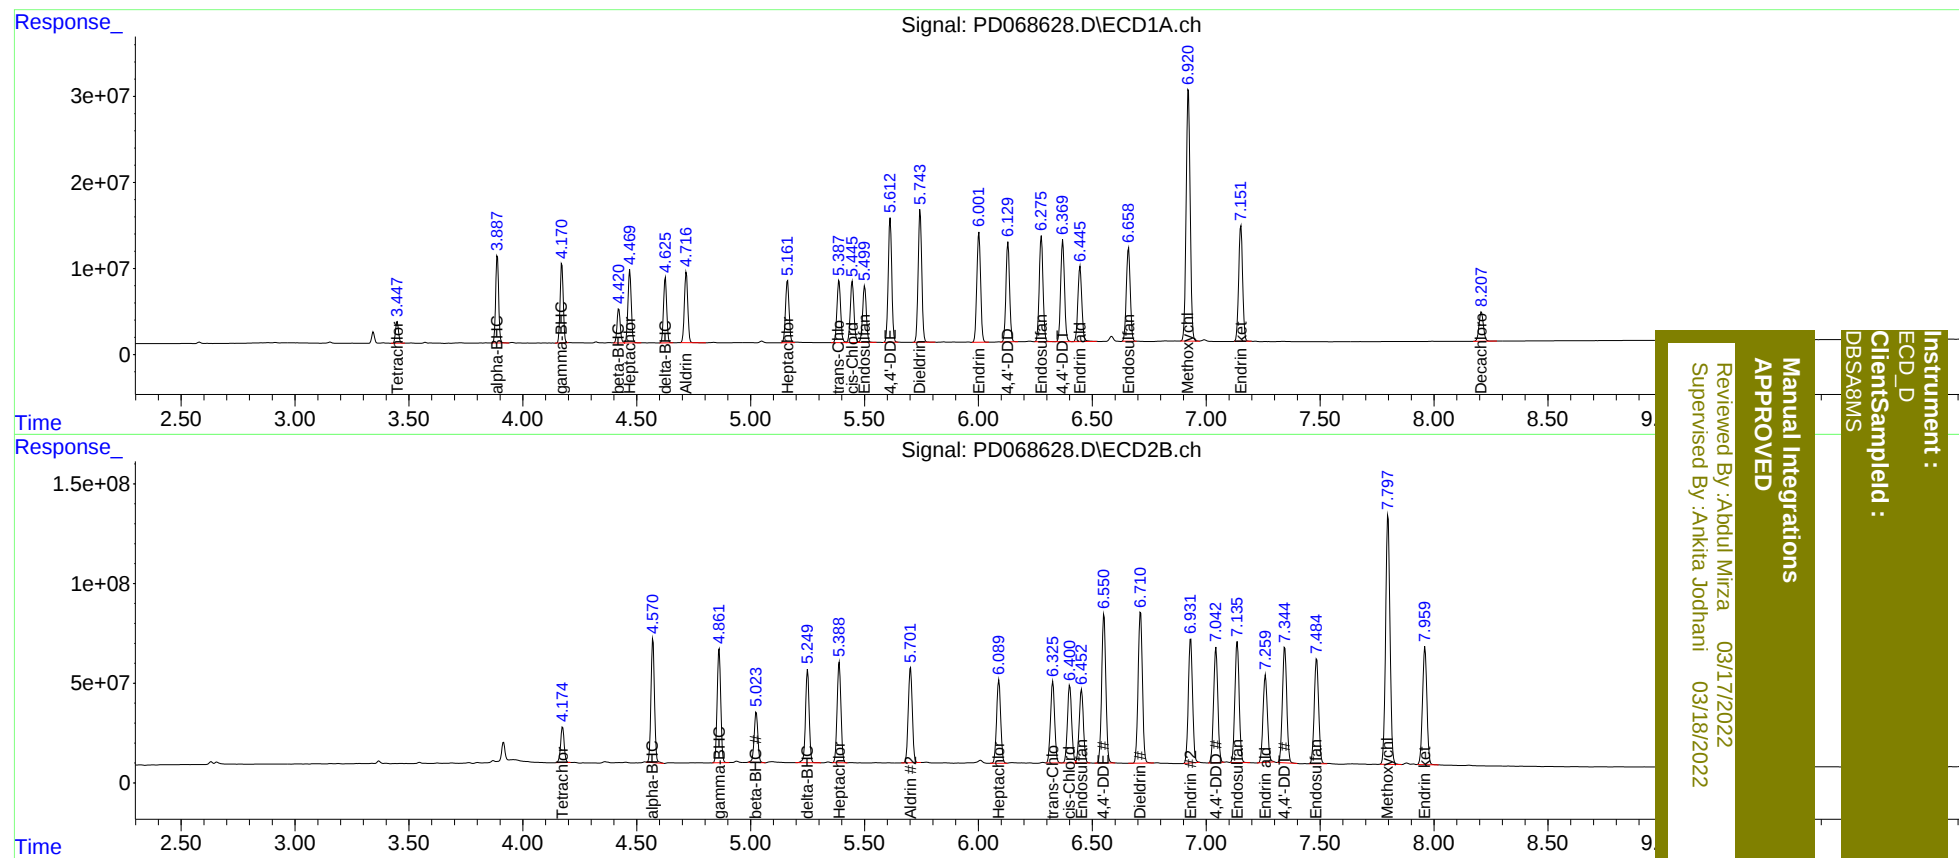

Reviewed By: Abdul Miza 03/17/2022
Supervised By: Ankita Jodhani 03/18/2022

Manual Integrations
APPROVED

Instrument :
ECD_D
ClientSampled :
DBSABMS