

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031522\
 Data File : PD068629.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Mar 2022 20:07
 Operator : AR\AJ
 Sample : N1883-11MSD
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 DBSA8MSD

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 03/17/2022
 Supervised By : Ankita Jodhani 03/18/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 16 06:37:02 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031322CLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Mar 14 07:24:04 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.449	4.175	21439285	181.8E6	15.744	16.613
27)	SA Decachlor...	8.208	9.370	41040429	191.2E6	29.514	30.314
Target Compounds							
2)	A alpha-BHC	3.889	4.571	92865060	670.9E6	48.512	42.906
3)	MA gamma-BHC...	4.172	4.862	87299267	636.9E6	48.093	43.927
4)	MA Heptachlor	4.471	5.389	85304499	594.8E6	47.621	43.217
5)	MB Aldrin	4.718	5.702	85107915	593.4E6	48.392	43.971
6)	B beta-BHC	4.422	5.024	39050112	285.4E6	46.861	44.685
7)	B delta-BHC	4.626	5.250	73657125	525.8E6	41.657	37.146
8)	B Heptachlo...	5.163	6.090	78921221	526.3E6	48.596	43.693
9)	A Endosulfan I	5.501	6.453	73686694	473.9E6	47.861	43.542
10)	B trans-Chl...	5.389	6.325	81147659	521.4E6	48.623	43.836m
11)	B cis-Chlor...	5.447	6.402	79206790	504.7E6	48.250	44.007
12)	B 4,4'-DDE	5.613	6.551	155.3E6	947.3E6	104.421	92.728
13)	MA Dieldrin	5.746	6.710	169.0E6	1003.1E6	101.183	90.275m
14)	MA Endrin	6.003	6.931	147.3E6	802.7E6	104.221	94.947
15)	B Endosulfa...	6.276	7.136	141.6E6	789.6E6	97.631	88.231
16)	A 4,4'-DDD	6.130	7.042	127.7E6	736.4E6	97.132	87.762
17)	MA 4,4'-DDT	6.371	7.345	137.3E6	766.5E6	102.832	97.256
18)	B Endrin al...	6.446	7.261	105.0E6	583.2E6	95.773	87.828
19)	B Endosulfa...	6.659	7.485	130.0E6	701.7E6	93.049	85.674
20)	A Methoxychlor	6.922	7.798	355.2E6	1654.1E6	501.862	472.186
21)	B Endrin ke...	7.153	7.959	161.7E6	785.7E6	101.359	92.018

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031522\
Data File : PD068629.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Mar 2022 20:07
Operator : AR\AJ
Sample : N1883-11MSD
Misc :
ALS Vial : 22 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 16 06:37:02 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031322CLP.M
Quant Title : GC Extractables
QLast Update : Mon Mar 14 07:24:04 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

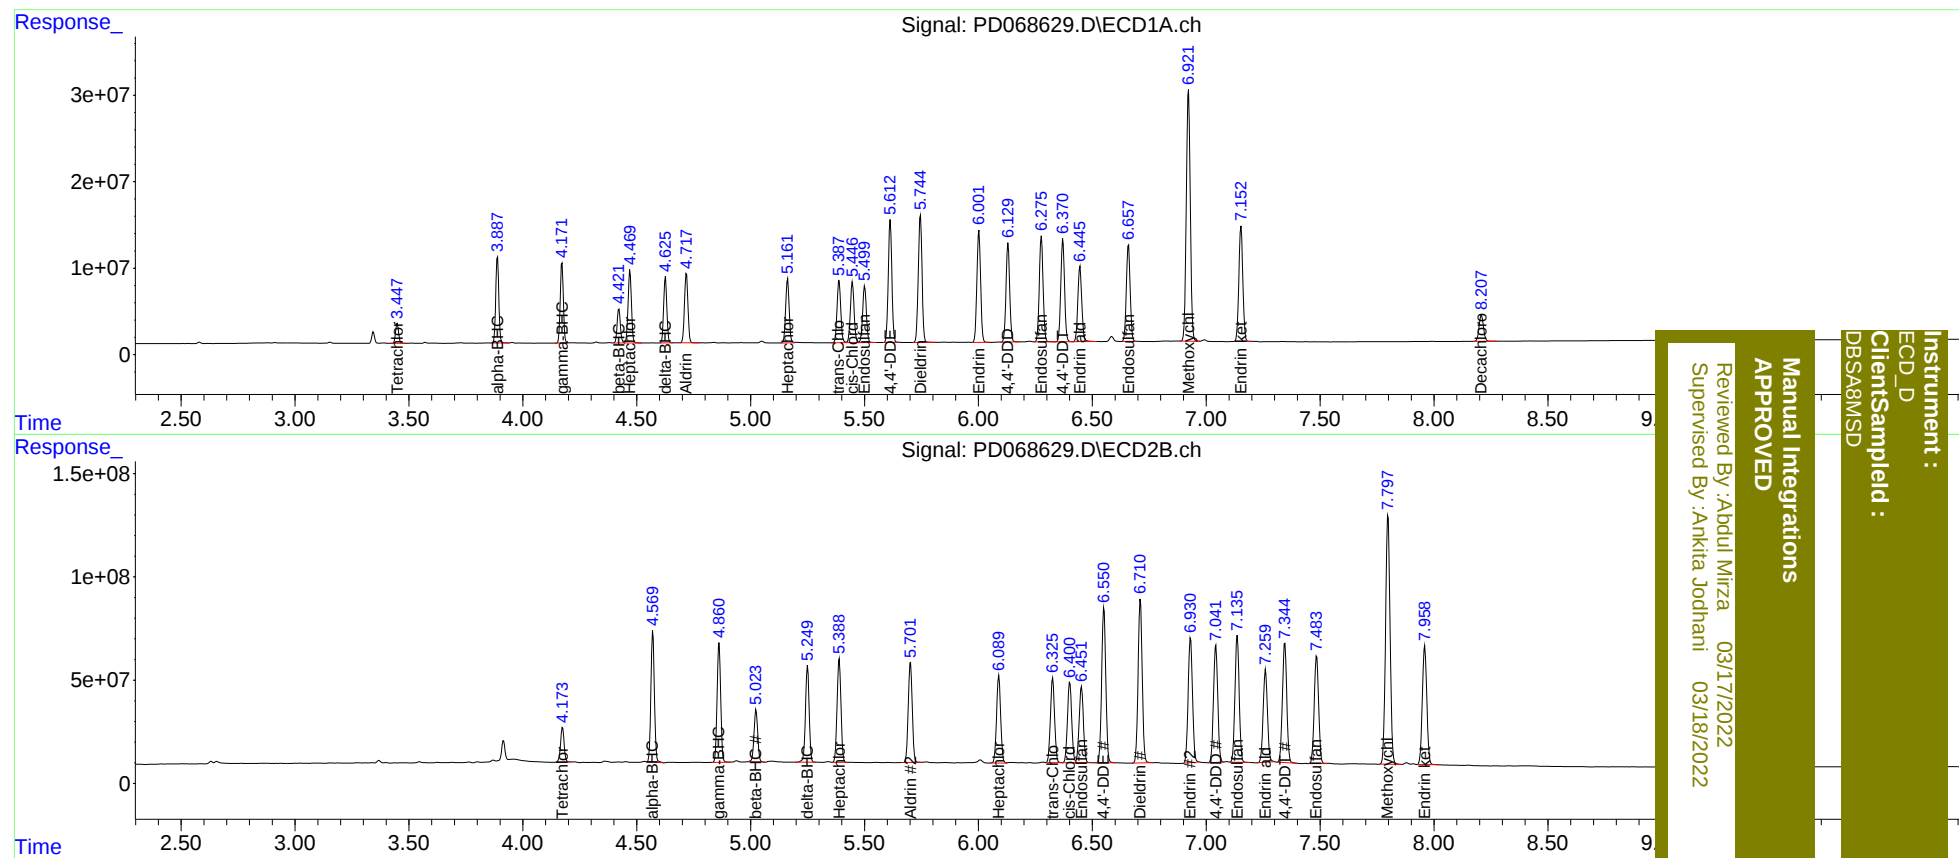

Reviewed By: Abdul Miza 03/17/2022
Supervised By: Ankita Jodhani 03/18/2022

Manual Integrations
APPROVED

Instrument :
ECD_D
Client Sampled :
DBSABMSD