

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Data\PD031522\  
 Data File : PD068616.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 15 Mar 2022 14:54  
 Operator : AR\AJ  
 Sample : INDA340  
 Misc :  
 ALS Vial : 9 Sample Multiplier: 1

Instrument :  
 ECD\_D  
 ClientSampleId :  
 INDA3153

Manual Integrations  
 APPROVED

Reviewed By : Abdul Mirza 03/17/2022  
 Supervised By : Ankita Jodhani 03/18/2022

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Mar 16 06:32:45 2022  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Method\PD031322CLP.M  
 Quant Title : GC Extractables  
 QLast Update : Mon Mar 14 07:24:04 2022  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1 µl  
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1  
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm


|                             | Compound        | RT#1  | RT#2  | Resp#1   | Resp#2  | ng/ml   | ng/ml   |
|-----------------------------|-----------------|-------|-------|----------|---------|---------|---------|
| -----                       |                 |       |       |          |         |         |         |
| System Monitoring Compounds |                 |       |       |          |         |         |         |
| 1)                          | SA Tetrachlo... | 3.456 | 4.176 | 25094905 | 207.1E6 | 18.428  | 18.919  |
| 27)                         | SA Decachlor... | 8.217 | 9.373 | 50956761 | 236.5E6 | 36.645  | 37.492  |
| Target Compounds            |                 |       |       |          |         |         |         |
| 2)                          | A alpha-BHC     | 3.896 | 4.572 | 35266652 | 289.8E6 | 18.423  | 18.535  |
| 3)                          | MA gamma-BHC... | 4.179 | 4.863 | 33566916 | 270.5E6 | 18.492  | 18.659  |
| 4)                          | MA Heptachlor   | 4.478 | 5.391 | 34287094 | 263.4E6 | 19.141  | 19.138  |
| 9)                          | A Endosulfan I  | 5.510 | 6.455 | 28885011 | 204.2E6 | 18.762  | 18.765  |
| 13)                         | MA Dieldrin     | 5.754 | 6.713 | 63533539 | 417.3E6 | 38.034  | 37.555  |
| 14)                         | MA Endrin       | 6.012 | 6.933 | 57208943 | 309.0E6 | 40.465  | 36.552  |
| 16)                         | A 4,4'-DDD      | 6.140 | 7.043 | 49234858 | 316.1E6 | 37.457  | 37.675m |
| 17)                         | MA 4,4'-DDT     | 6.380 | 7.348 | 50821880 | 302.0E6 | 38.057  | 38.313  |
| 20)                         | A Methoxychlor  | 6.931 | 7.800 | 141.1E6  | 696.2E6 | 199.365 | 198.753 |
| -----                       |                 |       |       |          |         |         |         |

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Data\PD031522\  
Data File : PD068616.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 15 Mar 2022 14:54  
Operator : AR\AJ  
Sample : INDA340  
Misc :  
ALS Vial : 9 Sample Multiplier: 1

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Mar 16 06:32:45 2022  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Method\PD031322CLP.M  
Quant Title : GC Extractables  
QLast Update : Mon Mar 14 07:24:04 2022  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 µl  
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1  
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

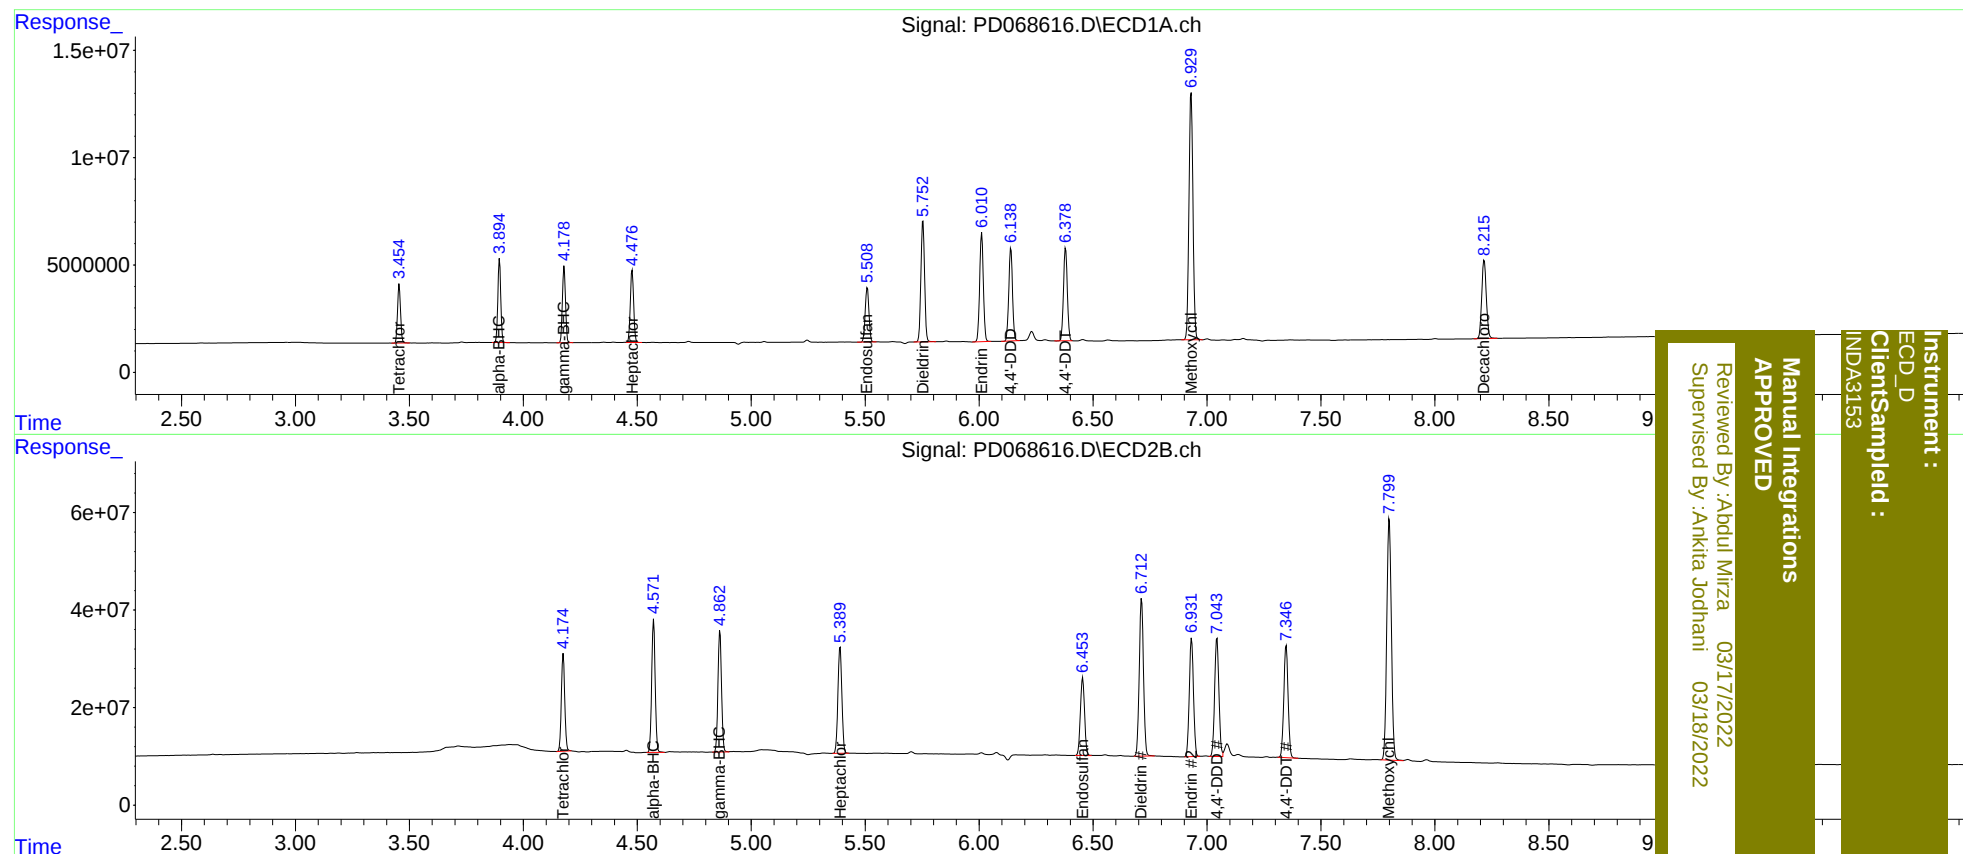

Reviewed By :Abdul Mirza 03/17/2022  
Supervised By :Ankita Jodhani 03/18/2022

Manual Integrations  
APPROVED

Instrument :  
ECD\_D  
ClientSampled :  
INDA3153