

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031523\
 Data File : PD074237.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Mar 2023 14:32
 Operator : AR\AJ
 Sample : PB151305BL
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 15 21:55:03 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031423.M
 Quant Title : GC Extractables
 QLast Update : Wed Mar 15 12:23:31 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.551	2.771	46958641	23108287	20.131	18.988
28)	SA Decachlor...	9.100	7.927	54900785	25652514	20.527	20.908
Target Compounds							
6)	B beta-BHC	4.570f	0.000	171247	0	0.116	N.D. #
7)	B delta-BHC	4.779	0.000	4905622	0	1.788	N.D. #
8)	B Heptachlo...	5.699	0.000	5422746	0	1.928	N.D. #
14)	MA Endrin	0.000	5.660f	0	373059	N.D.	0.285 #
15)	B Endosulfa...	6.842f	0.000	143202	0	0.056	N.D. #
21)	B Endrin ke...	7.699f	0.000	894701	0	0.321	N.D. #
22)	Mirex	8.159	0.000	536496	0	0.253	N.D. #
24)	Chlordane-2	0.000	4.329f	0	371670	N.D.	6.397 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031523\
Data File : PD074237.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Mar 2023 14:32
Operator : AR\AJ
Sample : PB151305BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 15 21:55:03 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031423.M
Quant Title : GC Extractables
QLast Update : Wed Mar 15 12:23:31 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

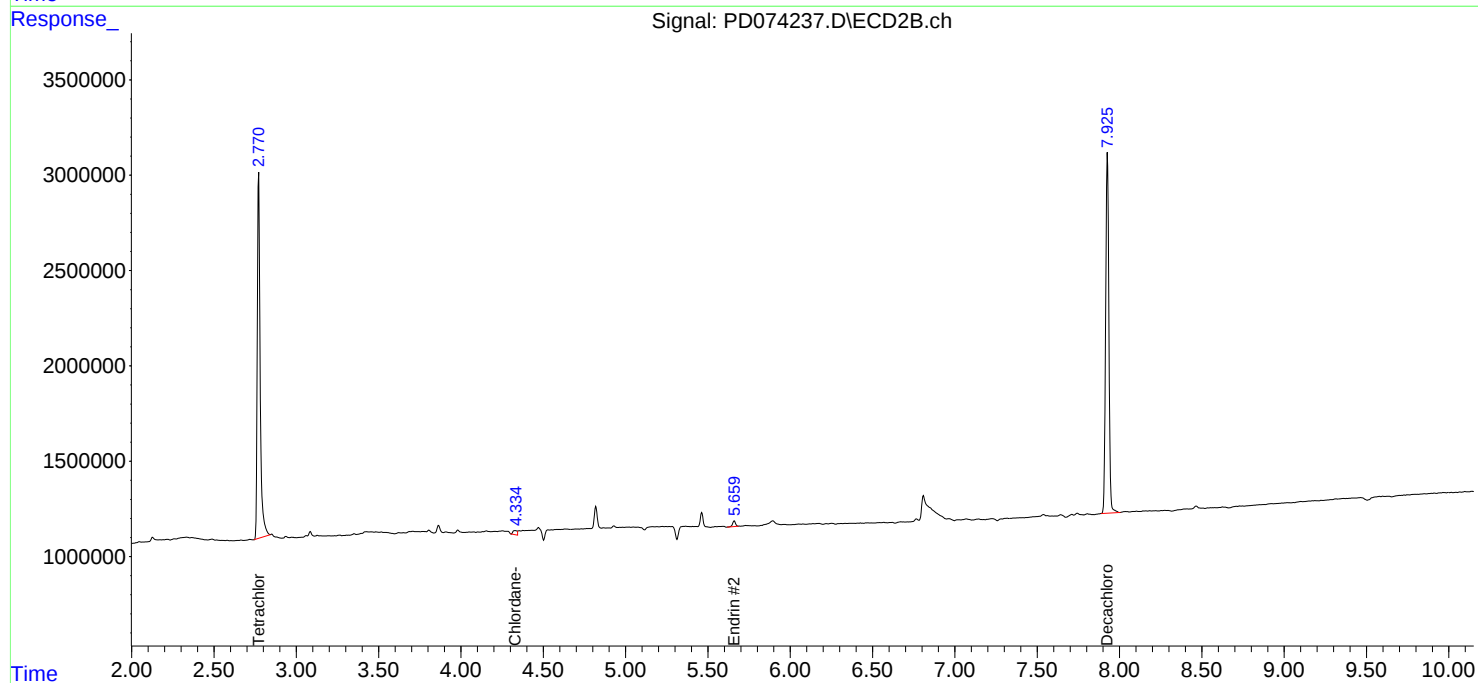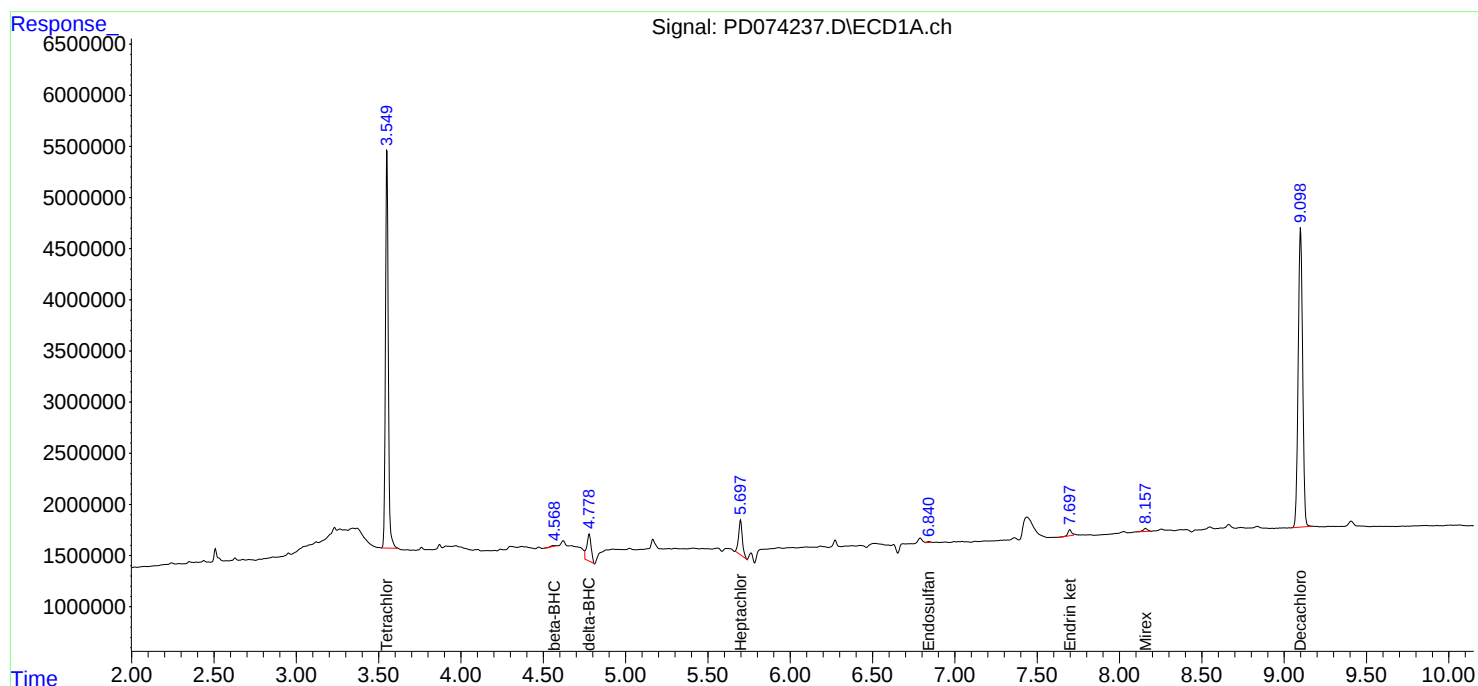


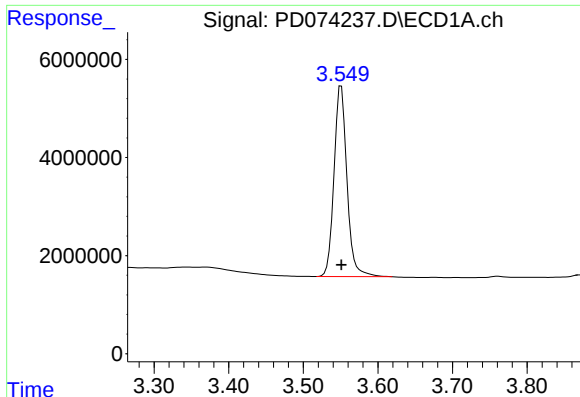

#1 Tetrachloro-m-xylene


R.T.: 3.551 min
Delta R.T.: 0.000 min
Response: 46958641
Conc: 20.13 ng/ml

Instrument :
ECD_D
ClientSampleId :

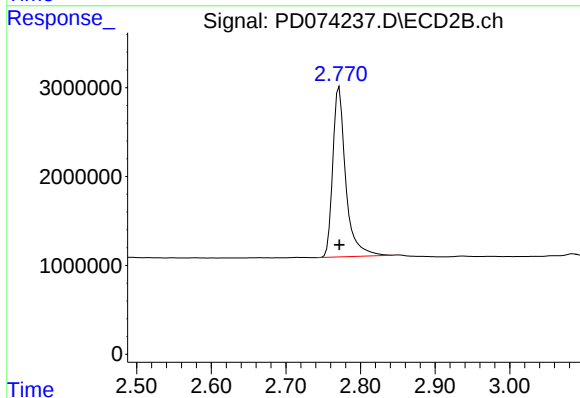


#1 Tetrachloro-m-xylene

R.T.: 2.771 min
Delta R.T.: 0.000 min
Response: 23108287
Conc: 18.99 ng/ml

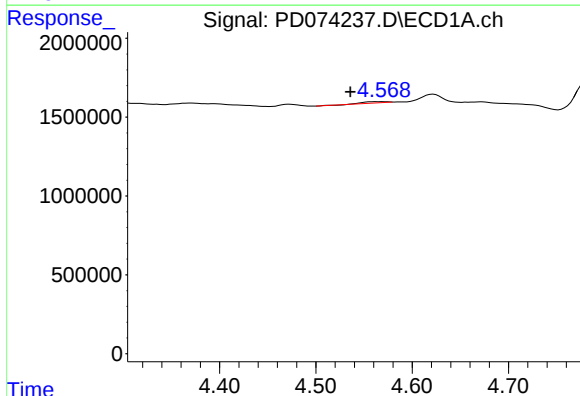


#6 beta-BHC

R.T.: 4.570 min
Delta R.T.: 0.034 min
Response: 171247
Conc: 0.12 ng/ml

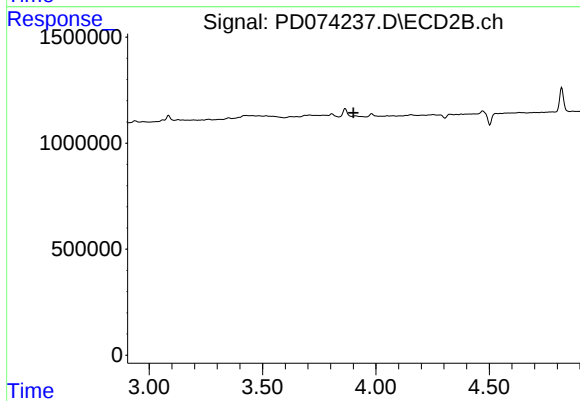

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 3.901 min
Response: 0
Conc: N.D.

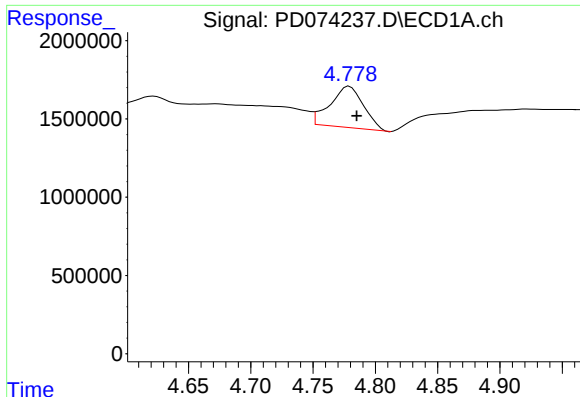

#7 delta-BHC


R.T.: 4.779 min
Delta R.T.: -0.006 min
Response: 4905622
Conc: 1.79 ng/ml

Instrument :
ECD_D
ClientSampleId :

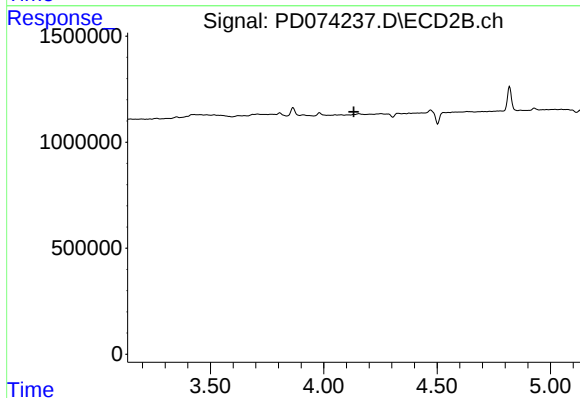


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.132 min
Response: 0
Conc: N.D.

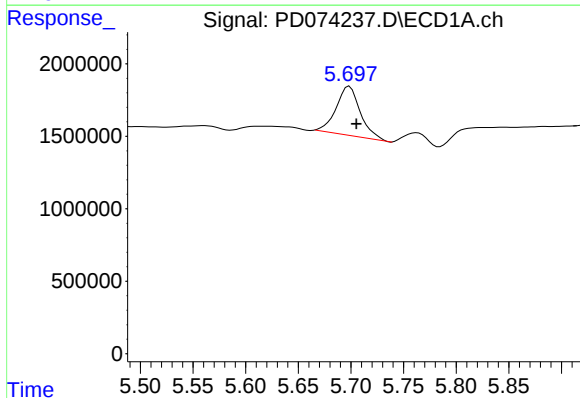


#8 Heptachlor epoxide

R.T.: 5.699 min
Delta R.T.: -0.006 min
Response: 5422746
Conc: 1.93 ng/ml

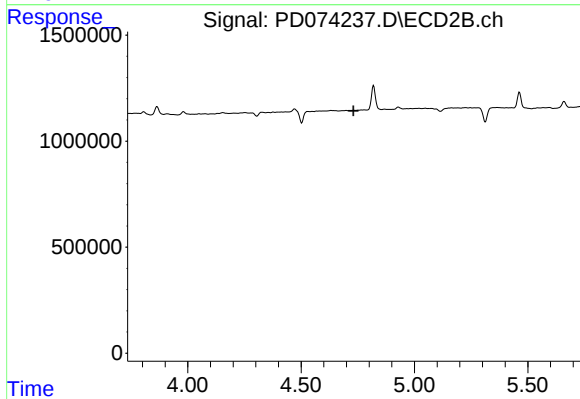

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T. : 4.731 min
Response: 0
Conc: N.D.

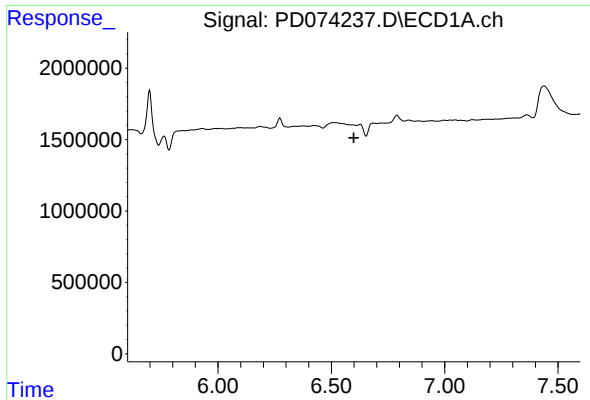

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 6.598 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

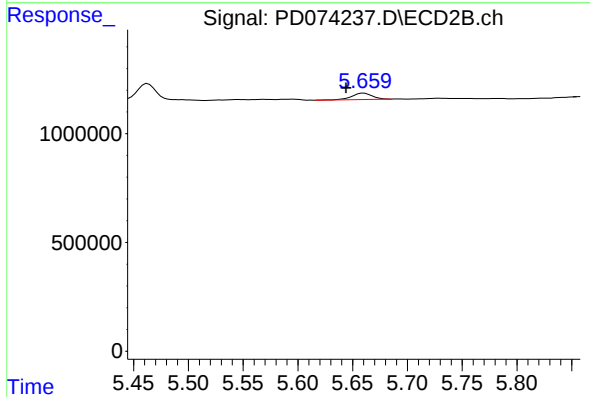


#14 Endrin

R.T.: 5.660 min
Delta R.T.: 0.016 min
Response: 373059
Conc: 0.29 ng/ml

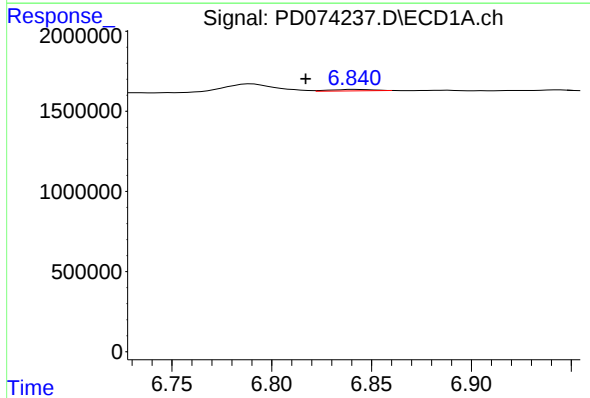


#15 Endosulfan II

R.T.: 6.842 min
Delta R.T.: 0.025 min
Response: 143202
Conc: 0.06 ng/ml

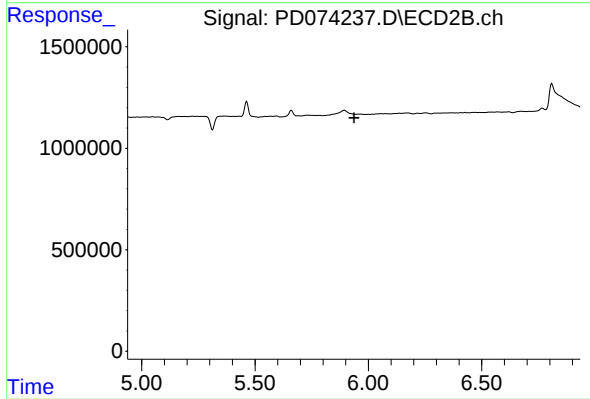

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 5.937 min
Response: 0
Conc: N.D.

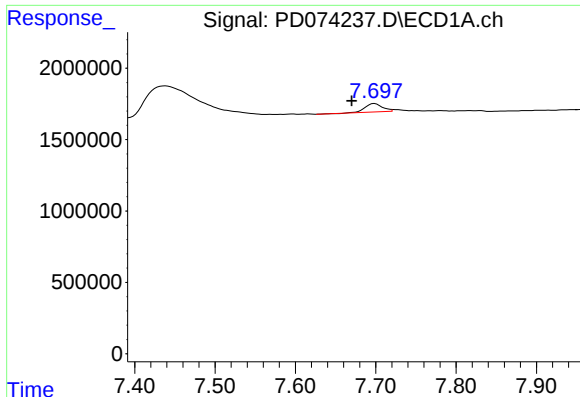

#21 Endrin ketone


R.T.: 7.699 min
Delta R.T.: 0.028 min
Response: 894701
Conc: 0.32 ng/ml

Instrument :
ECD_D
ClientSampleId :

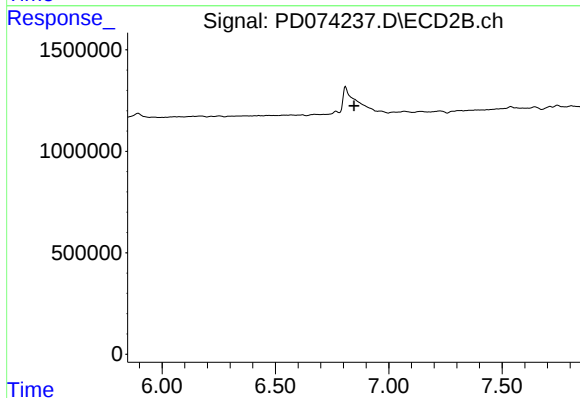


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 6.847 min
Response: 0
Conc: N.D.

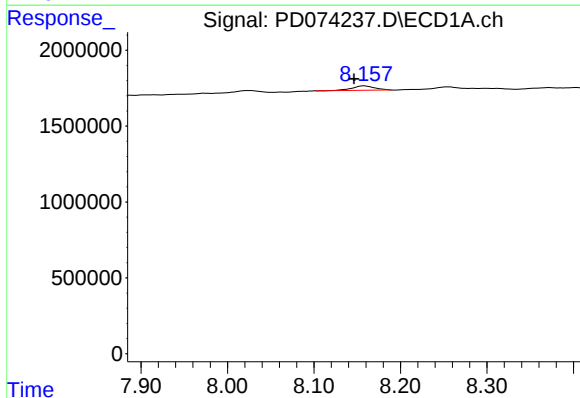


#22 Mirex

R.T.: 8.159 min
Delta R.T.: 0.012 min
Response: 536496
Conc: 0.25 ng/ml

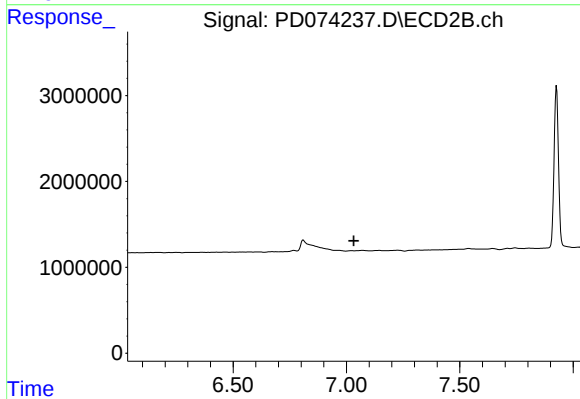

#22 Mirex


R.T.: 0.000 min
Exp R.T. : 7.032 min
Response: 0
Conc: N.D.

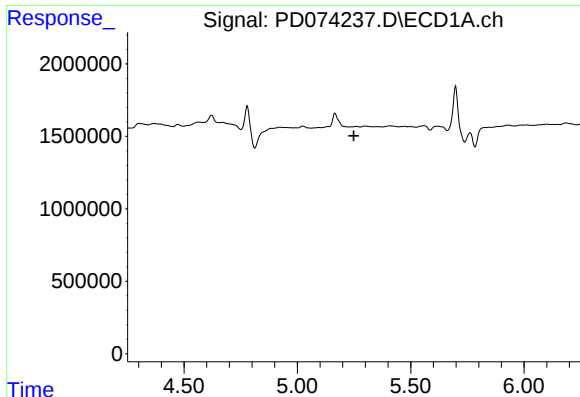

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T.: 5.249 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

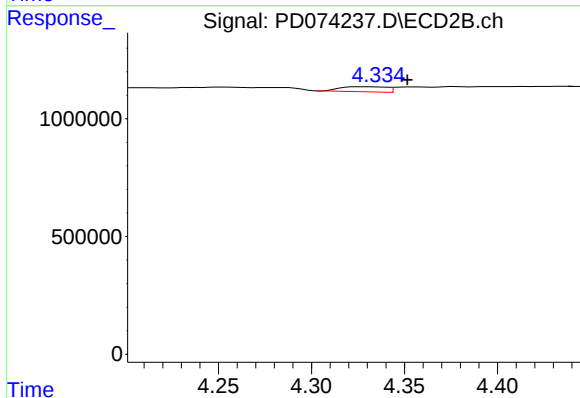


#24 Chlordane-2

R.T.: 4.329 min
Delta R.T.: -0.022 min
Response: 371670
Conc: 6.40 ng/ml

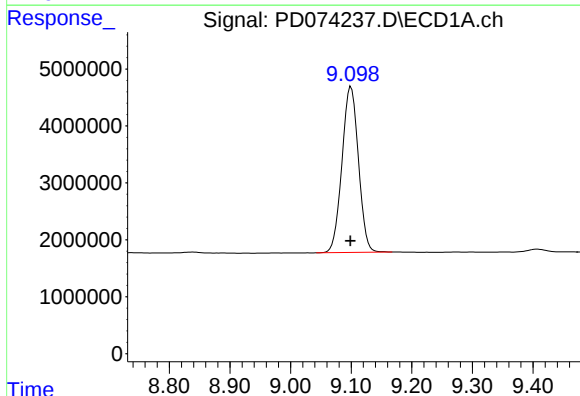

#28 Decachlorobiphenyl

R.T.: 9.100 min
Delta R.T.: 0.000 min
Response: 54900785
Conc: 20.53 ng/ml

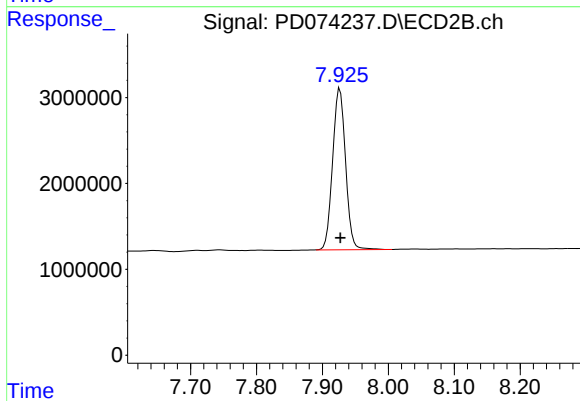

#28 Decachlorobiphenyl

R.T.: 7.927 min
Delta R.T.: 0.000 min
Response: 25652514
Conc: 20.91 ng/ml