

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031523\
 Data File : PD074226.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Mar 2023 09:47
 Operator : AR\AJ
 Sample : RESCHK
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 RESCHK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 15 17:42:27 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031423.M
 Quant Title : GC Extractables
 QLast Update : Wed Mar 15 12:23:31 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.551	2.772	55176908	28399049	23.655	23.335
28)	SA Decachlor...	9.099	7.926	59361108	28867072	22.195	23.528
Target Compounds							
9)	A Endosulfan I	6.092	5.102	33579805	16391157	11.811	11.390
10)	B gamma-Chl...	5.961	4.982	37541672	17962986	12.509	11.569
12)	B 4,4'-DDE	6.213	5.236	62154086	31698942	22.543	22.463
13)	MA Dieldrin	6.368	5.367	69055262	34944318	23.409	23.240
19)	B Endosulfa...	7.182	6.339	52889804	25929600	21.422	21.239
20)	A Methoxychlor	7.522	6.620	149.8E6	71955645	107.048	106.345
21)	B Endrin ke...	7.669	6.847	64248129	34172921	23.080	23.167



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031523\
Data File : PD074226.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Mar 2023 09:47
Operator : AR\AJ
Sample : RESCHK
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESCHK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 15 17:42:27 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031423.M
Quant Title : GC Extractables
QLast Update : Wed Mar 15 12:23:31 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

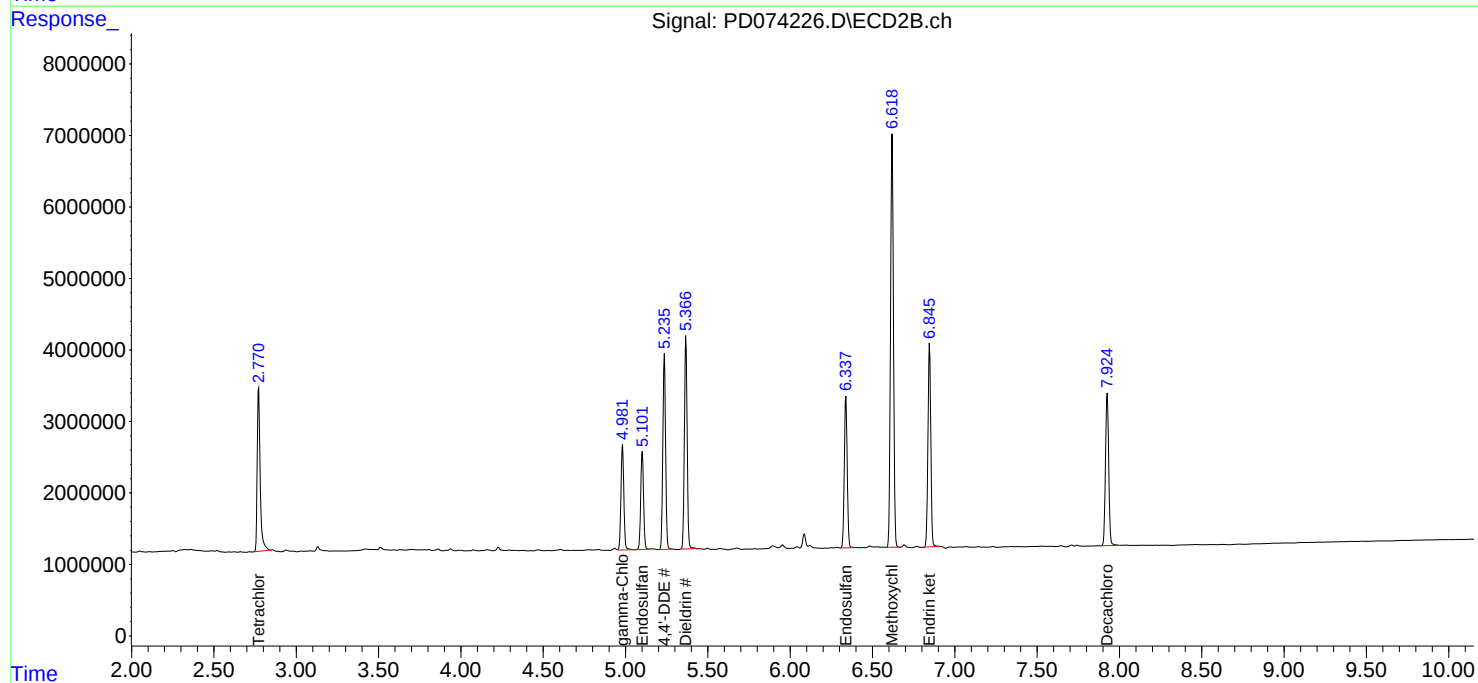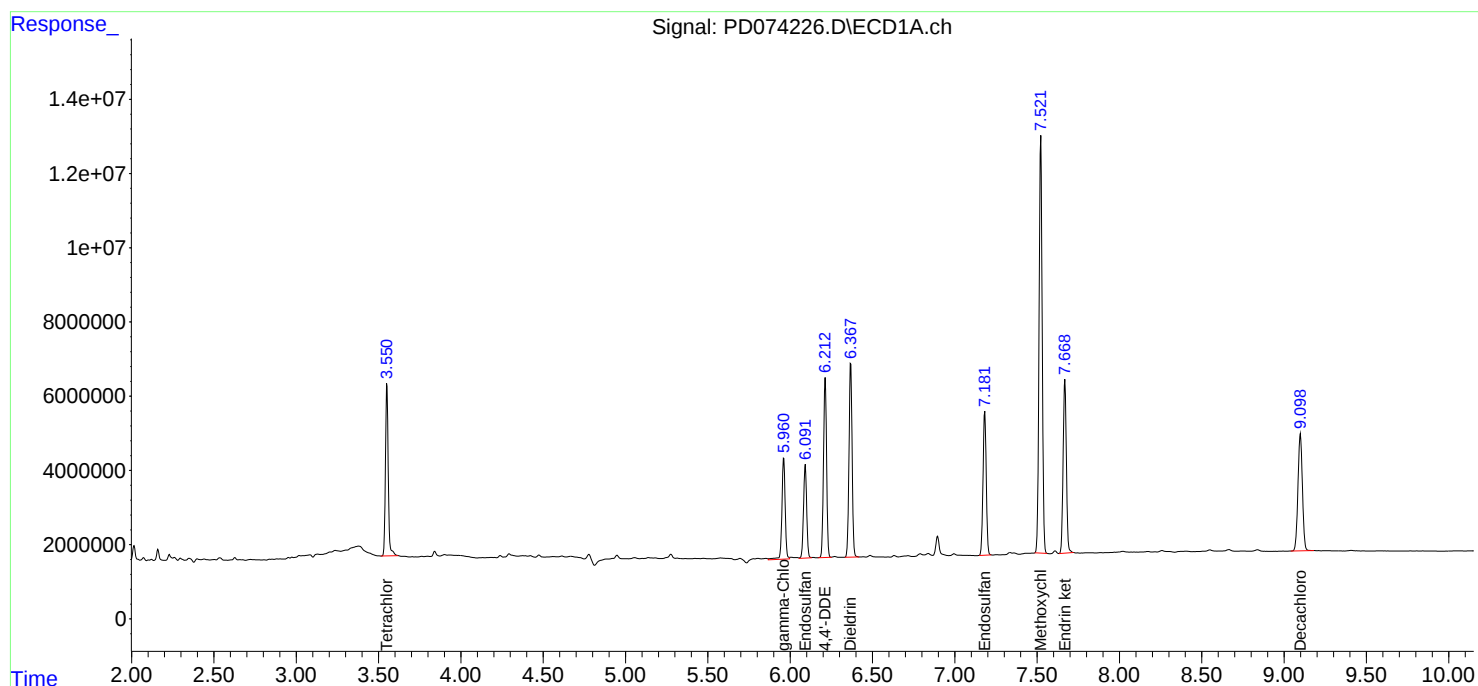


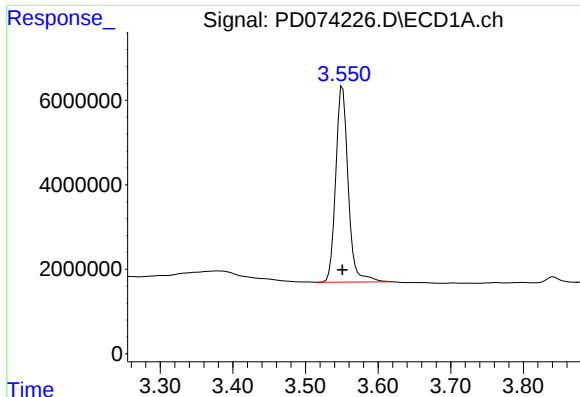

#1 Tetrachloro-m-xylene


R.T.: 3.551 min
Delta R.T.: 0.000 min
Response: 55176908
Conc: 23.65 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

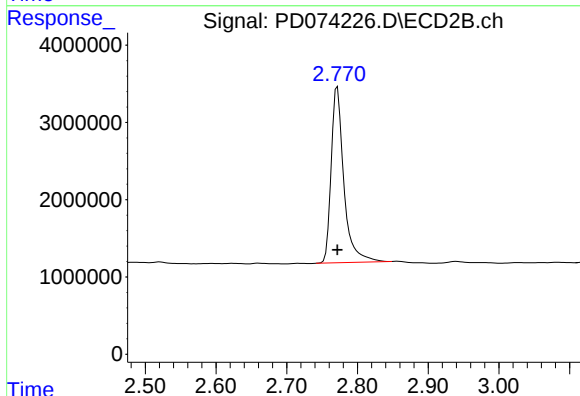


#1 Tetrachloro-m-xylene

R.T.: 2.772 min
Delta R.T.: 0.000 min
Response: 28399049
Conc: 23.34 ng/ml

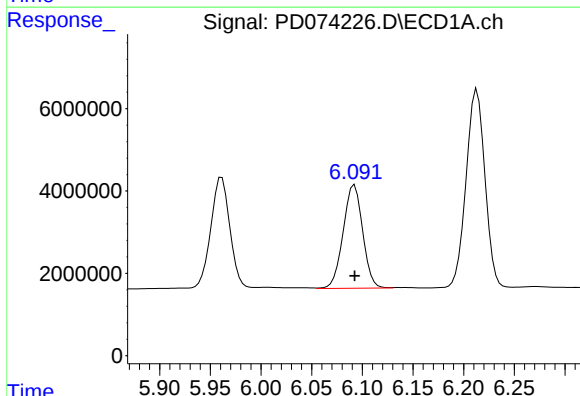


#9 Endosulfan I

R.T.: 6.092 min
Delta R.T.: 0.000 min
Response: 33579805
Conc: 11.81 ng/ml

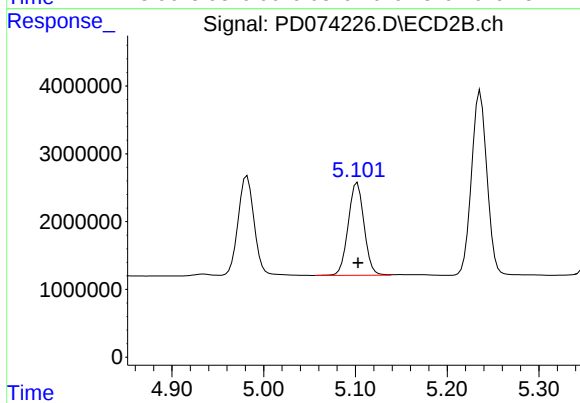

#9 Endosulfan I


R.T.: 5.102 min
Delta R.T.: 0.000 min
Response: 16391157
Conc: 11.39 ng/ml

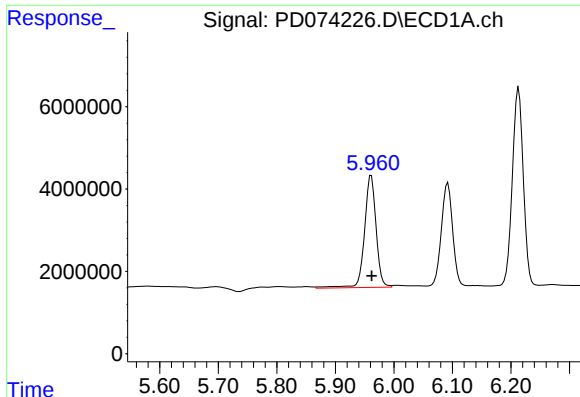

#10 gamma-Chlordane


R.T.: 5.961 min
Delta R.T.: 0.000 min
Response: 37541672
Conc: 12.51 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

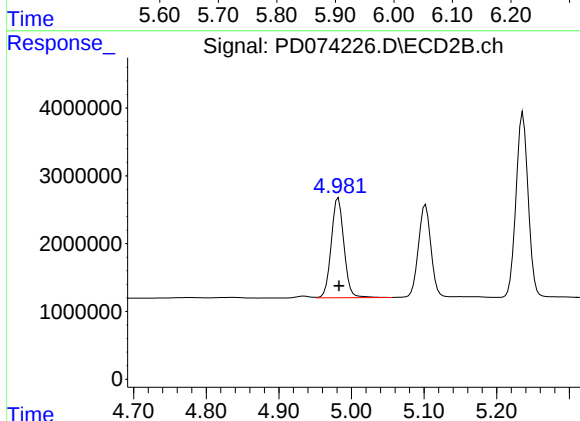


#10 gamma-Chlordane

R.T.: 4.982 min
Delta R.T.: -0.001 min
Response: 17962986
Conc: 11.57 ng/ml

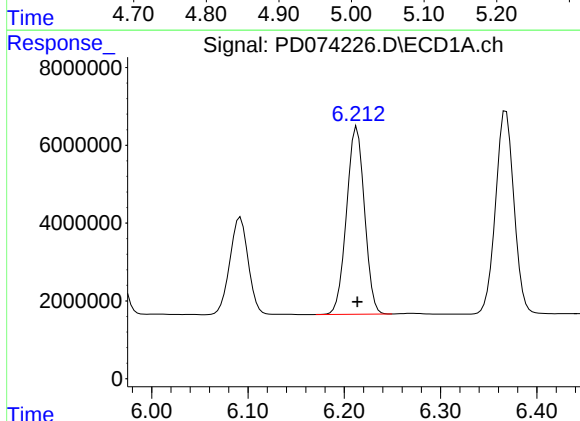


#12 4,4'-DDE

R.T.: 6.213 min
Delta R.T.: 0.000 min
Response: 62154086
Conc: 22.54 ng/ml

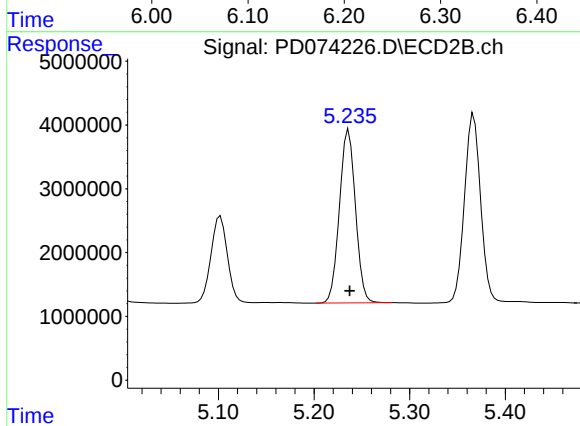

#12 4,4'-DDE


R.T.: 5.236 min
Delta R.T.: -0.001 min
Response: 31698942
Conc: 22.46 ng/ml

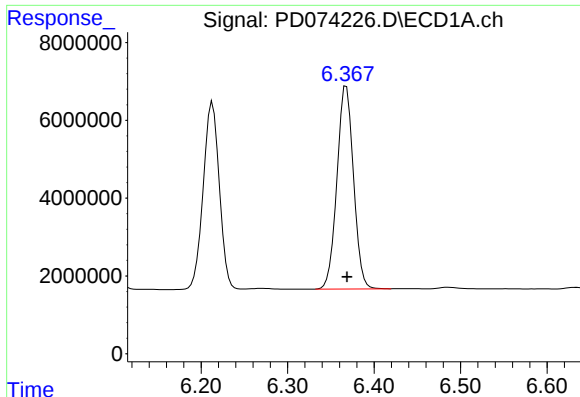

#13 Dieldrin


R.T.: 6.368 min
Delta R.T.: 0.000 min
Response: 69055262
Conc: 23.41 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

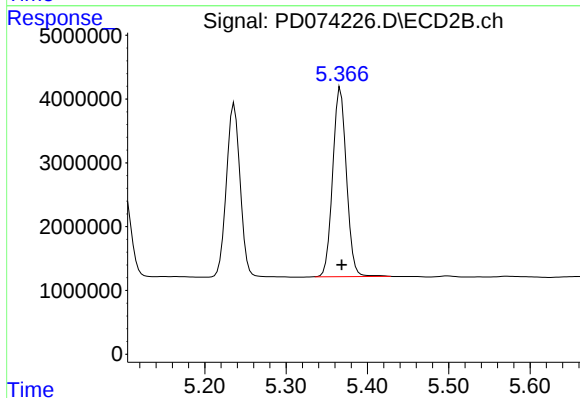


#13 Dieldrin

R.T.: 5.367 min
Delta R.T.: -0.002 min
Response: 34944318
Conc: 23.24 ng/ml

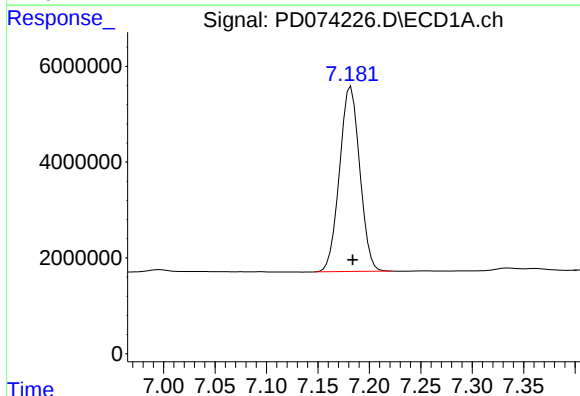


#19 Endosulfan Sulfate

R.T.: 7.182 min
Delta R.T.: -0.002 min
Response: 52889804
Conc: 21.42 ng/ml

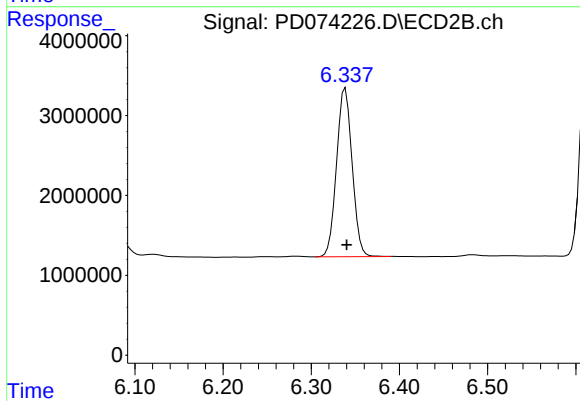

#19 Endosulfan Sulfate


R.T.: 6.339 min
Delta R.T.: -0.002 min
Response: 25929600
Conc: 21.24 ng/ml

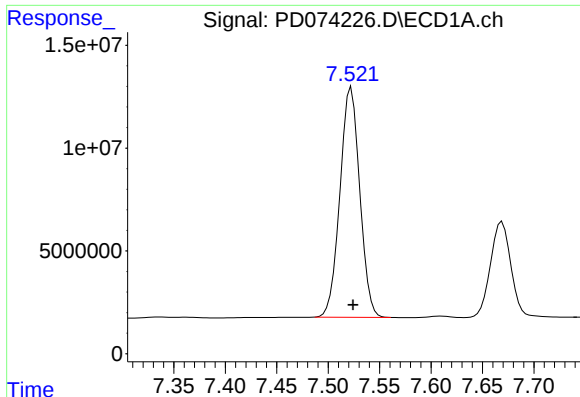

#20 Methoxychlor


R.T.: 7.522 min
Delta R.T.: -0.002 min
Response: 149780037
Conc: 107.05 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

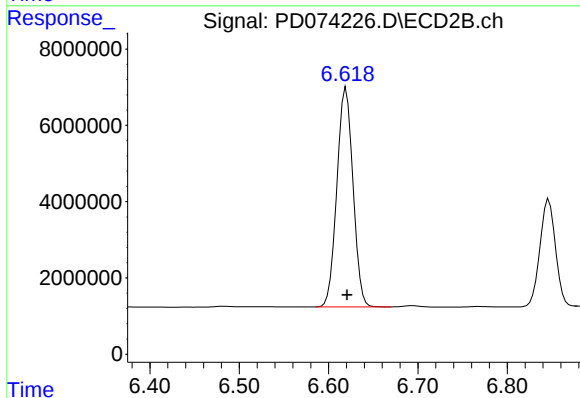


#20 Methoxychlor

R.T.: 6.620 min
Delta R.T.: -0.001 min
Response: 71955645
Conc: 106.34 ng/ml

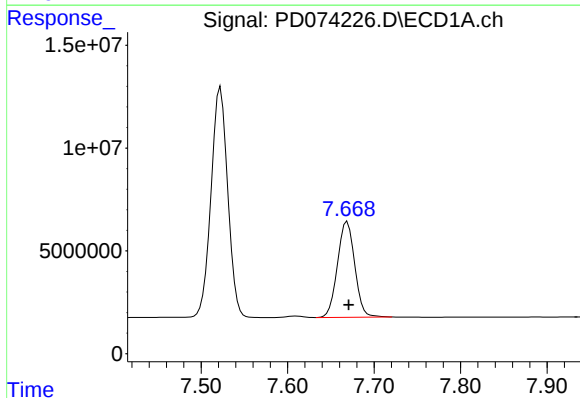


#21 Endrin ketone

R.T.: 7.669 min
Delta R.T.: -0.002 min
Response: 64248129
Conc: 23.08 ng/ml

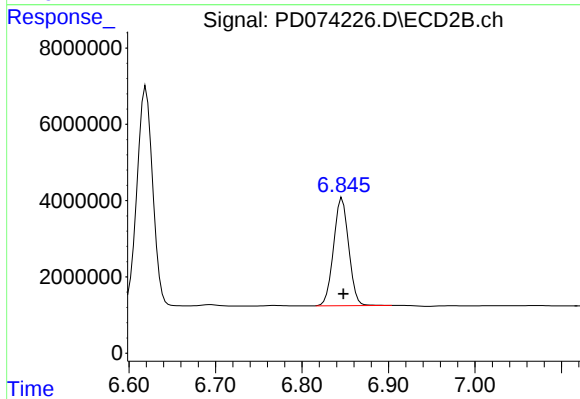

#21 Endrin ketone


R.T.: 6.847 min
Delta R.T.: -0.001 min
Response: 34172921
Conc: 23.17 ng/ml

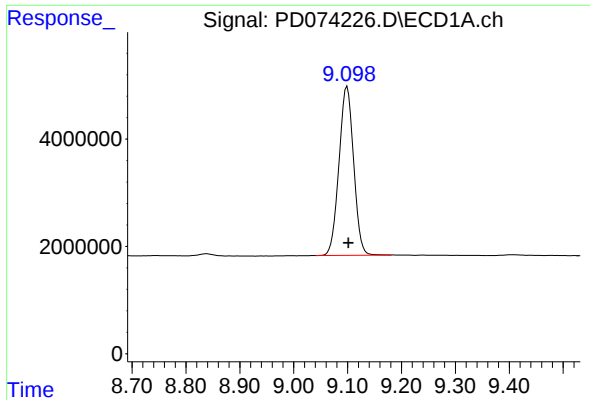

#28 Decachlorobiphenyl

R.T.: 9.099 min
Delta R.T.: -0.002 min
Response: 59361108
Conc: 22.19 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

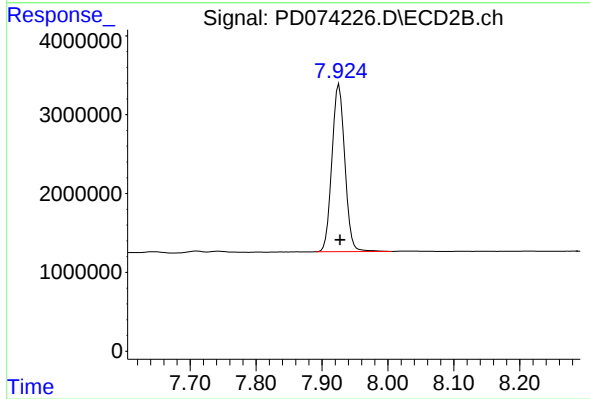

#28 Decachlorobiphenyl

R.T.: 7.926 min
Delta R.T.: -0.001 min
Response: 28867072
Conc: 23.53 ng/ml