

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031523\
 Data File : PD074228.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Mar 2023 10:21
 Operator : AR\AJ
 Sample : PCHLORICC750
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 15 12:01:59 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031423.M
 Quant Title : GC Extractables
 QLast Update : Wed Mar 15 12:01:09 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.551	2.771	174.0E6	109.9E6	74.268	74.106
28)	SA Decachlor...	9.099	7.926	174.4E6	87904432	71.081	71.444
Target Compounds							
23)	Chlordane-1	4.719	3.773	93910930	37943254	739.154	738.345
24)	Chlordane-2	5.250	4.351	95131564	42401039	718.072	719.138
25)	Chlordane-3	5.962	4.982	383.8E6	128.7E6	753.914	745.509
26)	Chlordane-4	6.045	5.046	458.3E6	123.1E6	747.722	751.405
27)	Chlordane-5	6.897	5.943	76303530	45833349	734.971	736.873



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031523\
Data File : PD074228.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Mar 2023 10:21
Operator : AR\AJ
Sample : PCHLORICC750
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 15 12:01:59 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031423.M
Quant Title : GC Extractables
QLast Update : Wed Mar 15 12:01:09 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

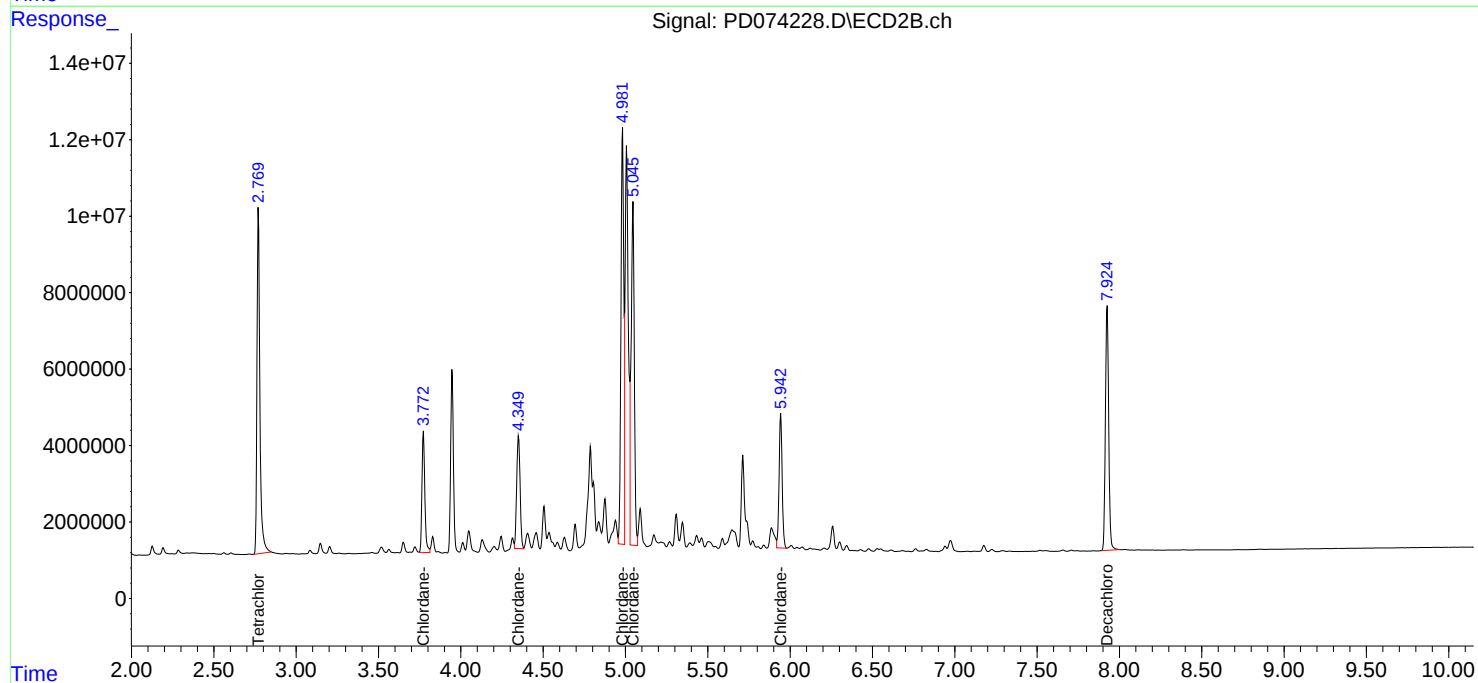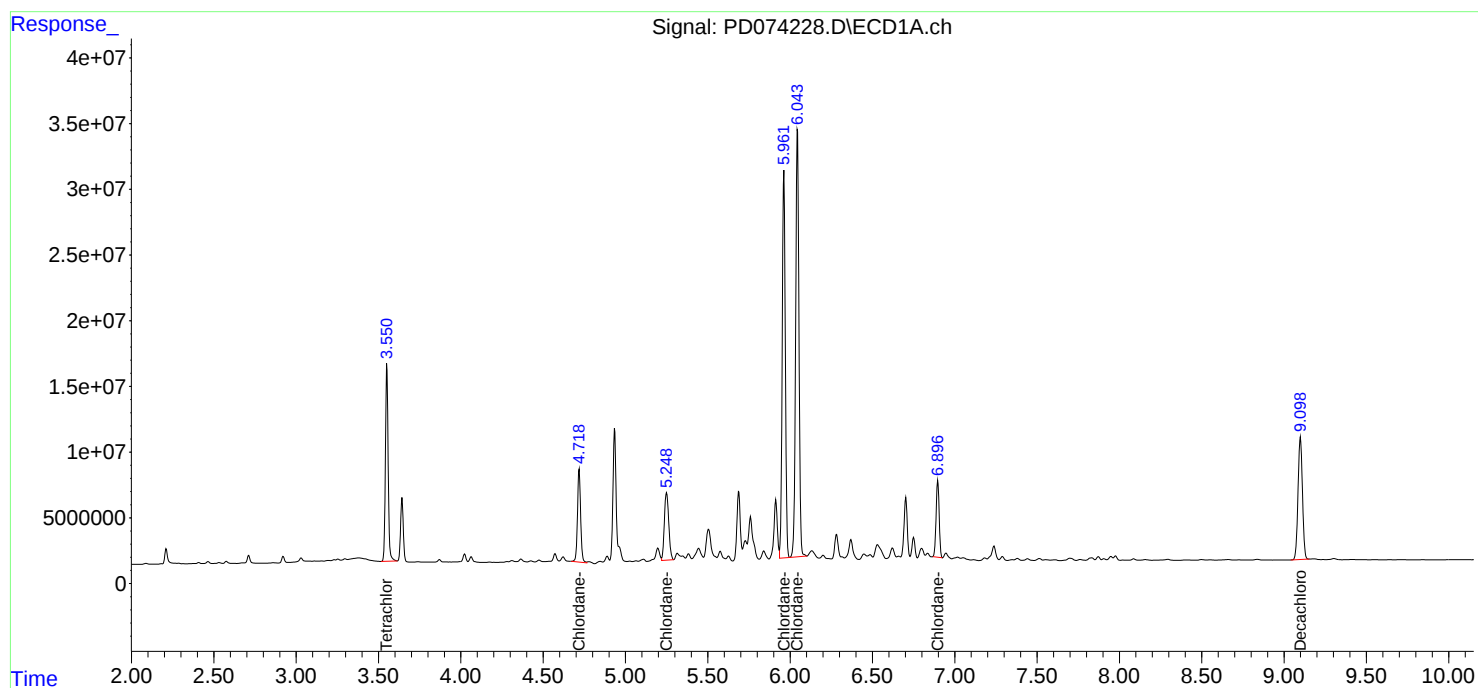


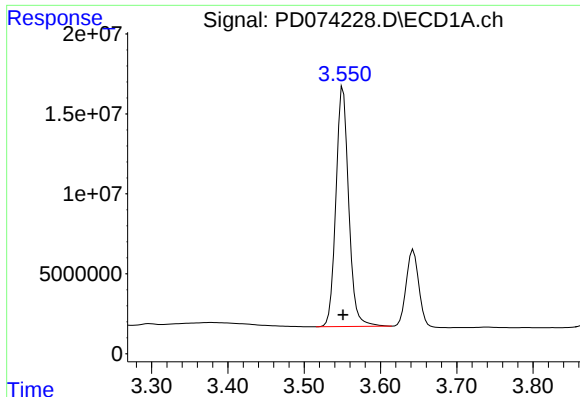

#1 Tetrachloro-m-xylene


R.T.: 3.551 min
Delta R.T.: 0.000 min
Response: 174020302
Conc: 74.27 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

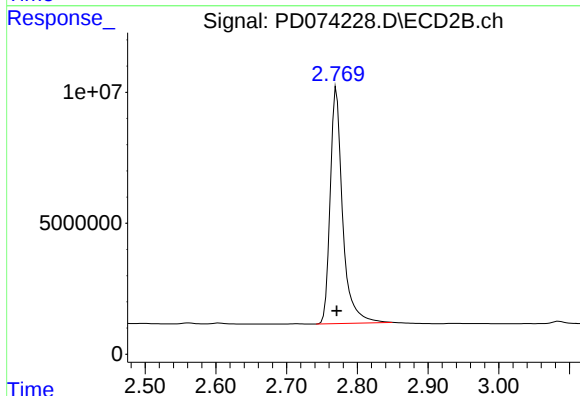


#1 Tetrachloro-m-xylene

R.T.: 2.771 min
Delta R.T.: 0.000 min
Response: 109923338
Conc: 74.11 ng/ml

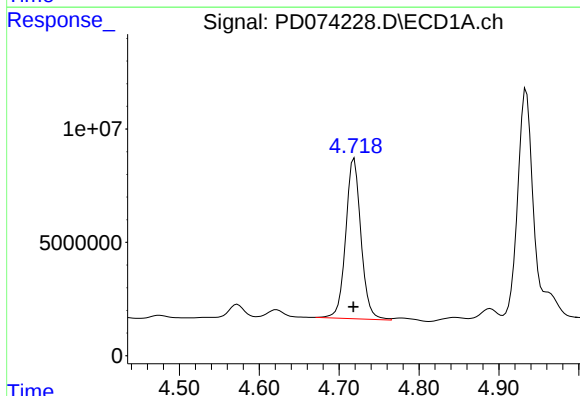


#23 Chlordane-1

R.T.: 4.719 min
Delta R.T.: 0.001 min
Response: 93910930
Conc: 739.15 ng/ml

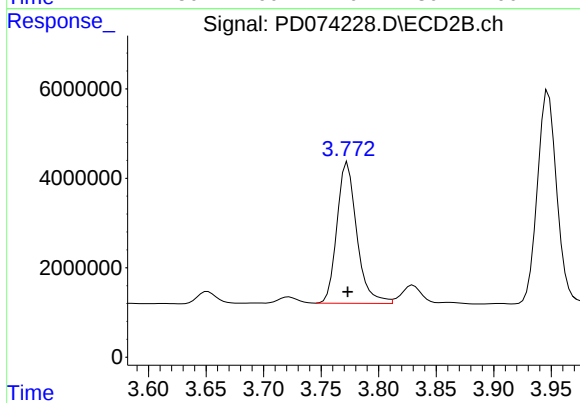

#23 Chlordane-1


R.T.: 3.773 min
Delta R.T.: 0.000 min
Response: 37943254
Conc: 738.35 ng/ml

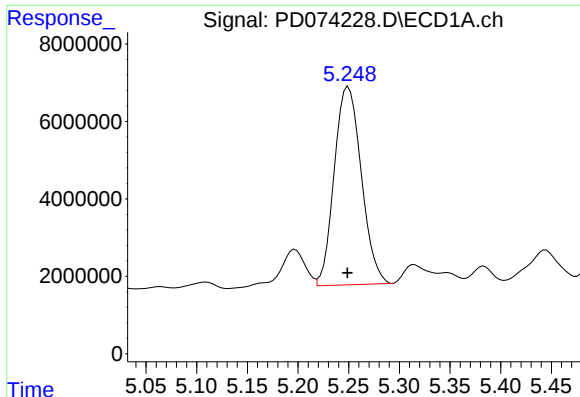

#24 Chlordane-2


R.T.: 5.250 min
Delta R.T.: 0.001 min
Response: 95131564
Conc: 718.07 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

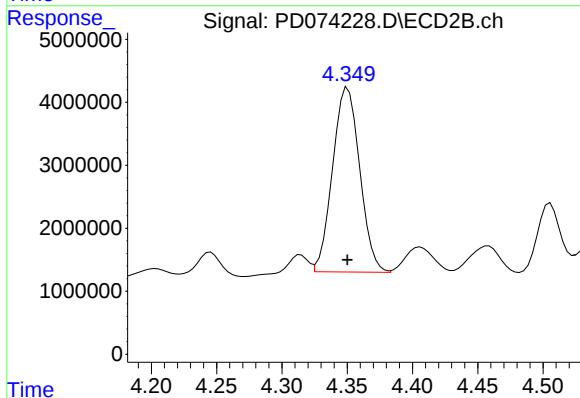


#24 Chlordane-2

R.T.: 4.351 min
Delta R.T.: 0.000 min
Response: 42401039
Conc: 719.14 ng/ml

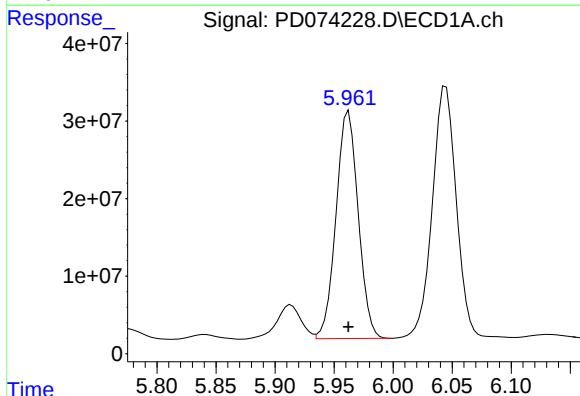


#25 Chlordane-3

R.T.: 5.962 min
Delta R.T.: 0.000 min
Response: 383819677
Conc: 753.91 ng/ml

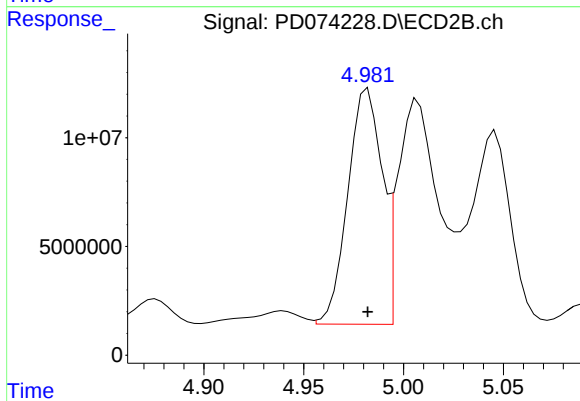

#25 Chlordane-3


R.T.: 4.982 min
Delta R.T.: 0.000 min
Response: 128731742
Conc: 745.51 ng/ml

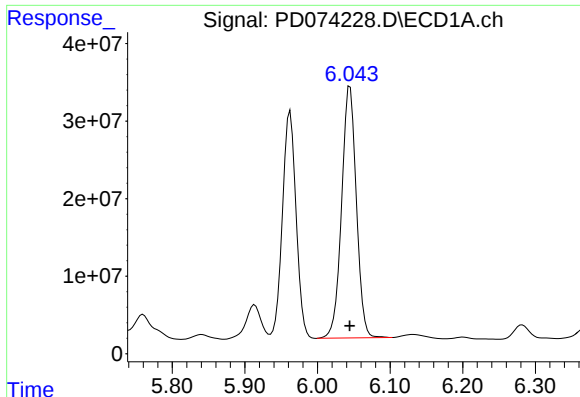

#26 Chlordane-4


R.T.: 6.045 min
Delta R.T.: 0.000 min
Response: 458330487
Conc: 747.72 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

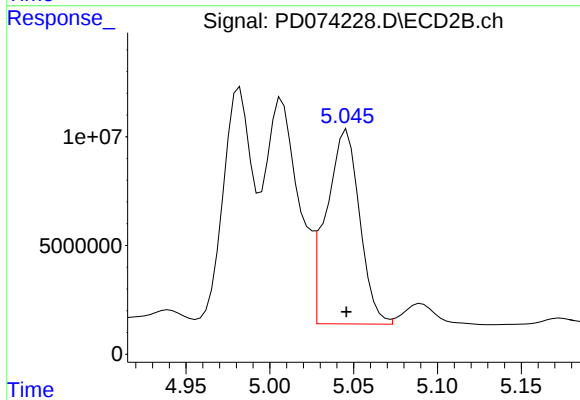


#26 Chlordane-4

R.T.: 5.046 min
Delta R.T.: 0.000 min
Response: 123067751
Conc: 751.40 ng/ml

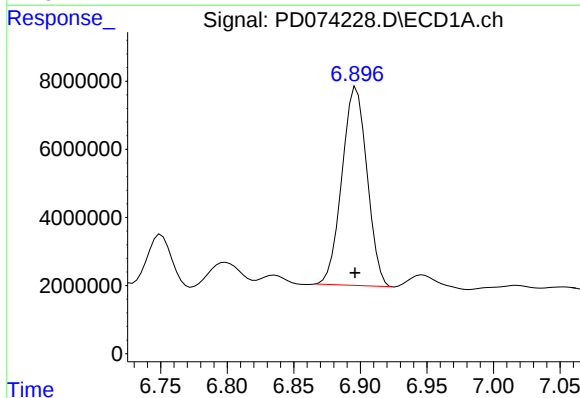


#27 Chlordane-5

R.T.: 6.897 min
Delta R.T.: 0.001 min
Response: 76303530
Conc: 734.97 ng/ml

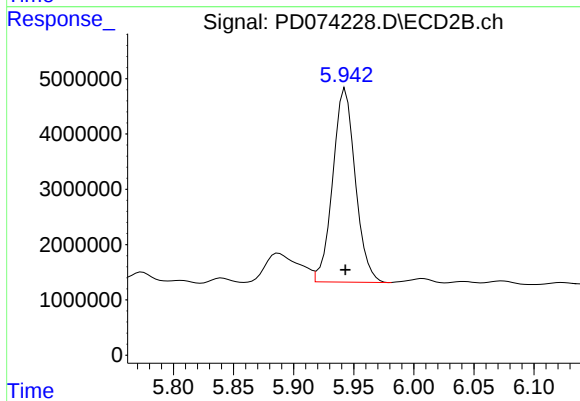

#27 Chlordane-5


R.T.: 5.943 min
Delta R.T.: 0.000 min
Response: 45833349
Conc: 736.87 ng/ml

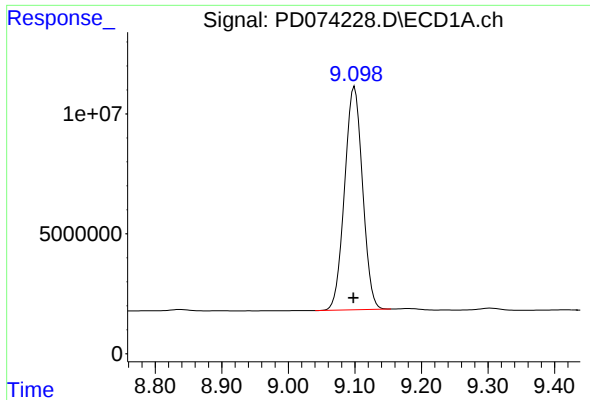

#28 Decachlorobiphenyl

R.T.: 9.099 min
Delta R.T.: 0.002 min
Response: 174362901
Conc: 71.08 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

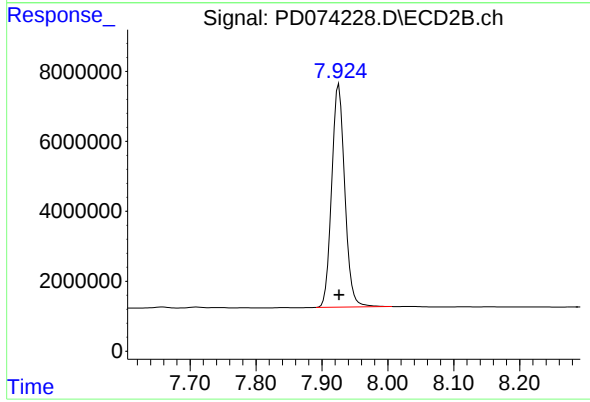

#28 Decachlorobiphenyl

R.T.: 7.926 min
Delta R.T.: 0.000 min
Response: 87904432
Conc: 71.44 ng/ml