

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031523\
 Data File : PD074229.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Mar 2023 10:34
 Operator : AR\AJ
 Sample : PCHLORICC500
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 15 12:02:08 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031423.M
 Quant Title : GC Extractables
 QLast Update : Wed Mar 15 12:01:09 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.551	2.771	117.2E6	74165998	50.000	50.000
28)	SA Decachlor...	9.098	7.926	122.7E6	61519985	50.000	50.000
Target Compounds							
23)	Chlordane-1	4.718	3.773	63525940	25694790	500.000	500.000
24)	Chlordane-2	5.249	4.350	66240973	29480446	500.000	500.000
25)	Chlordane-3	5.962	4.982	254.6E6	86338157	500.000	500.000
26)	Chlordane-4	6.045	5.046	306.5E6	81891806	500.000	500.000
27)	Chlordane-5	6.896	5.943	51909196	31099909	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031523\
Data File : PD074229.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Mar 2023 10:34
Operator : AR\AJ
Sample : PCHLORICC500
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 15 12:02:08 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031423.M
Quant Title : GC Extractables
QLast Update : Wed Mar 15 12:01:09 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

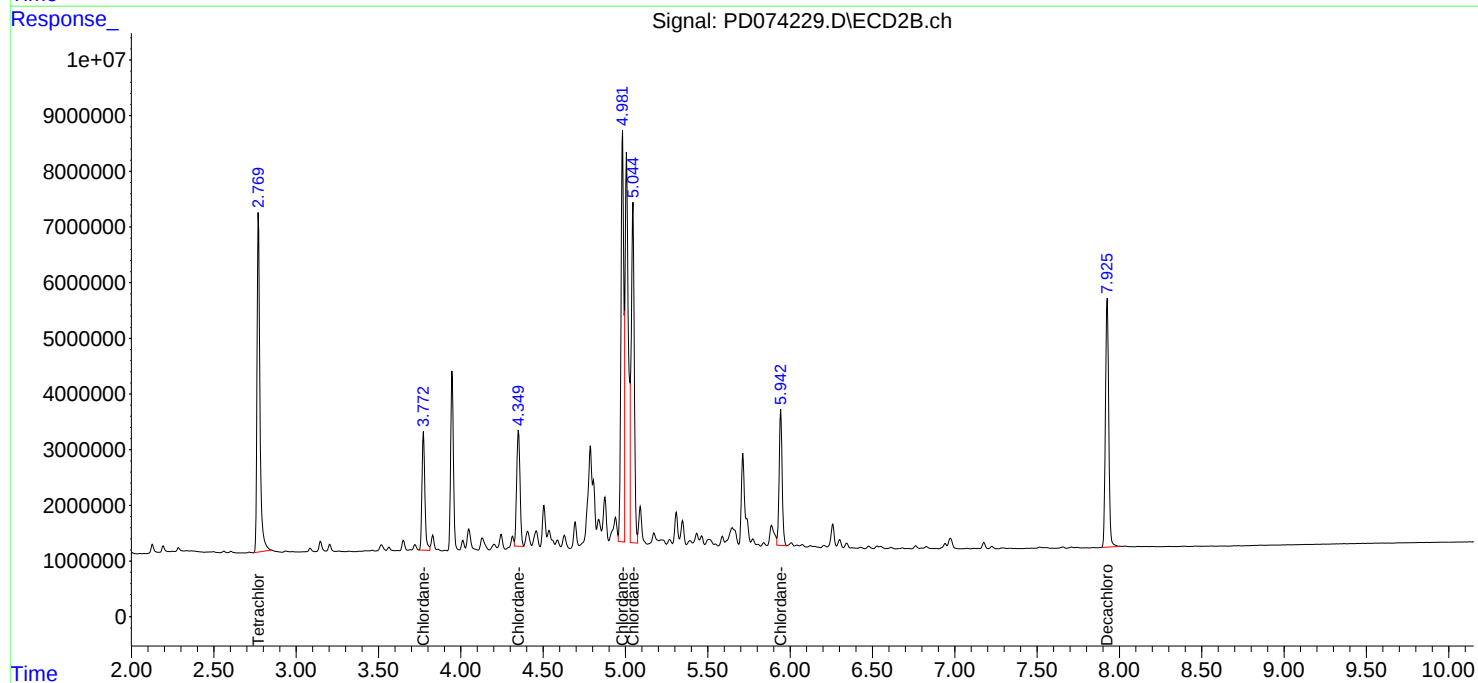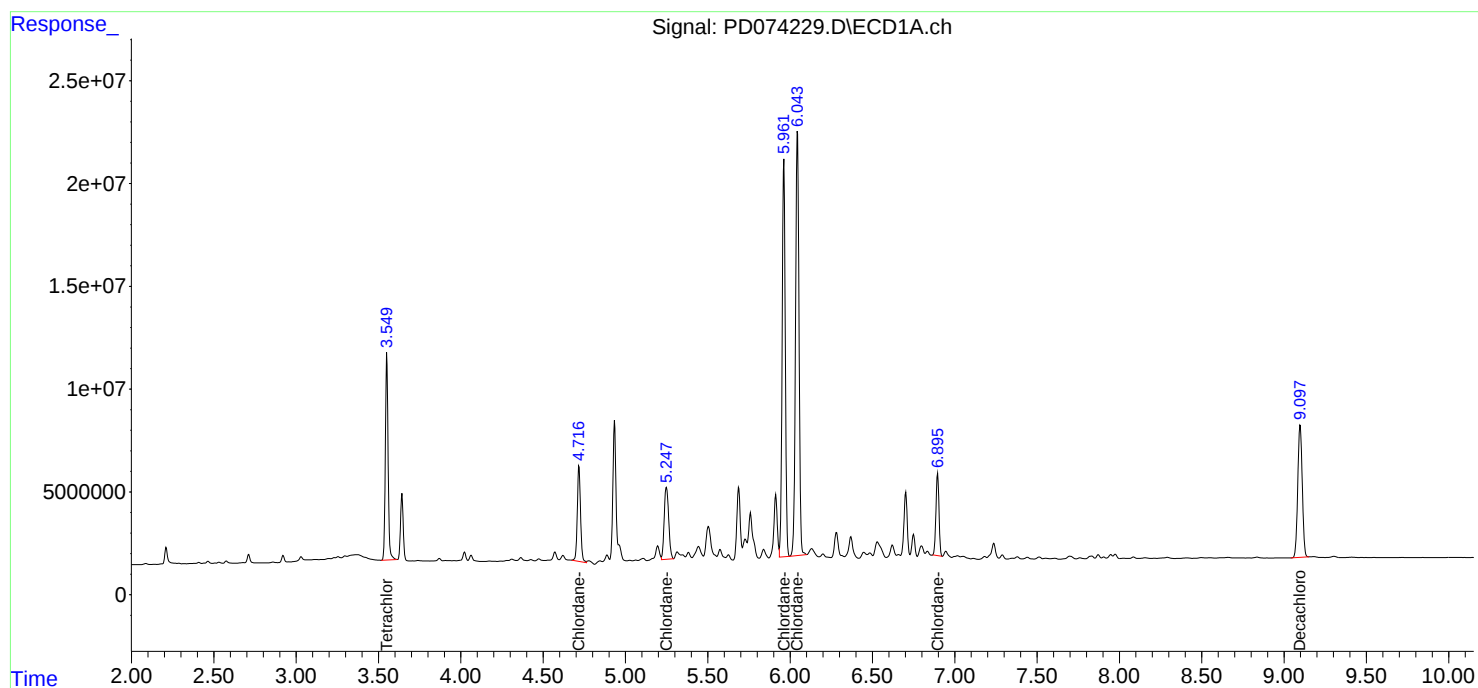


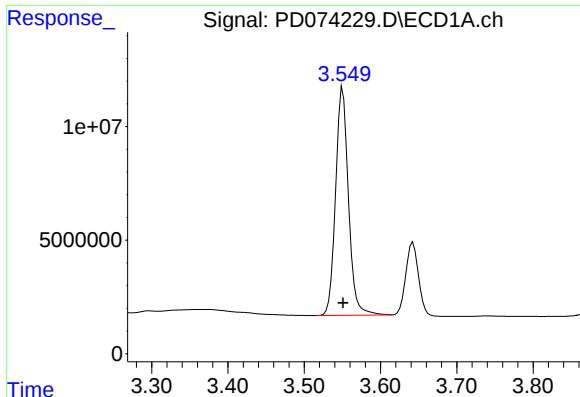

#1 Tetrachloro-m-xylene


R.T.: 3.551 min
Delta R.T.: 0.000 min
Response: 117156407
Conc: 50.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

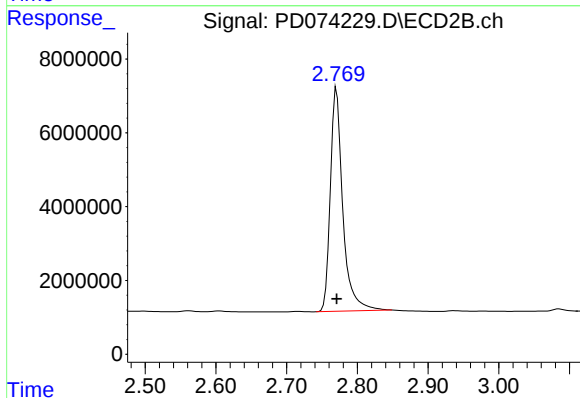


#1 Tetrachloro-m-xylene

R.T.: 2.771 min
Delta R.T.: 0.000 min
Response: 74165998
Conc: 50.00 ng/ml

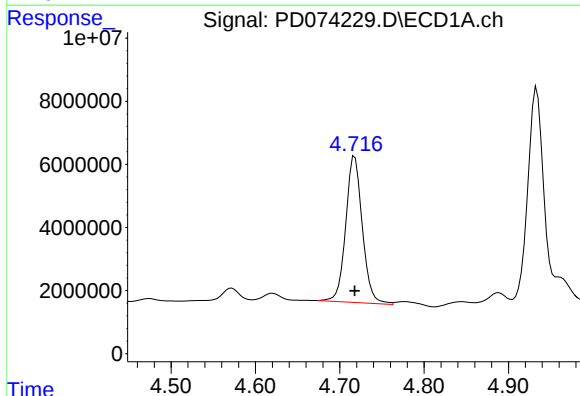


#23 Chlordane-1

R.T.: 4.718 min
Delta R.T.: 0.000 min
Response: 63525940
Conc: 500.00 ng/ml

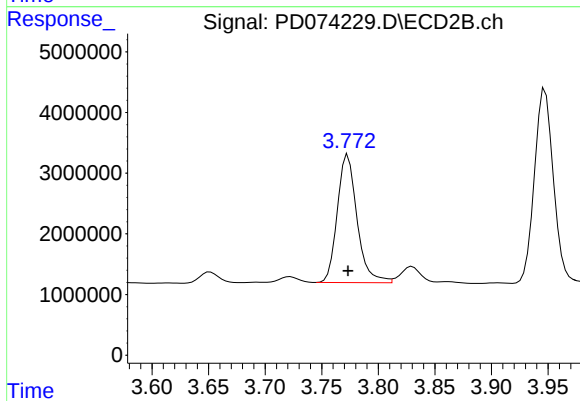

#23 Chlordane-1


R.T.: 3.773 min
Delta R.T.: 0.000 min
Response: 25694790
Conc: 500.00 ng/ml

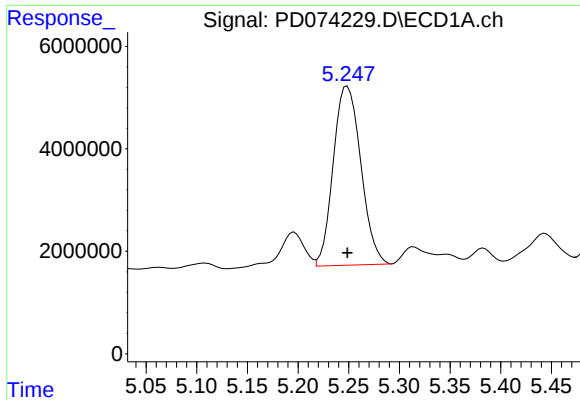

#24 Chlordane-2


R.T.: 5.249 min
Delta R.T.: 0.000 min
Response: 66240973
Conc: 500.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

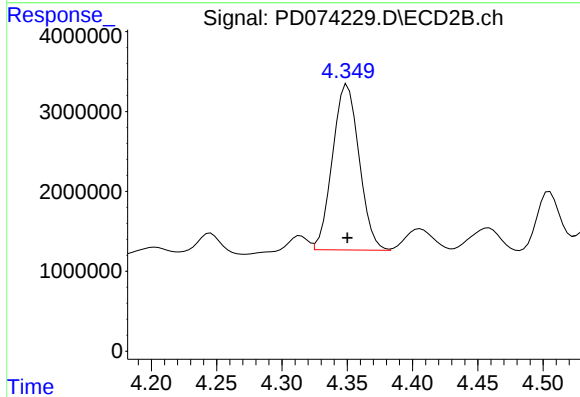


#24 Chlordane-2

R.T.: 4.350 min
Delta R.T.: 0.000 min
Response: 29480446
Conc: 500.00 ng/ml

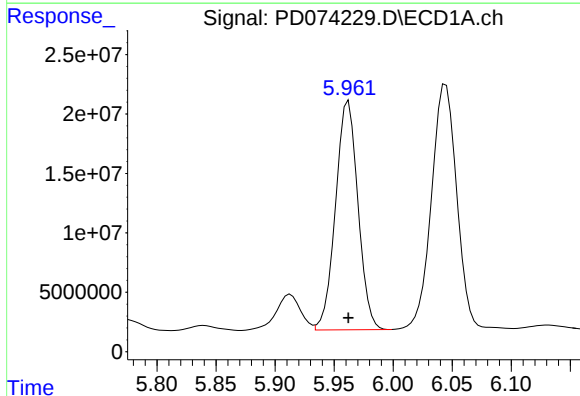


#25 Chlordane-3

R.T.: 5.962 min
Delta R.T.: 0.000 min
Response: 254551273
Conc: 500.00 ng/ml

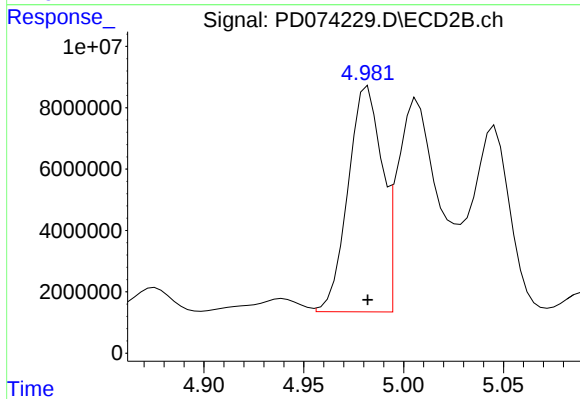

#25 Chlordane-3


R.T.: 4.982 min
Delta R.T.: 0.000 min
Response: 86338157
Conc: 500.00 ng/ml

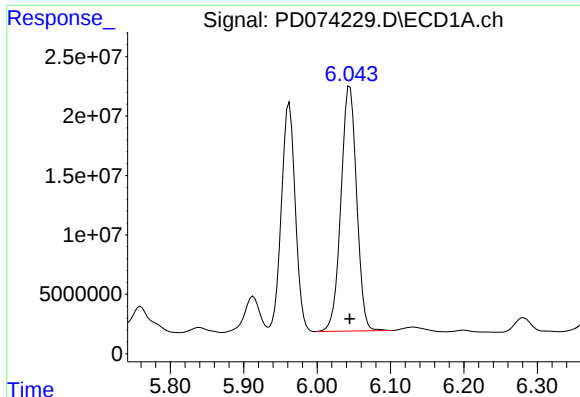

#26 Chlordane-4


R.T.: 6.045 min
Delta R.T.: 0.000 min
Response: 306484624
Conc: 500.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

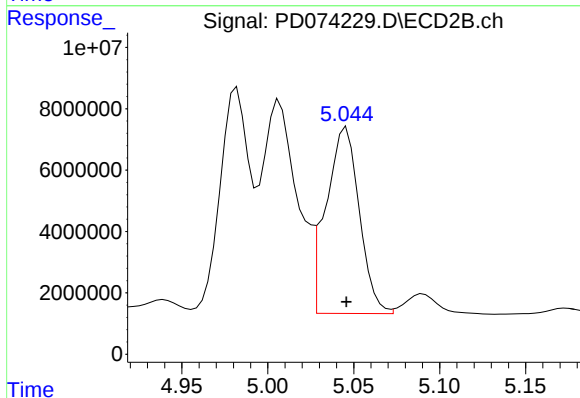


#26 Chlordane-4

R.T.: 5.046 min
Delta R.T.: 0.000 min
Response: 81891806
Conc: 500.00 ng/ml

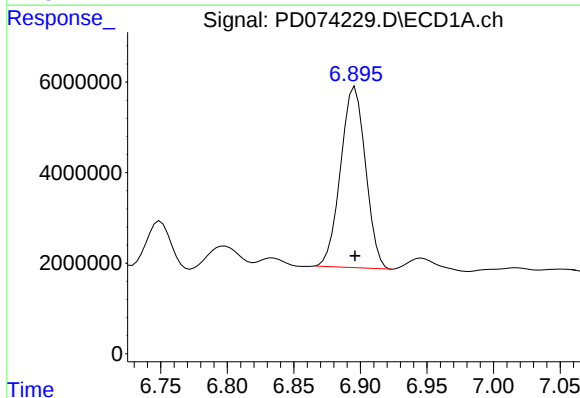


#27 Chlordane-5

R.T.: 6.896 min
Delta R.T.: 0.000 min
Response: 51909196
Conc: 500.00 ng/ml

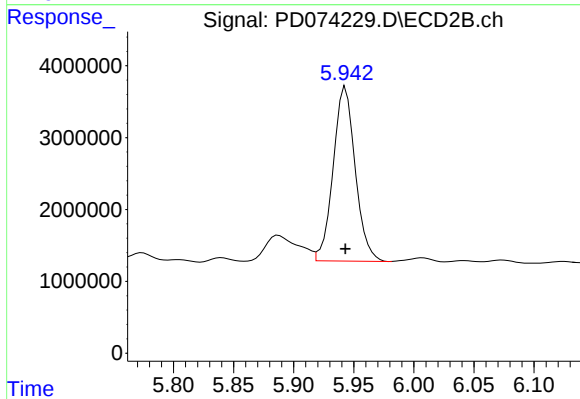

#27 Chlordane-5


R.T.: 5.943 min
Delta R.T.: 0.000 min
Response: 31099909
Conc: 500.00 ng/ml

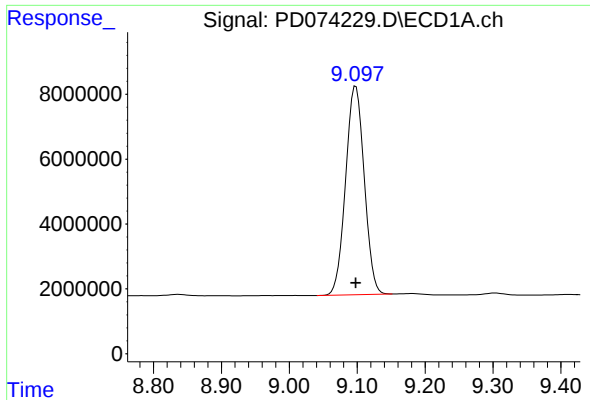

#28 Decachlorobiphenyl

R.T.: 9.098 min
Delta R.T.: 0.000 min
Response: 122650845
Conc: 50.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

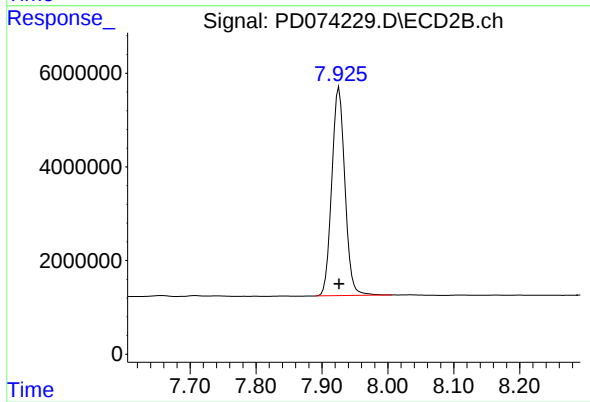

#28 Decachlorobiphenyl

R.T.: 7.926 min
Delta R.T.: 0.000 min
Response: 61519985
Conc: 50.00 ng/ml