

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031523\
 Data File : PD074230.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Mar 2023 11:03
 Operator : AR\AJ
 Sample : PCHLORICC250
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 15 12:02:14 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031423.M
 Quant Title : GC Extractables
 QLast Update : Wed Mar 15 12:01:09 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.557	2.769	56904545	36475311	24.286	24.590
28)	SA Decachlor...	9.106	7.928	65220102	31660152	26.588	25.732
Target Compounds							
23)	Chlordane-1	4.724	3.772	29398264	12545772	231.388	244.131
24)	Chlordane-2	5.255	4.350	33676697	14682006	254.198	249.013
25)	Chlordane-3	5.968	4.982	119.1E6	40953625	233.973	237.170
26)	Chlordane-4	6.050	5.046	145.9E6	40331863	238.029	246.251
27)	Chlordane-5	6.903	5.943	25508225	14995872	245.700	241.092



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031523\
Data File : PD074230.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Mar 2023 11:03
Operator : AR\AJ
Sample : PCHLORICC250
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 15 12:02:14 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031423.M
Quant Title : GC Extractables
QLast Update : Wed Mar 15 12:01:09 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

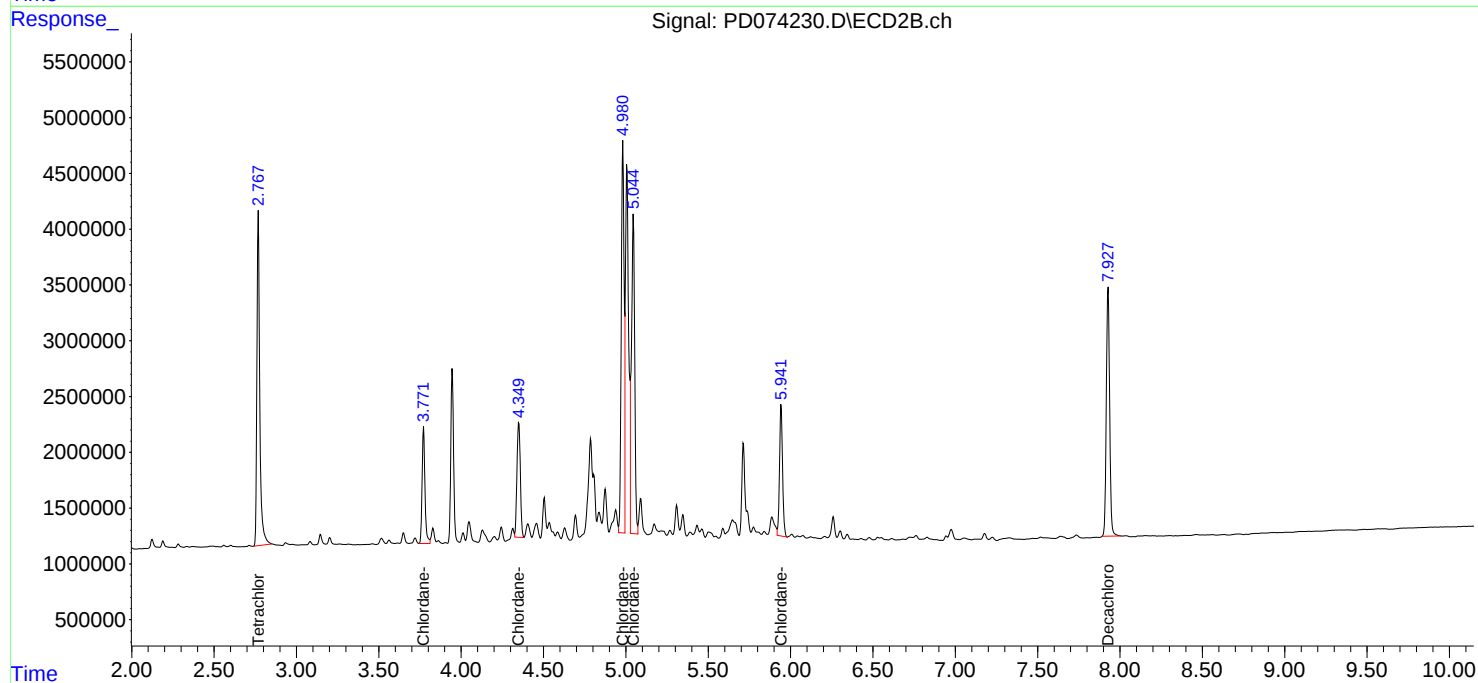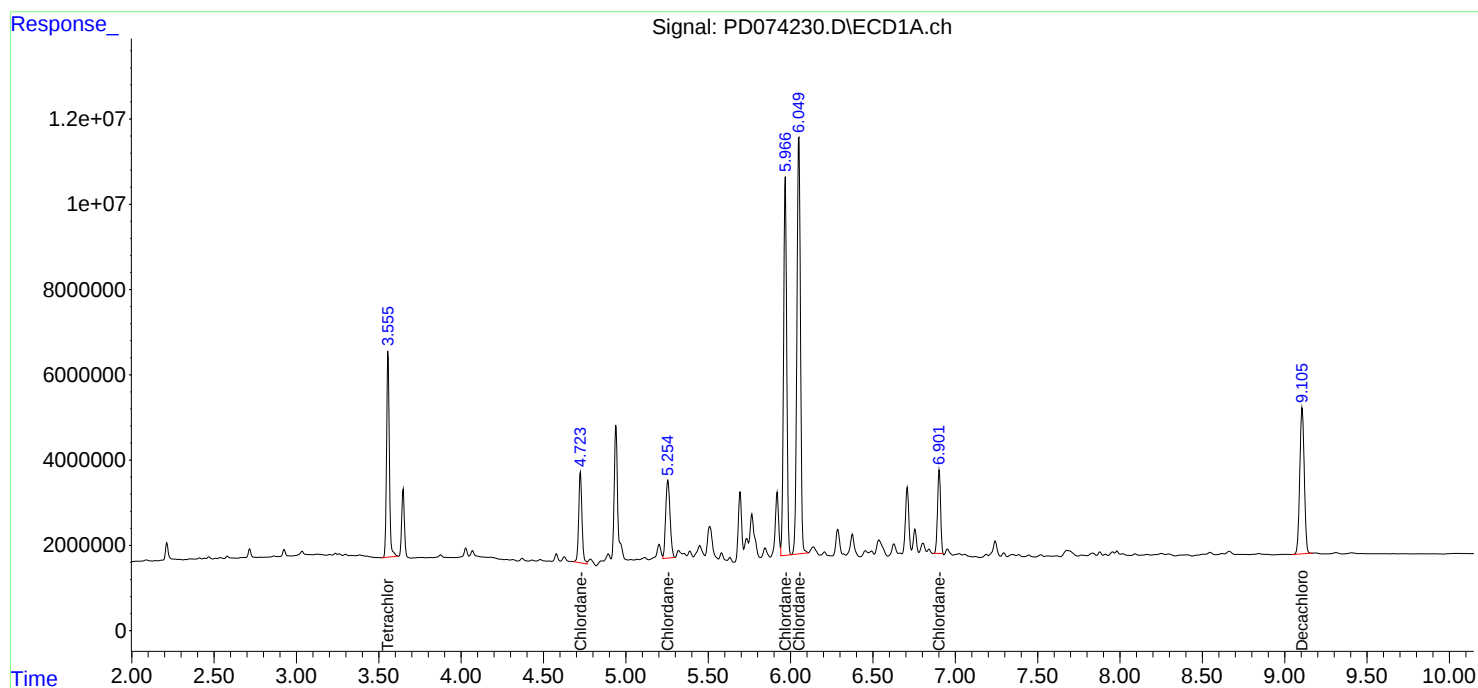


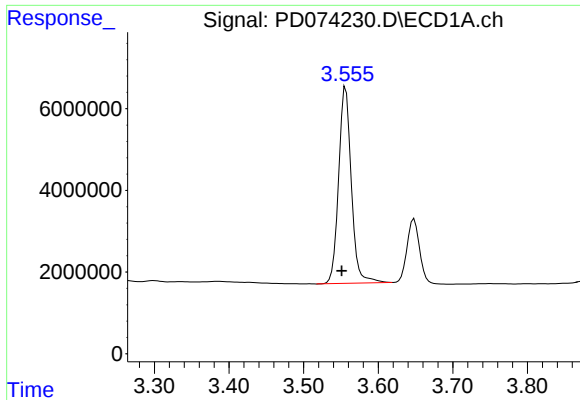

#1 Tetrachloro-m-xylene


R.T.: 3.557 min
Delta R.T.: 0.006 min
Response: 56904545
Conc: 24.29 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

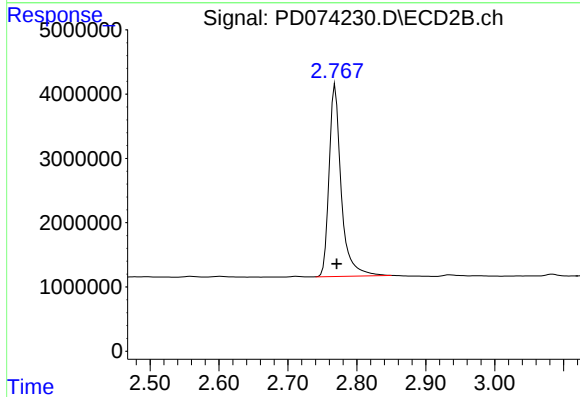


#1 Tetrachloro-m-xylene

R.T.: 2.769 min
Delta R.T.: -0.002 min
Response: 36475311
Conc: 24.59 ng/ml

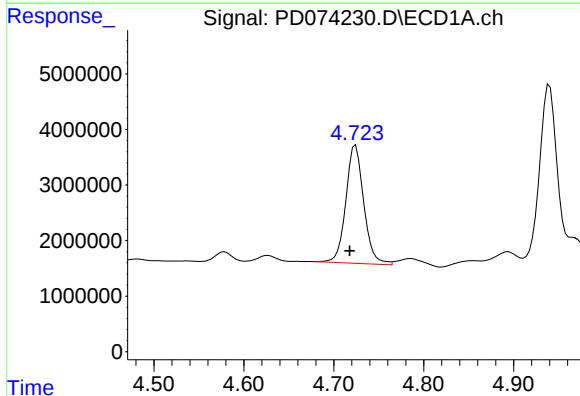


#23 Chlordane-1

R.T.: 4.724 min
Delta R.T.: 0.006 min
Response: 29398264
Conc: 231.39 ng/ml

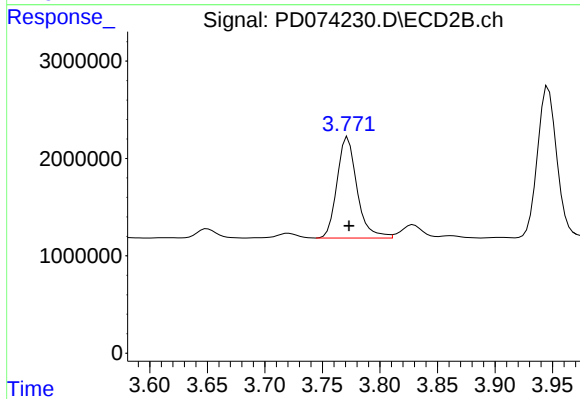

#23 Chlordane-1


R.T.: 3.772 min
Delta R.T.: -0.001 min
Response: 12545772
Conc: 244.13 ng/ml

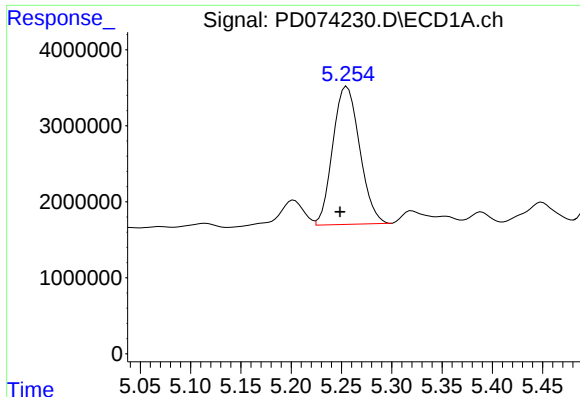

#24 Chlordane-2


R.T.: 5.255 min
Delta R.T.: 0.007 min
Response: 33676697
Conc: 254.20 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

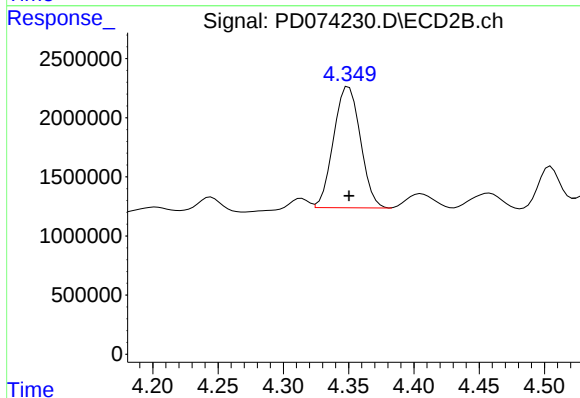


#24 Chlordane-2

R.T.: 4.350 min
Delta R.T.: 0.000 min
Response: 14682006
Conc: 249.01 ng/ml

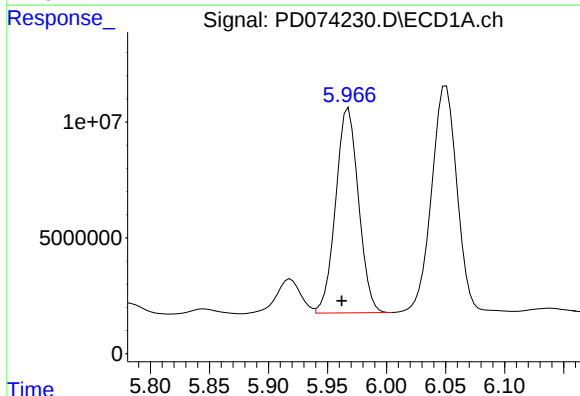


#25 Chlordane-3

R.T.: 5.968 min
Delta R.T.: 0.006 min
Response: 119116242
Conc: 233.97 ng/ml

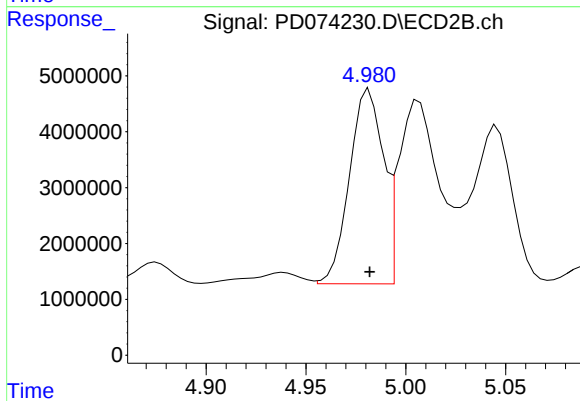

#25 Chlordane-3


R.T.: 4.982 min
Delta R.T.: 0.000 min
Response: 40953625
Conc: 237.17 ng/ml

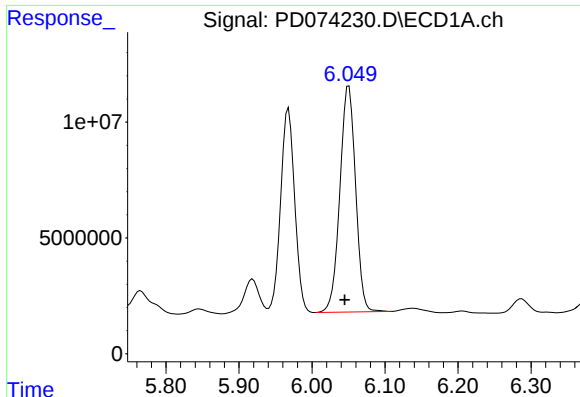

#26 Chlordane-4


R.T.: 6.050 min
Delta R.T.: 0.006 min
Response: 145904568
Conc: 238.03 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

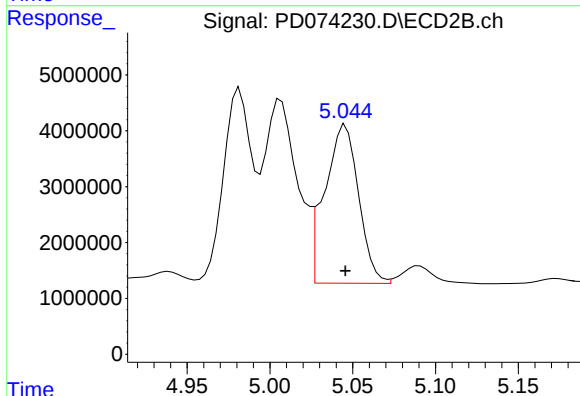


#26 Chlordane-4

R.T.: 5.046 min
Delta R.T.: 0.000 min
Response: 40331863
Conc: 246.25 ng/ml

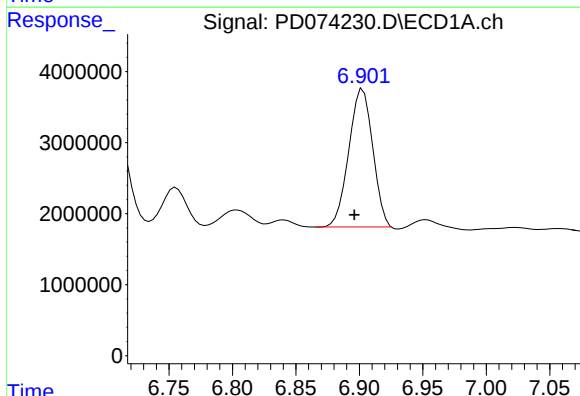


#27 Chlordane-5

R.T.: 6.903 min
Delta R.T.: 0.007 min
Response: 25508225
Conc: 245.70 ng/ml

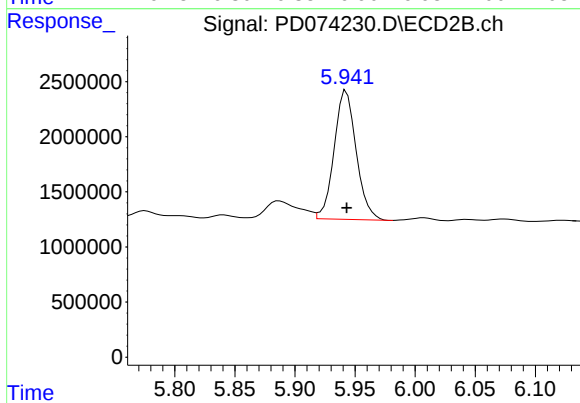

#27 Chlordane-5


R.T.: 5.943 min
Delta R.T.: 0.000 min
Response: 14995872
Conc: 241.09 ng/ml

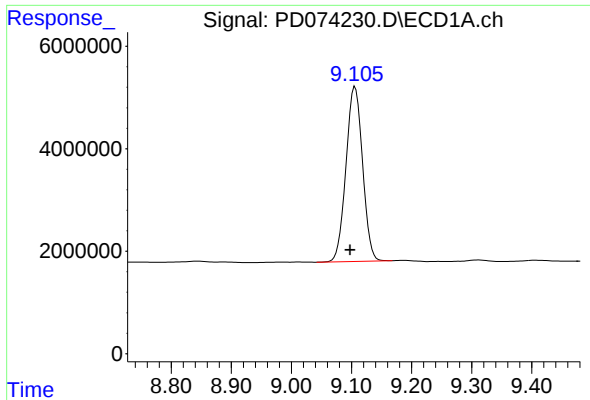

#28 Decachlorobiphenyl

R.T.: 9.106 min
Delta R.T.: 0.008 min
Response: 65220102
Conc: 26.59 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

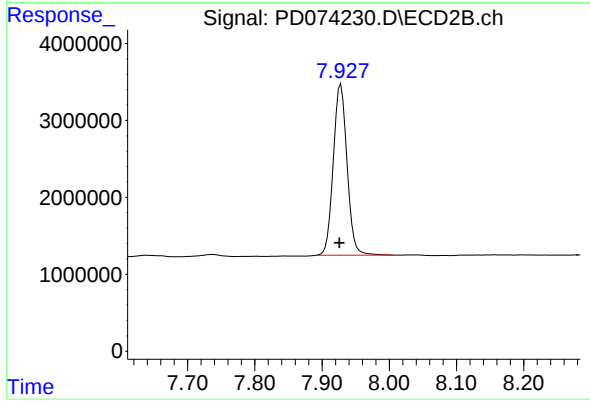

#28 Decachlorobiphenyl

R.T.: 7.928 min
Delta R.T.: 0.002 min
Response: 31660152
Conc: 25.73 ng/ml