

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031523\
 Data File : PD074232.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Mar 2023 12:01
 Operator : AR\AJ
 Sample : PCHLORICV500
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 ICVPD031523

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 15 12:20:52 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031423.M
 Quant Title : GC Extractables
 QLast Update : Wed Mar 15 12:20:10 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.555	2.770	115.0E6	73203321	50.126	50.324
28)	SA Decachlor...	9.101	7.926	123.3E6	61205279	48.849	49.611
Target Compounds							
23)	Chlordane-1	4.722	3.773	56724975	25043979	475.725	496.979
24)	Chlordane-2	5.252	4.350	65159216	28846359	486.299	494.952
25)	Chlordane-3	5.965	4.982	251.8E6	84417801	508.914	502.916
26)	Chlordane-4	6.047	5.046	303.6E6	81356295	505.376	504.273
27)	Chlordane-5	6.899	5.943	51349206	30557421	498.329	506.228



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031523\
Data File : PD074232.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Mar 2023 12:01
Operator : AR\AJ
Sample : PCHLORICV500
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
ICVPD031523

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 15 12:20:52 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031423.M
Quant Title : GC Extractables
QLast Update : Wed Mar 15 12:20:10 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

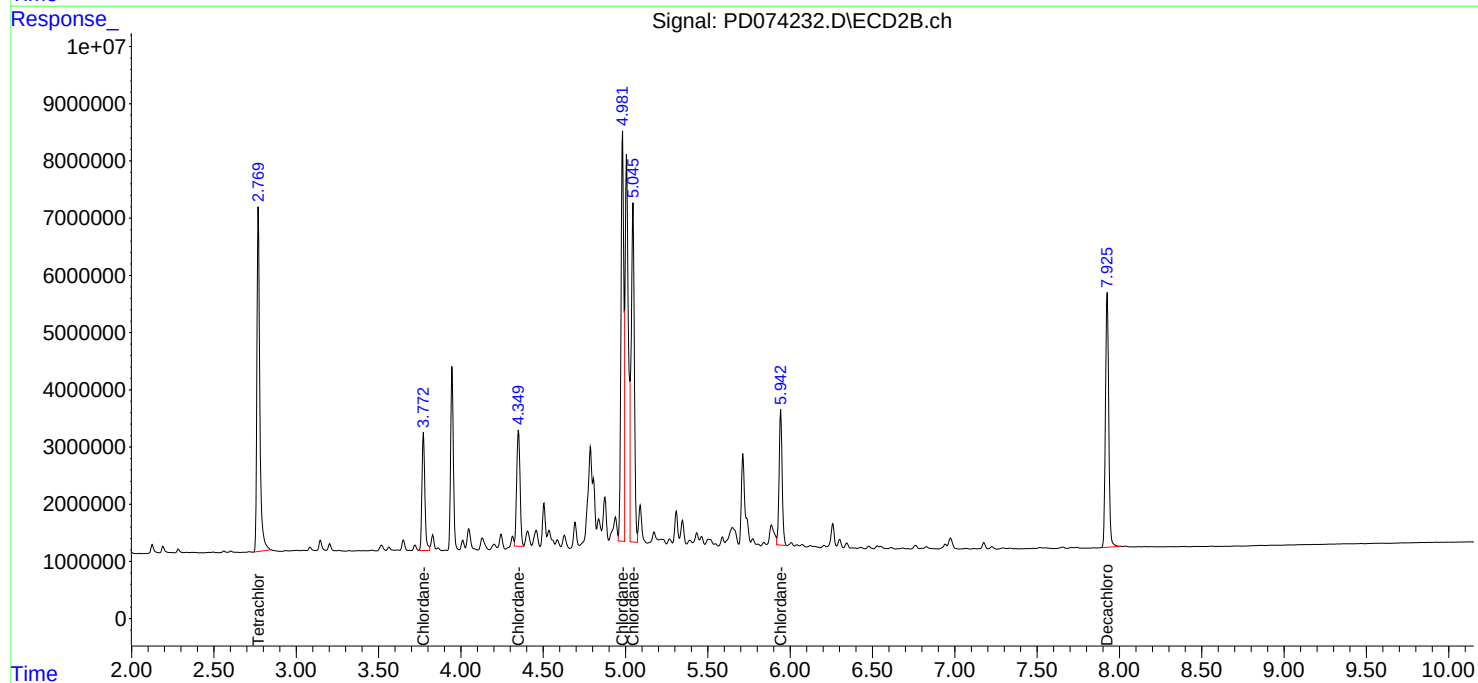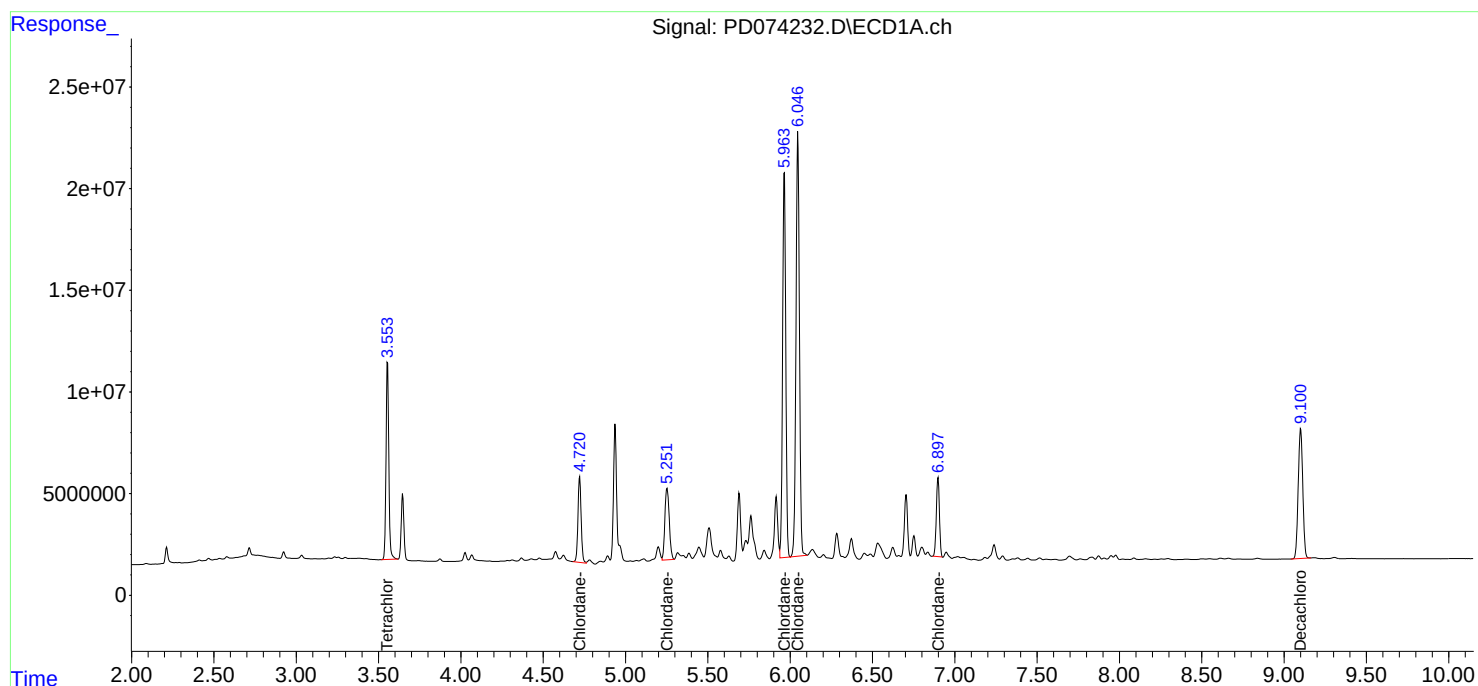


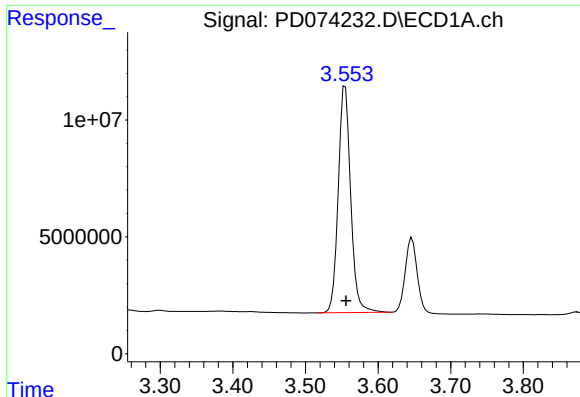

#1 Tetrachloro-m-xylene


R.T.: 3.555 min
Delta R.T.: -0.001 min
Response: 115047895
Conc: 50.13 ng/ml

Instrument :
ECD_D
ClientSampleId :
ICVPD031523

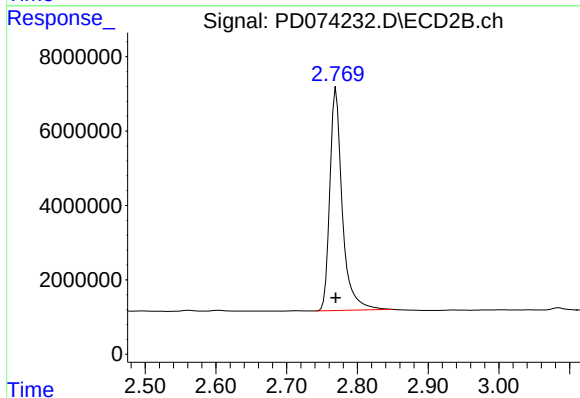


#1 Tetrachloro-m-xylene

R.T.: 2.770 min
Delta R.T.: 0.000 min
Response: 73203321
Conc: 50.32 ng/ml

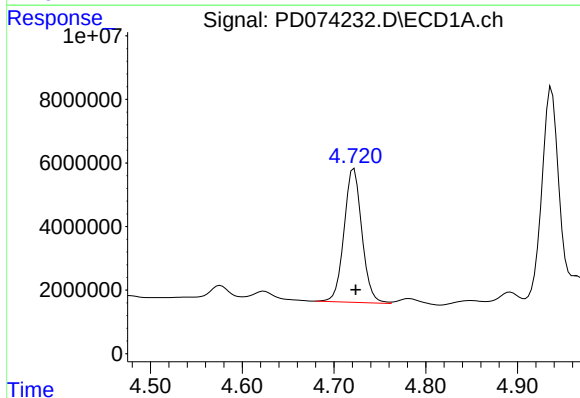


#23 Chlordane-1

R.T.: 4.722 min
Delta R.T.: -0.002 min
Response: 56724975
Conc: 475.72 ng/ml

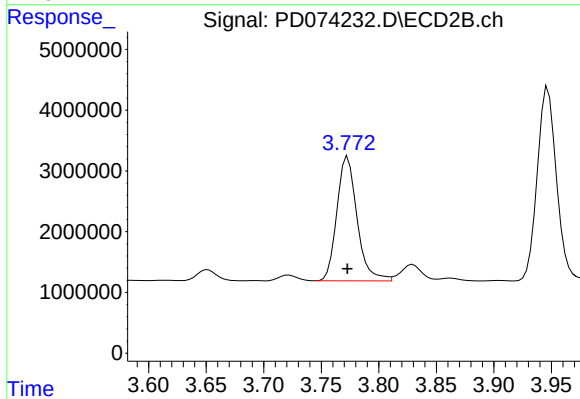

#23 Chlordane-1


R.T.: 3.773 min
Delta R.T.: 0.000 min
Response: 25043979
Conc: 496.98 ng/ml

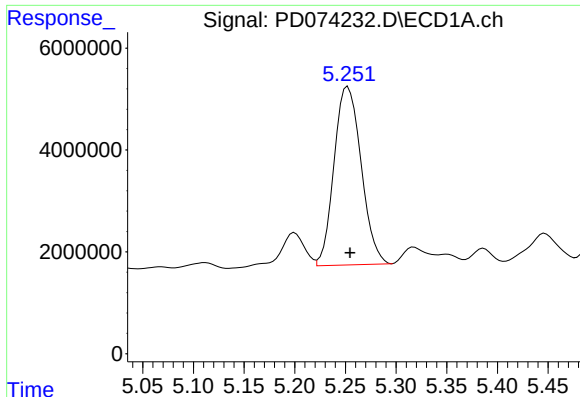

#24 Chlordane-2


R.T.: 5.252 min
Delta R.T.: -0.002 min
Response: 65159216
Conc: 486.30 ng/ml

Instrument :
ECD_D
ClientSampleId :
ICVPD031523

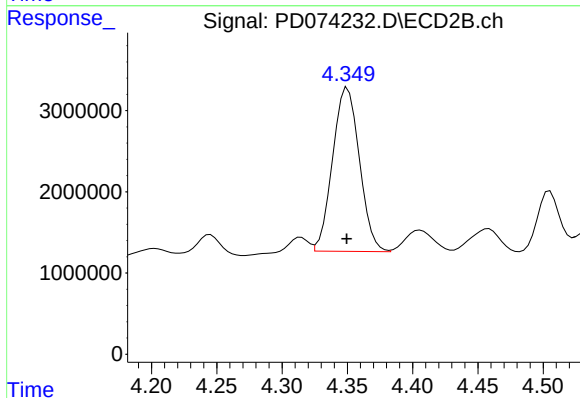


#24 Chlordane-2

R.T.: 4.350 min
Delta R.T.: 0.000 min
Response: 28846359
Conc: 494.95 ng/ml

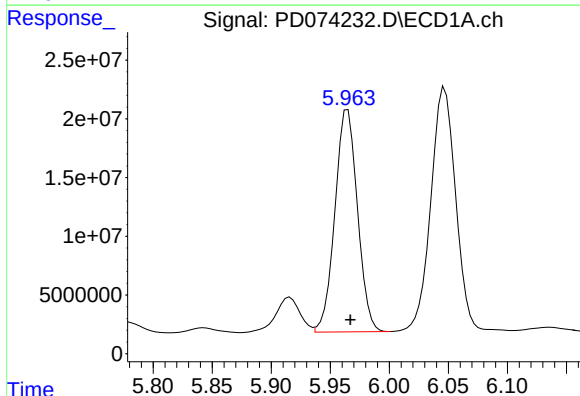


#25 Chlordane-3

R.T.: 5.965 min
Delta R.T.: -0.002 min
Response: 251756458
Conc: 508.91 ng/ml

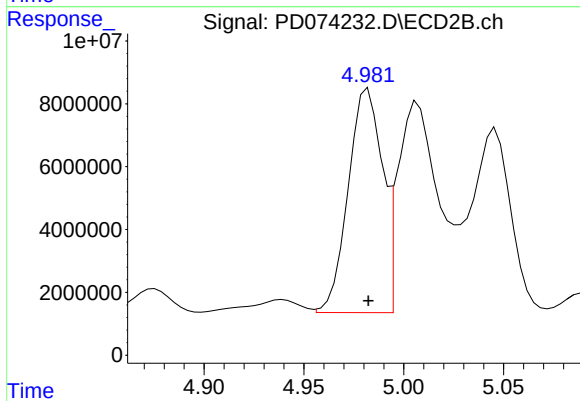

#25 Chlordane-3


R.T.: 4.982 min
Delta R.T.: 0.000 min
Response: 84417801
Conc: 502.92 ng/ml

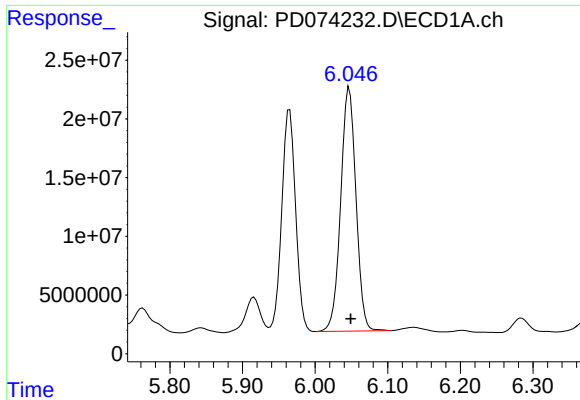

#26 Chlordane-4


R.T.: 6.047 min
Delta R.T.: -0.002 min
Response: 303598010
Conc: 505.38 ng/ml

Instrument :
ECD_D
ClientSampleId :
ICVPD031523

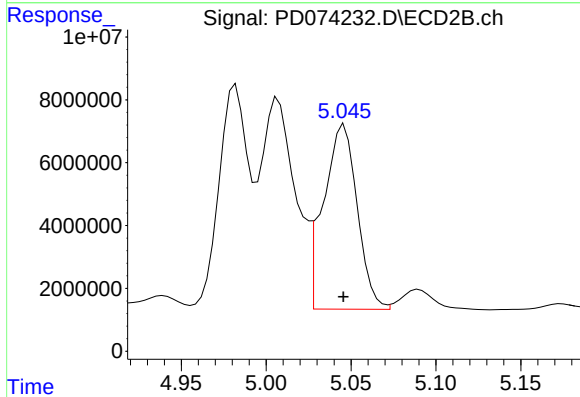


#26 Chlordane-4

R.T.: 5.046 min
Delta R.T.: 0.000 min
Response: 81356295
Conc: 504.27 ng/ml

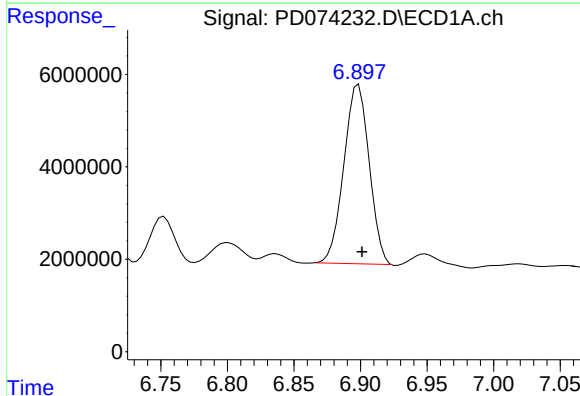


#27 Chlordane-5

R.T.: 6.899 min
Delta R.T.: -0.003 min
Response: 51349206
Conc: 498.33 ng/ml

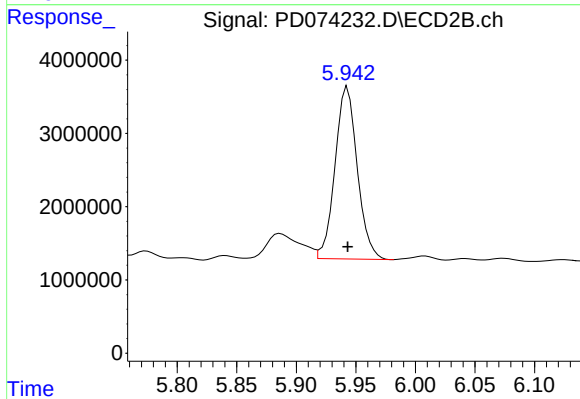

#27 Chlordane-5


R.T.: 5.943 min
Delta R.T.: 0.000 min
Response: 30557421
Conc: 506.23 ng/ml

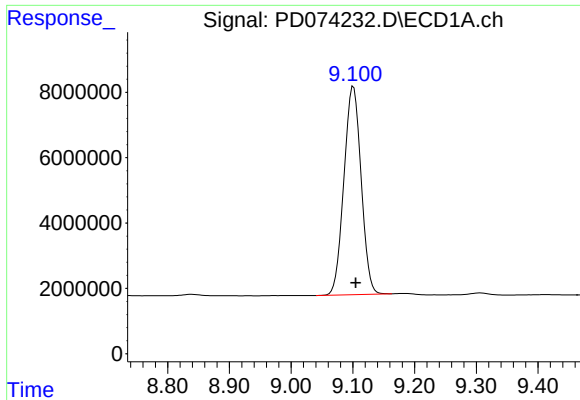

#28 Decachlorobiphenyl

R.T.: 9.101 min
Delta R.T.: -0.004 min
Response: 123328014
Conc: 48.85 ng/ml

Instrument :
ECD_D
ClientSampleId :
ICVPD031523

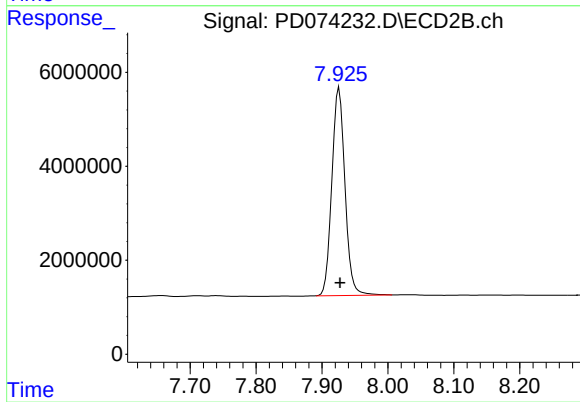

#28 Decachlorobiphenyl

R.T.: 7.926 min
Delta R.T.: -0.001 min
Response: 61205279
Conc: 49.61 ng/ml