

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD032322\
 Data File : PD068738.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Mar 2022 18:14
 Operator : AR\AJ
 Sample : PIBLK251
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 23 06:54:53 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031322CLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Mar 14 07:24:04 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.445	4.171	26492479	214.3E6	19.454	19.577
2)	SA Decachlor...	8.204	9.367	55527703	259.8E6	39.932	41.187
Target Compounds							
7)	B delta-BHC	0.000	5.225f	0	1040199	N.D.	<MDL
8)	B Heptachlo...	0.000	6.148f	0	2382427	N.D.	0.198


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD032322\
Data File : PD068738.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Mar 2022 18:14
Operator : AR\AJ
Sample : PIBLK251
Misc :
ALS Vial : 2 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 23 06:54:53 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031322CLP.M
Quant Title : GC Extractables
QLast Update : Mon Mar 14 07:24:04 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

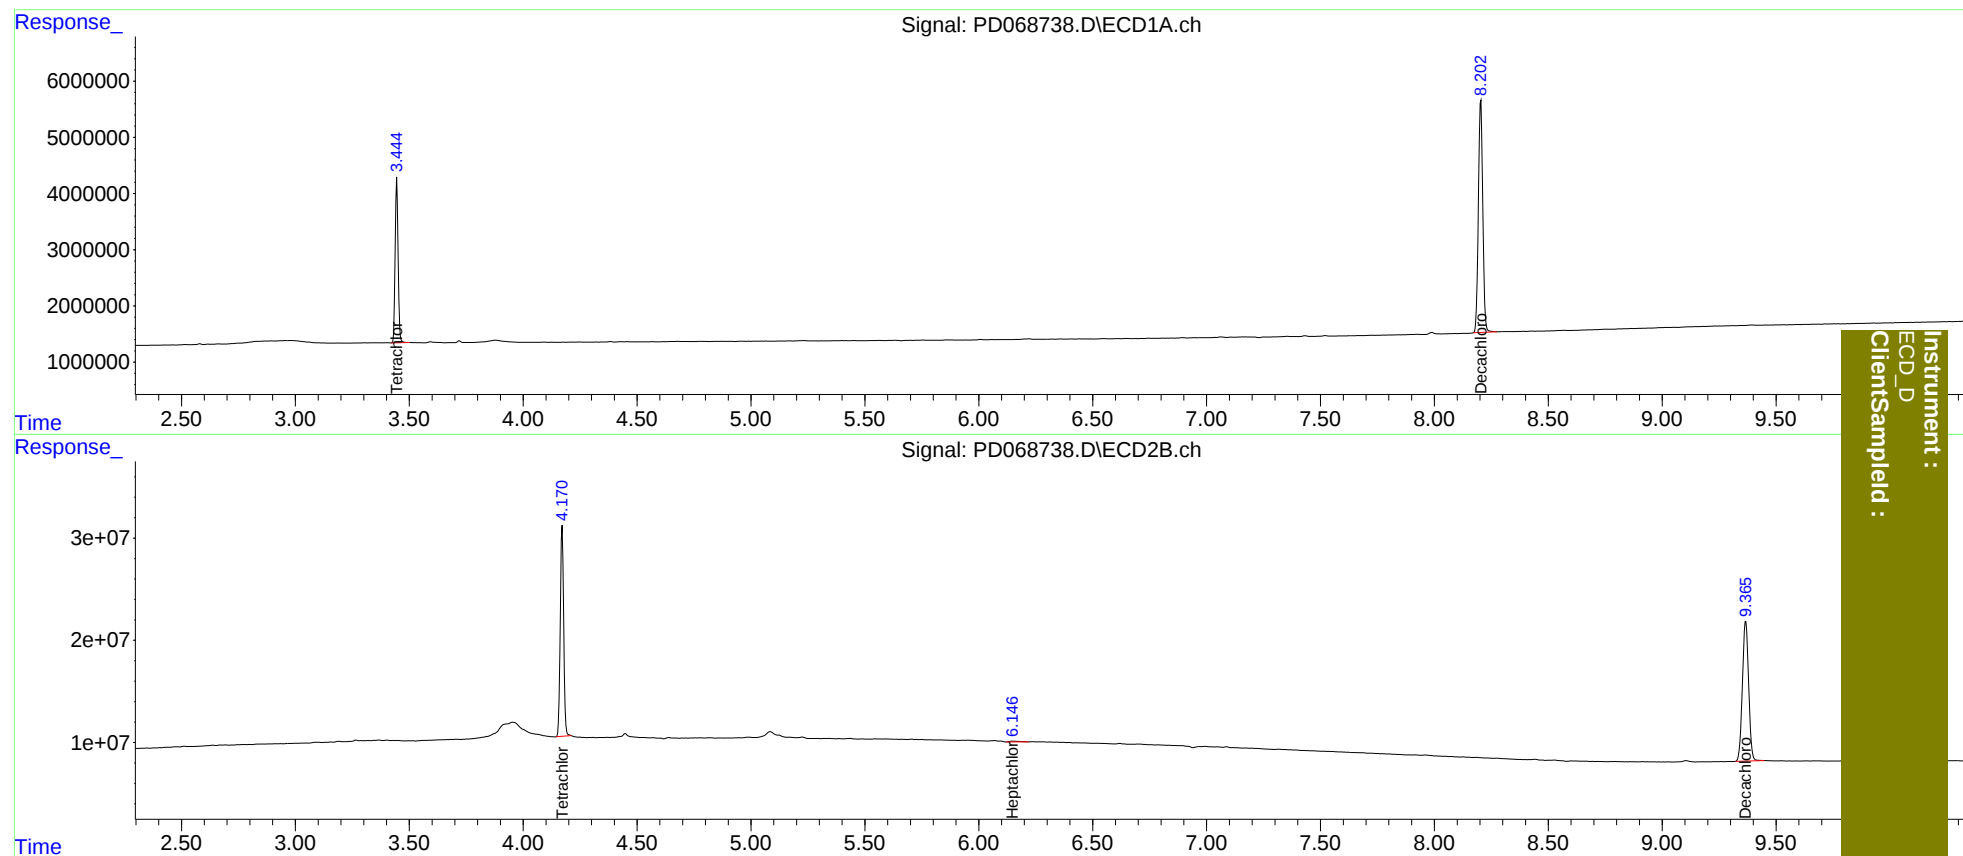


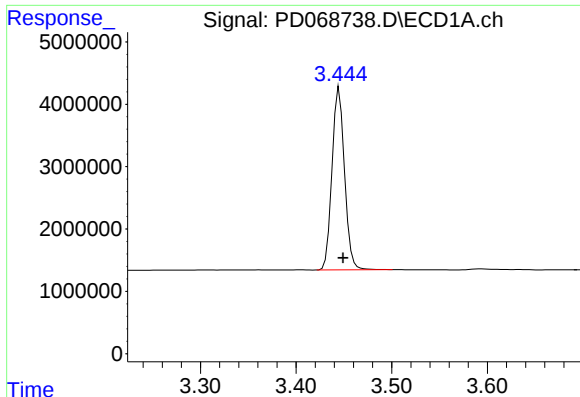

#1 Tetrachloro-m-xylene


R.T.: 3.445 min
Delta R.T.: -0.004 min
Response: 26492479
Conc: 19.45 ng/ml

Instrument :
ECD_D
ClientSampleId :

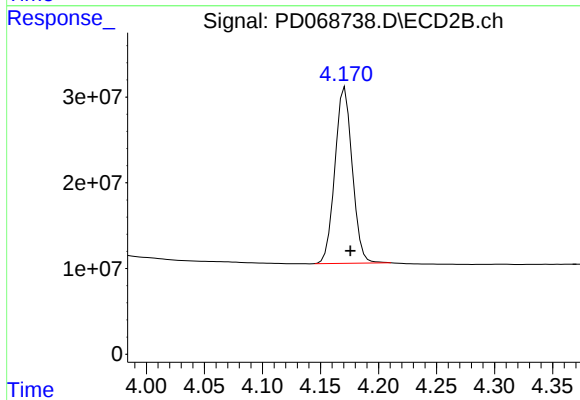


#1 Tetrachloro-m-xylene

R.T.: 4.171 min
Delta R.T.: -0.005 min
Response: 214275112
Conc: 19.58 ng/ml

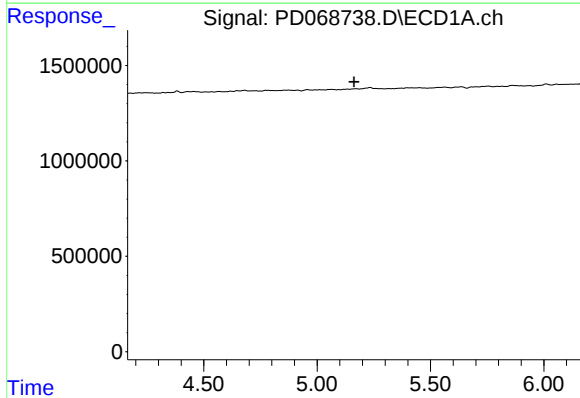


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.163 min
Response: 0
Conc: N.D.

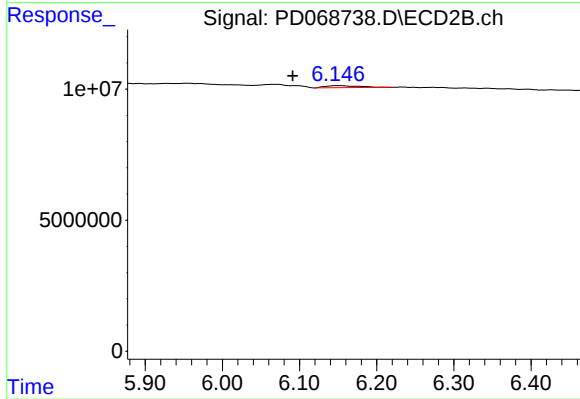

#8 Heptachlor epoxide


R.T.: 6.148 min
Delta R.T.: 0.057 min
Response: 2382427
Conc: 0.20 ng/ml

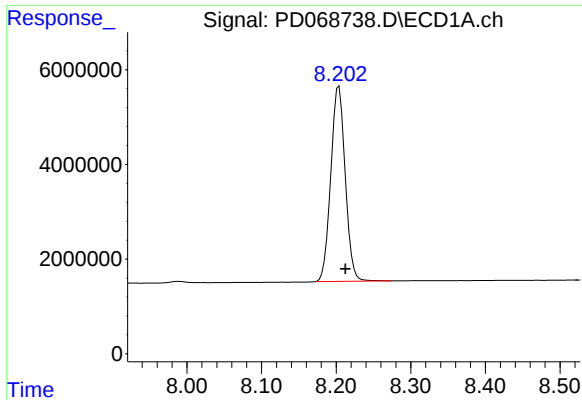

#27 Decachlorobiphenyl

R.T.: 8.204 min
Delta R.T.: -0.008 min
Response: 55527703
Conc: 39.93 ng/ml

Instrument :
ECD_D
ClientSampleId :

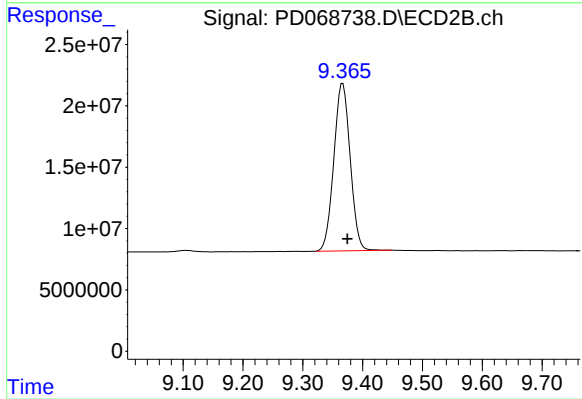

#27 Decachlorobiphenyl

R.T.: 9.367 min
Delta R.T.: -0.008 min
Response: 259772448
Conc: 41.19 ng/ml