

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD033021\
 Data File : PD061879.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Mar 2021 17:46
 Operator : AR\AJ
 Sample : M1828-05
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 31 04:29:57 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032921.M
 Quant Title : GC Extractables
 QLast Update : Tue Mar 30 04:47:56 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.485	3.982	9802794	94567136	11.708	10.884
28)	SA Decachlor...	8.256	9.039	11850813	75498455	9.631	7.997
Target Compounds							
2)	A alpha-BHC	0.000	4.368	0	2585109	N.D.	0.192 #
5)	MB Aldrin	4.747f	5.470	8799244	9107760	7.332	0.732 #
6)	B beta-BHC	4.458	0.000	4839943	0	8.875	N.D. #
7)	B delta-BHC	0.000	5.014f	0	56713270	N.D.	4.288 #
8)	B Heptachlo...	5.211	0.000	7287769	0	6.357	N.D. #
9)	A Endosulfan I	0.000	6.235f	0	9834377	N.D.	0.907 #
15)	B Endosulfa...	0.000	6.897	0	9193930	N.D.	0.968 #
24)	Chlordane-2	0.000	5.470f	0	9107760	N.D.	23.736 #
27)	Chlordane-5	0.000	6.946f	0	12773161	N.D.	35.442 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD033021\
 Data File : PD061879.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Mar 2021 17:46
 Operator : AR\AJ
 Sample : M1828-05
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampled :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 31 04:29:57 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032921.M
 Quant Title : GC Extractables
 QLast Update : Tue Mar 30 04:47:56 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

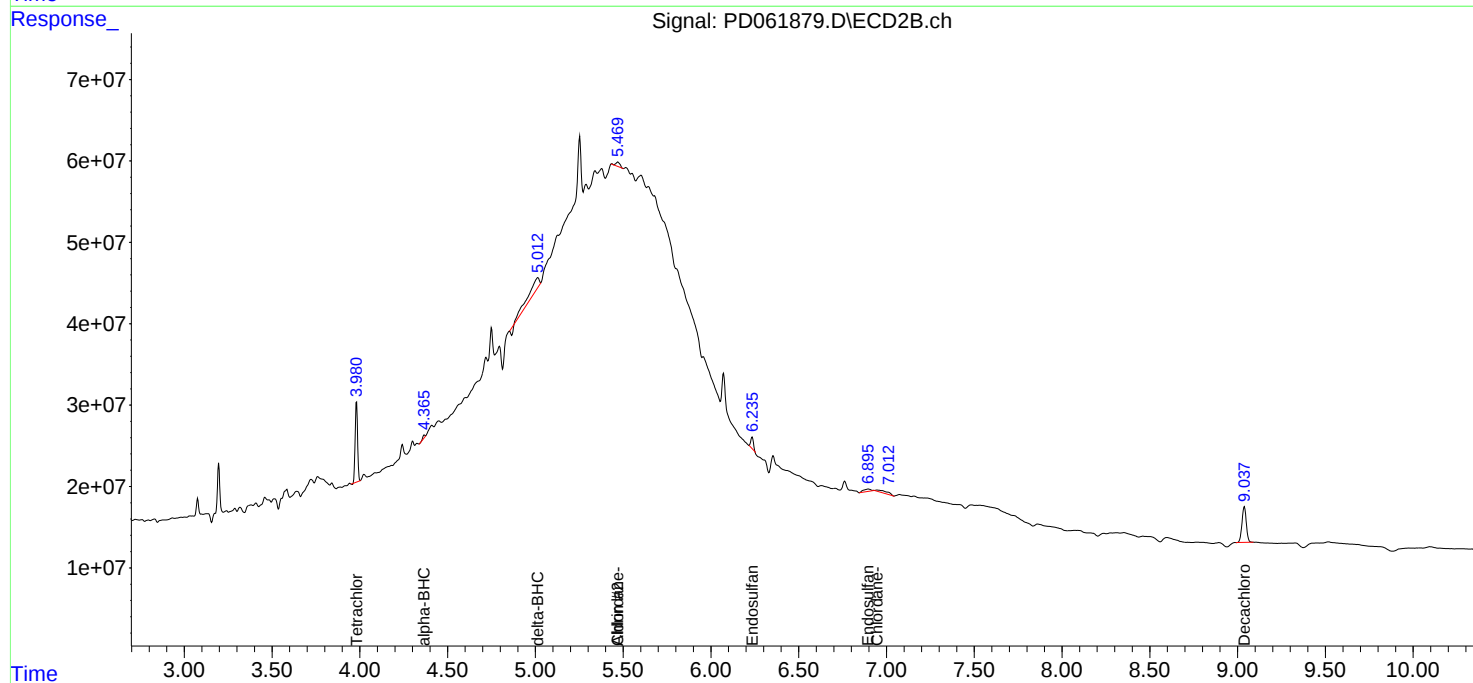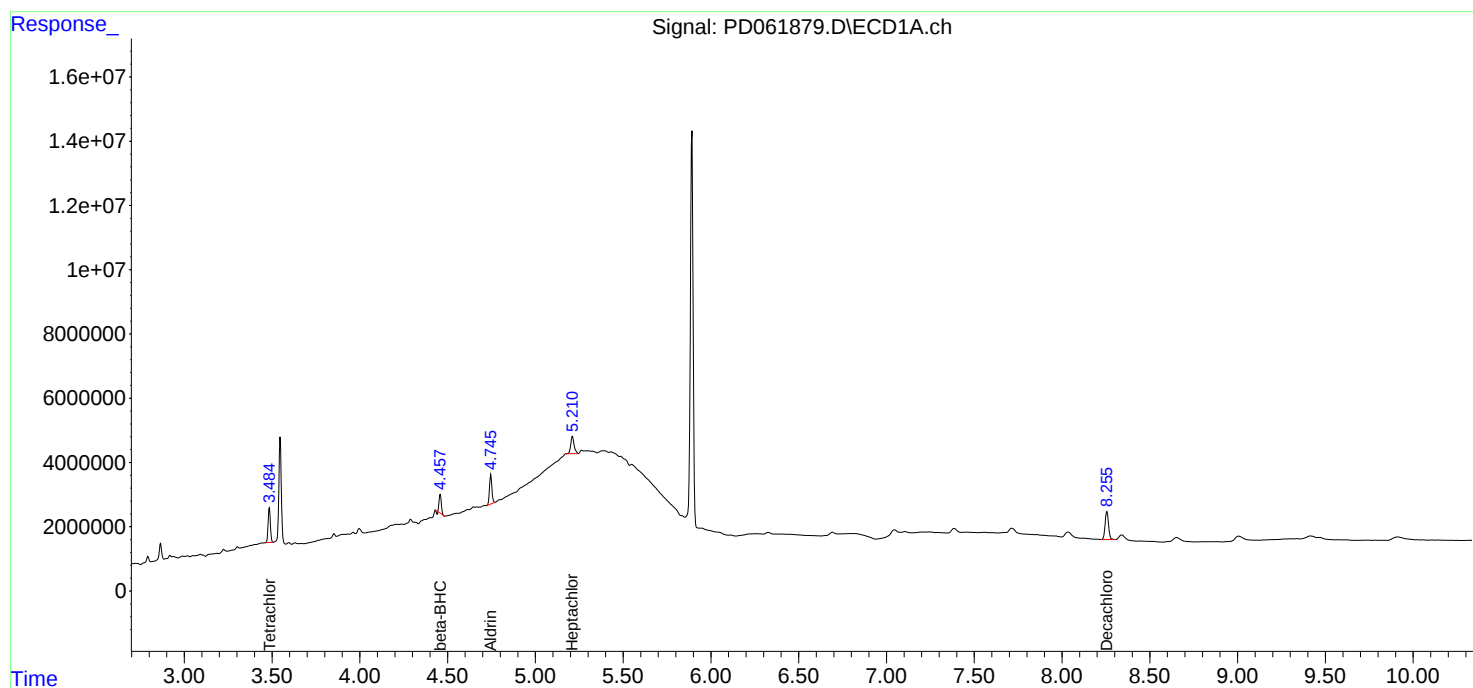


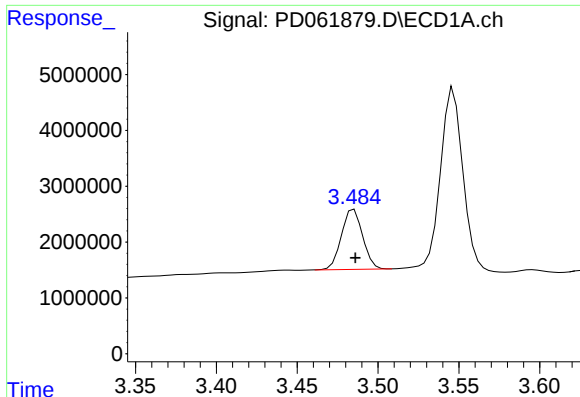

#1 Tetrachloro-m-xylene


R.T.: 3.485 min
Delta R.T.: 0.000 min
Response: 9802794
Conc: 11.71 ng/ml

Instrument :
ECD_D
ClientSampleId :

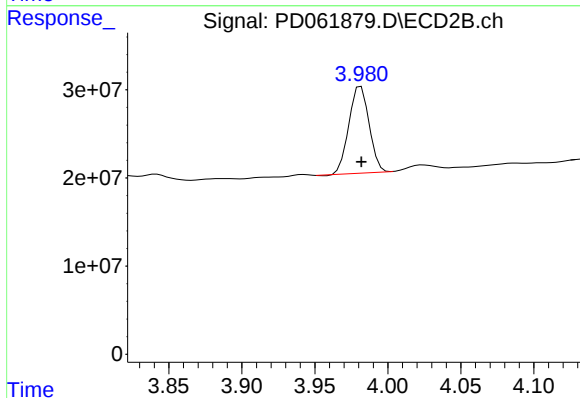


#1 Tetrachloro-m-xylene

R.T.: 3.982 min
Delta R.T.: 0.000 min
Response: 94567136
Conc: 10.88 ng/ml

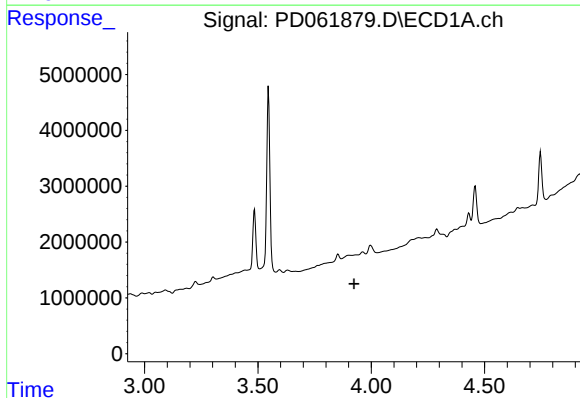


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 3.925 min
Response: 0
Conc: N.D.

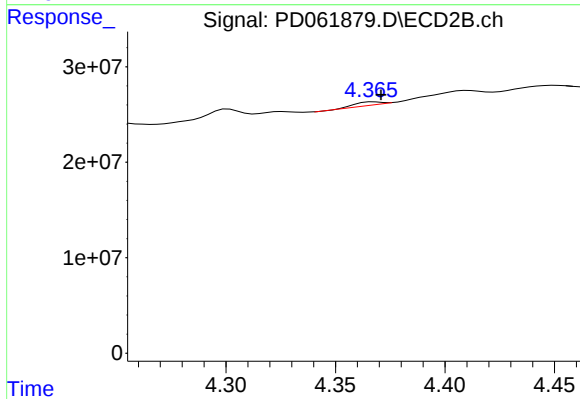

#2 alpha-BHC


R.T.: 4.368 min
Delta R.T.: -0.003 min
Response: 2585109
Conc: 0.19 ng/ml

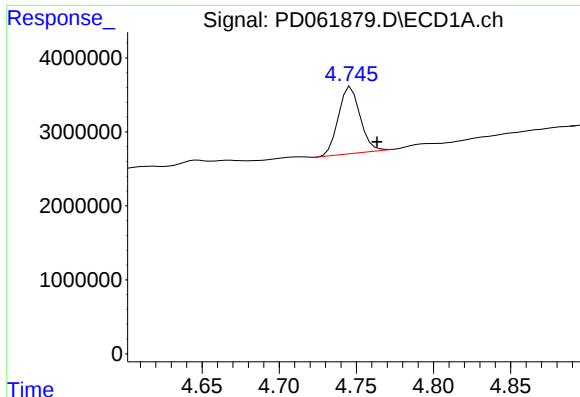

#5 Aldrin


R.T.: 4.747 min
Delta R.T.: -0.017 min
Response: 8799244
Conc: 7.33 ng/ml

Instrument :
ECD_D
ClientSampleId :

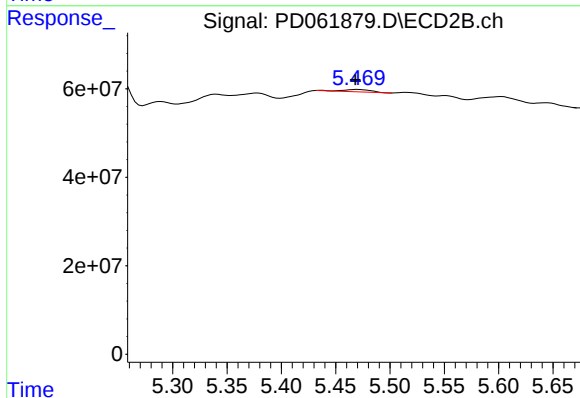


#5 Aldrin

R.T.: 5.470 min
Delta R.T.: 0.002 min
Response: 9107760
Conc: 0.73 ng/ml

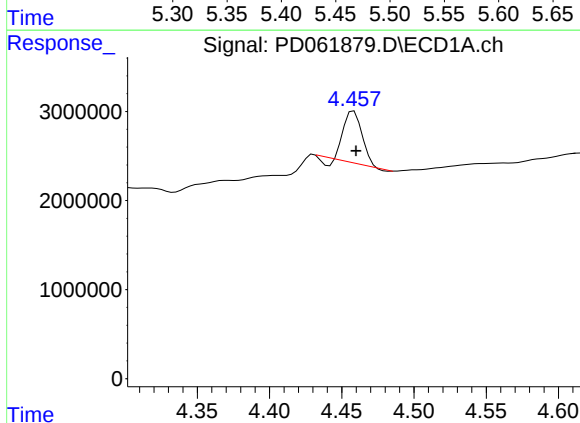


#6 beta-BHC

R.T.: 4.458 min
Delta R.T.: -0.002 min
Response: 4839943
Conc: 8.88 ng/ml

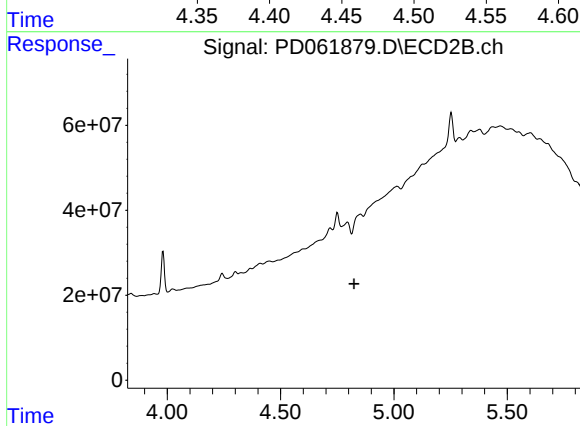

#6 beta-BHC


R.T.: 0.000 min
Exp R.T. : 4.824 min
Response: 0
Conc: N.D.

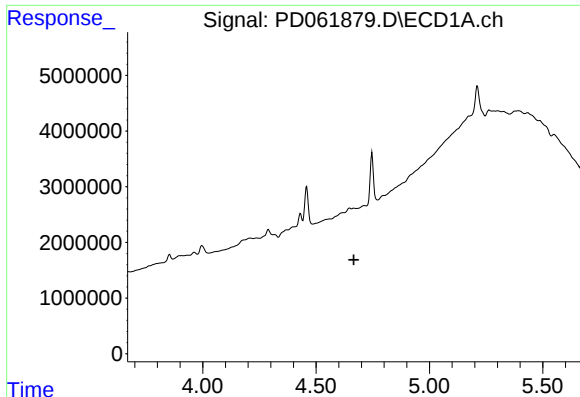

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 4.666 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

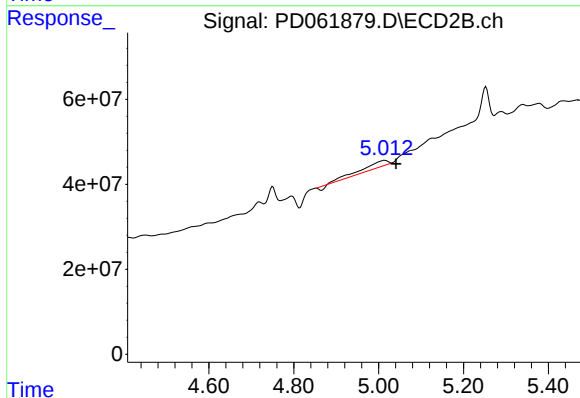


#7 delta-BHC

R.T.: 5.014 min
Delta R.T.: -0.027 min
Response: 56713270
Conc: 4.29 ng/ml

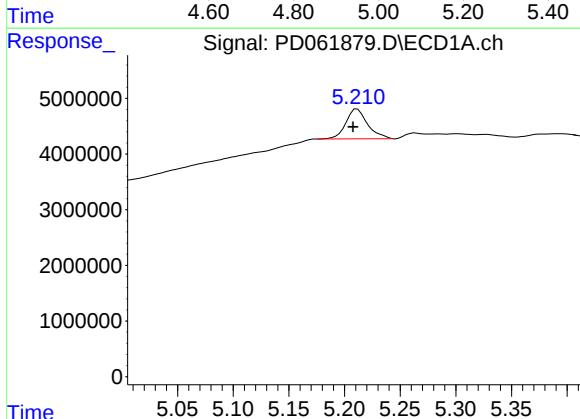


#8 Heptachlor epoxide

R.T.: 5.211 min
Delta R.T.: 0.004 min
Response: 7287769
Conc: 6.36 ng/ml

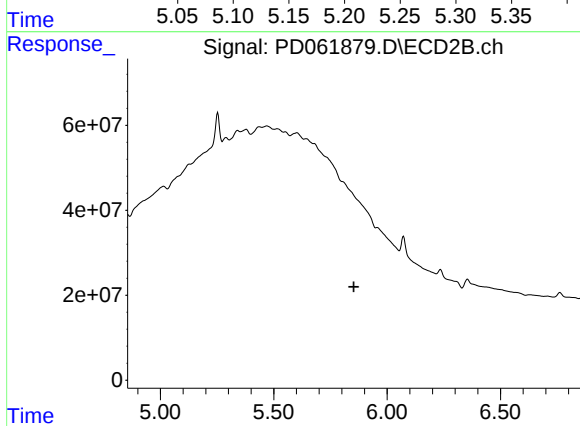

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 5.854 min
Response: 0
Conc: N.D.

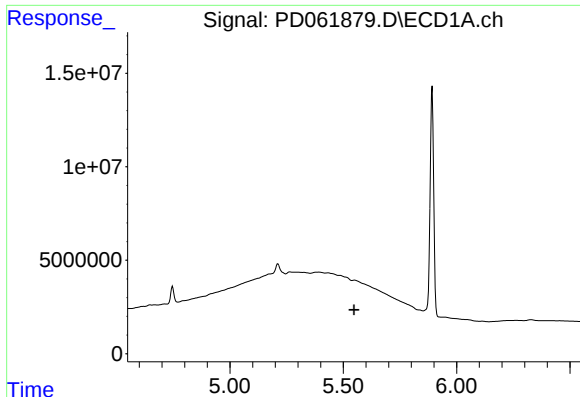

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T. : 5.548 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

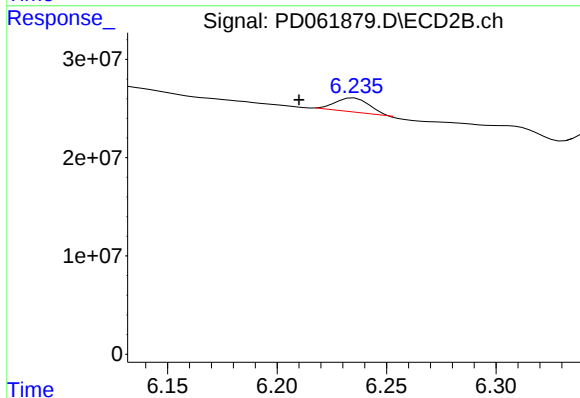


#9 Endosulfan I

R.T.: 6.235 min
Delta R.T.: 0.025 min
Response: 9834377
Conc: 0.91 ng/ml

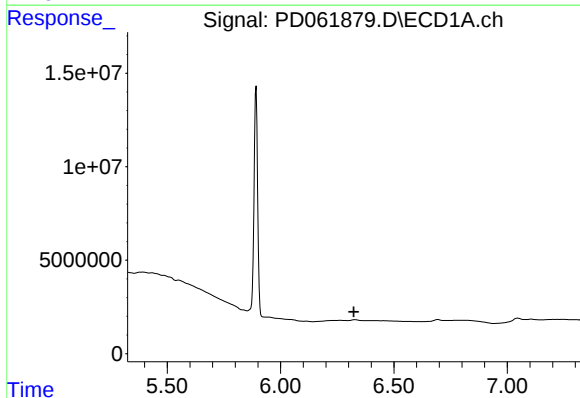


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.323 min
Response: 0
Conc: N.D.

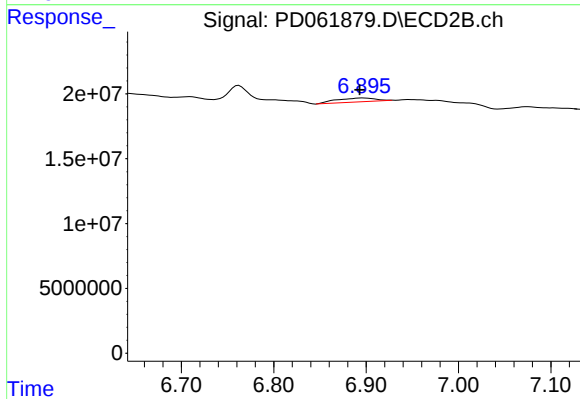

#15 Endosulfan II


R.T.: 6.897 min
Delta R.T.: 0.004 min
Response: 9193930
Conc: 0.97 ng/ml

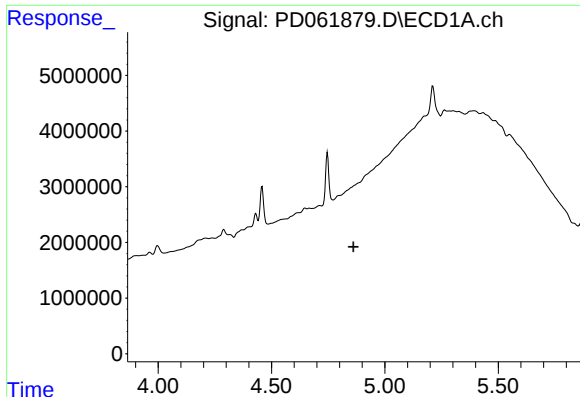

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T.: 4.862 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

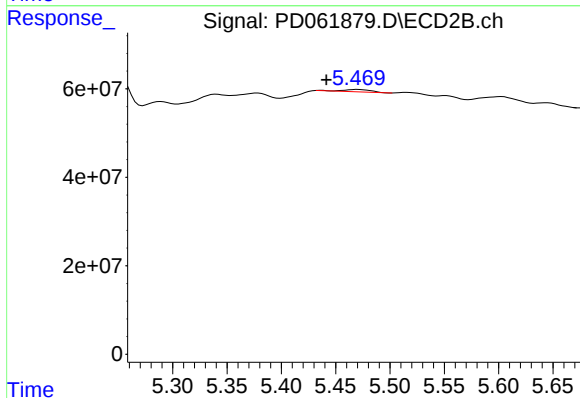


#24 Chlordane-2

R.T.: 5.470 min
Delta R.T.: 0.029 min
Response: 9107760
Conc: 23.74 ng/ml

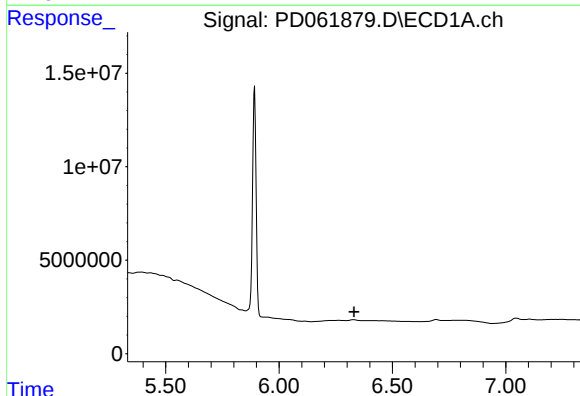


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T.: 6.332 min
Response: 0
Conc: N.D.

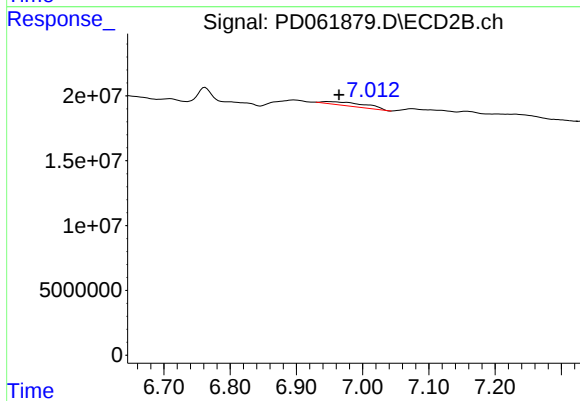

#27 Chlordane-5


R.T.: 6.946 min
Delta R.T.: -0.018 min
Response: 12773161
Conc: 35.44 ng/ml

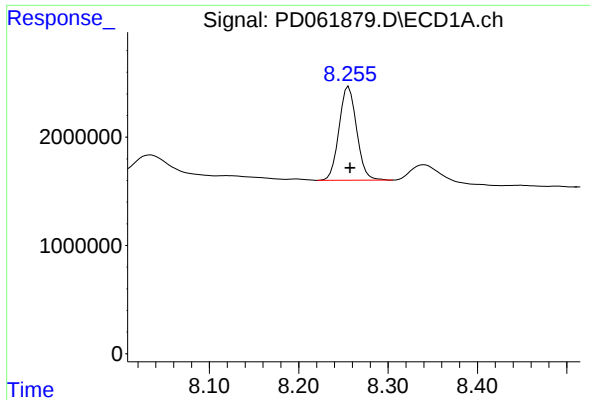

#28 Decachlorobiphenyl

R.T.: 8.256 min
Delta R.T.: -0.001 min
Response: 11850813
Conc: 9.63 ng/ml

Instrument :
ECD_D
ClientSampleId :

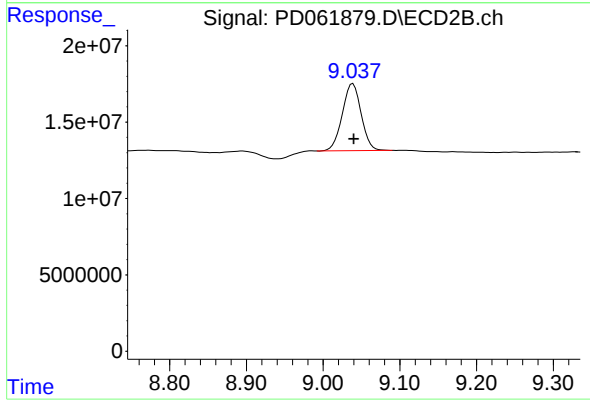

#28 Decachlorobiphenyl

R.T.: 9.039 min
Delta R.T.: -0.001 min
Response: 75498455
Conc: 8.00 ng/ml