

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD033021\
 Data File : PD061892.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Mar 2021 21:16
 Operator : AR\AJ
 Sample : M1836-01
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 B1-0-2

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 31 04:44:20 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032921.M
 Quant Title : GC Extractables
 QLast Update : Tue Mar 30 04:47:56 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.485	3.981	10270810	104.7E6	12.267	12.056
28)	SA Decachlor...	8.256	9.038	16221730	100.0E6	13.184	10.594
Target Compounds							
5)	MB Aldrin	4.747f	5.486f	13251463	15232578	11.042	1.224 #
7)	B delta-BHC	0.000	5.021f	0	49998104	N.D.	3.780 #
8)	B Heptachlo...	5.220	0.000	20869872	0	18.206	N.D. #
9)	A Endosulfan I	0.000	6.235f	0	23824858	N.D.	2.198 #
16)	A 4,4'-DDD	0.000	6.808	0	5532775	N.D.	0.584 #
20)	A Methoxychlor	6.947f	7.590f	1296487	1708832	2.744	0.379 #
21)	B Endrin ke...	7.223f	0.000	1186289	0	0.930	N.D. #
22)	Mirex	0.000	8.188f	0	10874817	N.D.	1.687 #
24)	Chlordane-2	0.000	5.445	0	5596574	N.D.	14.585 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD033021\
Data File : PD061892.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Mar 2021 21:16
Operator : AR\AJ
Sample : M1836-01
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampled :
B1-0-2

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 31 04:44:20 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032921.M
Quant Title : GC Extractables
QLast Update : Tue Mar 30 04:47:56 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

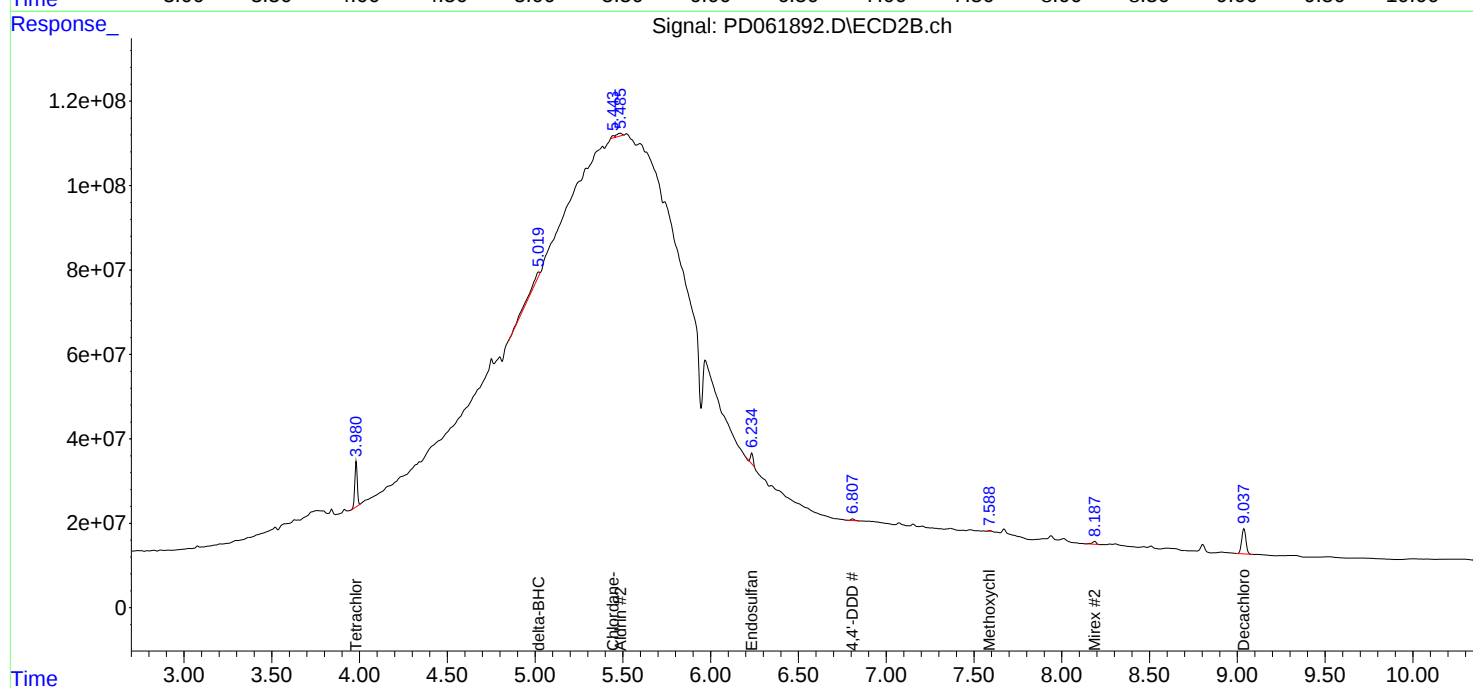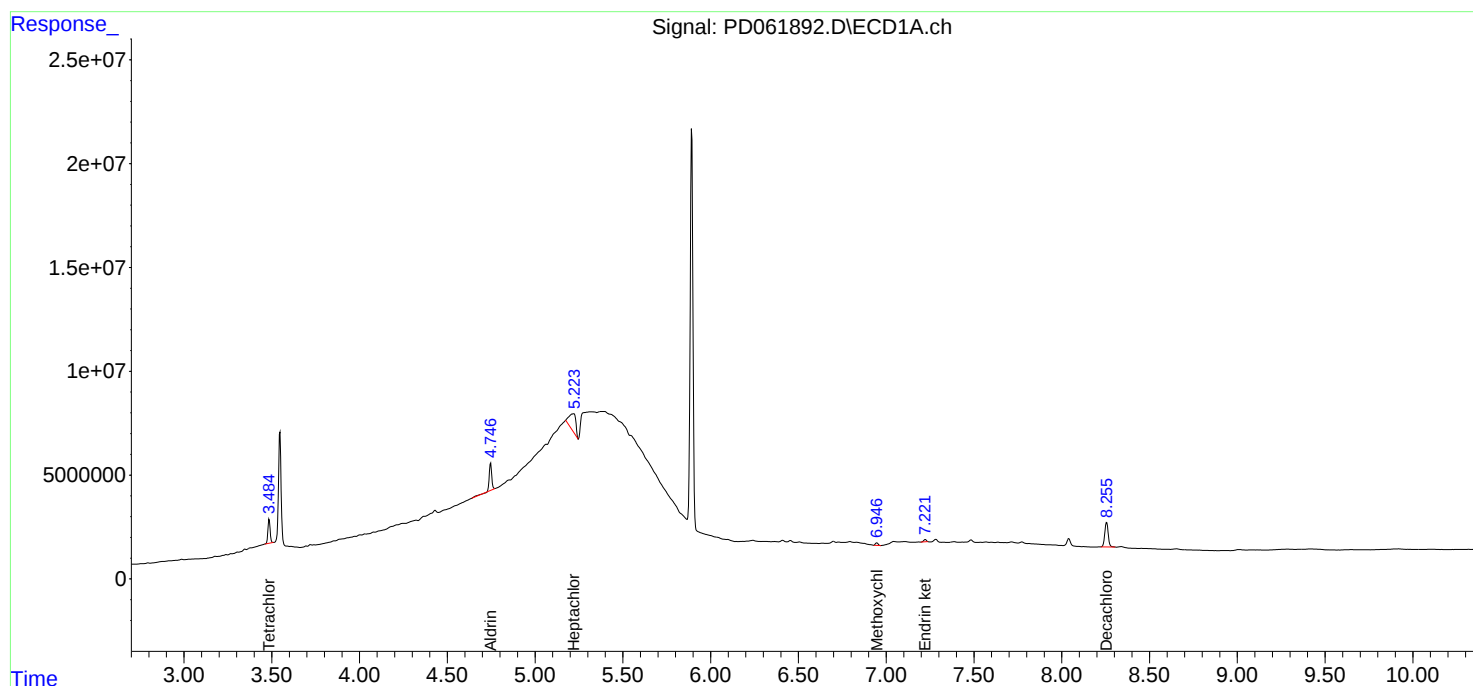


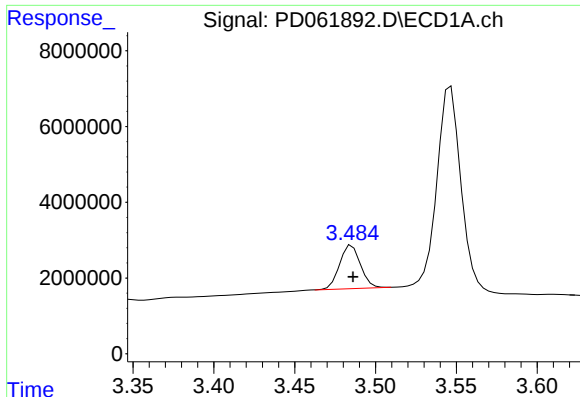

#1 Tetrachloro-m-xylene


R.T.: 3.485 min
Delta R.T.: 0.000 min
Response: 10270810
Conc: 12.27 ng/ml

Instrument :
ECD_D
ClientSampleId :
B1-0-2

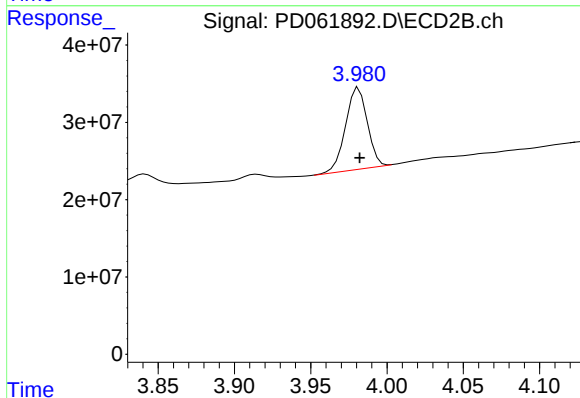


#1 Tetrachloro-m-xylene

R.T.: 3.981 min
Delta R.T.: 0.000 min
Response: 104749939
Conc: 12.06 ng/ml

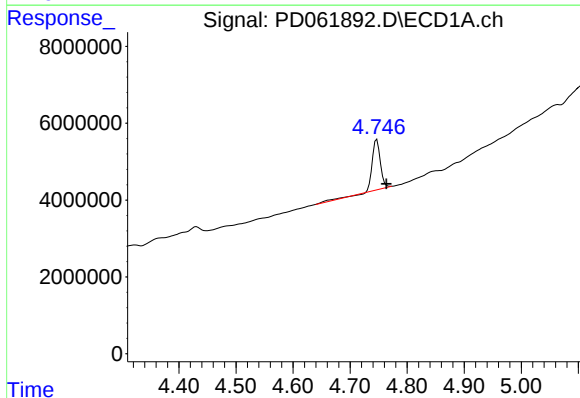


#5 Aldrin

R.T.: 4.747 min
Delta R.T.: -0.016 min
Response: 13251463
Conc: 11.04 ng/ml

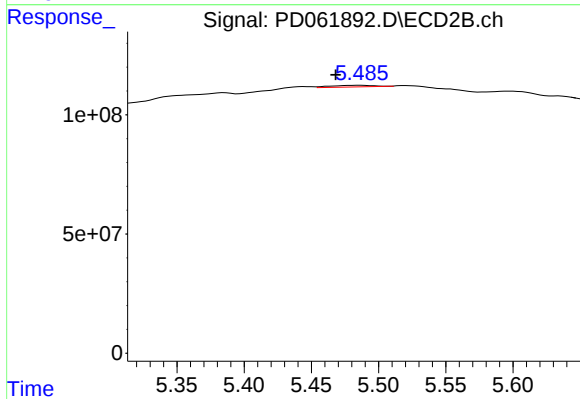

#5 Aldrin


R.T.: 5.486 min
Delta R.T.: 0.018 min
Response: 15232578
Conc: 1.22 ng/ml

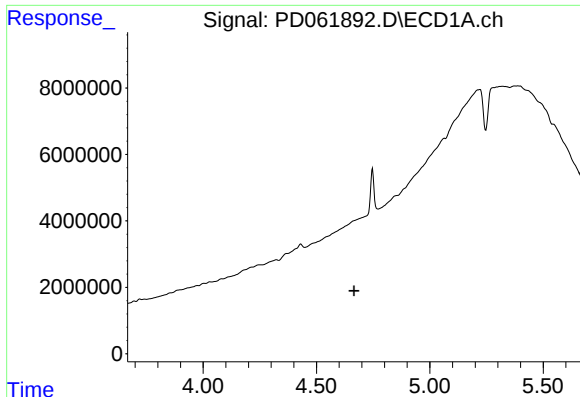

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 4.666 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
B1-0-2

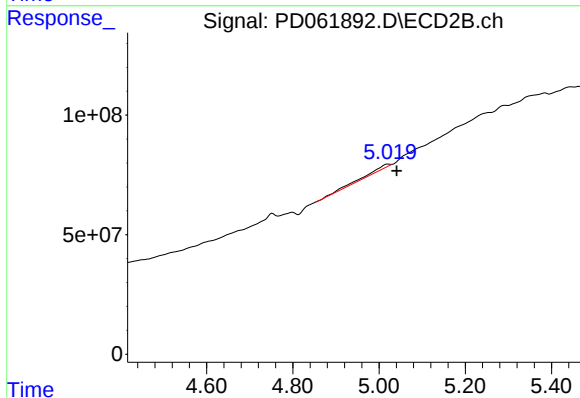


#7 delta-BHC

R.T.: 5.021 min
Delta R.T.: -0.020 min
Response: 49998104
Conc: 3.78 ng/ml

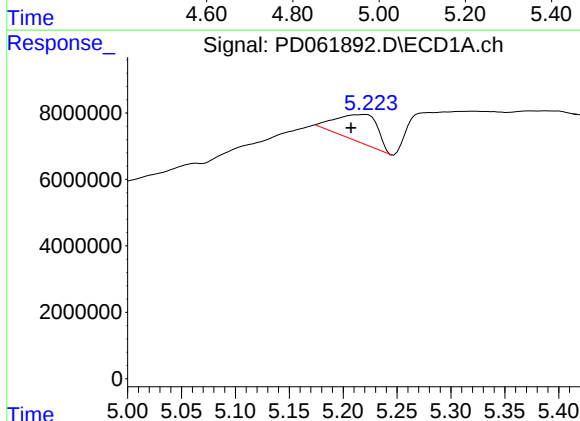


#8 Heptachlor epoxide

R.T.: 5.220 min
Delta R.T.: 0.013 min
Response: 20869872
Conc: 18.21 ng/ml

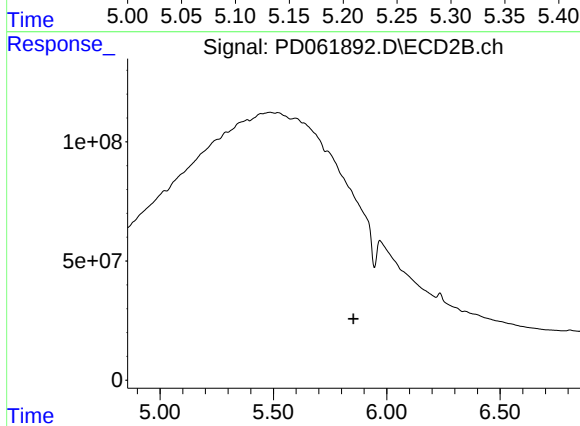

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 5.854 min
Response: 0
Conc: N.D.

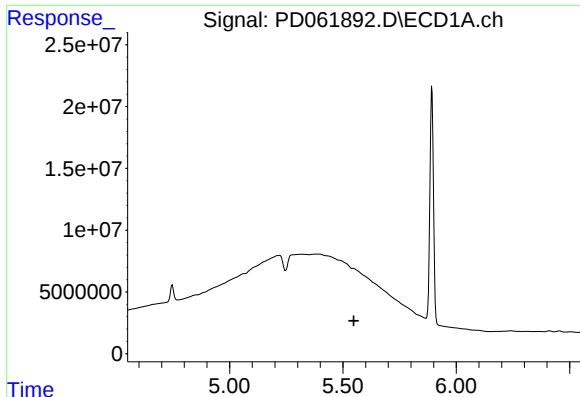

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 5.548 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
B1-0-2

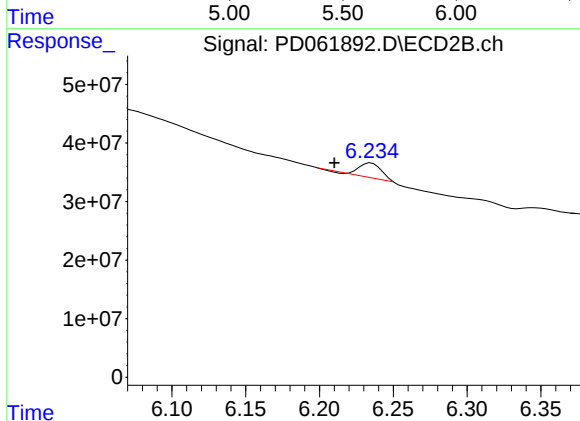


#9 Endosulfan I

R.T.: 6.235 min
Delta R.T.: 0.025 min
Response: 23824858
Conc: 2.20 ng/ml

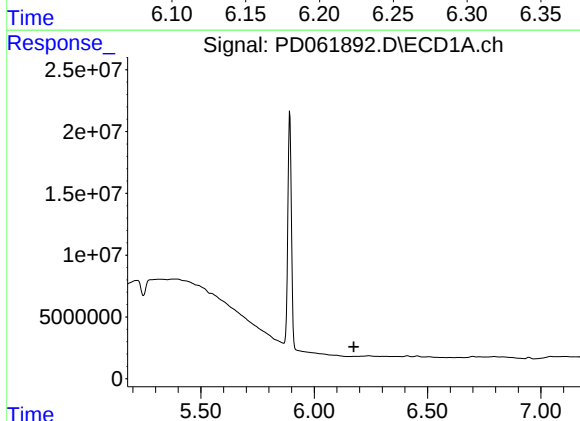


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T.: 6.174 min
Response: 0
Conc: N.D.

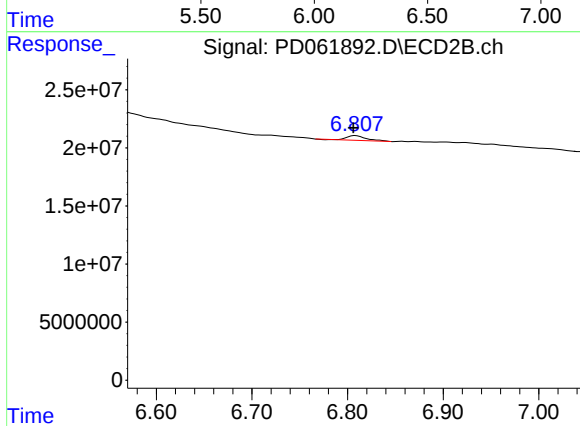

#16 4,4'-DDD


R.T.: 6.808 min
Delta R.T.: 0.002 min
Response: 5532775
Conc: 0.58 ng/ml

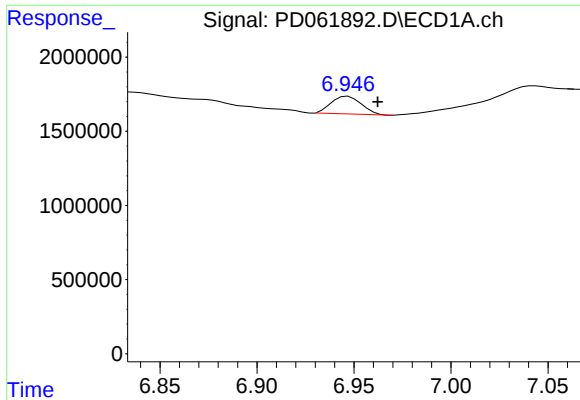

#20 Methoxychlor


R.T.: 6.947 min
Delta R.T.: -0.015 min
Response: 1296487
Conc: 2.74 ng/ml

Instrument :
ECD_D
ClientSampleId :
B1-0-2

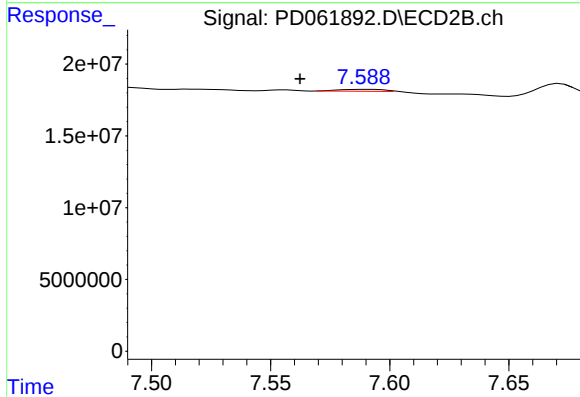


#20 Methoxychlor

R.T.: 7.590 min
Delta R.T.: 0.028 min
Response: 1708832
Conc: 0.38 ng/ml

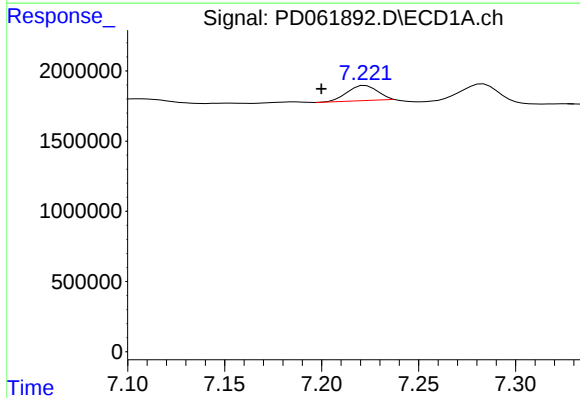


#21 Endrin ketone

R.T.: 7.223 min
Delta R.T.: 0.023 min
Response: 1186289
Conc: 0.93 ng/ml

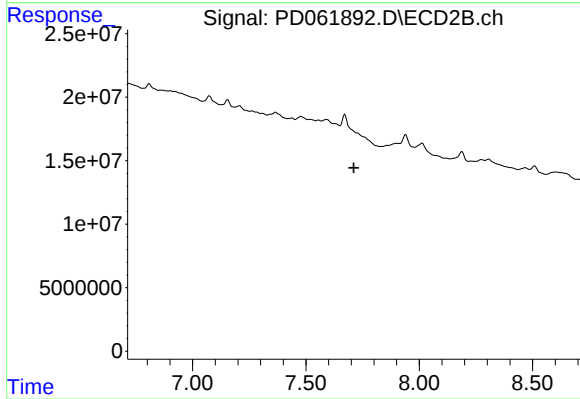

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T.: 7.711 min
Response: 0
Conc: N.D.

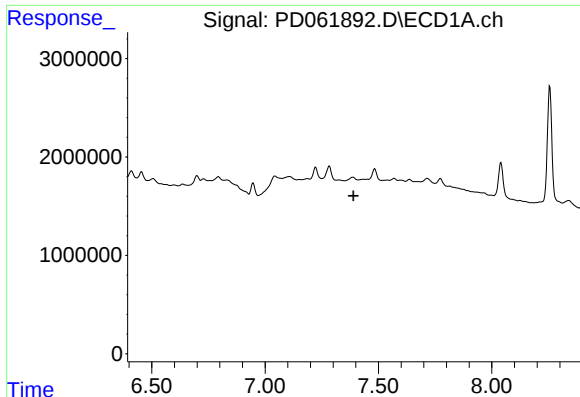

#22 Mirex


R.T.: 0.000 min
Exp R.T.: 7.390 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
B1-0-2

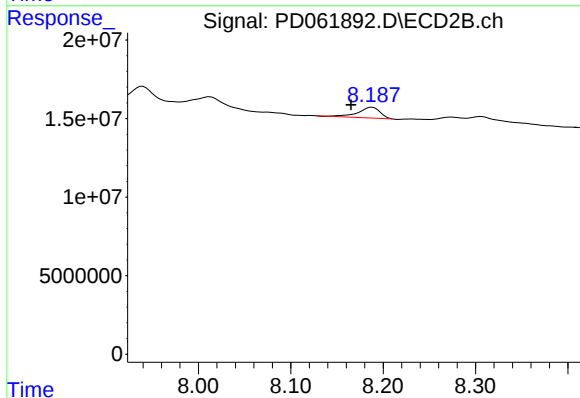


#22 Mirex

R.T.: 8.188 min
Delta R.T.: 0.023 min
Response: 10874817
Conc: 1.69 ng/ml

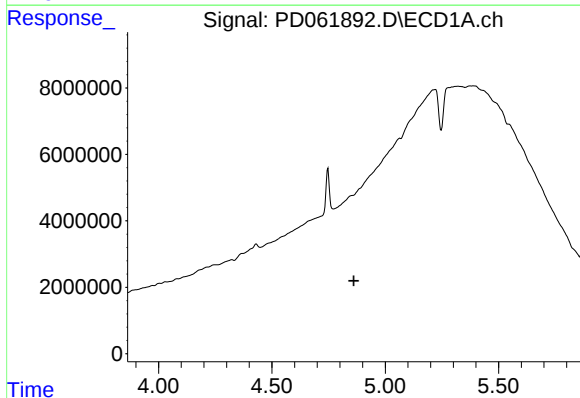


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T.: 4.862 min
Response: 0
Conc: N.D.

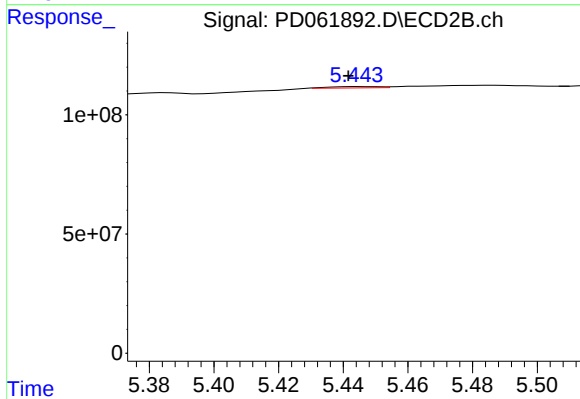

#24 Chlordane-2


R.T.: 5.445 min
Delta R.T.: 0.004 min
Response: 5596574
Conc: 14.59 ng/ml

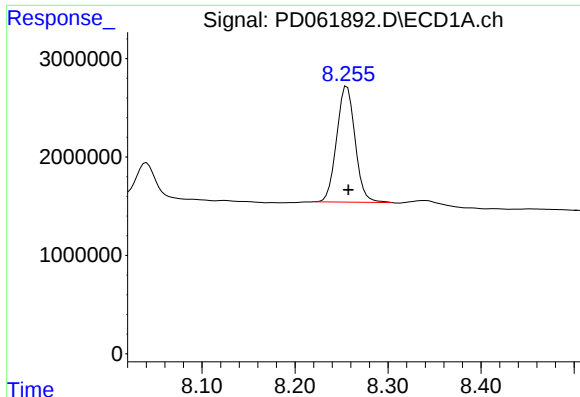

#28 Decachlorobiphenyl

R.T.: 8.256 min
Delta R.T.: -0.001 min
Response: 16221730
Conc: 13.18 ng/ml

Instrument :
ECD_D
ClientSampleId :
B1-0-2

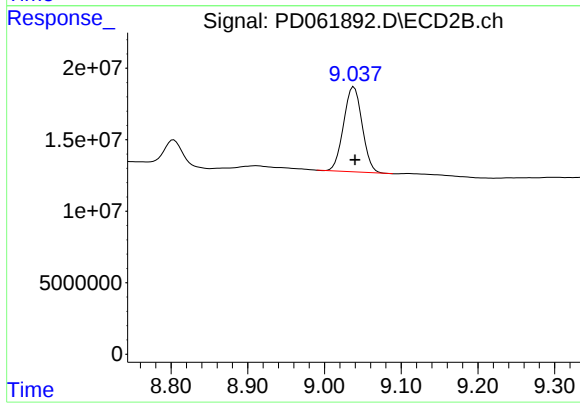

#28 Decachlorobiphenyl

R.T.: 9.038 min
Delta R.T.: -0.002 min
Response: 100012218
Conc: 10.59 ng/ml