

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD033021\
 Data File : PD061896.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Mar 2021 22:12
 Operator : AR\AJ
 Sample : M1836-03
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 B2-0-2

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 31 04:49:13 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032921.M
 Quant Title : GC Extractables
 QLast Update : Tue Mar 30 04:47:56 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.485	3.981	11273894	115.1E6	13.465	13.241
28)	SA Decachlor...	8.255	9.039	16121713	105.8E6	13.103	11.204
Target Compounds							
4)	MA Heptachlor	0.000	5.189f	0	1473986	N.D.	0.113 #
5)	MB Aldrin	4.747f	5.484f	955717	1267102	0.796	0.102 #
7)	B delta-BHC	0.000	5.040	0	5947566	N.D.	0.450 #
9)	A Endosulfan I	0.000	6.236f	0	2824600	N.D.	0.261 #
16)	A 4,4'-DDD	0.000	6.809	0	7339862	N.D.	0.775 #
17)	MA 4,4'-DDT	0.000	7.129f	0	1269614	N.D.	0.133 #
20)	A Methoxychlor	0.000	7.534f	0	536819	N.D.	0.119 #
22)	Mirex	0.000	8.164	0	2741437	N.D.	0.425 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD033021\
Data File : PD061896.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Mar 2021 22:12
Operator : AR\AJ
Sample : M1836-03
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
B2-0-2

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 31 04:49:13 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032921.M
Quant Title : GC Extractables
QLast Update : Tue Mar 30 04:47:56 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

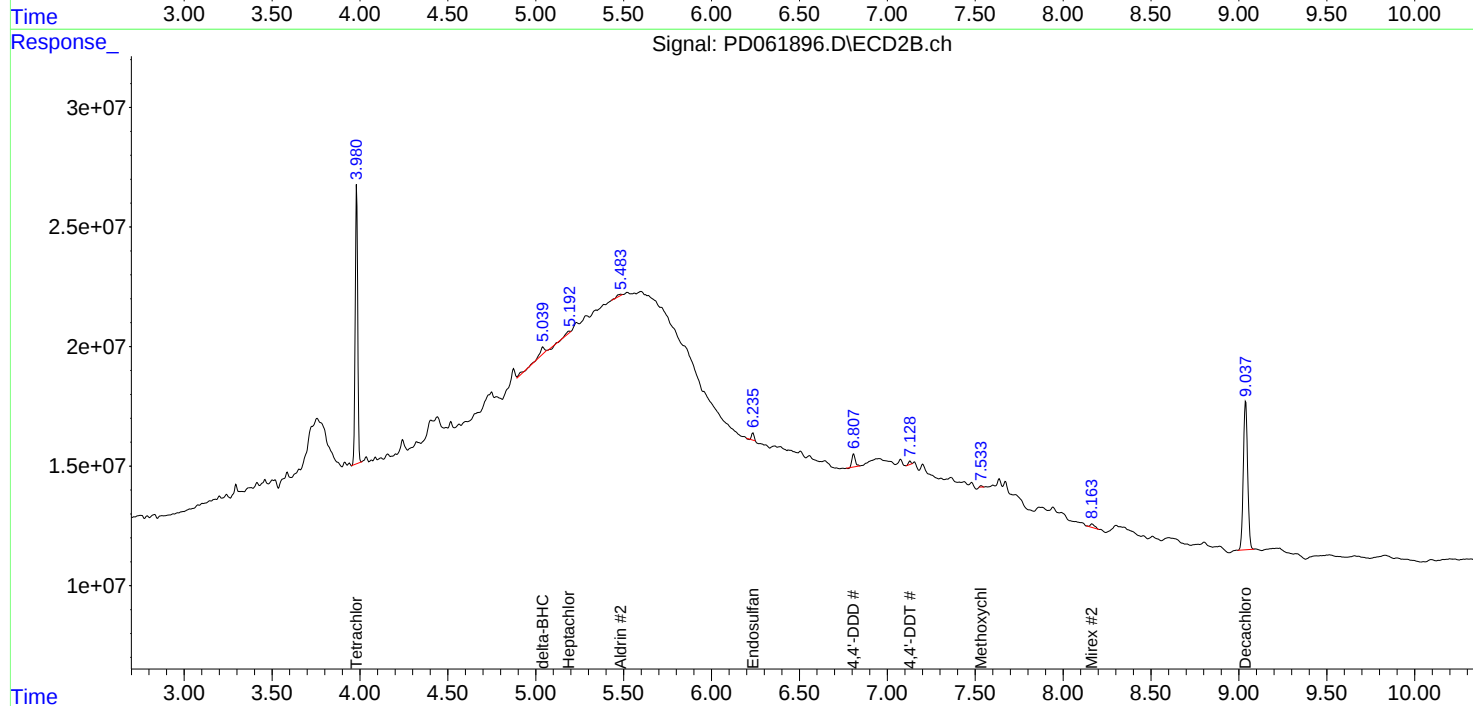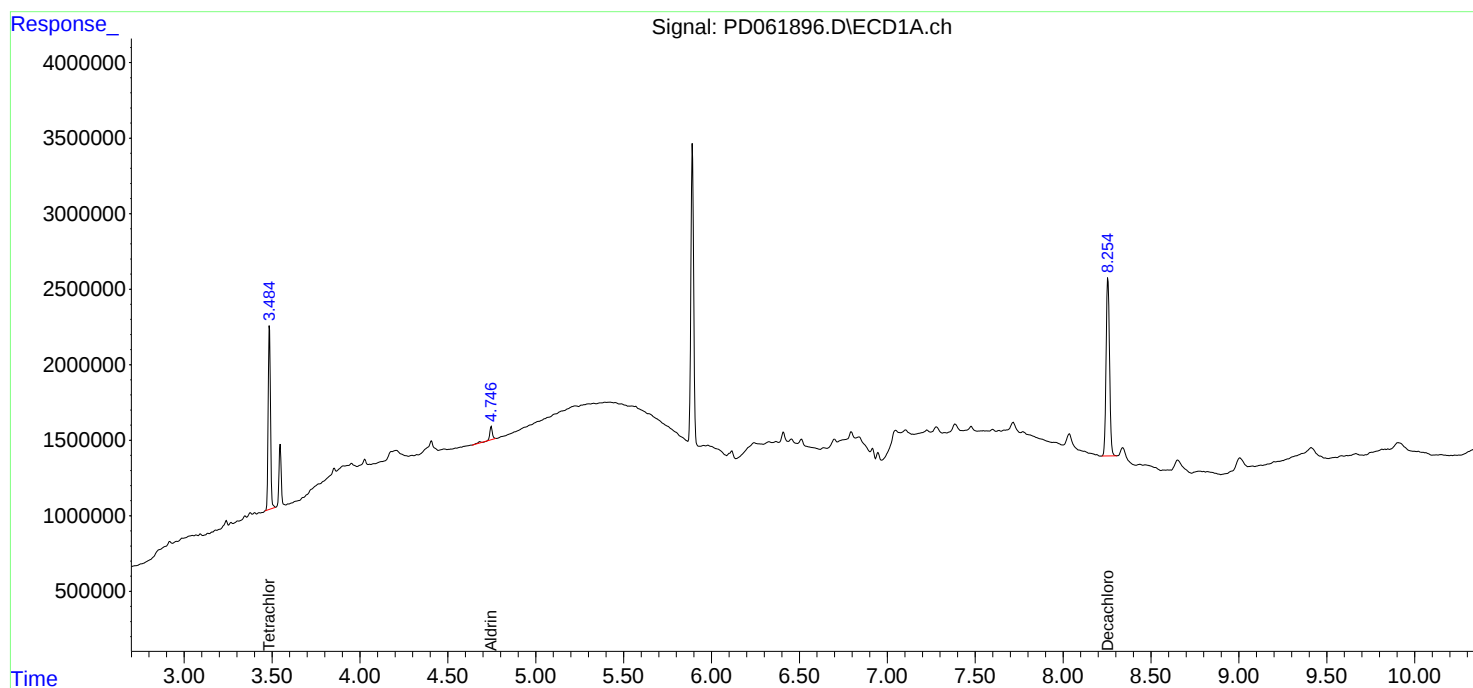


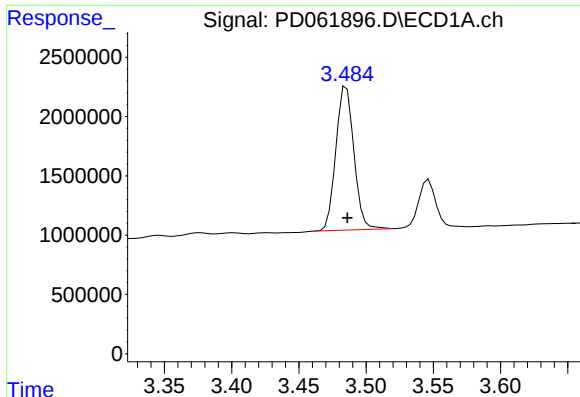

#1 Tetrachloro-m-xylene


R.T.: 3.485 min
Delta R.T.: 0.000 min
Response: 11273894
Conc: 13.46 ng/ml

Instrument :
ECD_D
ClientSampleId :
B2-0-2

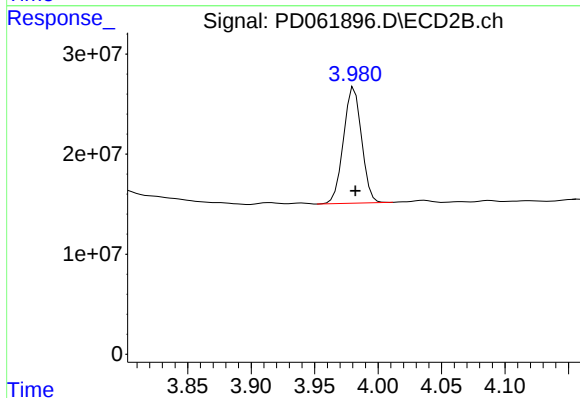


#1 Tetrachloro-m-xylene

R.T.: 3.981 min
Delta R.T.: 0.000 min
Response: 115052855
Conc: 13.24 ng/ml

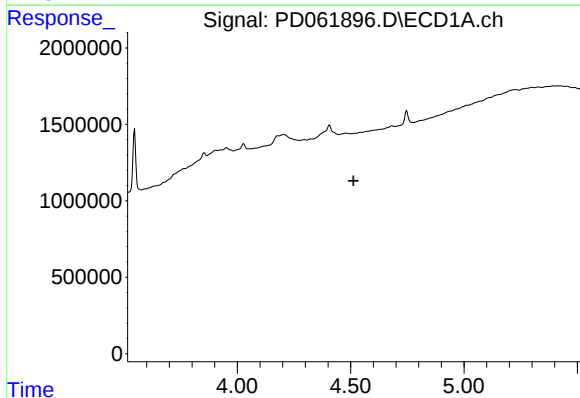


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 4.513 min
Response: 0
Conc: N.D.

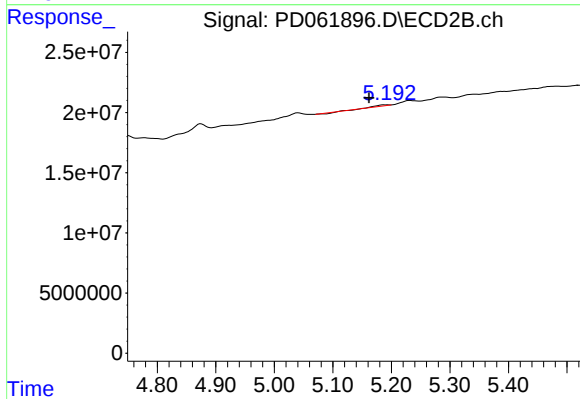

#4 Heptachlor


R.T.: 5.189 min
Delta R.T.: 0.027 min
Response: 1473986
Conc: 0.11 ng/ml

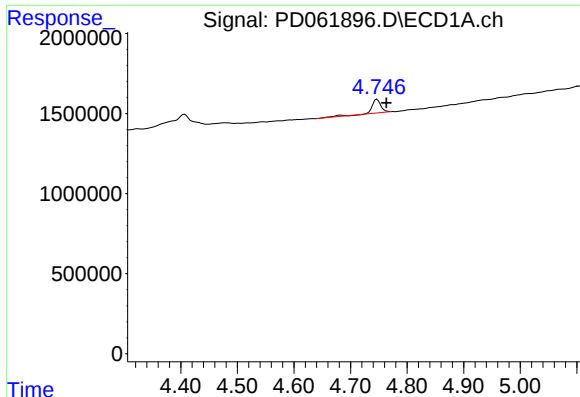

#5 Aldrin


R.T.: 4.747 min
Delta R.T.: -0.016 min
Response: 955717
Conc: 0.80 ng/ml

Instrument :
ECD_D
ClientSampleId :
B2-0-2

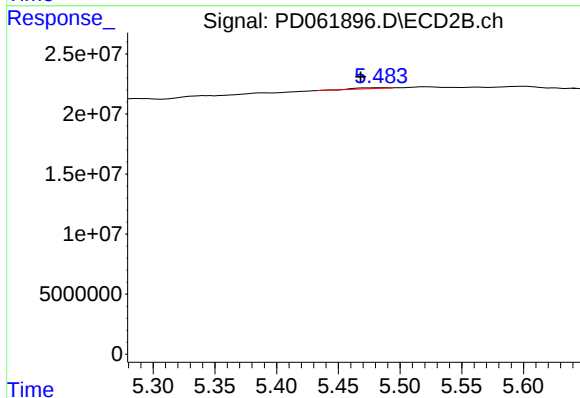


#5 Aldrin

R.T.: 5.484 min
Delta R.T.: 0.016 min
Response: 1267102
Conc: 0.10 ng/ml

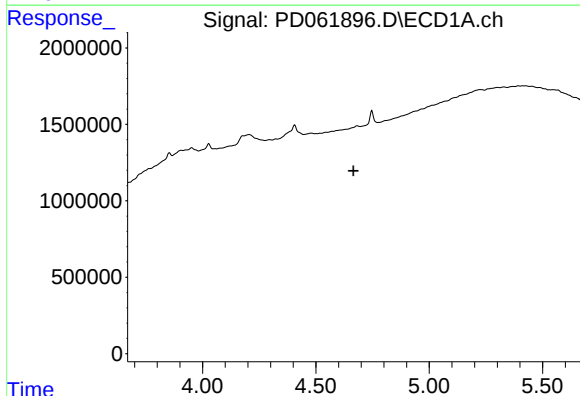


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.666 min
Response: 0
Conc: N.D.

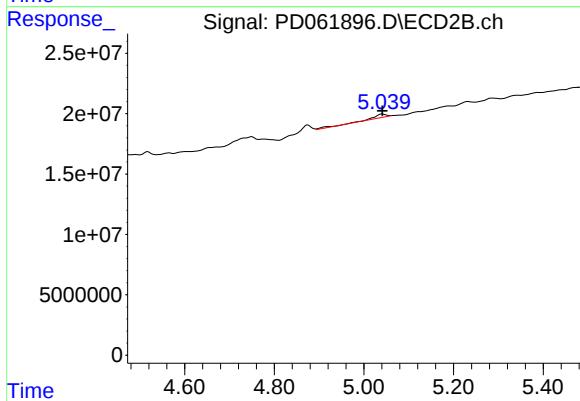

#7 delta-BHC


R.T.: 5.040 min
Delta R.T.: 0.000 min
Response: 5947566
Conc: 0.45 ng/ml

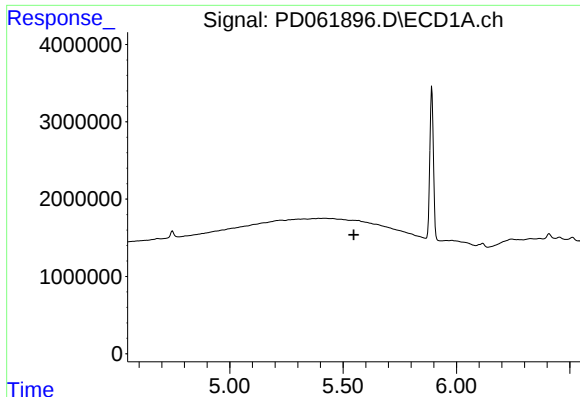

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 5.548 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
B2-0-2

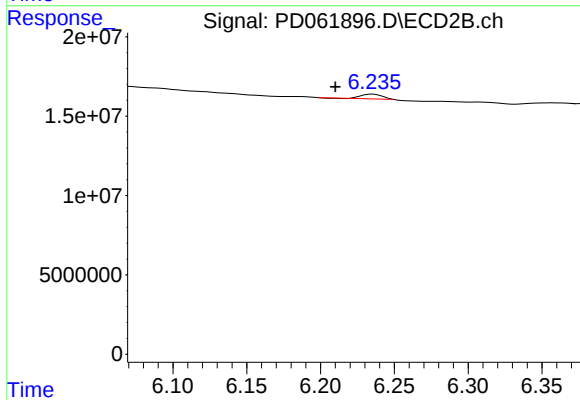


#9 Endosulfan I

R.T.: 6.236 min
Delta R.T.: 0.026 min
Response: 2824600
Conc: 0.26 ng/ml

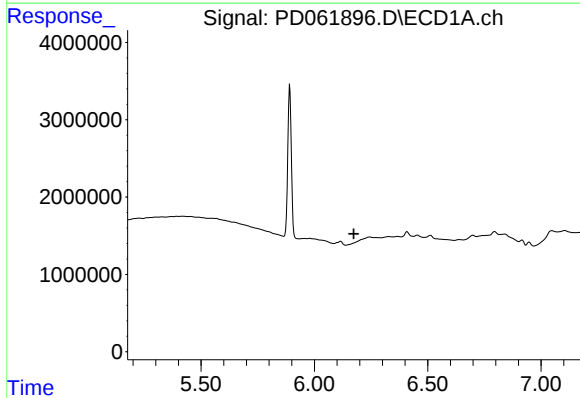


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T.: 6.174 min
Response: 0
Conc: N.D.

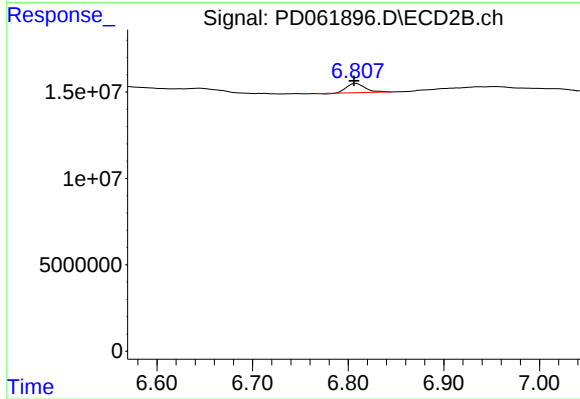

#16 4,4'-DDD


R.T.: 6.809 min
Delta R.T.: 0.002 min
Response: 7339862
Conc: 0.78 ng/ml

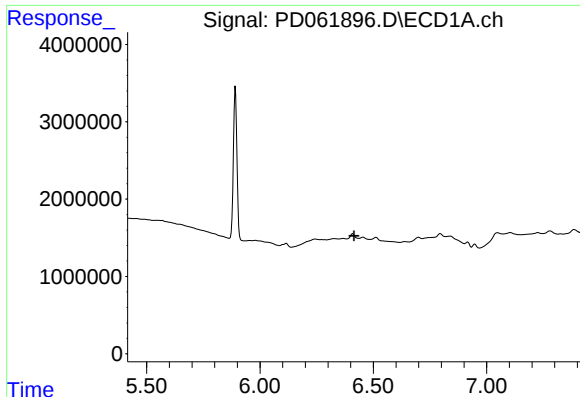

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T.: 6.416 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
B2-0-2

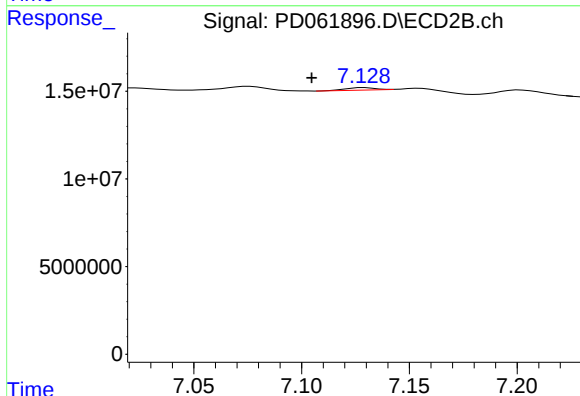


#17 4,4'-DDT

R.T.: 7.129 min
Delta R.T.: 0.024 min
Response: 1269614
Conc: 0.13 ng/ml

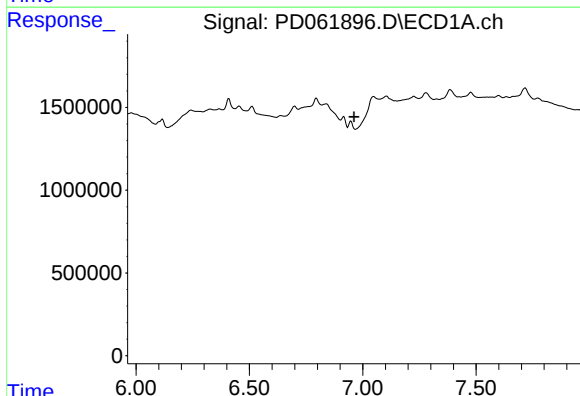


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T.: 6.962 min
Response: 0
Conc: N.D.

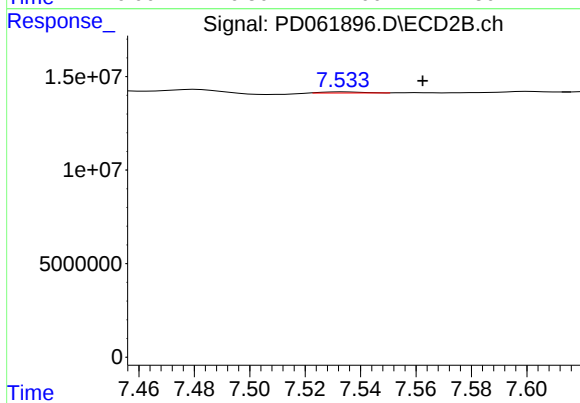

#20 Methoxychlor


R.T.: 7.534 min
Delta R.T.: -0.028 min
Response: 536819
Conc: 0.12 ng/ml

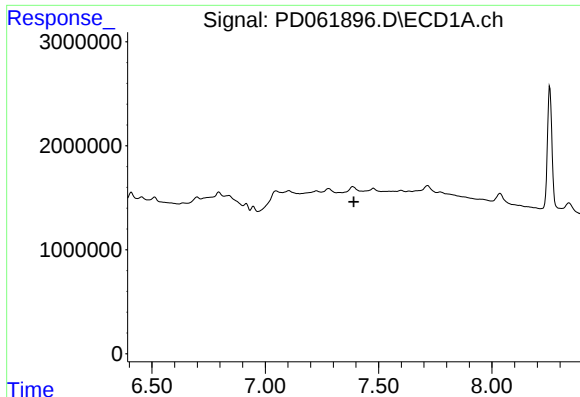

#22 Mirex


R.T.: 0.000 min
Exp R.T.: 7.390 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
B2-0-2

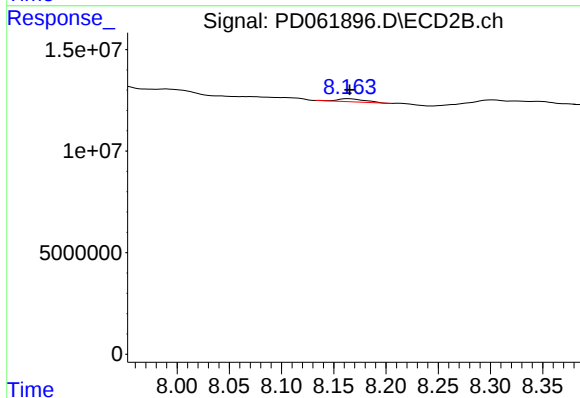


#22 Mirex

R.T.: 8.164 min
Delta R.T.: -0.001 min
Response: 2741437
Conc: 0.43 ng/ml

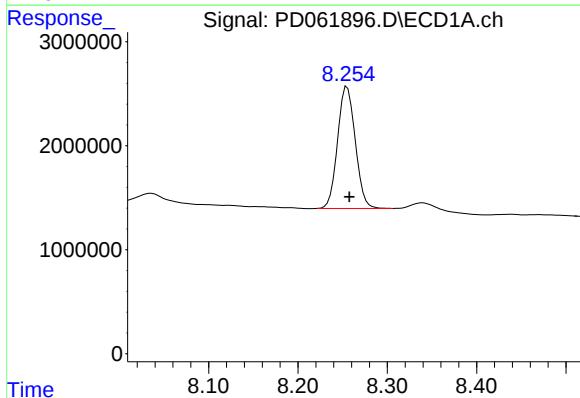

#28 Decachlorobiphenyl

R.T.: 8.255 min
Delta R.T.: -0.002 min
Response: 16121713
Conc: 13.10 ng/ml

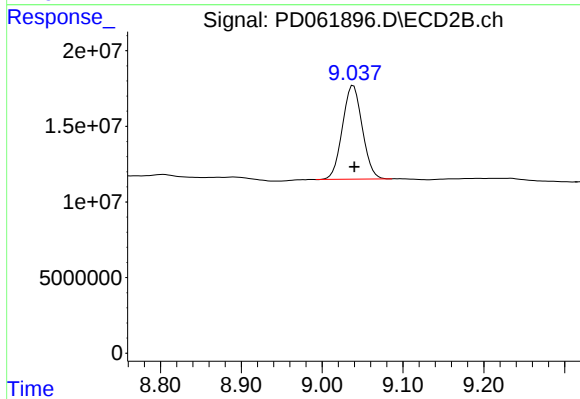

#28 Decachlorobiphenyl

R.T.: 9.039 min
Delta R.T.: -0.001 min
Response: 105773604
Conc: 11.20 ng/ml