

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD033021\
 Data File : PD061901.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Mar 2021 23:22
 Operator : AR\AJ
 Sample : M1836-08
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 B4-0-2

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 31 04:54:44 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032921.M
 Quant Title : GC Extractables
 QLast Update : Tue Mar 30 04:47:56 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.485	3.981	10197823	94632753	12.179	10.891
28)	SA Decachlor...	8.256	9.038	19473985	133.5E6	15.827	14.144
Target Compounds							
5)	MB Aldrin	4.747f	5.481	6552358	5339053	5.460	0.429 #
8)	B Heptachlo...	5.228f	0.000	1611883	0	1.406	N.D. #
9)	A Endosulfan I	0.000	6.235f	0	16375972	N.D.	1.511 #
12)	B 4,4'-DDE	0.000	6.313	0	5401385	N.D.	0.469 #
15)	B Endosulfa...	0.000	6.894	0	647920	N.D.	0.068 #
16)	A 4,4'-DDD	0.000	6.810	0	4821749	N.D.	0.509 #
17)	MA 4,4'-DDT	0.000	7.111	0	1859285	N.D.	0.195 #
22)	Mirex	0.000	8.187f	0	10309242	N.D.	1.600 #
24)	Chlordane-2	0.000	5.442	0	2890980	N.D.	7.534 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD033021\
Data File : PD061901.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Mar 2021 23:22
Operator : AR\AJ
Sample : M1836-08
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
B4-0-2

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 31 04:54:44 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032921.M
Quant Title : GC Extractables
QLast Update : Tue Mar 30 04:47:56 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

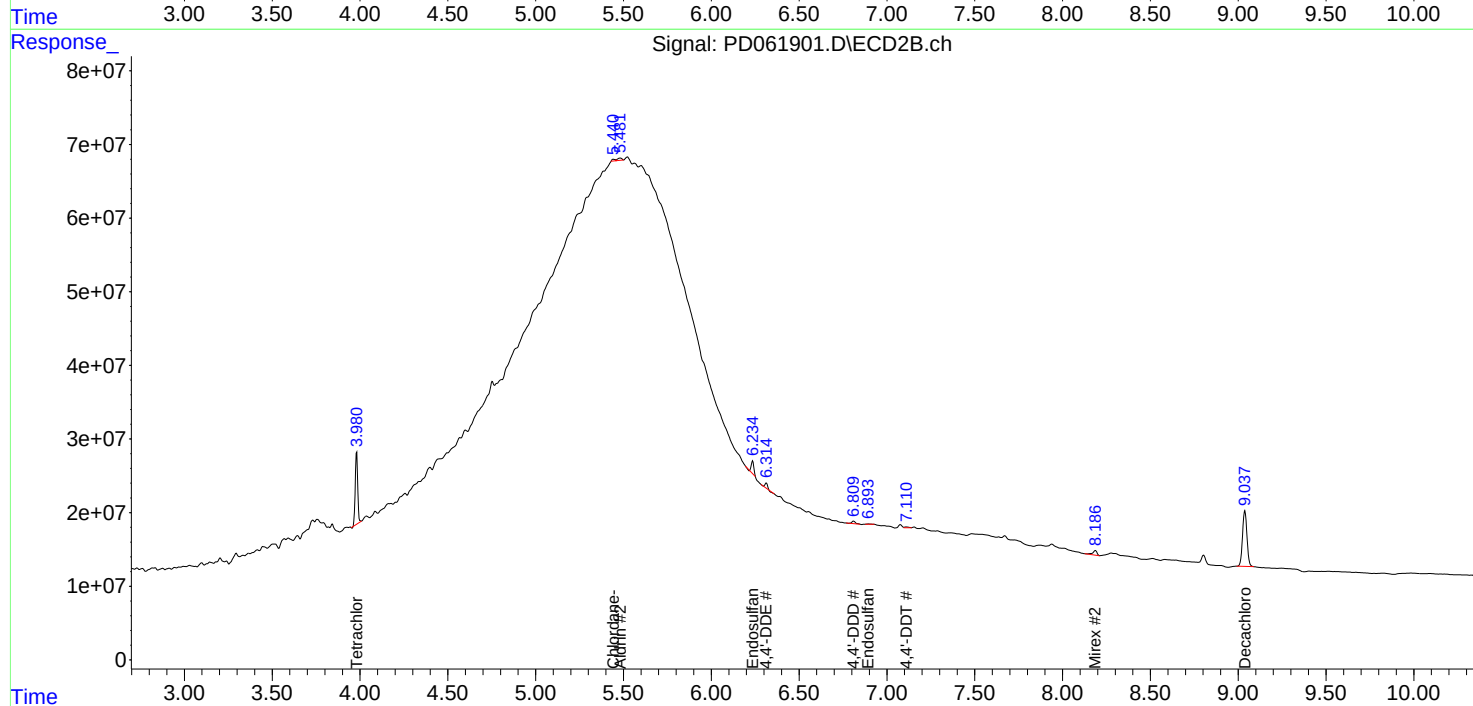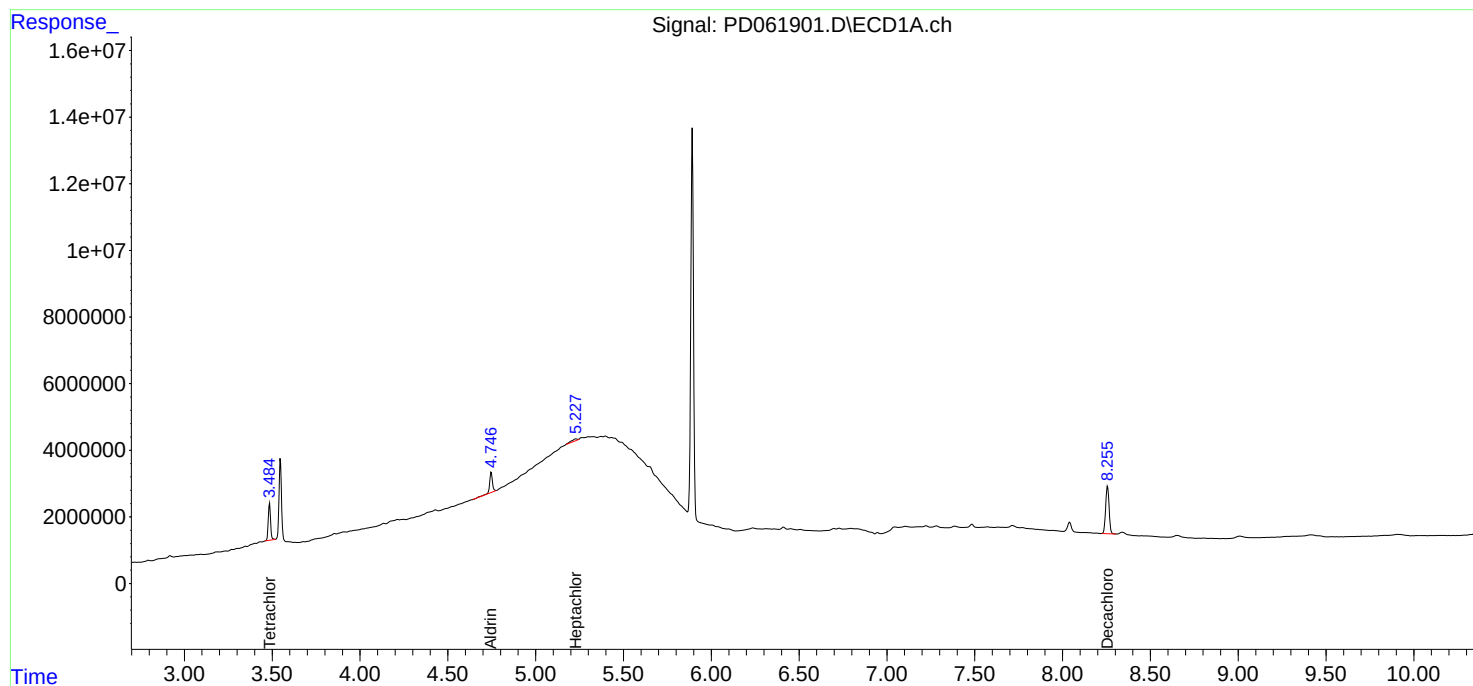


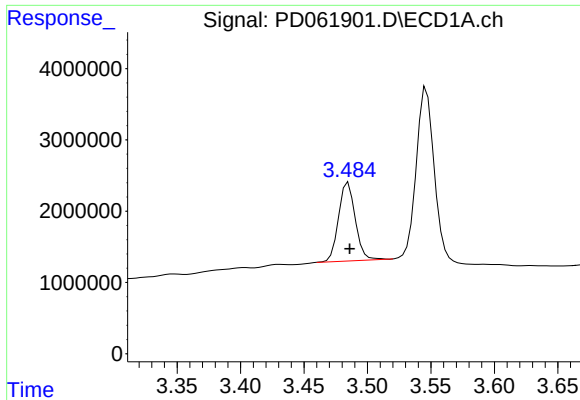

#1 Tetrachloro-m-xylene


R.T.: 3.485 min
Delta R.T.: -0.001 min
Response: 10197823
Conc: 12.18 ng/ml

Instrument :
ECD_D
ClientSampleId :
B4-0-2

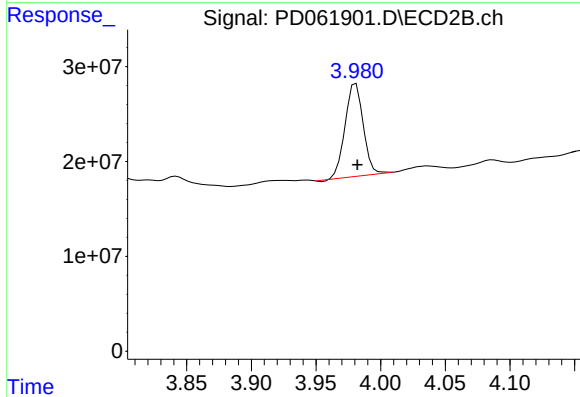


#1 Tetrachloro-m-xylene

R.T.: 3.981 min
Delta R.T.: -0.001 min
Response: 94632753
Conc: 10.89 ng/ml

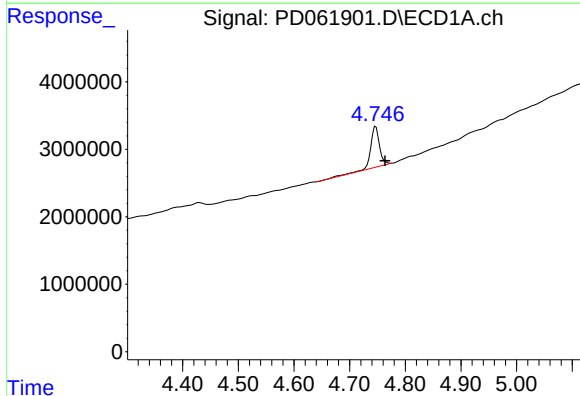


#5 Aldrin

R.T.: 4.747 min
Delta R.T.: -0.016 min
Response: 6552358
Conc: 5.46 ng/ml

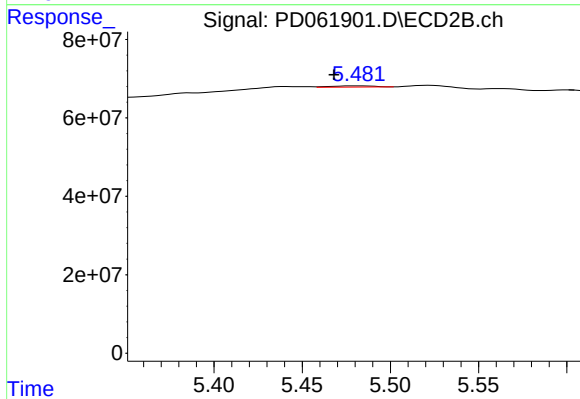

#5 Aldrin


R.T.: 5.481 min
Delta R.T.: 0.013 min
Response: 5339053
Conc: 0.43 ng/ml

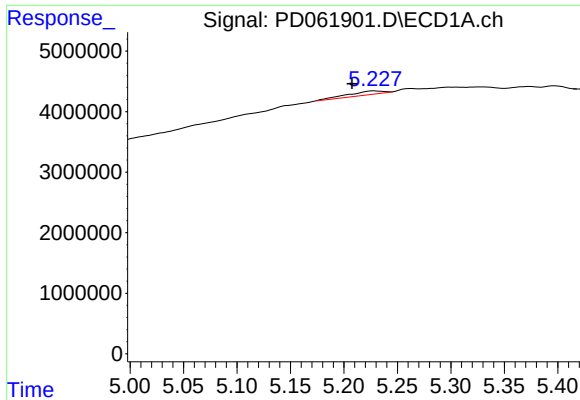

#8 Heptachlor epoxide


R.T.: 5.228 min
Delta R.T.: 0.021 min
Response: 1611883
Conc: 1.41 ng/ml

Instrument :
ECD_D
ClientSampleId :
B4-0-2

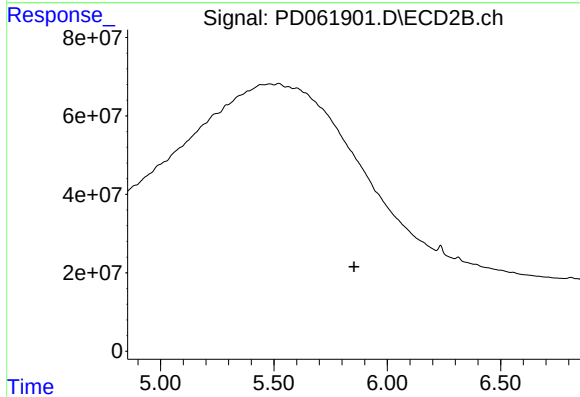


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.854 min
Response: 0
Conc: N.D.

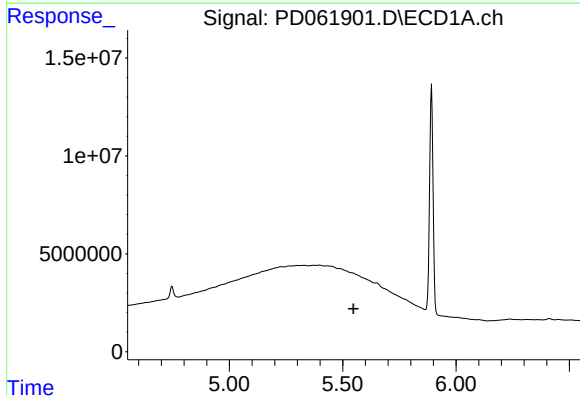


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 5.548 min
Response: 0
Conc: N.D.

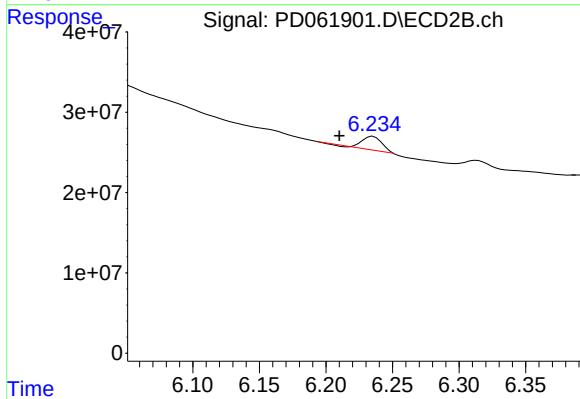

#9 Endosulfan I


R.T.: 6.235 min
Delta R.T.: 0.025 min
Response: 16375972
Conc: 1.51 ng/ml

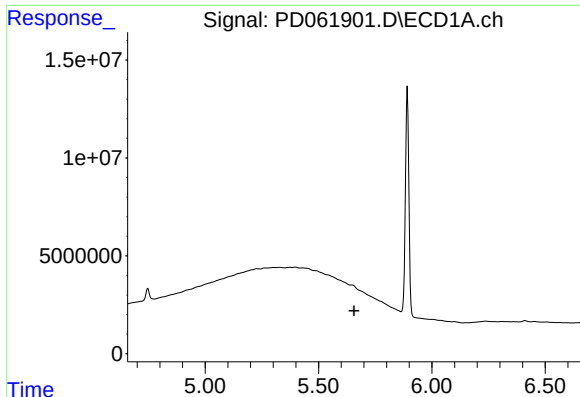

#12 4,4'-DDE


R.T.: 0.000 min
Exp R.T.: 5.657 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
B4-0-2

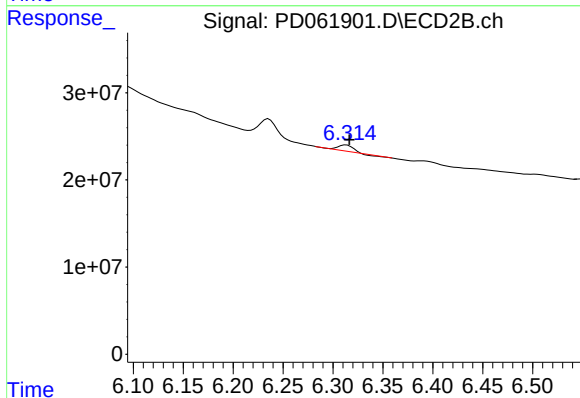


#12 4,4'-DDE

R.T.: 6.313 min
Delta R.T.: -0.003 min
Response: 5401385
Conc: 0.47 ng/ml

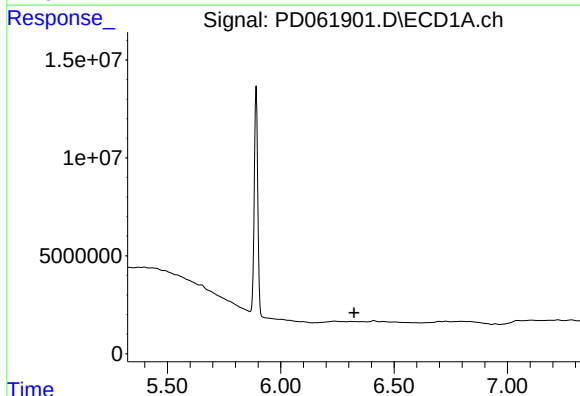


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T.: 6.323 min
Response: 0
Conc: N.D.

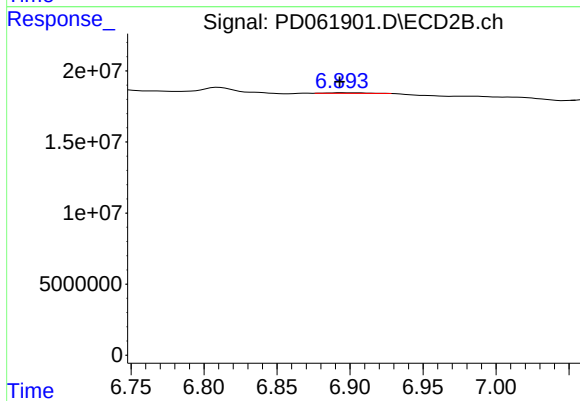

#15 Endosulfan II


R.T.: 6.894 min
Delta R.T.: 0.001 min
Response: 647920
Conc: 0.07 ng/ml

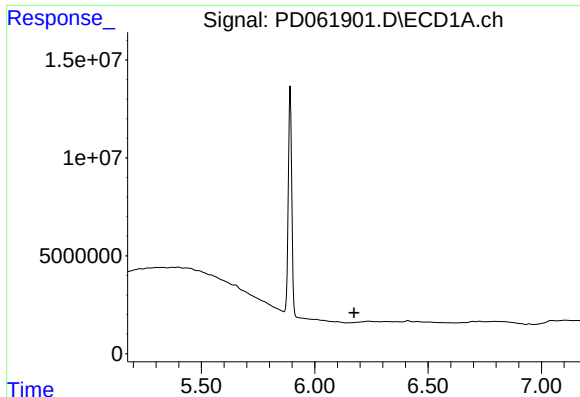

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 6.174 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
B4-0-2

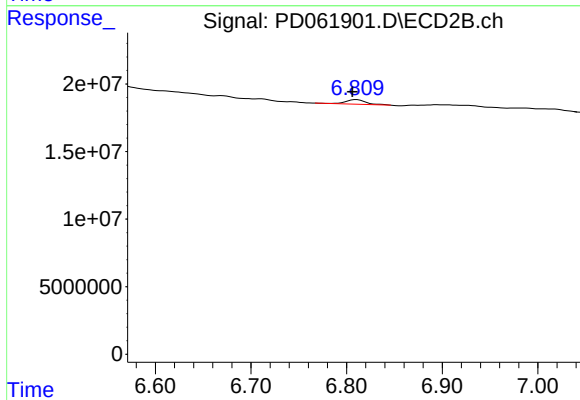


#16 4,4'-DDD

R.T.: 6.810 min
Delta R.T.: 0.004 min
Response: 4821749
Conc: 0.51 ng/ml

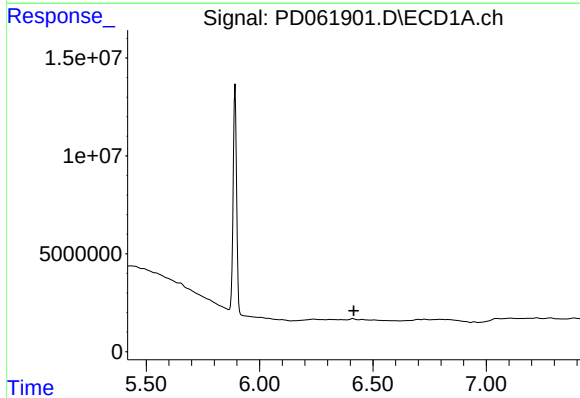


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T.: 6.416 min
Response: 0
Conc: N.D.

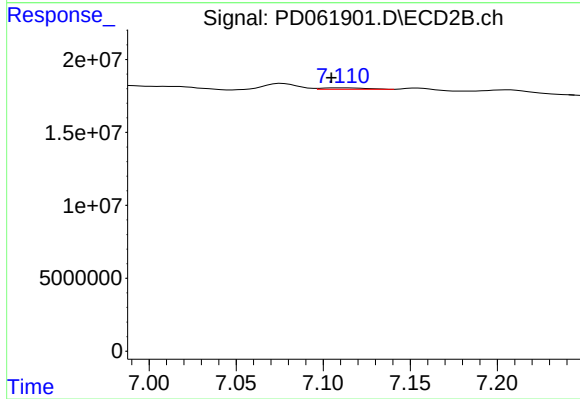

#17 4,4'-DDT


R.T.: 7.111 min
Delta R.T.: 0.006 min
Response: 1859285
Conc: 0.19 ng/ml

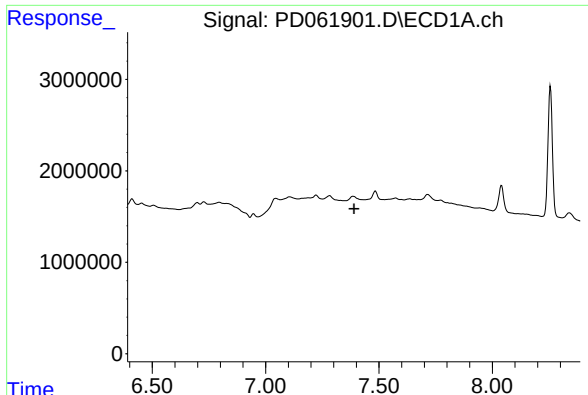

#22 Mirex


R.T.: 0.000 min
Exp R.T.: 7.390 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
B4-0-2

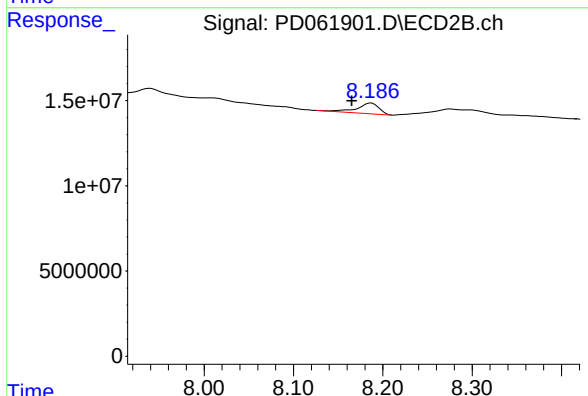


#22 Mirex

R.T.: 8.187 min
Delta R.T.: 0.022 min
Response: 10309242
Conc: 1.60 ng/ml

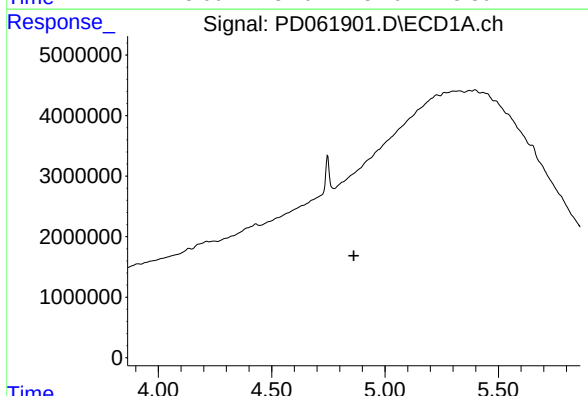


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T.: 4.862 min
Response: 0
Conc: N.D.

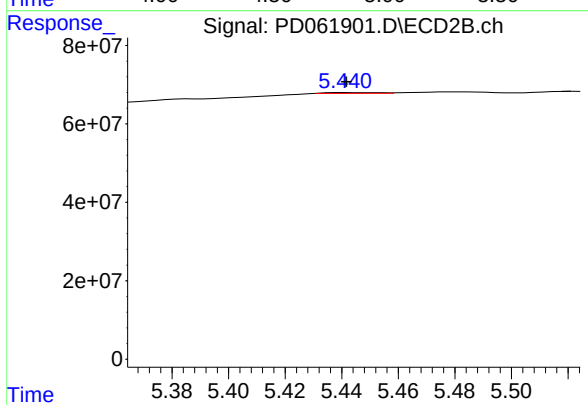

#24 Chlordane-2


R.T.: 5.442 min
Delta R.T.: 0.000 min
Response: 2890980
Conc: 7.53 ng/ml

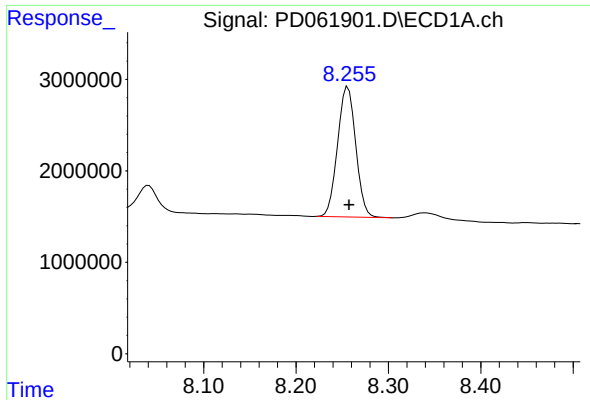

#28 Decachlorobiphenyl

R.T.: 8.256 min
Delta R.T.: -0.001 min
Response: 19473985
Conc: 15.83 ng/ml

Instrument :
ECD_D
ClientSampleId :
B4-0-2

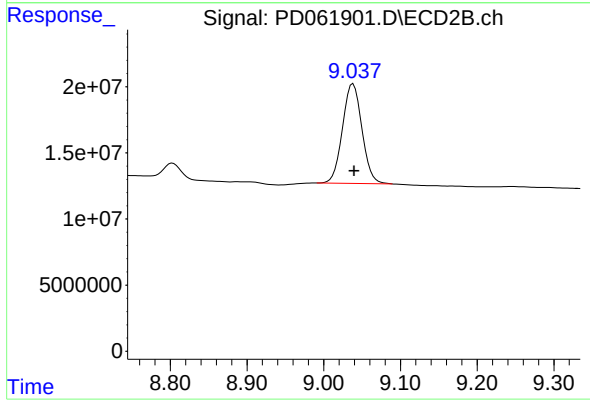

#28 Decachlorobiphenyl

R.T.: 9.038 min
Delta R.T.: -0.002 min
Response: 133525245
Conc: 14.14 ng/ml