

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD033021\
 Data File : PD061863.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Mar 2021 11:36
 Operator : AR\AJ
 Sample : PTOXCCC500
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PTOXCCC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 31 05:55:25 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\DTX032921.M
 Quant Title : GC Extractables
 QLast Update : Tue Mar 30 05:22:59 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.488	3.980	40891466	424.4E6	51.516	51.723
7) SA Decachlor...	8.260	9.040	56492982	411.5E6	47.305	45.812
Target Compounds						
2) Toxaphene-1	5.973	6.556	5618313	52569799	527.314	499.504
3) Toxaphene-2	6.241	7.062	4162694	42237546	472.864	480.836
4) Toxaphene-3	6.606	7.139	9769283	123.6E6	505.363	496.868
5) Toxaphene-4	6.751	7.225	3426823	77212771	494.510	490.666
6) Toxaphene-5	7.032	7.638	4254869	50402096	493.148	463.481

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD033021\
Data File : PD061863.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Mar 2021 11:36
Operator : AR\AJ
Sample : PTOXCCC500
Misc :
ALS Vial : 6 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 31 05:55:25 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\DTX032921.M
Quant Title : GC Extractables
QLast Update : Tue Mar 30 05:22:59 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

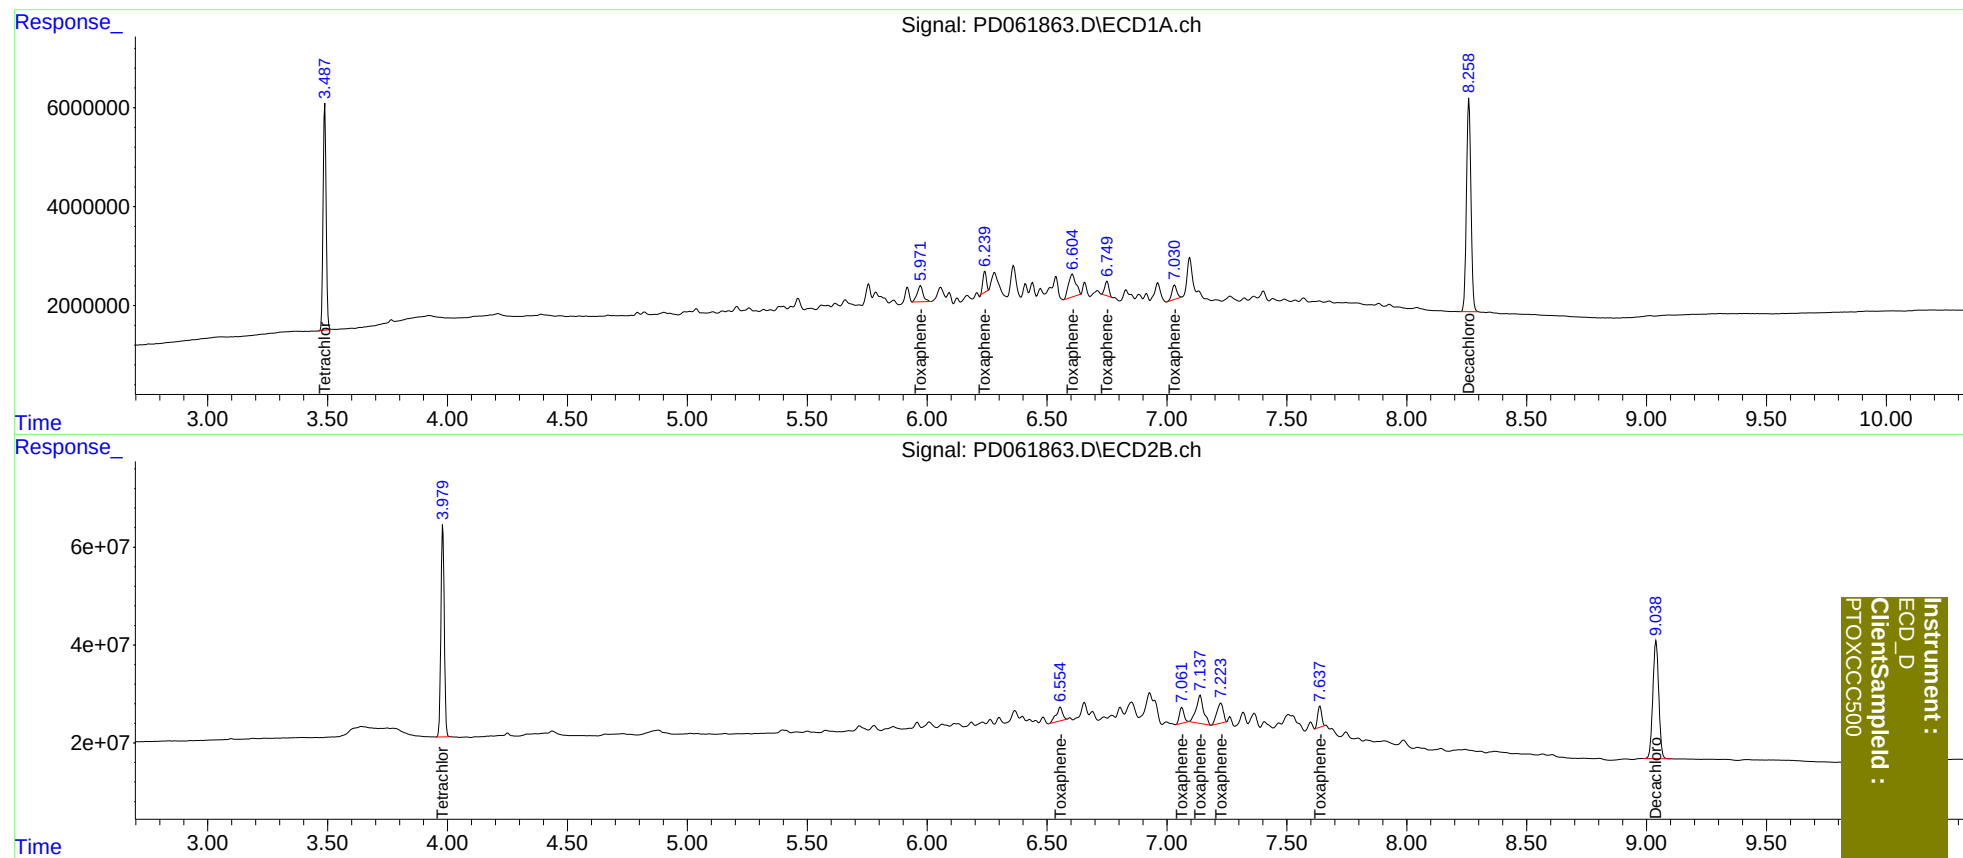

Instrument :
ECD_D
ClientSampled :
PTOXCCC500