

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD033021\
 Data File : PD061863.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Mar 2021 11:36
 Operator : AR\AJ
 Sample : PTOXCCC500
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PTOXCCC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 31 05:55:25 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\DTX032921.M
 Quant Title : GC Extractables
 QLast Update : Tue Mar 30 05:22:59 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.488	3.980	40891466	424.4E6	51.516	51.723
7) SA Decachlor...	8.260	9.040	56492982	411.5E6	47.305	45.812
Target Compounds						
2) Toxaphene-1	5.973	6.556	5618313	52569799	527.314	499.504
3) Toxaphene-2	6.241	7.062	4162694	42237546	472.864	480.836
4) Toxaphene-3	6.606	7.139	9769283	123.6E6	505.363	496.868
5) Toxaphene-4	6.751	7.225	3426823	77212771	494.510	490.666
6) Toxaphene-5	7.032	7.638	4254869	50402096	493.148	463.481

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD033021\
Data File : PD061863.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Mar 2021 11:36
Operator : AR\AJ
Sample : PTOXCCC500
Misc :
ALS Vial : 6 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 31 05:55:25 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\DTX032921.M
Quant Title : GC Extractables
QLast Update : Tue Mar 30 05:22:59 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

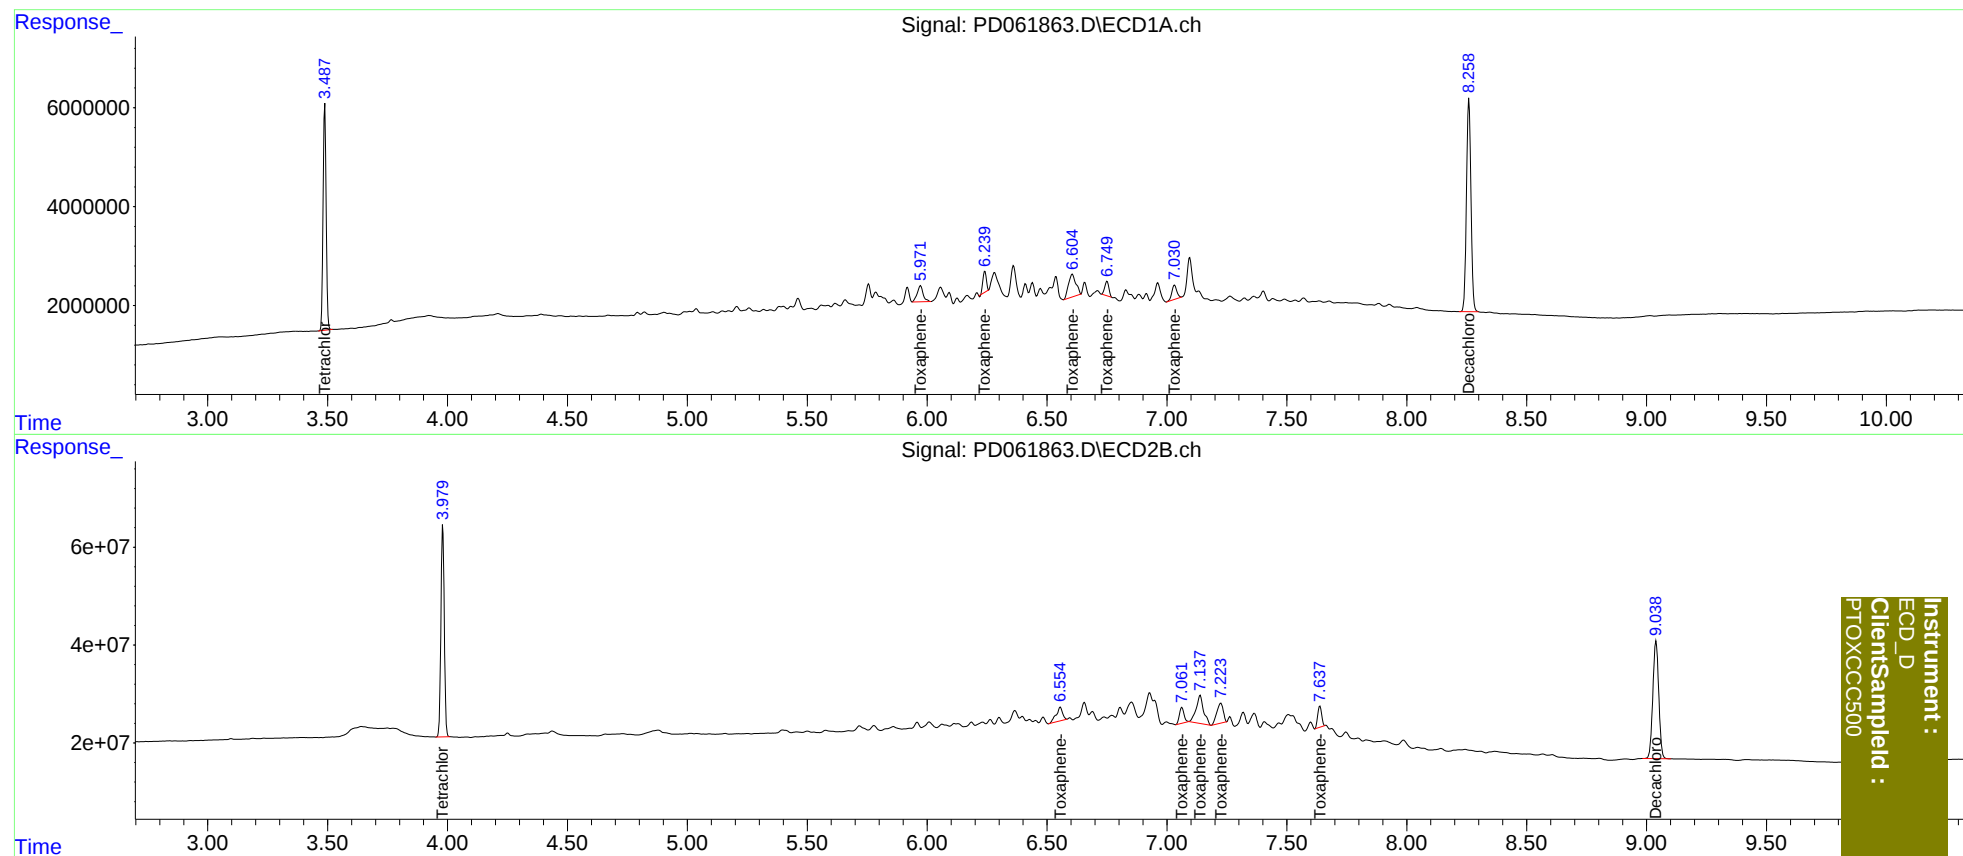


Instrument :
ECD_D
ClientSampled :
PTOXCCC500

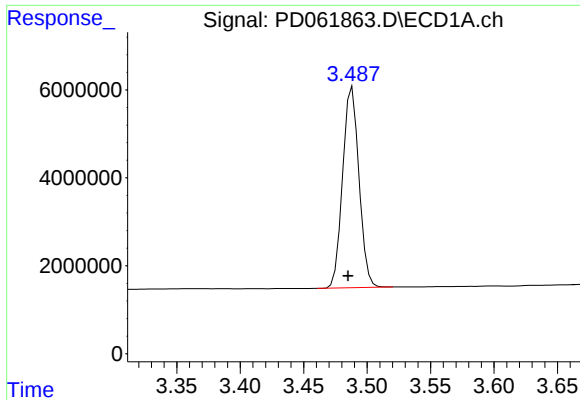

#1 Tetrachloro-m-xylene


R.T.: 3.488 min
Delta R.T.: 0.003 min
Response: 40891466
Conc: 51.52 ng/ml

Instrument :
ECD_D
ClientSampleId :
PTOXCCC500

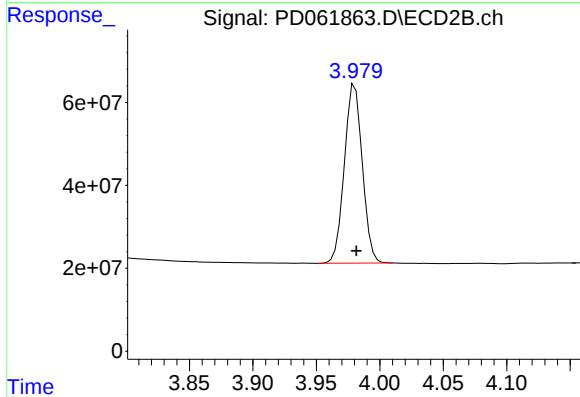


#1 Tetrachloro-m-xylene

R.T.: 3.980 min
Delta R.T.: -0.001 min
Response: 424362771
Conc: 51.72 ng/ml

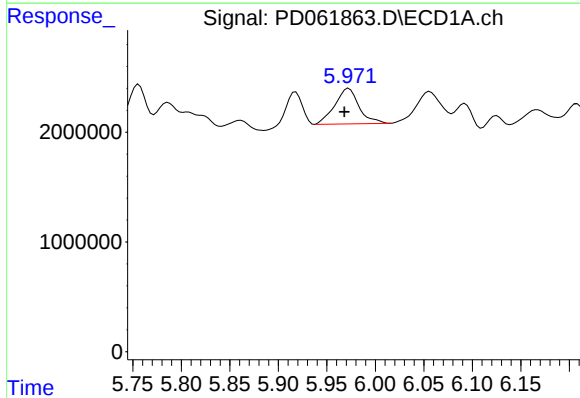


#2 Toxaphene-1

R.T.: 5.973 min
Delta R.T.: 0.005 min
Response: 5618313
Conc: 527.31 ng/ml

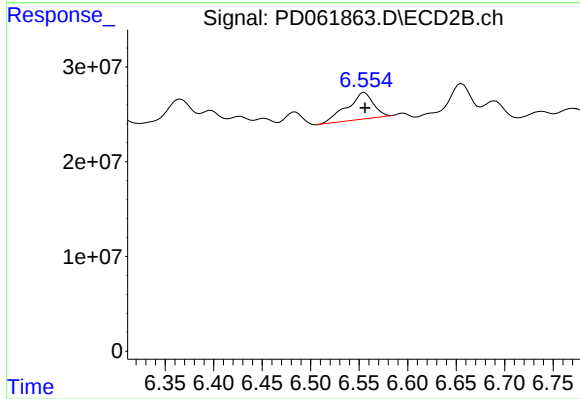

#2 Toxaphene-1


R.T.: 6.556 min
Delta R.T.: 0.000 min
Response: 52569799
Conc: 499.50 ng/ml

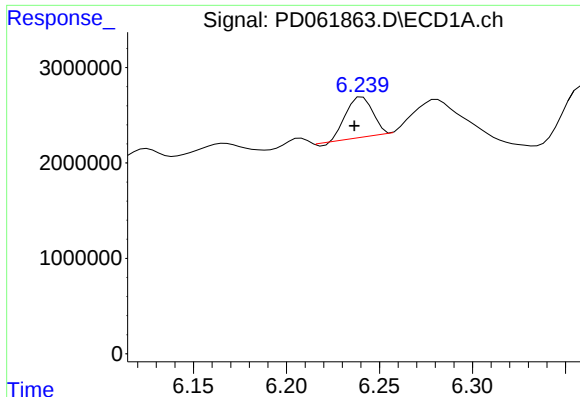

#3 Toxaphene-2


R.T.: 6.241 min
Delta R.T.: 0.004 min
Response: 4162694
Conc: 472.86 ng/ml

Instrument :
ECD_D
ClientSampleId :
PTOXCCC500

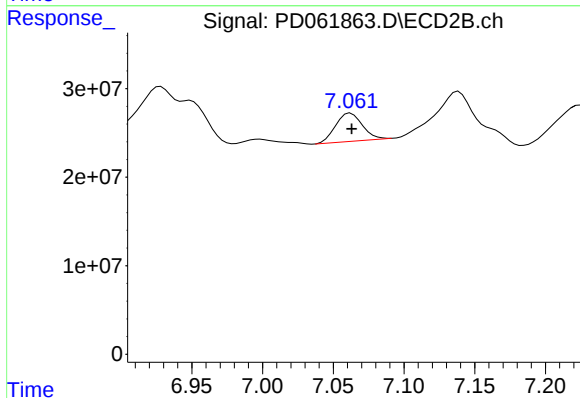


#3 Toxaphene-2

R.T.: 7.062 min
Delta R.T.: 0.000 min
Response: 42237546
Conc: 480.84 ng/ml

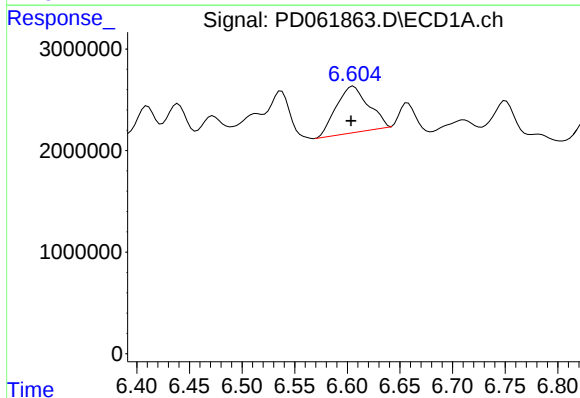


#4 Toxaphene-3

R.T.: 6.606 min
Delta R.T.: 0.002 min
Response: 9769283
Conc: 505.36 ng/ml

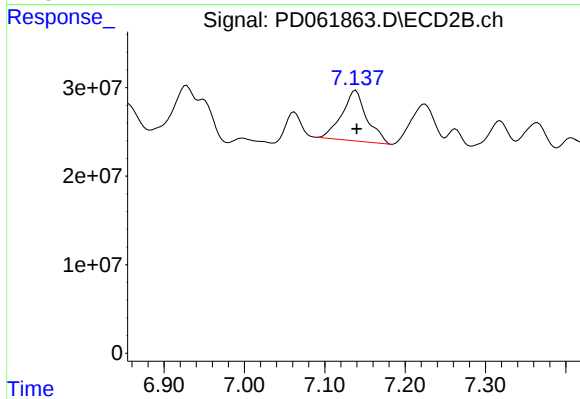

#4 Toxaphene-3


R.T.: 7.139 min
Delta R.T.: 0.000 min
Response: 123638478
Conc: 496.87 ng/ml

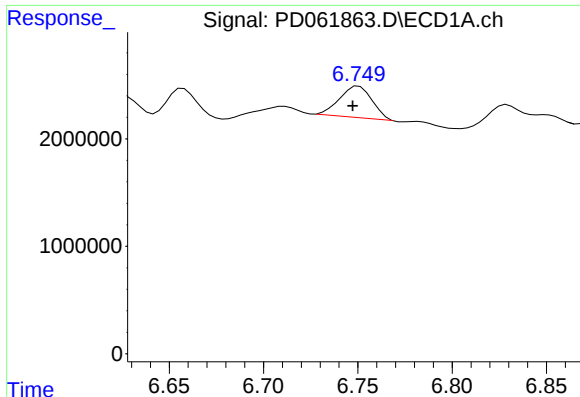

#5 Toxaphene-4


R.T.: 6.751 min
Delta R.T.: 0.003 min
Response: 3426823
Conc: 494.51 ng/ml

Instrument :
ECD_D
ClientSampleId :
PTOXCCC500

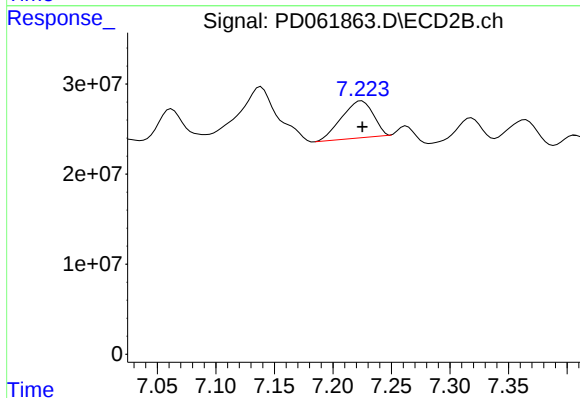


#5 Toxaphene-4

R.T.: 7.225 min
Delta R.T.: 0.000 min
Response: 77212771
Conc: 490.67 ng/ml

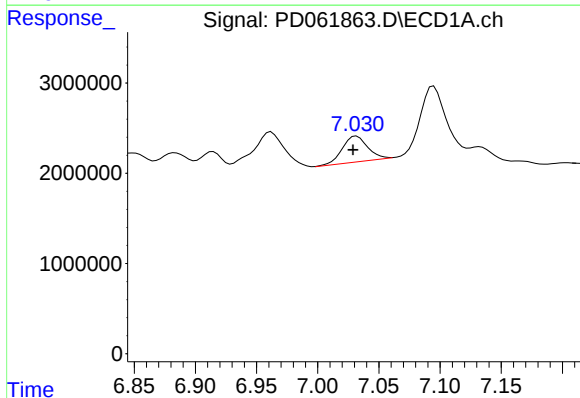


#6 Toxaphene-5

R.T.: 7.032 min
Delta R.T.: 0.003 min
Response: 4254869
Conc: 493.15 ng/ml

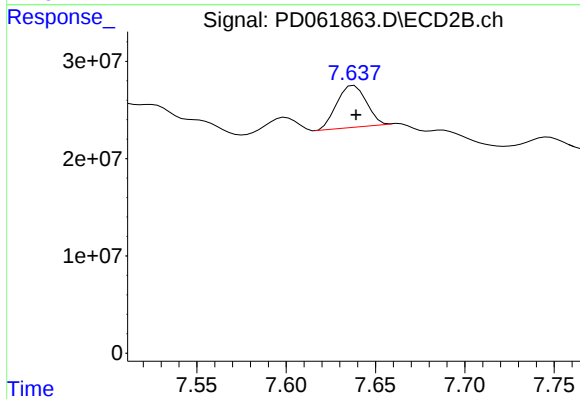

#6 Toxaphene-5


R.T.: 7.638 min
Delta R.T.: -0.001 min
Response: 50402096
Conc: 463.48 ng/ml

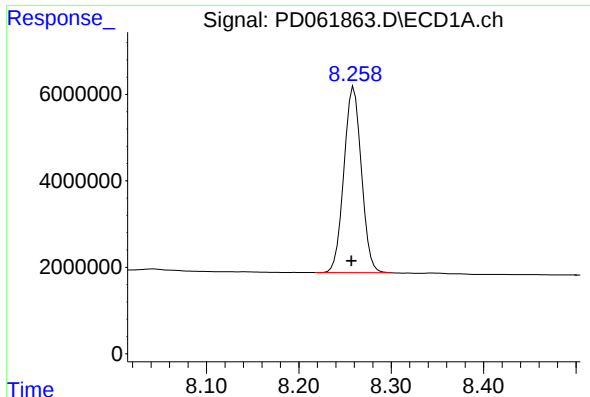

#7 Decachlorobiphenyl

R.T.: 8.260 min
Delta R.T.: 0.003 min
Response: 56492982
Conc: 47.31 ng/ml

Instrument :
ECD_D
ClientSampleId :
PTOXCCC500

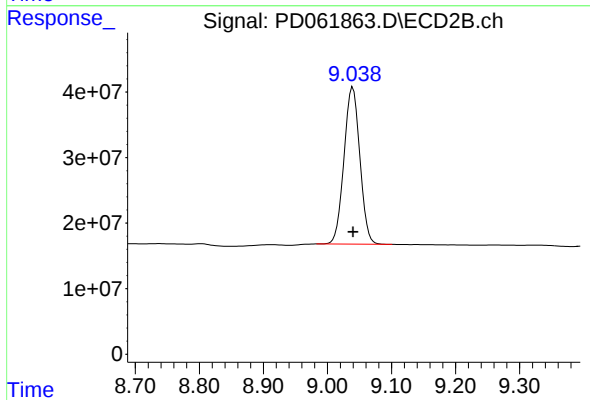

#7 Decachlorobiphenyl

R.T.: 9.040 min
Delta R.T.: 0.000 min
Response: 411453205
Conc: 45.81 ng/ml