

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD033021\
 Data File : PD061866.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Mar 2021 12:34
 Operator : AR\AJ
 Sample : PB135397BS
 Misc : CHLOR BS
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PB135397BS

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 01 13:23:10 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032921.M
 Quant Title : GC Extractables
 QLast Update : Tue Mar 30 04:47:56 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.485	3.981	20272591	195.4E6	24.212	22.487
28)	SA Decachlor...	8.255	9.037	27386468	199.7E6	22.258	21.157
Target Compounds							
23)	Chlordane-1	4.360	4.973	6464483	83032507	203.443	214.031
24)	Chlordane-2	4.863	5.440	8160524	72353652	209.185	188.561m
25)	Chlordane-3	5.434	6.085	22812559	328.7E6	196.641	198.261m
26)	Chlordane-4	5.492	6.160	18333190	388.9E6	190.559	202.666
27)	Chlordane-5	6.332	6.963	8545951	68708875	194.077	190.646



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD033021\
Data File : PD061866.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Mar 2021 12:34
Operator : AR\AJ
Sample : PB135397BS
Misc : CHLOR BS
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PB135397BS

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 01 13:23:10 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032921.M
Quant Title : GC Extractables
QLast Update : Tue Mar 30 04:47:56 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

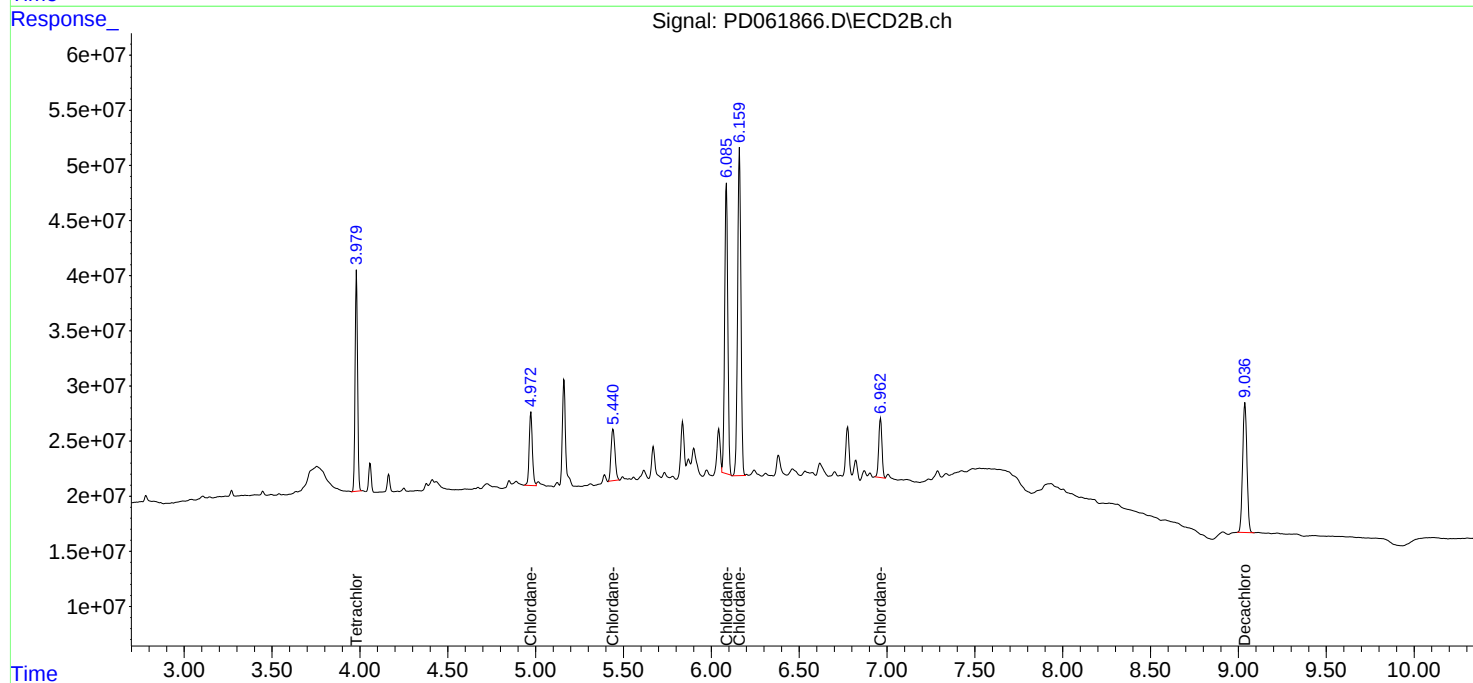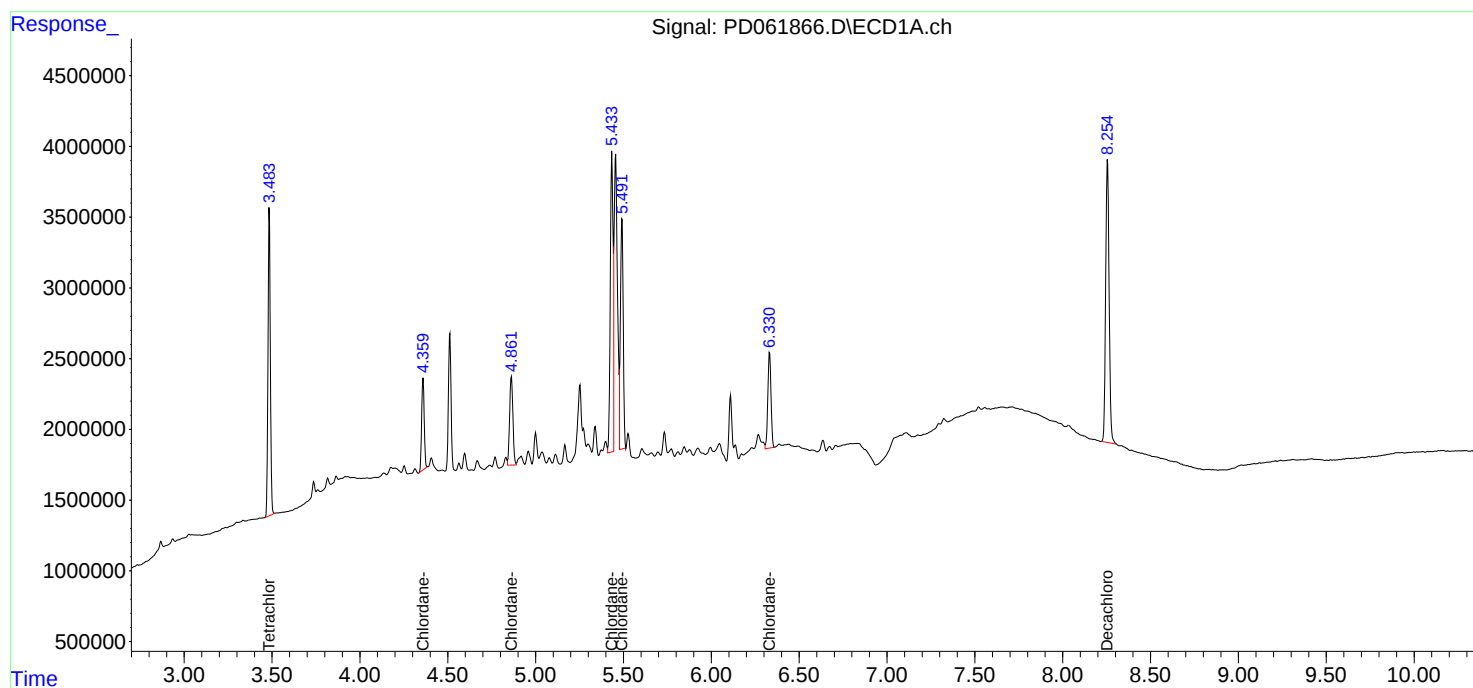


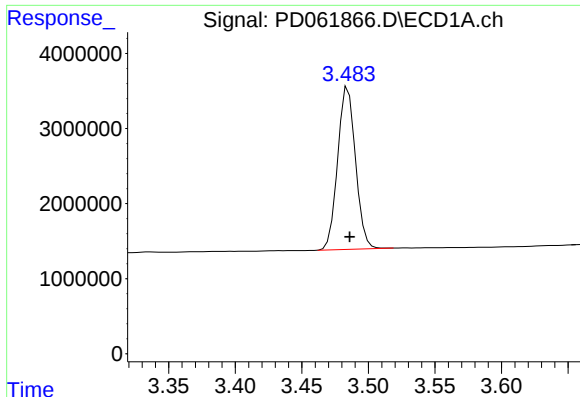

#1 Tetrachloro-m-xylene


R.T.: 3.485 min
Delta R.T.: -0.001 min
Response: 20272591
Conc: 24.21 ng/ml

Instrument :
ECD_D
ClientSampleId :
PB135397BS

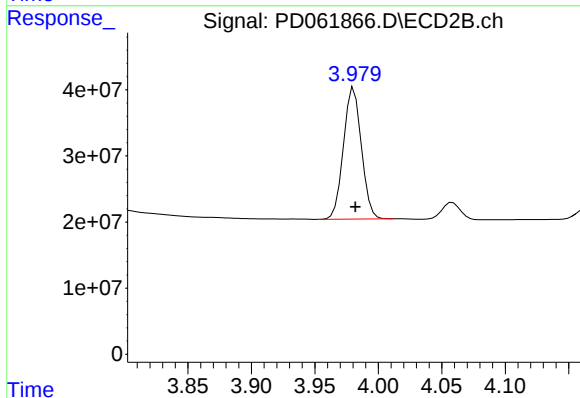


#1 Tetrachloro-m-xylene

R.T.: 3.981 min
Delta R.T.: -0.001 min
Response: 195387588
Conc: 22.49 ng/ml

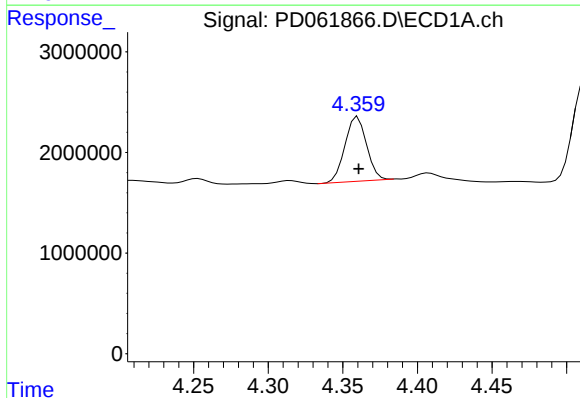


#23 Chlordane-1

R.T.: 4.360 min
Delta R.T.: 0.000 min
Response: 6464483
Conc: 203.44 ng/ml

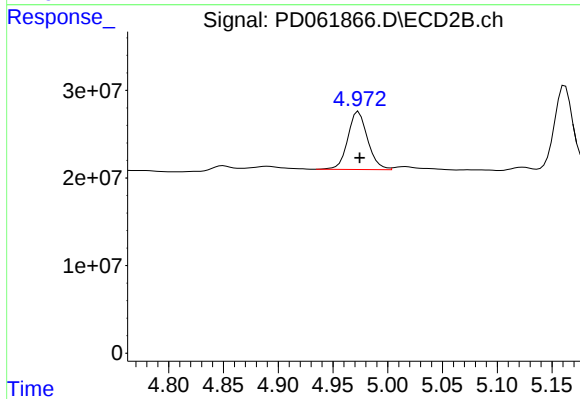

#23 Chlordane-1


R.T.: 4.973 min
Delta R.T.: -0.001 min
Response: 83032507
Conc: 214.03 ng/ml

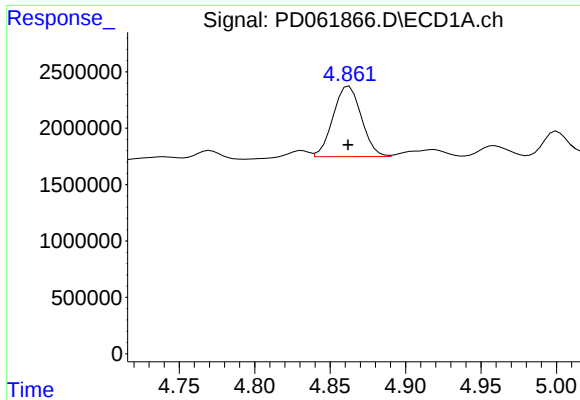

#24 Chlordane-2


R.T.: 4.863 min
Delta R.T.: 0.000 min
Response: 8160524
Conc: 209.18 ng/ml

Instrument :
ECD_D
ClientSampleId :
PB135397BS

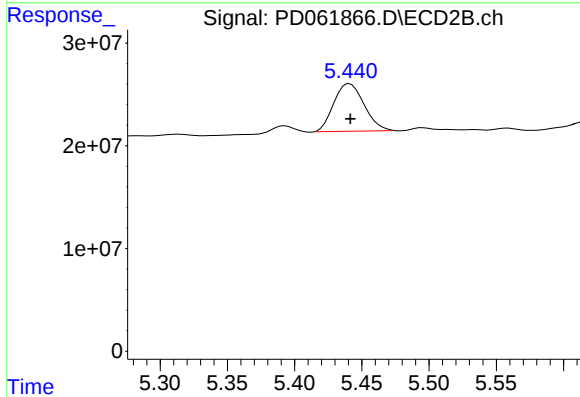


#24 Chlordane-2

R.T.: 5.440 min
Delta R.T.: -0.002 min
Response: 72353652
Conc: 188.56 ng/ml m

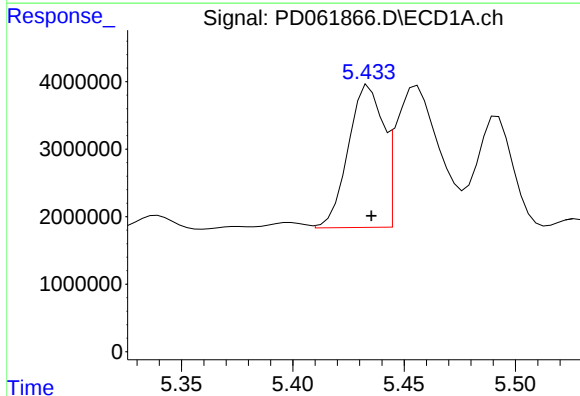


#25 Chlordane-3

R.T.: 5.434 min
Delta R.T.: 0.000 min
Response: 22812559
Conc: 196.64 ng/ml

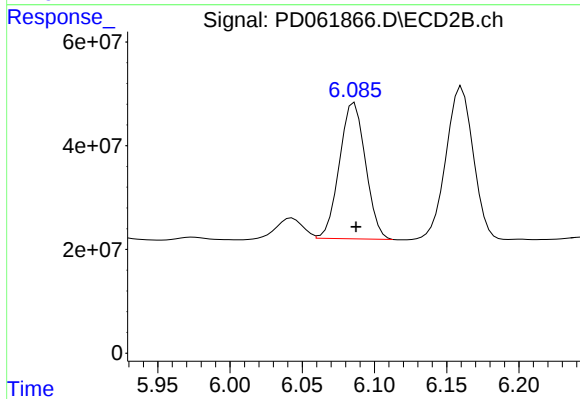

#25 Chlordane-3


R.T.: 6.085 min
Delta R.T.: -0.003 min
Response: 328665415
Conc: 198.26 ng/ml m

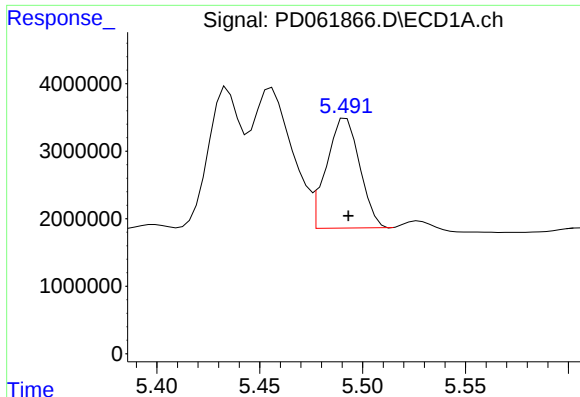

#26 Chlordane-4


R.T.: 5.492 min
Delta R.T.: 0.000 min
Response: 18333190
Conc: 190.56 ng/ml

Instrument :
ECD_D
ClientSampleId :
PB135397BS

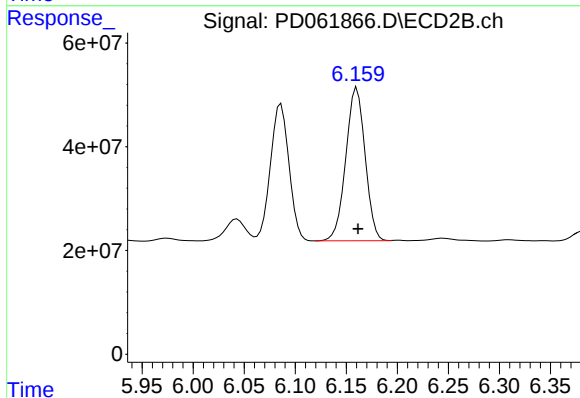


#26 Chlordane-4

R.T.: 6.160 min
Delta R.T.: 0.000 min
Response: 388905956
Conc: 202.67 ng/ml

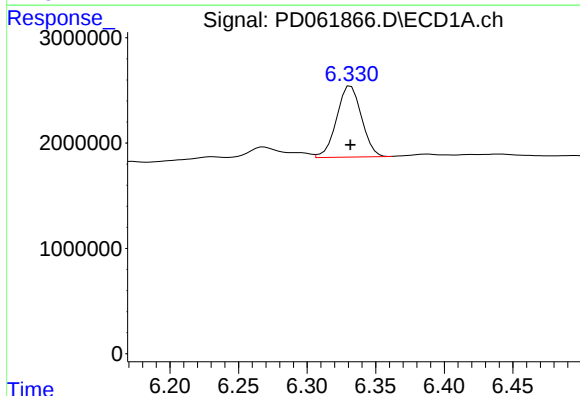


#27 Chlordane-5

R.T.: 6.332 min
Delta R.T.: 0.000 min
Response: 8545951
Conc: 194.08 ng/ml

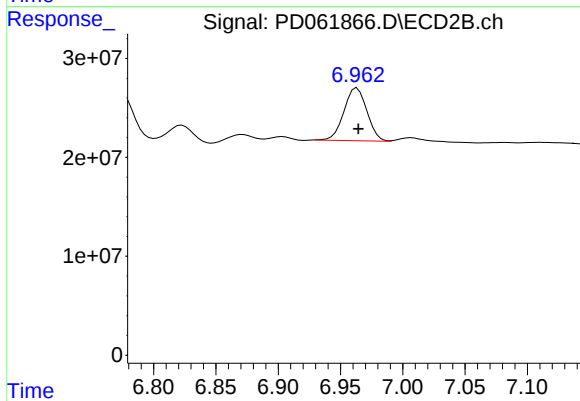

#27 Chlordane-5


R.T.: 6.963 min
Delta R.T.: -0.001 min
Response: 68708875
Conc: 190.65 ng/ml

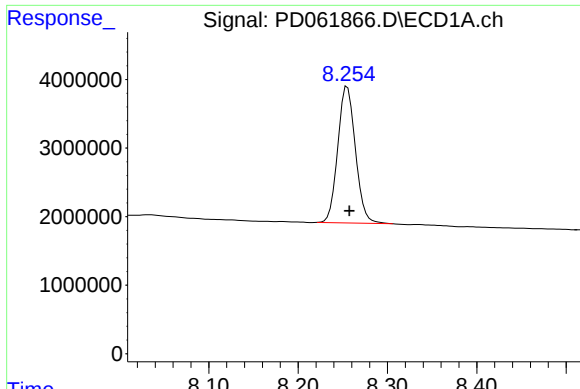

#28 Decachlorobiphenyl

R.T.: 8.255 min
Delta R.T.: -0.002 min
Response: 27386468
Conc: 22.26 ng/ml

Instrument :
ECD_D
ClientSampleId :
PB135397BS

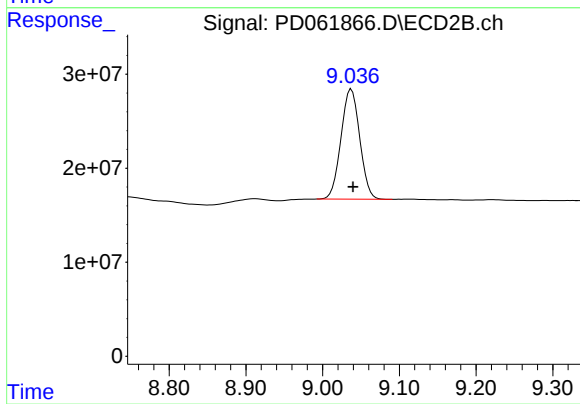

#28 Decachlorobiphenyl

R.T.: 9.037 min
Delta R.T.: -0.002 min
Response: 199736243
Conc: 21.16 ng/ml