

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD033021\
 Data File : PD061872.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Mar 2021 15:00
 Operator : AR\AJ
 Sample : M1828-01
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 FS-SB13(5-6)

Manual Integrations
 APPROVED

Ankita
 4/1/2021 2:36:29 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 31 04:21:29 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032921.M
 Quant Title : GC Extractables
 QLast Update : Tue Mar 30 04:47:56 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.486	3.981	16598079	169.6E6	19.823	19.515
28)	SA Decachlor...	8.257	9.037	17888147	138.0E6	14.538	14.614
Target Compounds							
12)	B 4,4'-DDE	5.656	6.313	2520816	29903848	2.243	2.595
17)	MA 4,4'-DDT	6.414	7.105	972326	8601466	1.079m	0.901

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD033021\
Data File : PD061872.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Mar 2021 15:00
Operator : AR\AJ
Sample : M1828-01
Misc :
ALS Vial : 12 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
FS-SB13(5-6)


Manual Integrations
APPROVED

Ankita
4/1/2021 2:36:29 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 31 04:21:29 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032921.M
Quant Title : GC Extractables
QLast Update : Tue Mar 30 04:47:56 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

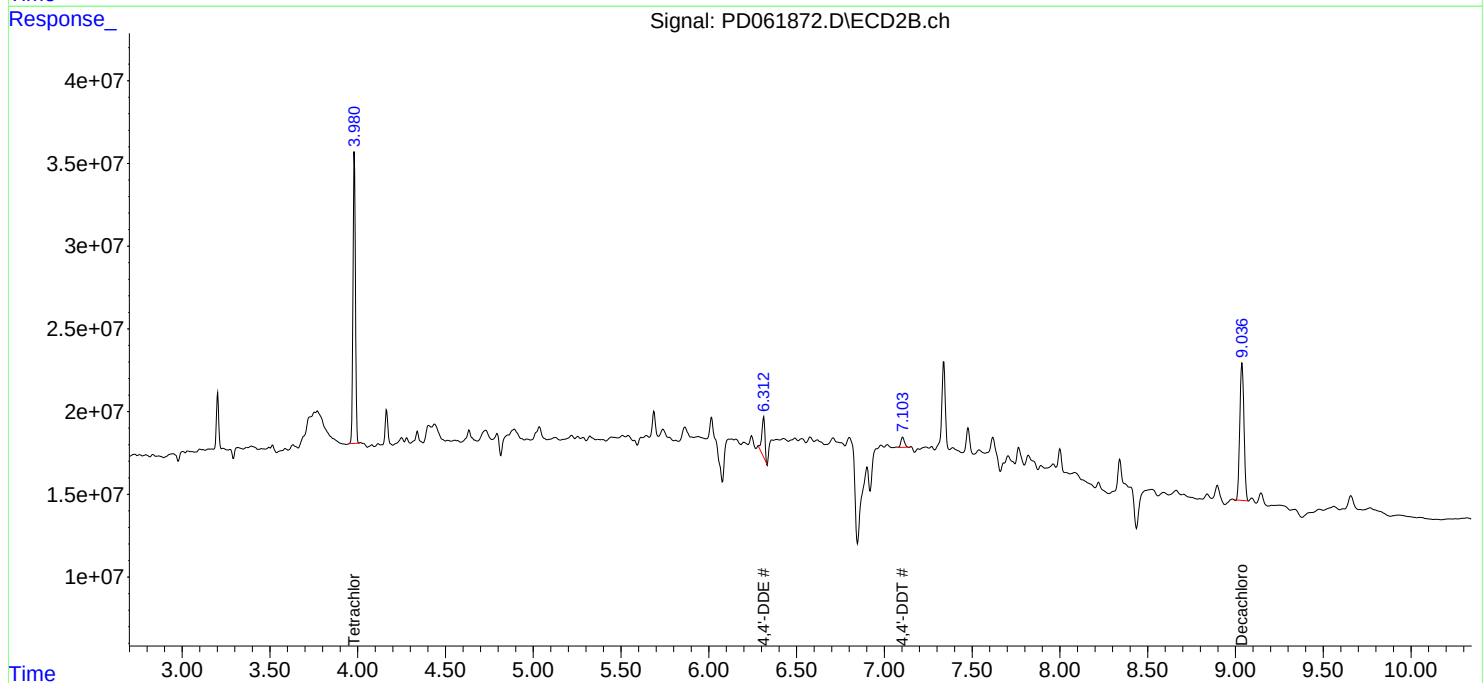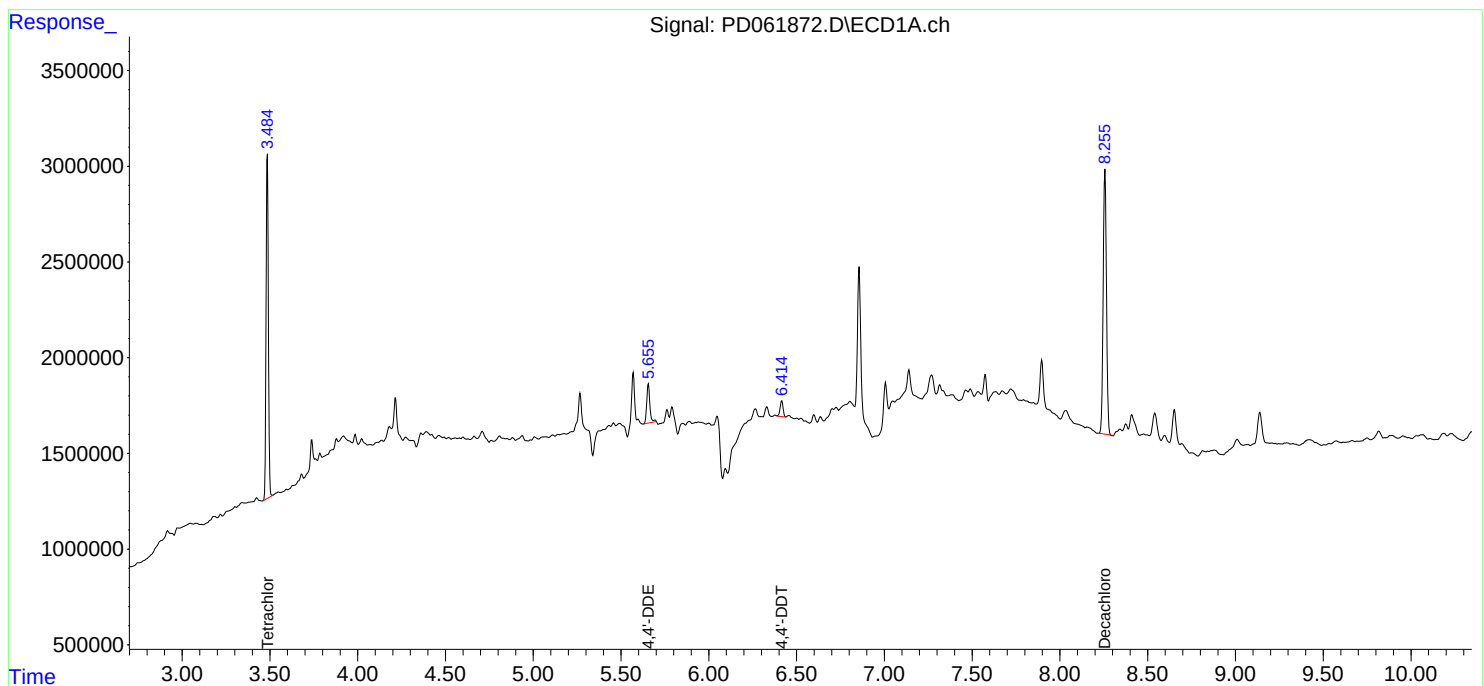

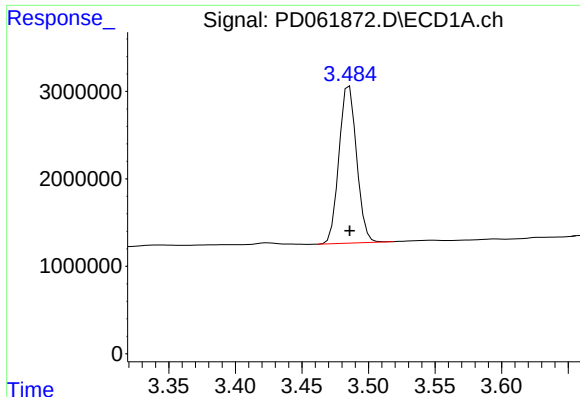


#1 Tetrachloro-m-xylene

R.T.: 3.486 min
Delta R.T.: 0.000 min
Response: 16598079
Conc: 19.82 ng/ml

Instrument :
ECD_D
ClientSampleId :
FS-SB13(5-6)


Manual Integrations
APPROVED

Ankita
4/1/2021 2:36:29 PM

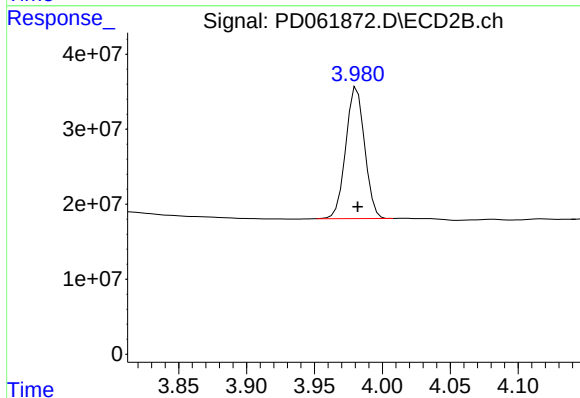


#1 Tetrachloro-m-xylene

R.T.: 3.981 min
Delta R.T.: 0.000 min
Response: 169561348
Conc: 19.51 ng/ml

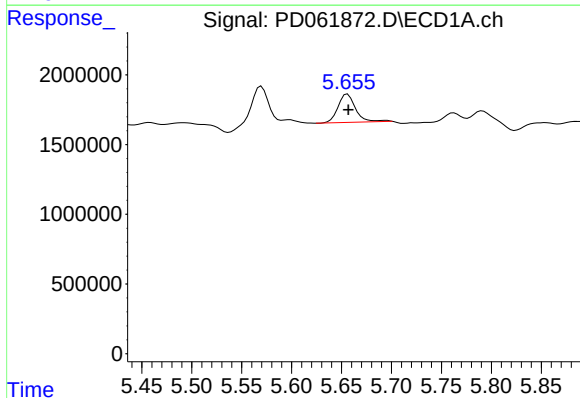


#12 4,4'-DDE

R.T.: 5.656 min
Delta R.T.: 0.000 min
Response: 2520816
Conc: 2.24 ng/ml

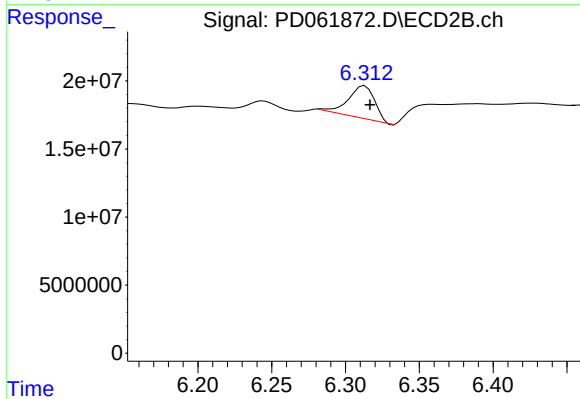

#12 4,4'-DDE

R.T.: 6.313 min
Delta R.T.: -0.004 min
Response: 29903848
Conc: 2.59 ng/ml

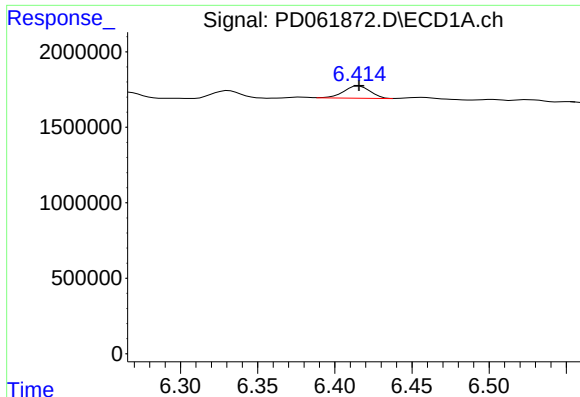


#17 4,4'-DDT

R.T.: 6.414 min
Delta R.T.: -0.002 min
Response: 972326
Conc: 1.08 ng/ml m

Instrument :
ECD_D
ClientSampleId :
FS-SB13(5-6)


Manual Integrations
APPROVED

Ankita
4/1/2021 2:36:29 PM

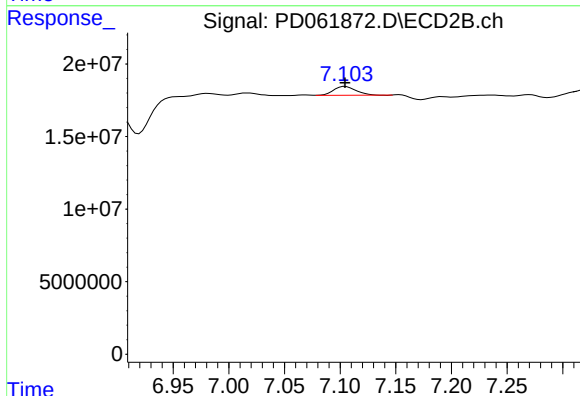


#17 4,4'-DDT

R.T.: 7.105 min
Delta R.T.: 0.000 min
Response: 8601466
Conc: 0.90 ng/ml

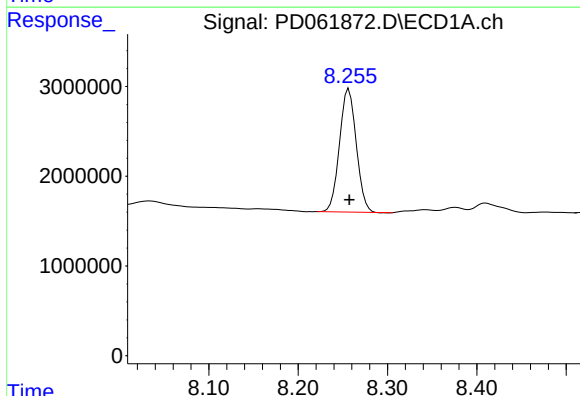

#28 Decachlorobiphenyl

R.T.: 8.257 min
Delta R.T.: 0.000 min
Response: 17888147
Conc: 14.54 ng/ml

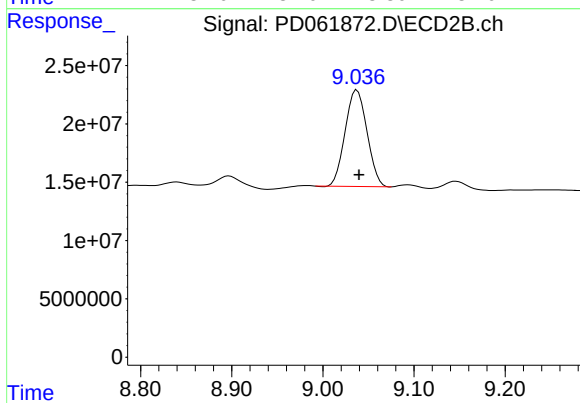

#28 Decachlorobiphenyl

R.T.: 9.037 min
Delta R.T.: -0.002 min
Response: 137967053
Conc: 14.61 ng/ml