

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD033021\
 Data File : PD061899.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Mar 2021 22:54
 Operator : AR\AJ
 Sample : M1836-06
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 B3-10-12

Manual Integrations
 APPROVED

Ankita
 4/1/2021 2:36:56 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 31 04:52:15 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032921.M
 Quant Title : GC Extractables
 QLast Update : Tue Mar 30 04:47:56 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.485	3.982	14382097	129.4E6	17.177	14.889
28)	SA Decachlor...	8.256	9.039	18759916	120.9E6	15.247	12.808
Target Compounds							
12)	B 4,4'-DDE	5.655	6.317	789616	5869998	0.703m	0.509 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD033021\
Data File : PD061899.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Mar 2021 22:54
Operator : AR\AJ
Sample : M1836-06
Misc :
ALS Vial : 35 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
B3-10-12


Manual Integrations
APPROVED

Ankita
4/1/2021 2:36:56 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 31 04:52:15 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032921.M
Quant Title : GC Extractables
QLast Update : Tue Mar 30 04:47:56 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

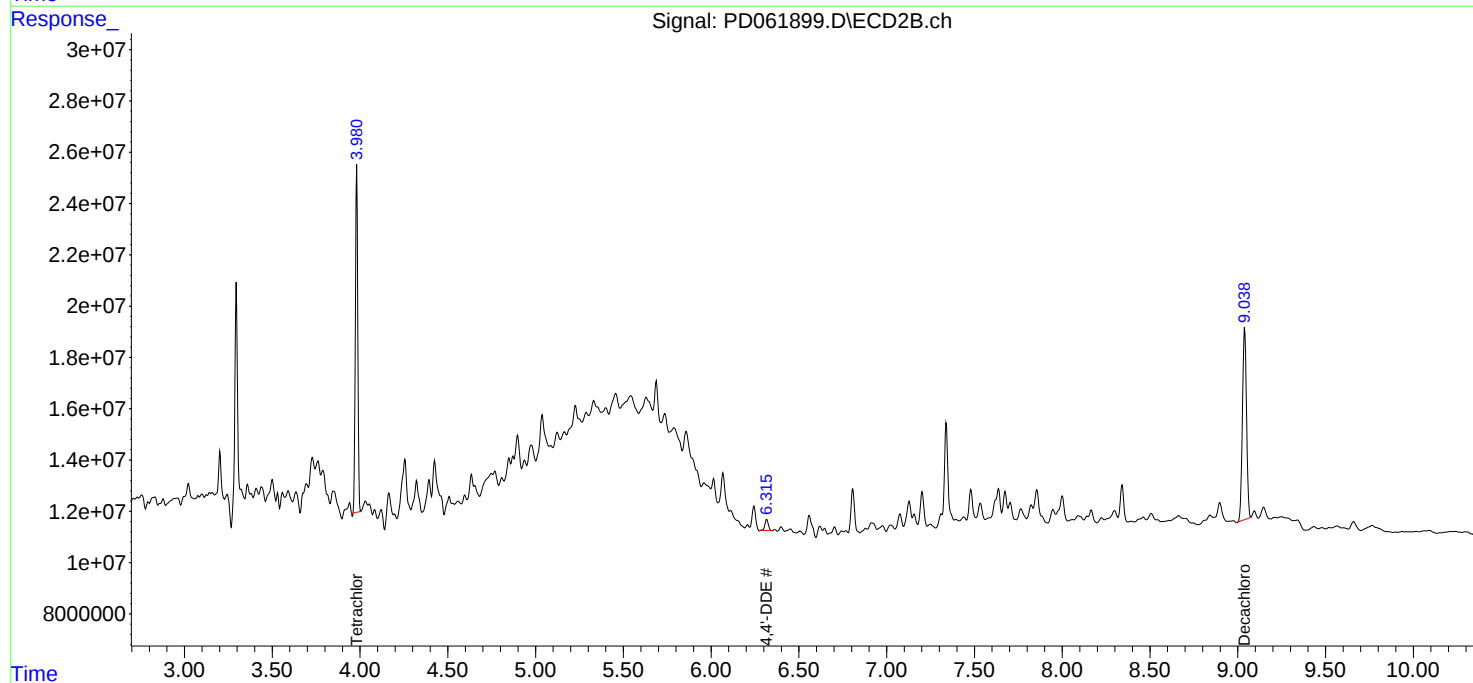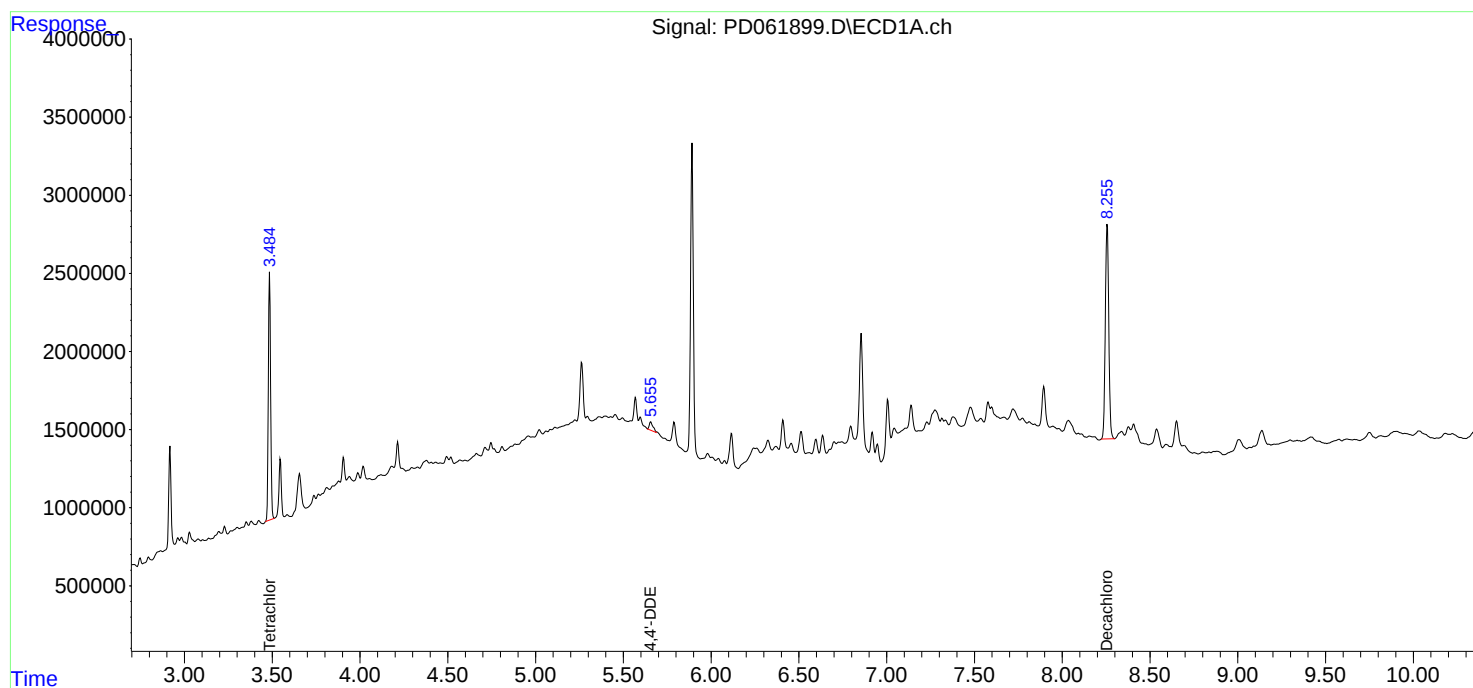

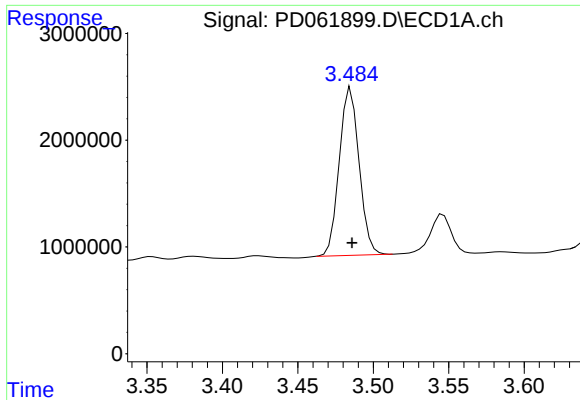


#1 Tetrachloro-m-xylene

R.T.: 3.485 min
Delta R.T.: 0.000 min
Response: 14382097
Conc: 17.18 ng/ml

Instrument :
ECD_D
ClientSampleId :
B3-10-12


Manual Integrations
APPROVED

Ankita
4/1/2021 2:36:56 PM

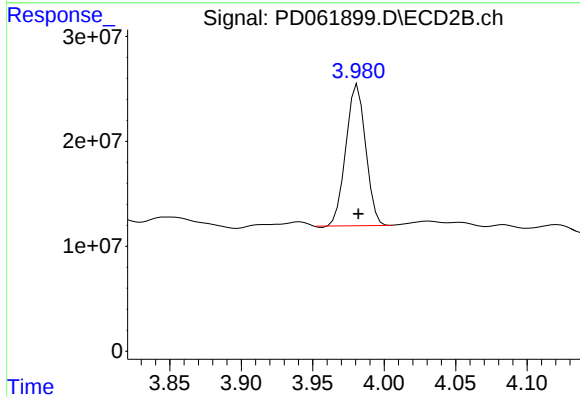


#1 Tetrachloro-m-xylene

R.T.: 3.982 min
Delta R.T.: 0.000 min
Response: 129366146
Conc: 14.89 ng/ml

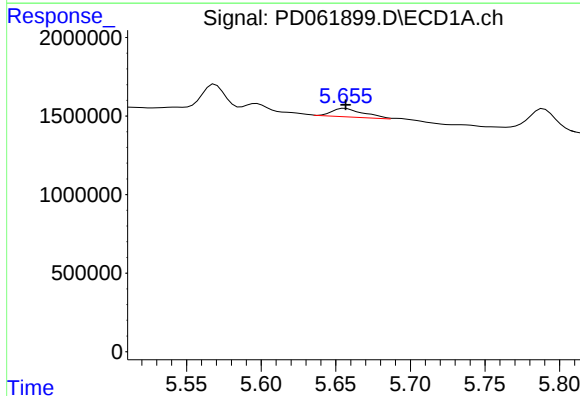


#12 4,4'-DDE

R.T.: 5.655 min
Delta R.T.: -0.002 min
Response: 789616
Conc: 0.70 ng/ml m

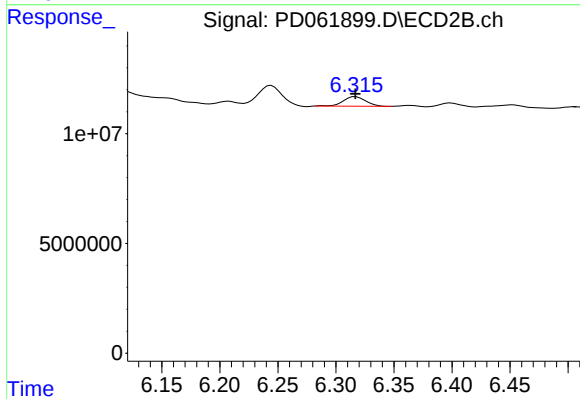

#12 4,4'-DDE

R.T.: 6.317 min
Delta R.T.: 0.000 min
Response: 5869998
Conc: 0.51 ng/ml

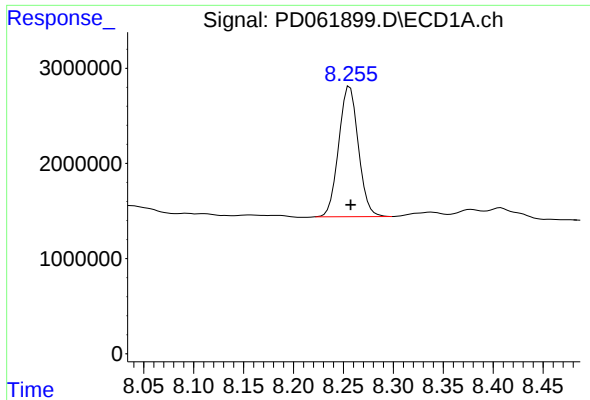

#28 Decachlorobiphenyl

R.T.: 8.256 min

Delta R.T.: -0.001 min


Response: 18759916

Conc: 15.25 ng/ml

Instrument :
ECD_D
ClientSampleId :
B3-10-12

Manual Integrations
APPROVED

Ankita
4/1/2021 2:36:56 PM

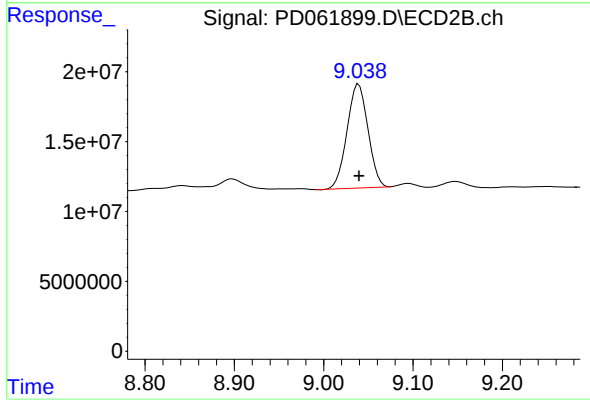

#28 Decachlorobiphenyl

R.T.: 9.039 min

Delta R.T.: 0.000 min

Response: 120912898

Conc: 12.81 ng/ml