

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD033021\
 Data File : PD061902.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Mar 2021 23:36
 Operator : AR\AJ
 Sample : M1836-09
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 B4-8-10

Manual Integrations
 APPROVED

Ankita
 4/1/2021 2:36:58 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 31 04:55:34 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032921.M
 Quant Title : GC Extractables
 QLast Update : Tue Mar 30 04:47:56 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.485	3.979	10406031	113.0E6	12.428	13.005m
28)	SA Decachlor...	8.256	9.037	16078902	104.5E6	13.068	11.065

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD033021\
Data File : PD061902.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Mar 2021 23:36
Operator : AR\AJ
Sample : M1836-09
Misc :
ALS Vial : 38 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
B4-8-10


Manual Integrations
APPROVED

Ankita
4/1/2021 2:36:58 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 31 04:55:34 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032921.M
Quant Title : GC Extractables
QLast Update : Tue Mar 30 04:47:56 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

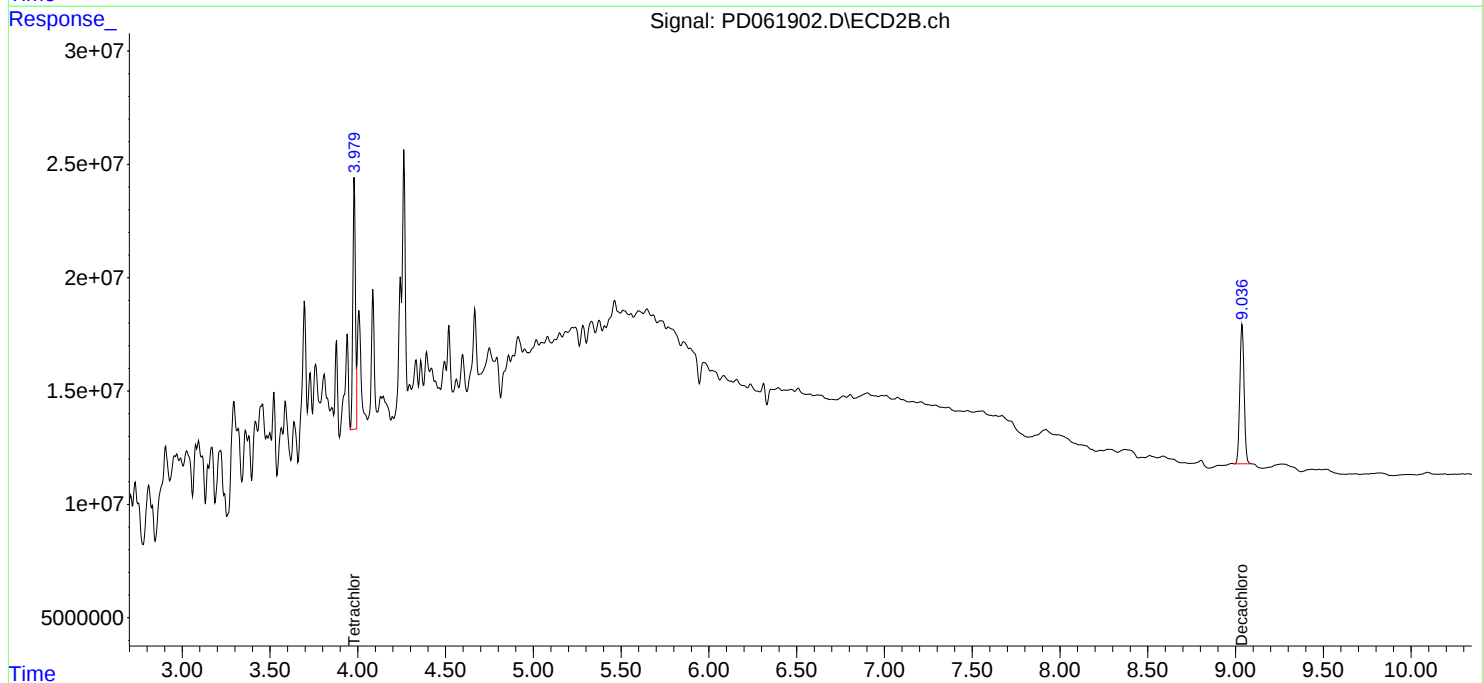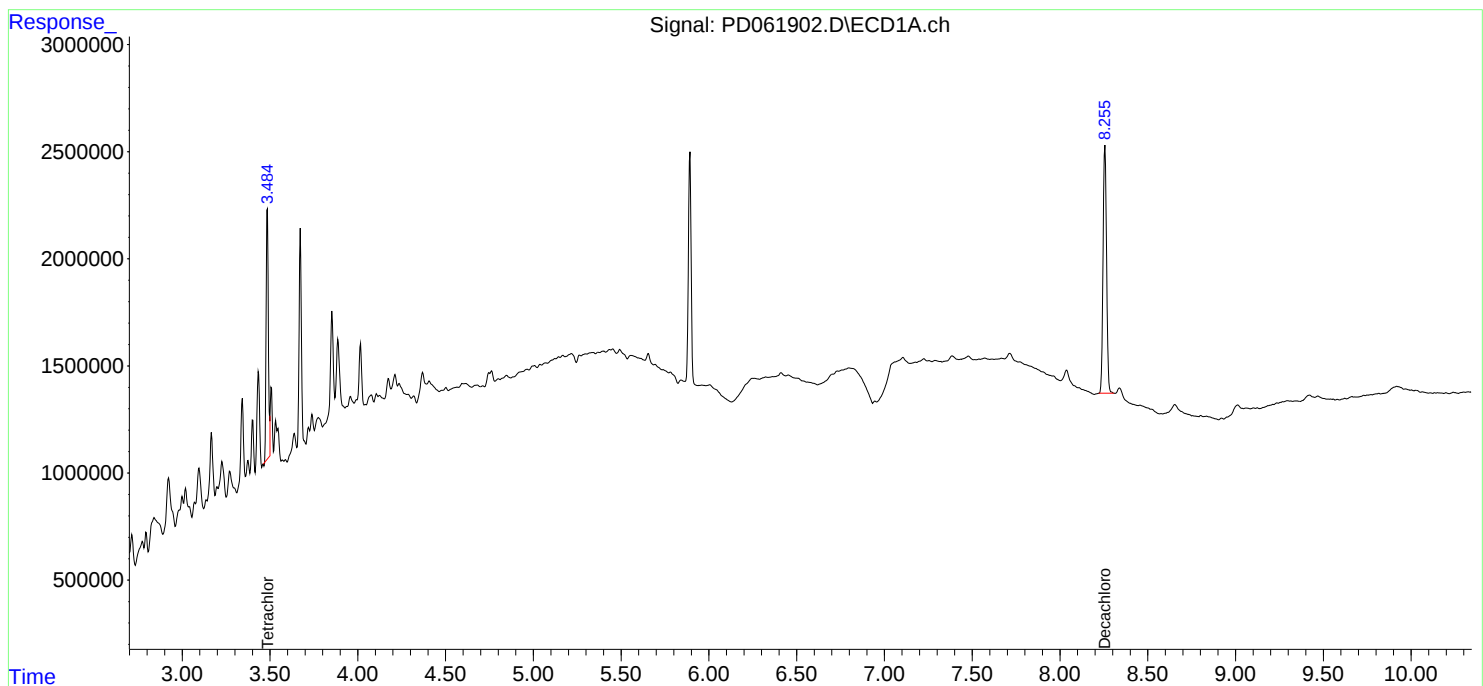

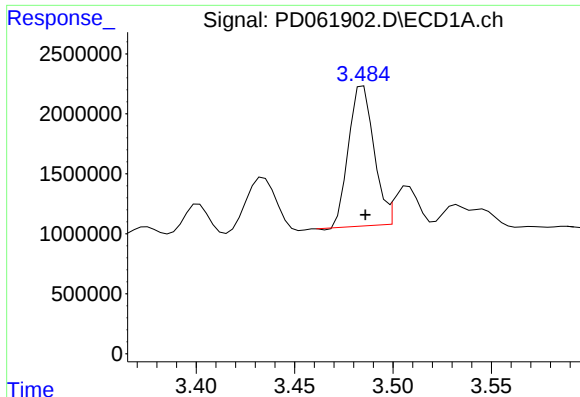


#1 Tetrachloro-m-xylene

R.T.: 3.485 min
Delta R.T.: -0.001 min
Response: 10406031
Conc: 12.43 ng/ml

Instrument :
ECD_D
ClientSampleId :
B4-8-10


Manual Integrations
APPROVED

Ankita
4/1/2021 2:36:58 PM

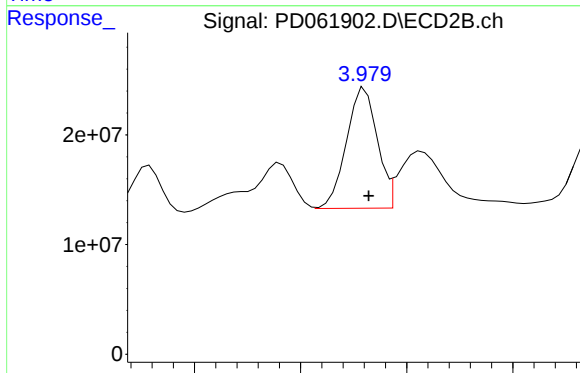


#1 Tetrachloro-m-xylene

R.T.: 3.979 min
Delta R.T.: -0.003 min
Response: 112998459
Conc: 13.00 ng/ml m

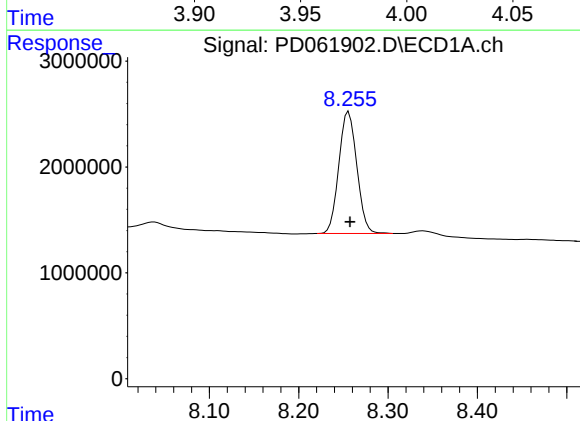

#28 Decachlorobiphenyl

R.T.: 8.256 min
Delta R.T.: -0.001 min
Response: 16078902
Conc: 13.07 ng/ml

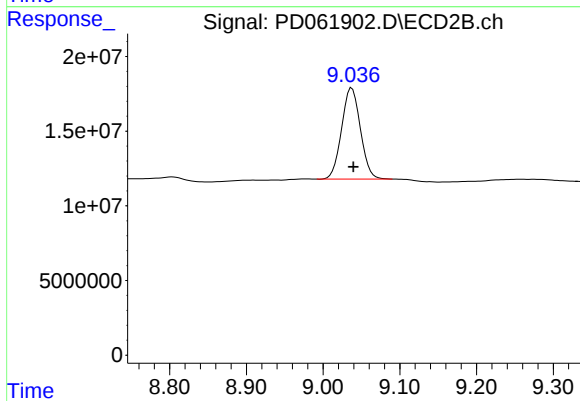

#28 Decachlorobiphenyl

R.T.: 9.037 min
Delta R.T.: -0.002 min
Response: 104457813
Conc: 11.06 ng/ml